

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\P0041320\
 Data File : P0067822.D
 Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
 Acq On : 13 Apr 2020 16:43
 Operator : DD\AJ
 Sample : I.BLK
 Misc :
 ALS Vial : 2 Sample Multiplier: 1

Instrument :
 ECD_O
 ClientSampleId :

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Apr 13 18:01:28 2020
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\P0040120.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Fri Apr 03 16:04:09 2020
 Response via : Initial Calibration
 Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	4.929	3.941	591711	776244	24.847	23.160
2)	SA Decachlor...	10.911	9.228	738190	894653	21.684	21.638
Target Compounds							
30)	L6 AR-1254-5	8.516	0.000	24100	0	14.047	N.D. #
33)	L7 AR-1260-3	8.516	0.000	24100	0	18.489	N.D. #
35)	L7 AR-1260-5	9.118	0.000	12375	0	3.923	N.D. #
36)	L8 AR-1262-1	8.516	0.000	24100	0	14.376	N.D. #
37)	L8 AR-1262-2	9.118	0.000	12375	0	4.313	N.D. #
43)	L9 AR-1268-3	9.701	0.000	389013	0	133.969	N.D. #
45)	L9 AR-1268-5	10.581	0.000	509602	0	51.400	N.D. #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\P0041320\
Data File : P0067822.D
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
Acq On : 13 Apr 2020 16:43
Operator : DD\AJ
Sample : I.BLK
Misc :
ALS Vial : 2 Sample Multiplier: 1

Instrument :
ECD_O
ClientSampleId :

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Apr 13 18:01:28 2020
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\P0040120.M
Quant Title : GC EXTRACTABLES
QLast Update : Fri Apr 03 16:04:09 2020
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µm Signal #2 Info : 30M x 0.32mm x 0.25µm

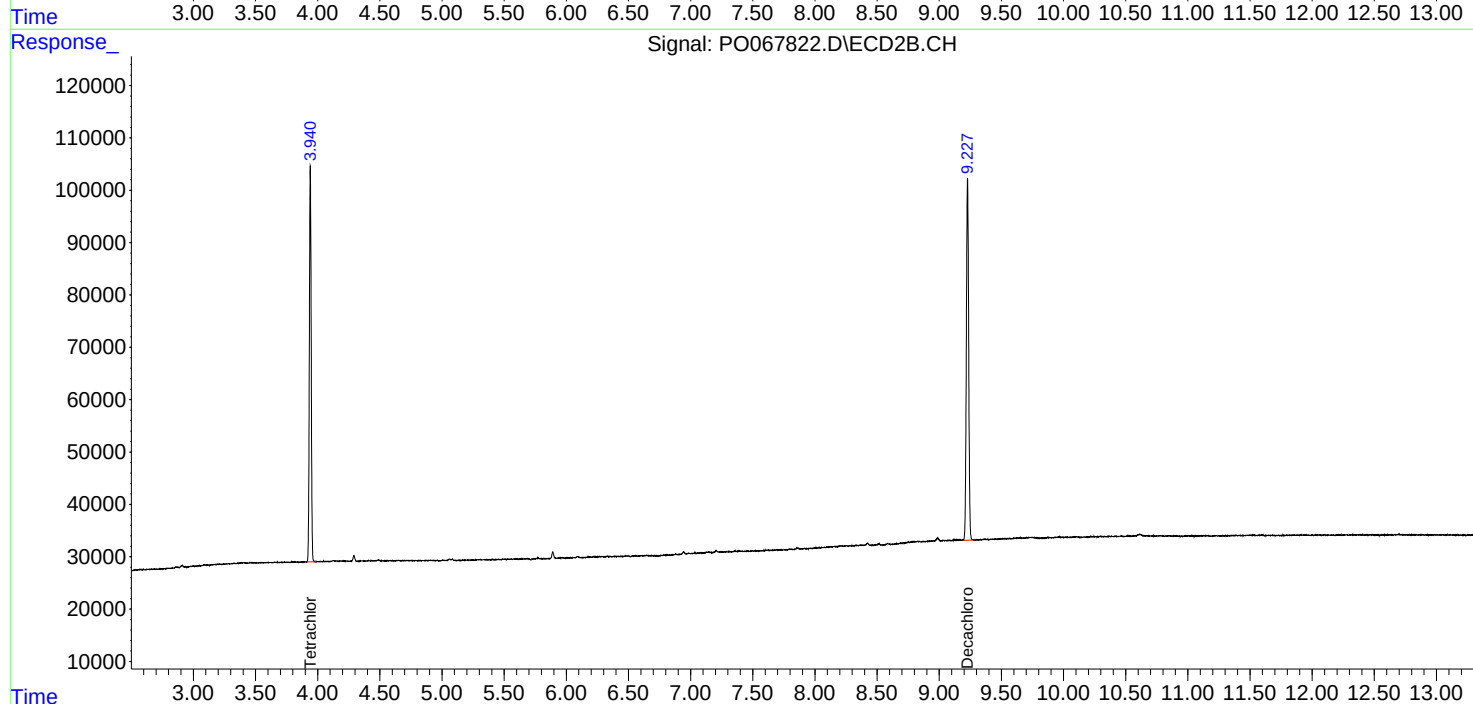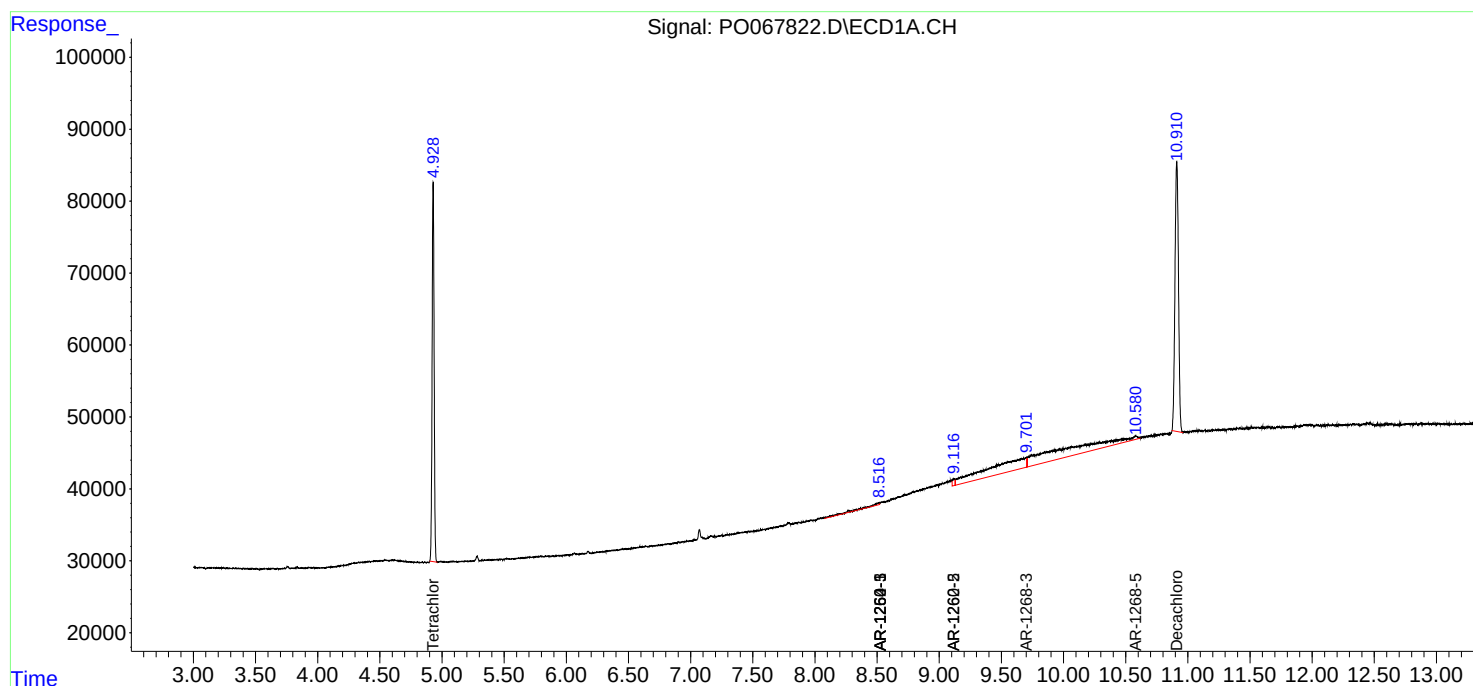


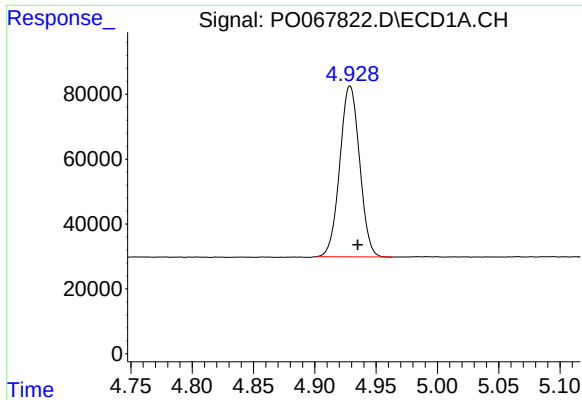

#1 Tetrachloro-m-xylene


R.T.: 4.929 min
Delta R.T.: -0.006 min
Response: 591711
Conc: 24.85 ng/ml

Instrument :
ECD_O
ClientSampleId :

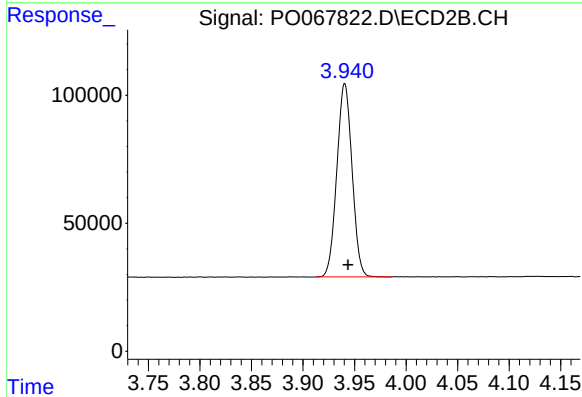


#1 Tetrachloro-m-xylene

R.T.: 3.941 min
Delta R.T.: -0.003 min
Response: 776244
Conc: 23.16 ng/ml

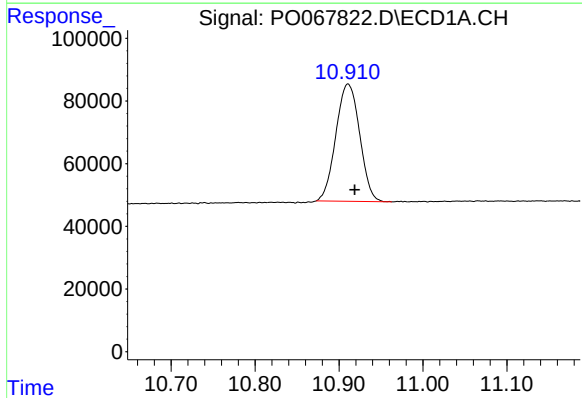


#2 Decachlorobiphenyl

R.T.: 10.911 min
Delta R.T.: -0.008 min
Response: 738190
Conc: 21.68 ng/ml

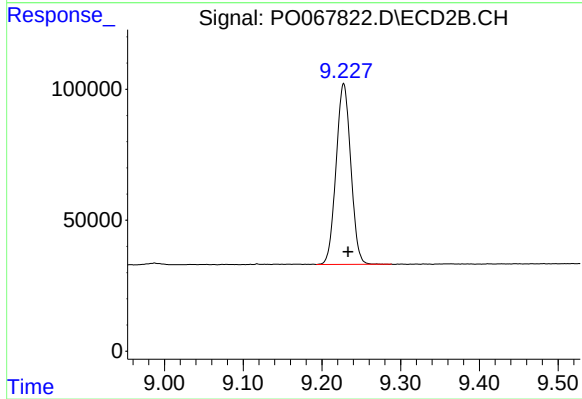

#2 Decachlorobiphenyl


R.T.: 9.228 min
Delta R.T.: -0.005 min
Response: 894653
Conc: 21.64 ng/ml

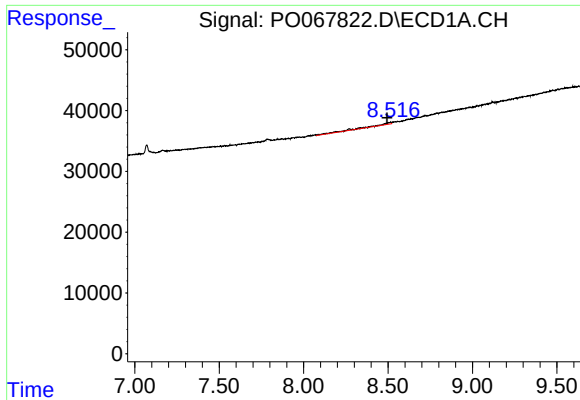

#30 AR-1254-5


R.T.: 8.516 min
Delta R.T.: 0.022 min
Response: 24100
Conc: 14.05 ng/ml

Instrument :
ECD_O
ClientSampleId :

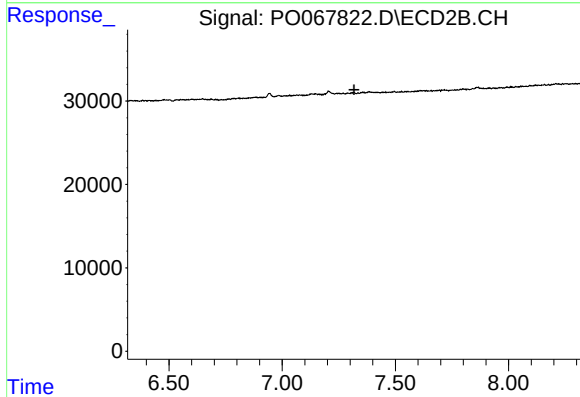


#30 AR-1254-5

R.T.: 0.000 min
Exp R.T. : 7.317 min
Response: 0
Conc: N.D.

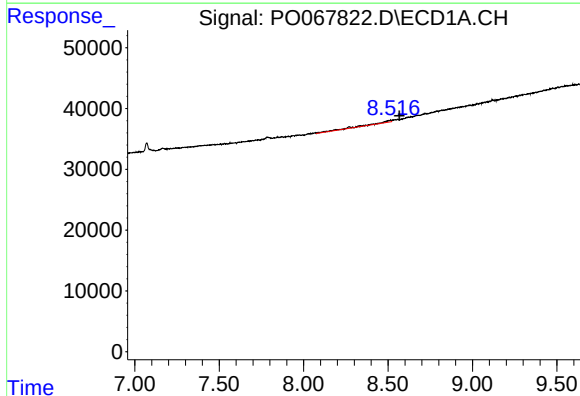


#33 AR-1260-3

R.T.: 8.516 min
Delta R.T.: -0.052 min
Response: 24100
Conc: 18.49 ng/ml

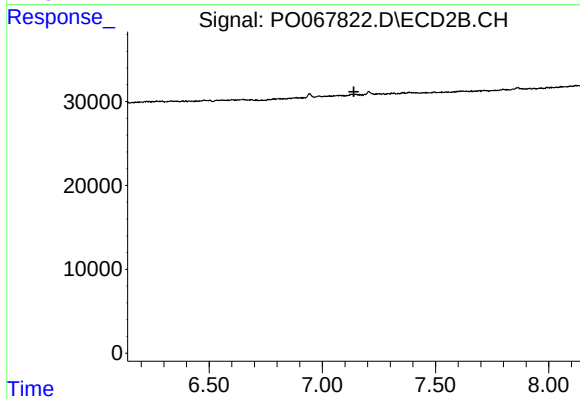

#33 AR-1260-3


R.T.: 0.000 min
Exp R.T. : 7.139 min
Response: 0
Conc: N.D.

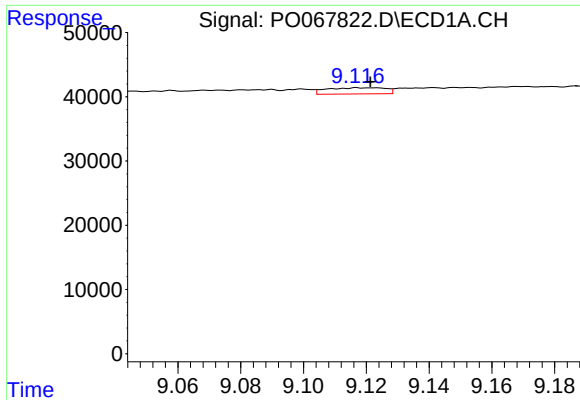

#35 AR-1260-5


R.T.: 9.118 min
Delta R.T.: -0.003 min
Response: 12375
Conc: 3.92 ng/ml

Instrument :
ECD_O
ClientSampleId :

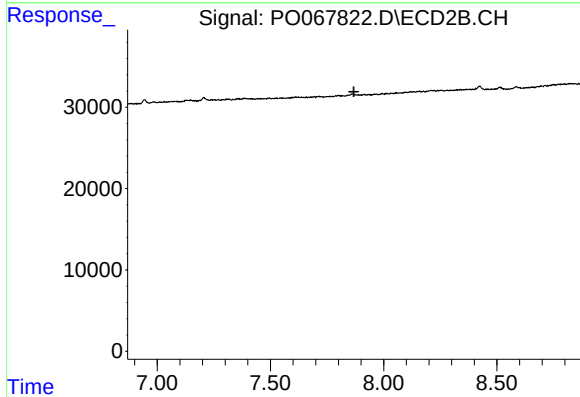


#35 AR-1260-5

R.T.: 0.000 min
Exp R.T. : 7.869 min
Response: 0
Conc: N.D.

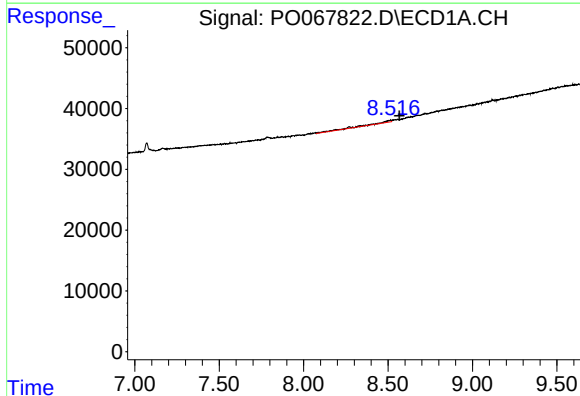


#36 AR-1262-1

R.T.: 8.516 min
Delta R.T.: -0.052 min
Response: 24100
Conc: 14.38 ng/ml

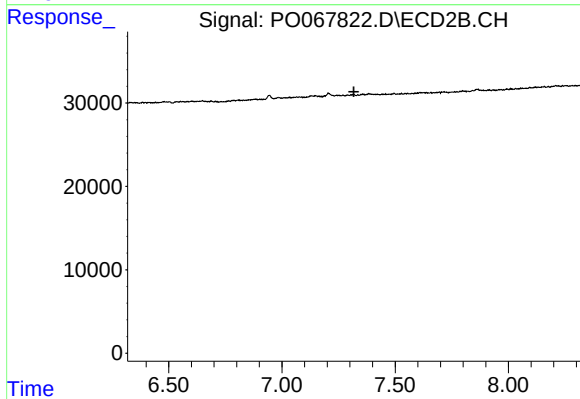

#36 AR-1262-1


R.T.: 0.000 min
Exp R.T. : 7.317 min
Response: 0
Conc: N.D.

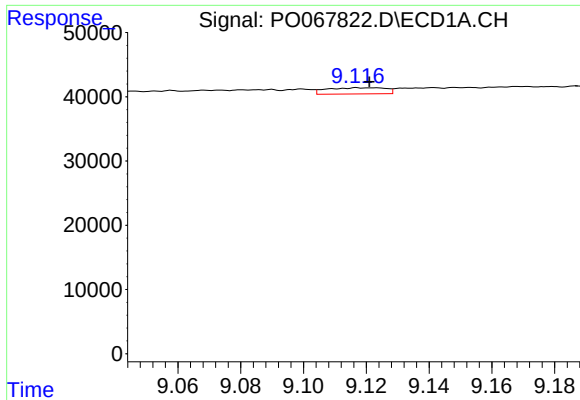

#37 AR-1262-2


R.T.: 9.118 min
Delta R.T.: -0.003 min
Response: 12375
Conc: 4.31 ng/ml

Instrument :
ECD_O
ClientSampleId :

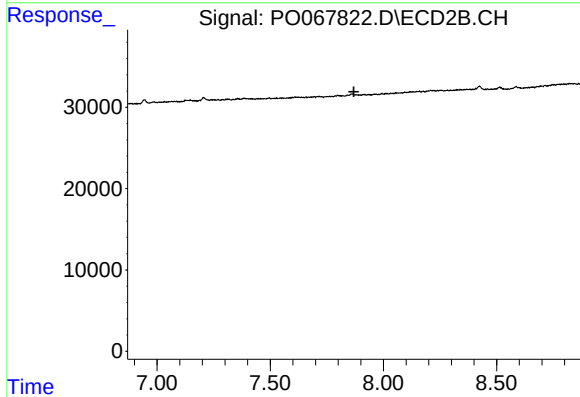


#37 AR-1262-2

R.T.: 0.000 min
Exp R.T. : 7.869 min
Response: 0
Conc: N.D.

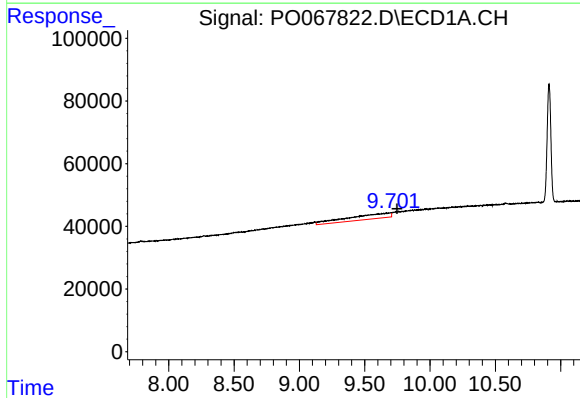


#43 AR-1268-3

R.T.: 9.701 min
Delta R.T.: -0.046 min
Response: 389013
Conc: 133.97 ng/ml

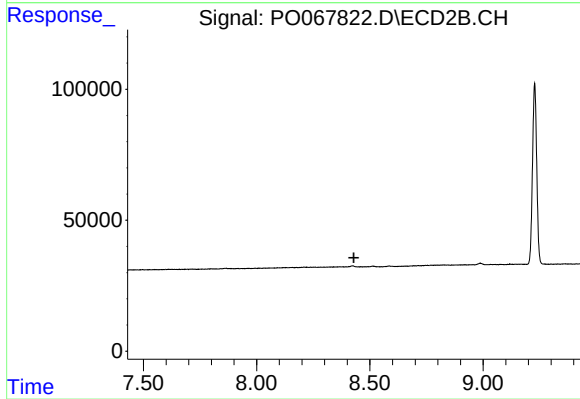

#43 AR-1268-3


R.T.: 0.000 min
Exp R.T. : 8.430 min
Response: 0
Conc: N.D.

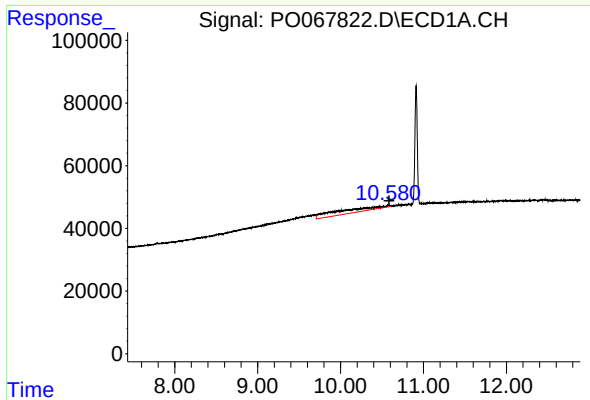

#45 AR-1268-5

R.T.: 10.581 min
Delta R.T.: -0.006 min
Response: 509602
Conc: 51.40 ng/ml

Instrument :
ECD_O
ClientSampleId :

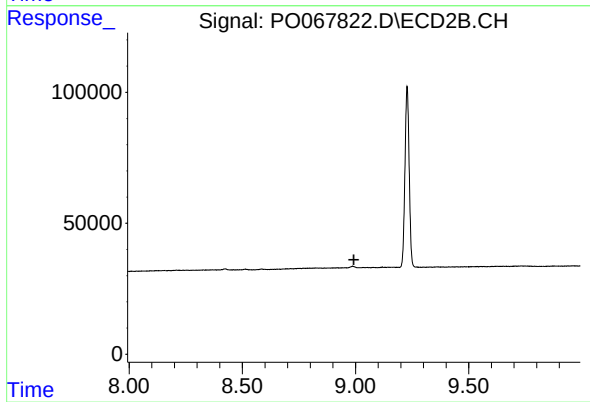

#45 AR-1268-5

R.T.: 0.000 min
Exp R.T. : 8.993 min
Response: 0
Conc: N.D.