

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\P0041519\
 Data File : P0055321.D
 Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
 Acq On : 15 Apr 2019 22:09
 Operator : SM/SJ
 Sample : K2389-04
 Misc :
 ALS Vial : 21 Sample Multiplier: 1

Instrument :
 ECD_O
 ClientSampleId :

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Apr 16 01:59:16 2019
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\P0032519.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Mon Mar 25 17:22:26 2019
 Response via : Initial Calibration
 Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	4.295	3.608	709388	701611	20.440	21.986
2)	SA Decachlor...	9.912	8.574	754657	533251	15.308	16.744
Target Compounds							
9)	L2 AR-1221-2	4.599	3.906	10898	12426	32.136	41.447 #
28)	L6 AR-1254-3	6.897	0.000	12738	0	4.051	N.D. #
32)	L7 AR-1260-2	7.375	0.000	52545	0	16.931	N.D. #
33)	L7 AR-1260-3	0.000	6.551	0	31984	N.D.	12.407 #
35)	L7 AR-1260-5	0.000	7.207	0	9063	N.D.	1.892 #
37)	L8 AR-1262-2	0.000	7.207	0	9063	N.D.	1.849 #
45)	L9 AR-1268-5	9.649	0.000	124394	0	7.550	N.D. #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\P0041519\
Data File : P0055321.D
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
Acq On : 15 Apr 2019 22:09
Operator : SM/SJ
Sample : K2389-04
Misc :
ALS Vial : 21 Sample Multiplier: 1

Instrument :
ECD_O
ClientSampleId :

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Apr 16 01:59:16 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\P0032519.M
Quant Title : GC EXTRACTABLES
QLast Update : Mon Mar 25 17:22:26 2019
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

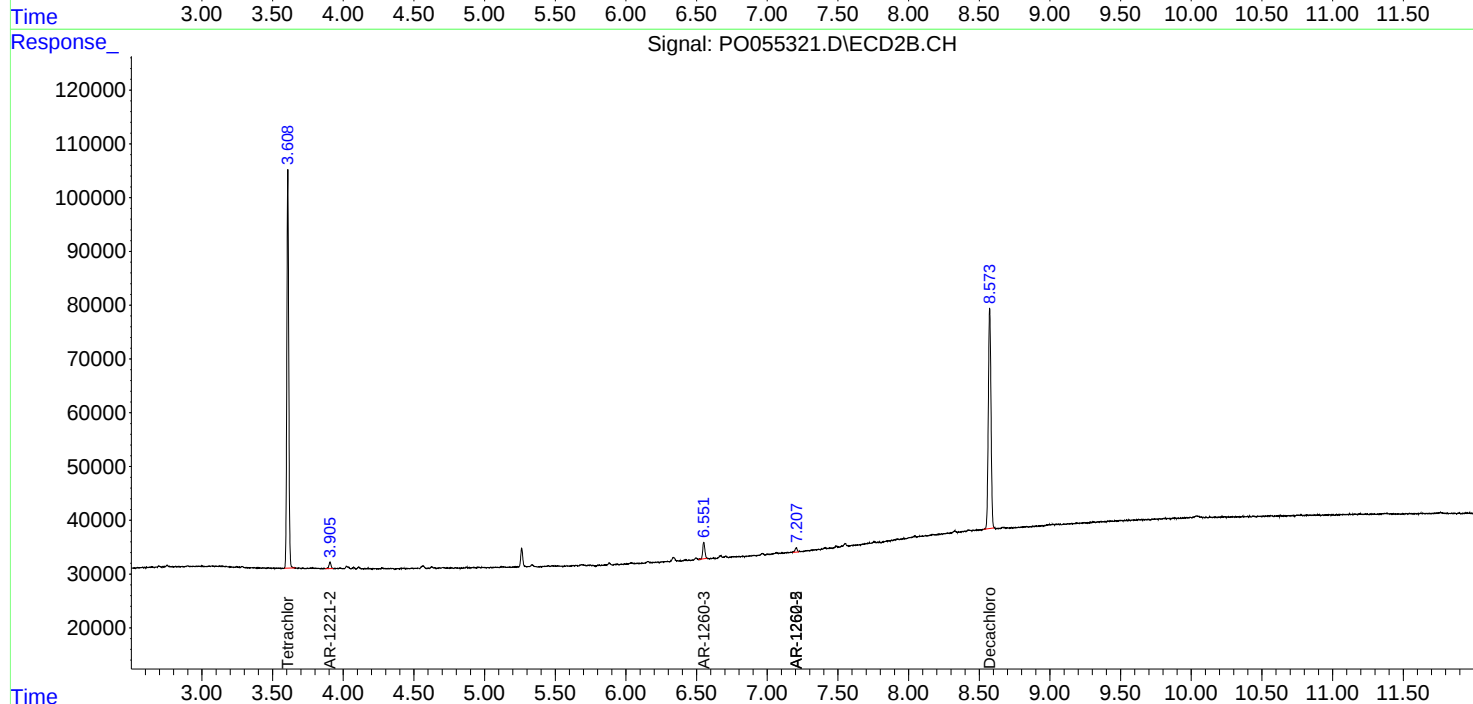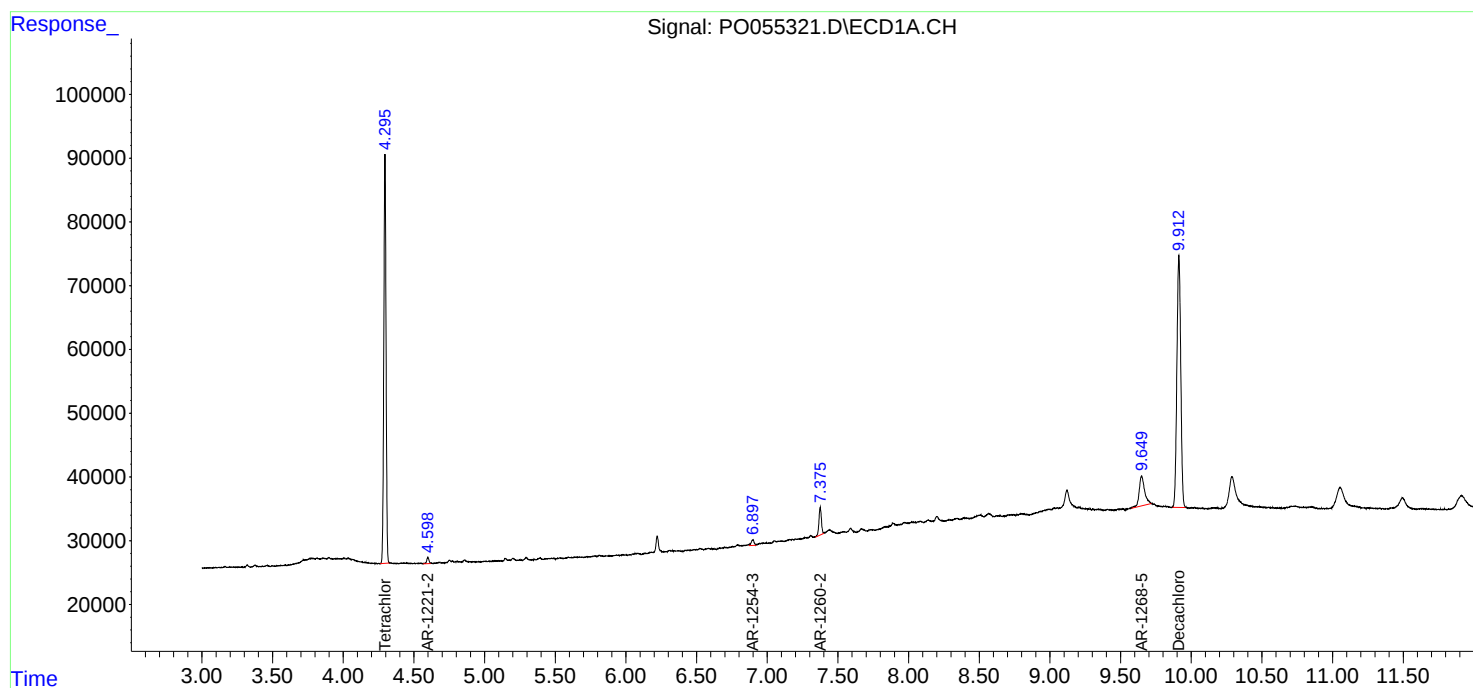


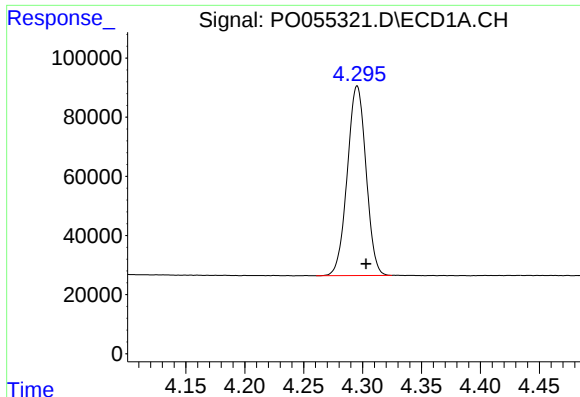

#1 Tetrachloro-m-xylene


R.T.: 4.295 min
Delta R.T.: -0.008 min
Response: 709388
Conc: 20.44 ng/ml

Instrument :
ECD_O
ClientSampleId :

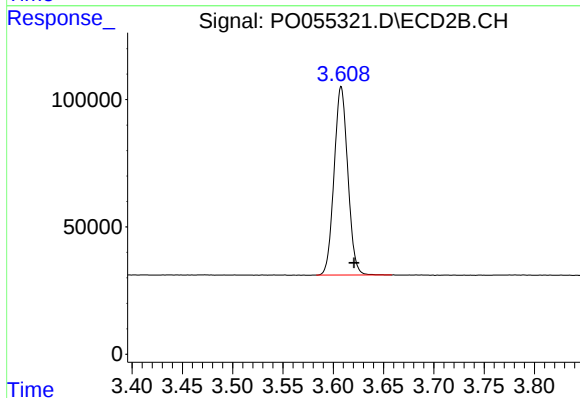


#1 Tetrachloro-m-xylene

R.T.: 3.608 min
Delta R.T.: -0.013 min
Response: 701611
Conc: 21.99 ng/ml

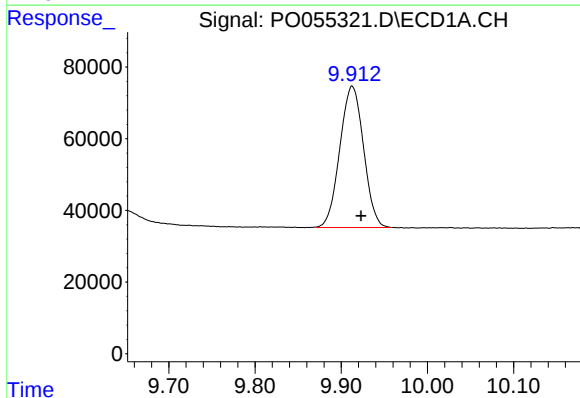


#2 Decachlorobiphenyl

R.T.: 9.912 min
Delta R.T.: -0.011 min
Response: 754657
Conc: 15.31 ng/ml

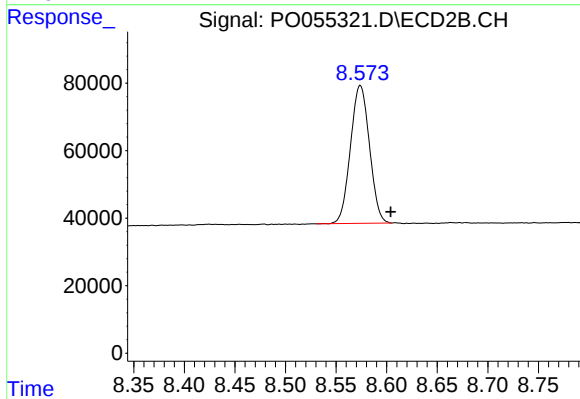

#2 Decachlorobiphenyl


R.T.: 8.574 min
Delta R.T.: -0.030 min
Response: 533251
Conc: 16.74 ng/ml

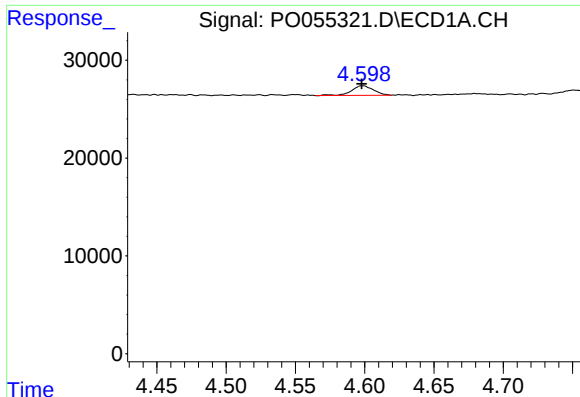

#9 AR-1221-2


R.T.: 4.599 min
Delta R.T.: 0.001 min
Response: 10898
Conc: 32.14 ng/ml

Instrument :
ECD_O
ClientSampleId :

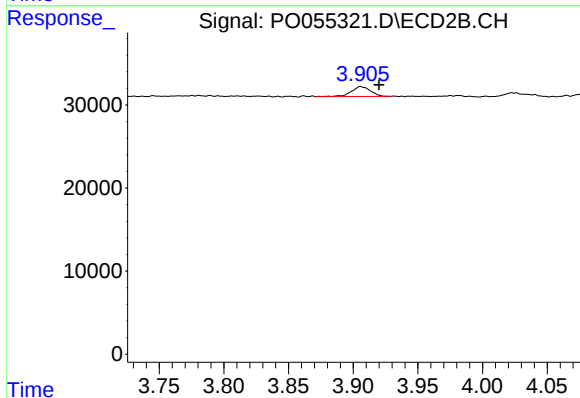


#9 AR-1221-2

R.T.: 3.906 min
Delta R.T.: -0.014 min
Response: 12426
Conc: 41.45 ng/ml

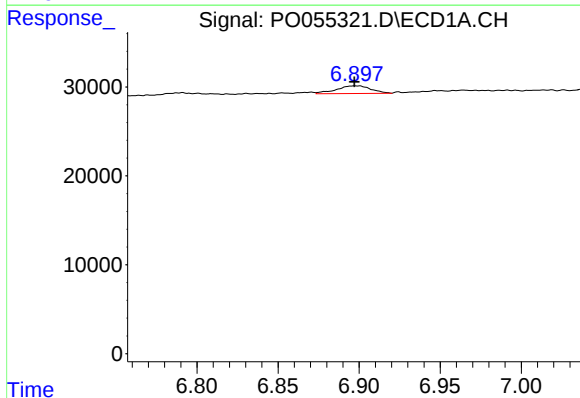


#28 AR-1254-3

R.T.: 6.897 min
Delta R.T.: 0.000 min
Response: 12738
Conc: 4.05 ng/ml

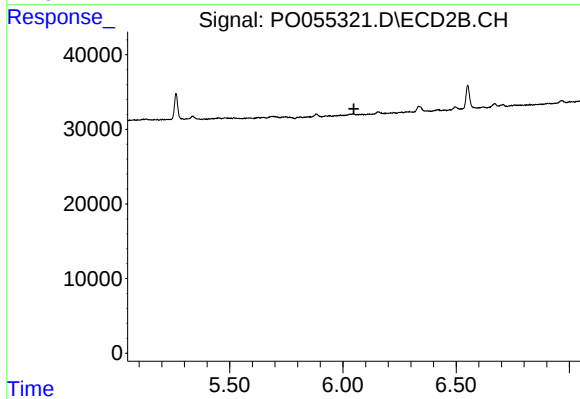

#28 AR-1254-3


R.T.: 0.000 min
Exp R.T.: 6.049 min
Response: 0
Conc: N.D.

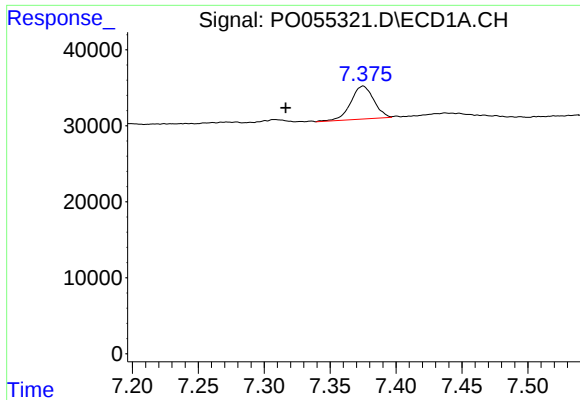

#32 AR-1260-2


R.T.: 7.375 min
Delta R.T.: 0.059 min
Response: 52545
Conc: 16.93 ng/ml

Instrument :
ECD_O
ClientSampleId :

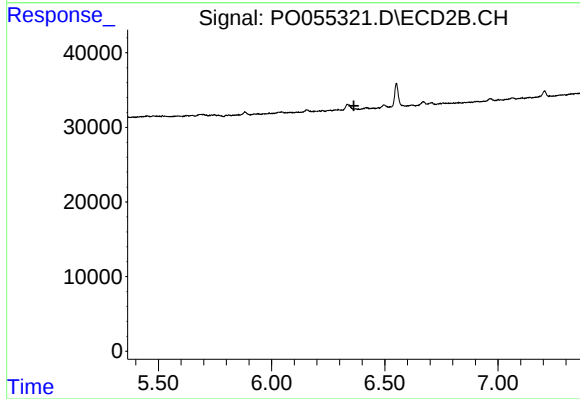


#32 AR-1260-2

R.T.: 0.000 min
Exp R.T. : 6.363 min
Response: 0
Conc: N.D.

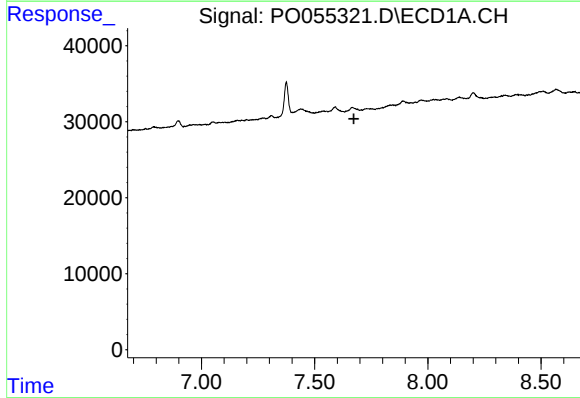


#33 AR-1260-3

R.T.: 0.000 min
Exp R.T. : 7.674 min
Response: 0
Conc: N.D.

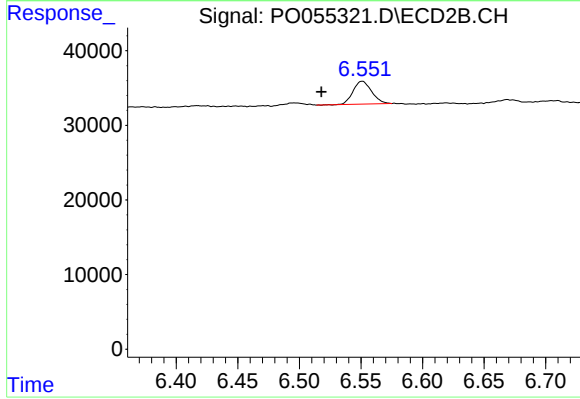

#33 AR-1260-3


R.T.: 6.551 min
Delta R.T.: 0.033 min
Response: 31984
Conc: 12.41 ng/ml

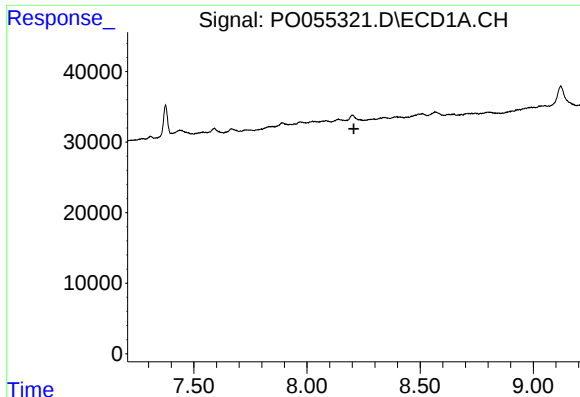

#35 AR-1260-5


R.T.: 0.000 min
Exp R.T.: 8.207 min
Response: 0
Conc: N.D.

Instrument :
ECD_O
ClientSampleId :

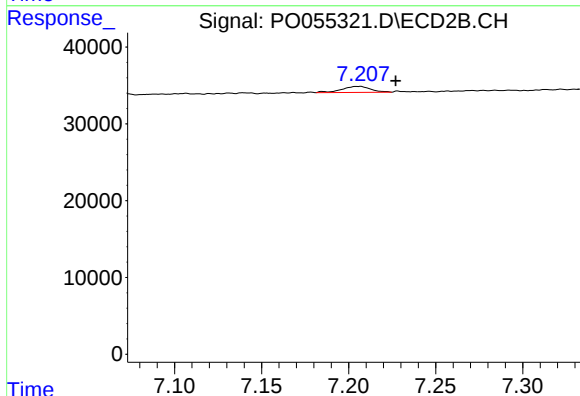


#35 AR-1260-5

R.T.: 7.207 min
Delta R.T.: -0.020 min
Response: 9063
Conc: 1.89 ng/ml

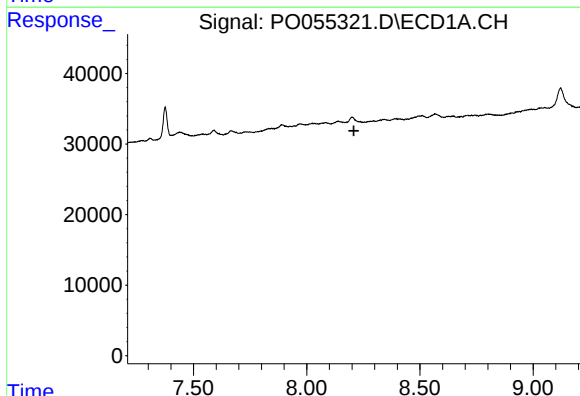


#37 AR-1262-2

R.T.: 0.000 min
Exp R.T.: 8.209 min
Response: 0
Conc: N.D.

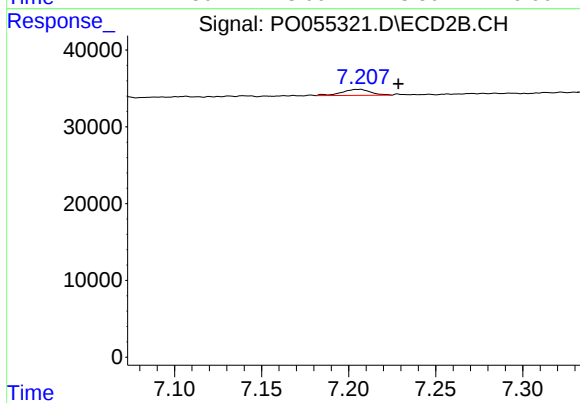

#37 AR-1262-2


R.T.: 7.207 min
Delta R.T.: -0.022 min
Response: 9063
Conc: 1.85 ng/ml

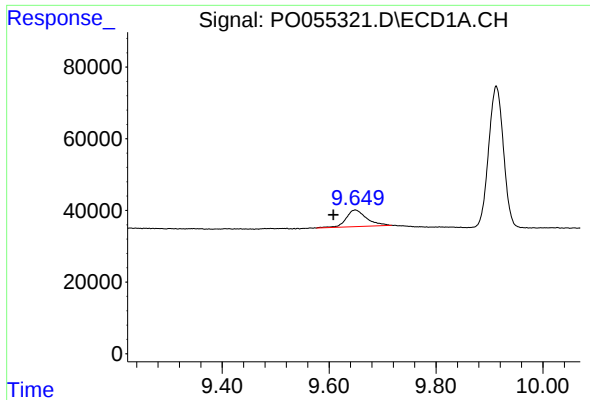

#45 AR-1268-5

R.T.: 9.649 min
Delta R.T.: 0.041 min
Response: 124394
Conc: 7.55 ng/ml

Instrument :
ECD_O
ClientSampleId :

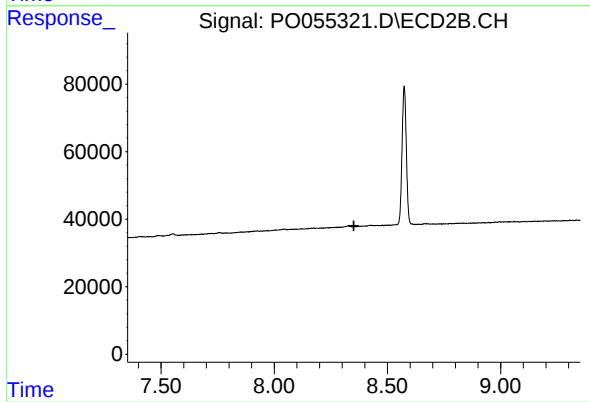

#45 AR-1268-5

R.T.: 0.000 min
Exp R.T. : 8.352 min
Response: 0
Conc: N.D.