

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\P0041519\
 Data File : P0055305.D
 Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
 Acq On : 15 Apr 2019 17:37
 Operator : SM/SJ
 Sample : K1560-09
 Misc : AR1221 MDL 25PPB
 ALS Vial : 7 Sample Multiplier: 1

Instrument :
 ECD_O
 ClientSampleId :
 MDL-MDL-WATER-03-QT1-2019

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Apr 16 01:51:50 2019
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\P0032519.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Mon Mar 25 17:22:26 2019
 Response via : Initial Calibration
 Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	4.297	3.609	594825	563037	17.139	17.643
2) SA Decachlor...	9.918	8.578	703957	518795	14.280	16.290
Target Compounds						
8) L2 AR-1221-1	4.507	3.822	19150	17030	43.864	43.803
9) L2 AR-1221-2	4.595	3.907	21445	21009	63.239	70.078
10) L2 AR-1221-3	4.669	3.982	50110	41778	48.239	45.323



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\PO041519\
Data File : PO055305.D
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
Acq On : 15 Apr 2019 17:37
Operator : SM/SJ
Sample : K1560-09
Misc : AR1221 MDL 25PPB
ALS Vial : 7 Sample Multiplier: 1

Instrument :
ECD_O
ClientSampleId :
MDL-MDL-WATER-03-QT1-2019

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Apr 16 01:51:50 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\PO032519.M
Quant Title : GC EXTRACTABLES
QLast Update : Mon Mar 25 17:22:26 2019
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

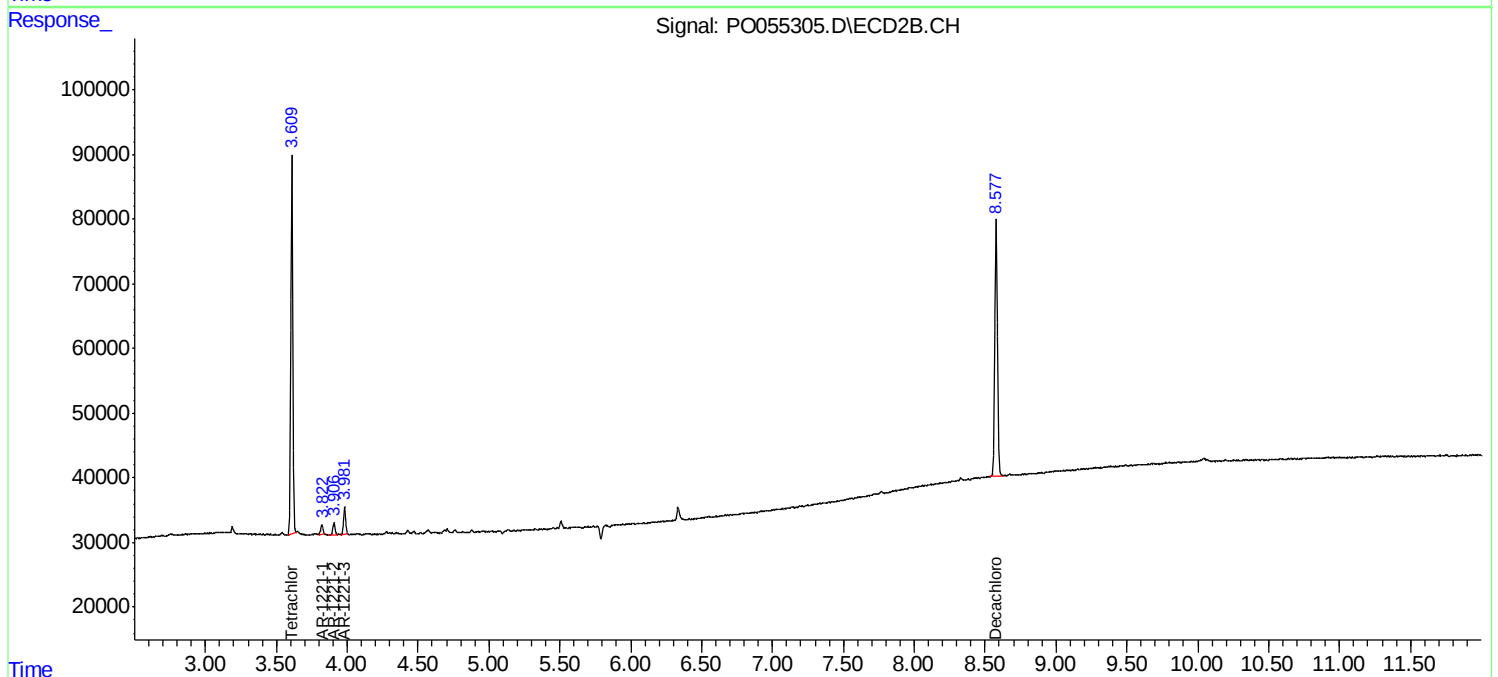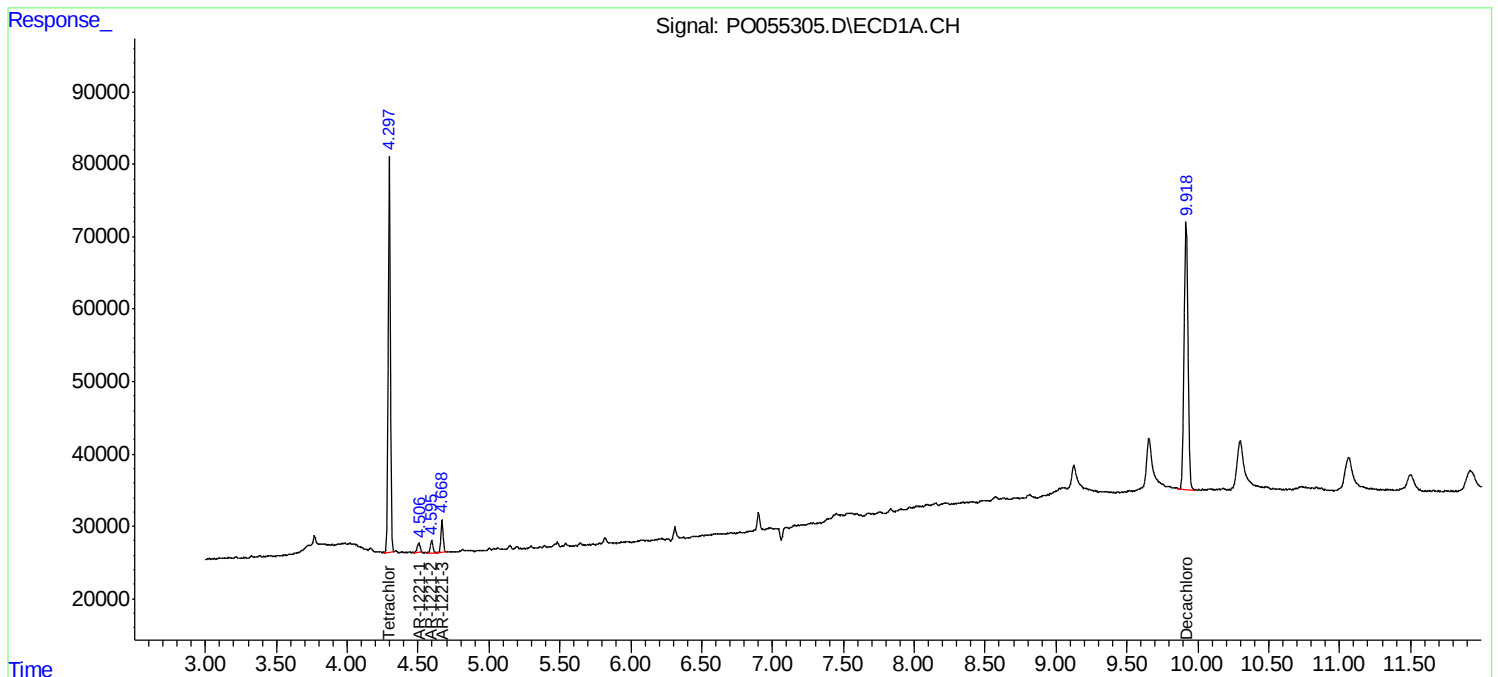


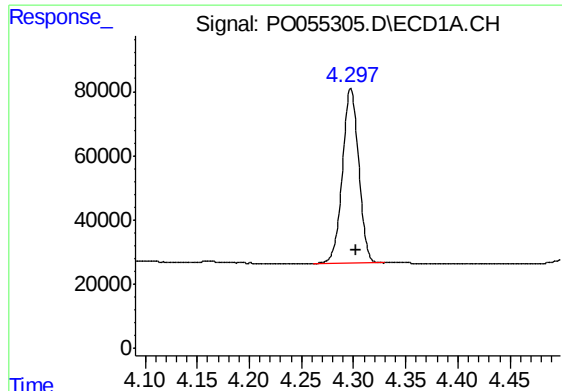

#1 Tetrachloro-m-xylene


R.T.: 4.297 min
Delta R.T.: -0.006 min
Response: 594825
Conc: 17.14 ng/ml

Instrument :
ECD_O
ClientSampleId :
MDL-MDL-WATER-03-QT1-2019

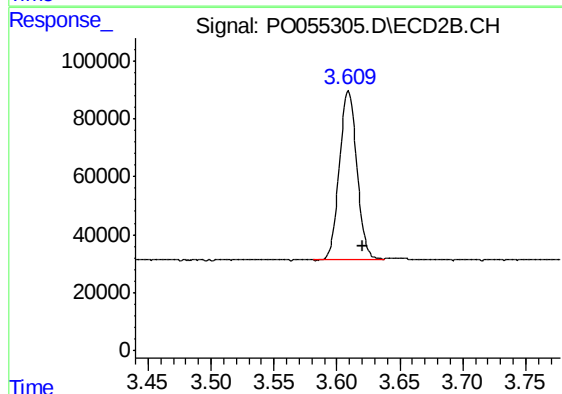


#1 Tetrachloro-m-xylene

R.T.: 3.609 min
Delta R.T.: -0.012 min
Response: 563037
Conc: 17.64 ng/ml

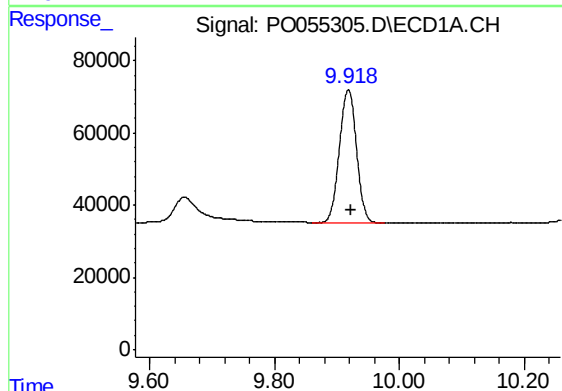


#2 Decachlorobiphenyl

R.T.: 9.918 min
Delta R.T.: -0.005 min
Response: 703957
Conc: 14.28 ng/ml

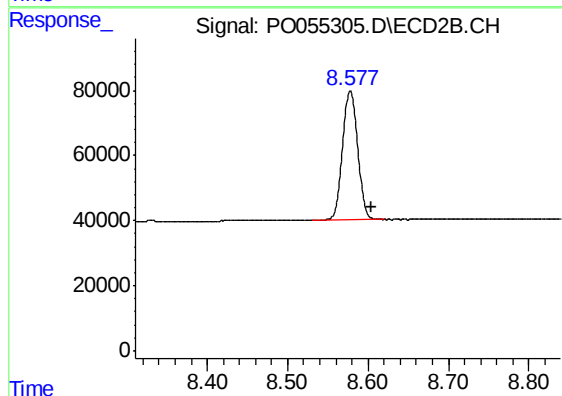

#2 Decachlorobiphenyl


R.T.: 8.578 min
Delta R.T.: -0.026 min
Response: 518795
Conc: 16.29 ng/ml

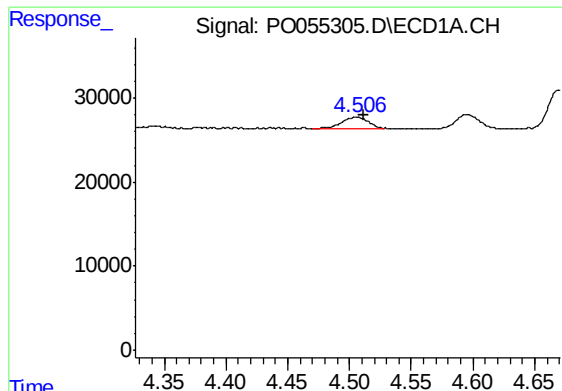

#8 AR-1221-1


R.T.: 4.507 min
Delta R.T.: -0.006 min
Response: 19150
Conc: 43.86 ng/ml

Instrument :
ECD_O
ClientSampleId :
MDL-MDL-WATER-03-QT1-2019

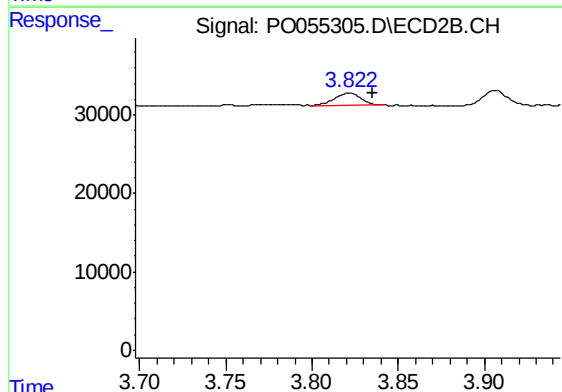


#8 AR-1221-1

R.T.: 3.822 min
Delta R.T.: -0.014 min
Response: 17030
Conc: 43.80 ng/ml

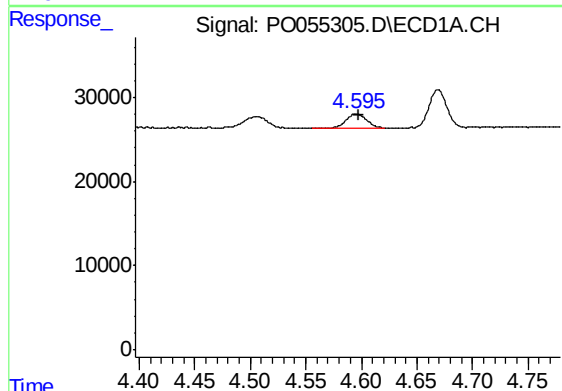


#9 AR-1221-2

R.T.: 4.595 min
Delta R.T.: -0.003 min
Response: 21445
Conc: 63.24 ng/ml

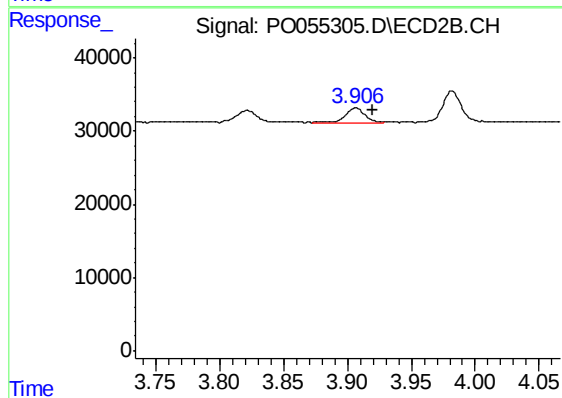

#9 AR-1221-2


R.T.: 3.907 min
Delta R.T.: -0.013 min
Response: 21009
Conc: 70.08 ng/ml

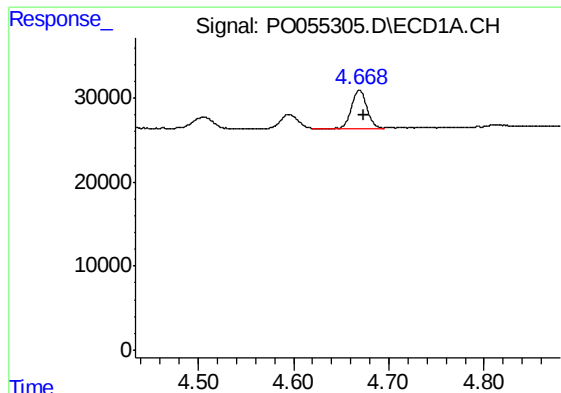

#10 AR-1221-3

R.T.: 4.669 min
Delta R.T.: -0.005 min
Response: 50110
Conc: 48.24 ng/ml

Instrument :
ECD_O
ClientSampleId :
MDL-MDL-WATER-03-QT1-2019

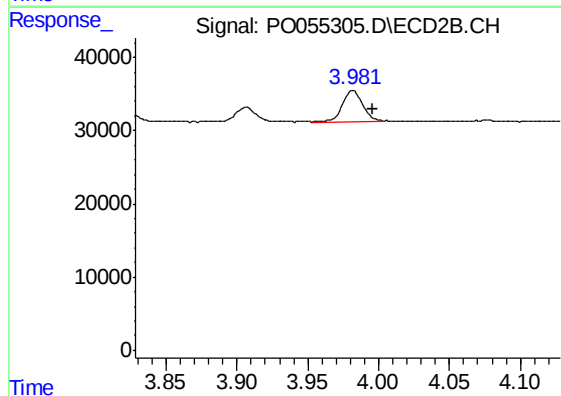

#10 AR-1221-3

R.T.: 3.982 min
Delta R.T.: -0.015 min
Response: 41778
Conc: 45.32 ng/ml