

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\P0041519\
 Data File : P0055308.D
 Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
 Acq On : 15 Apr 2019 18:28
 Operator : SM/SJ
 Sample : K1560-09
 Misc : AR1254 MDL 25PPB
 ALS Vial : 10 Sample Multiplier: 1

Instrument :
 ECD_O
 ClientSampleId :
 MDL-MDL-WATER-03-QT1-2019

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Apr 16 01:53:11 2019
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\P0032519.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Mon Mar 25 17:22:26 2019
 Response via : Initial Calibration
 Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	4.298	3.609	846489	817477	24.391	25.616
2)	SA Decachlor...	9.917	8.613	1049915	2409	21.297	0.076 #
Target Compounds							
26)	L6 AR-1254-1	6.310	5.480	63301	70769	34.911	32.382
27)	L6 AR-1254-2	6.527	5.626	94055	64232	32.947	33.127
28)	L6 AR-1254-3	6.892	6.029	97494	103240	31.002	32.205
29)	L6 AR-1254-4	7.177	6.256	85029	66787	34.757	34.111m
30)	L6 AR-1254-5	7.592	6.670	61976	80675	23.123m	28.064m



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\P0041519\
Data File : P0055308.D
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
Acq On : 15 Apr 2019 18:28
Operator : SM/SJ
Sample : K1560-09
Misc : AR1254 MDL 25PPB
ALS Vial : 10 Sample Multiplier: 1

Instrument :
ECD_O
ClientSampleId :
MDL-MDL-WATER-03-QT1-2019

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Apr 16 01:53:11 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\P0032519.M
Quant Title : GC EXTRACTABLES
QLast Update : Mon Mar 25 17:22:26 2019
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

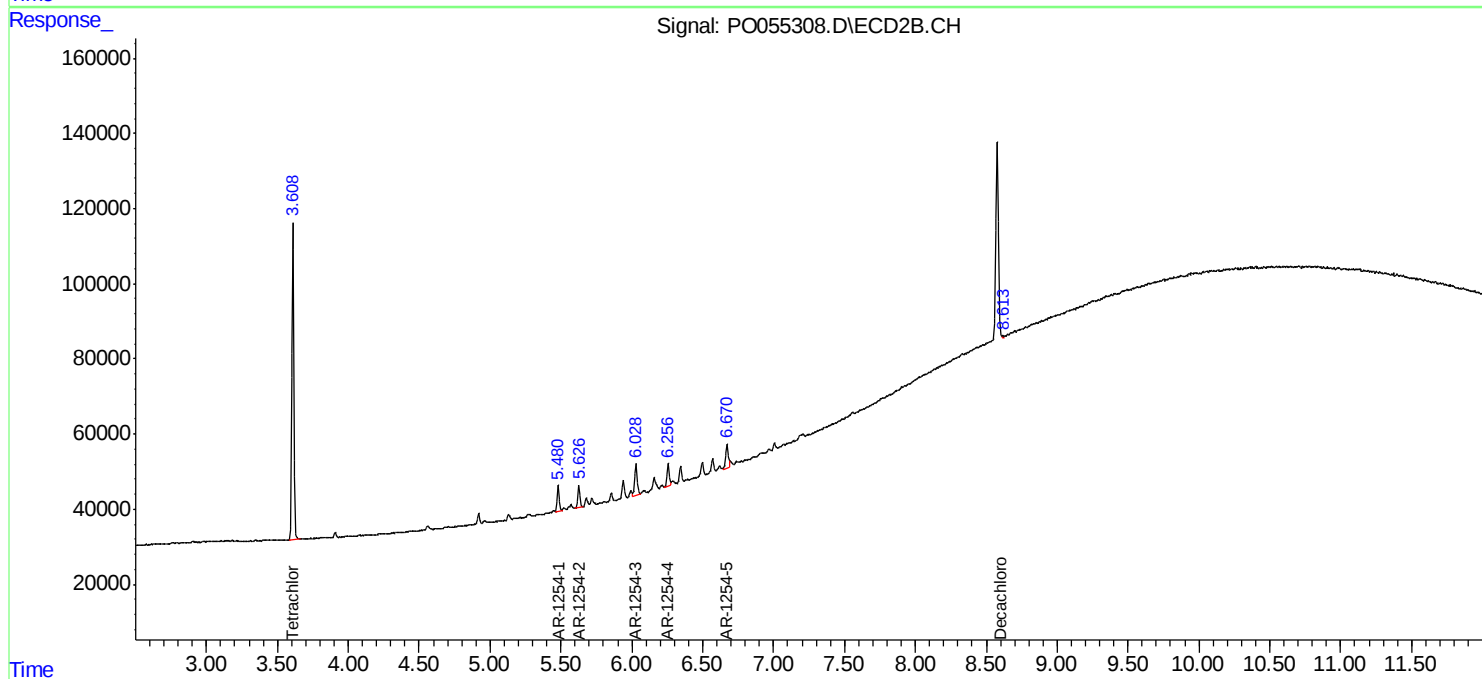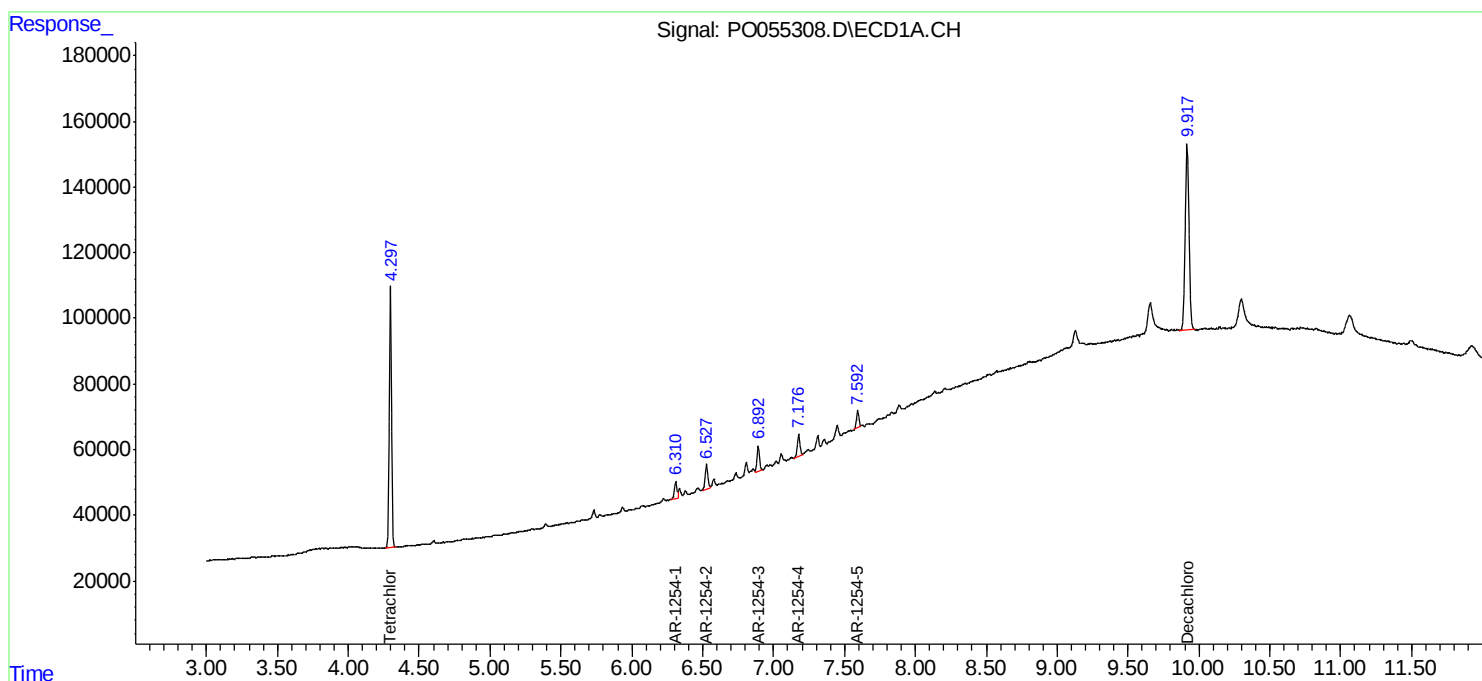


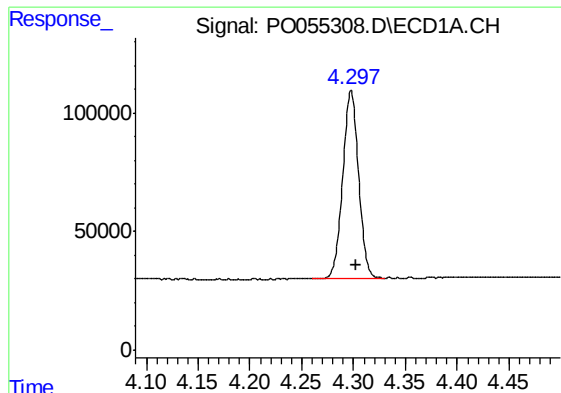

#1 Tetrachloro-m-xylene


R.T.: 4.298 min
Delta R.T.: -0.005 min
Response: 846489
Conc: 24.39 ng/ml

Instrument :
ECD_O
ClientSampleId :
MDL-MDL-WATER-03-QT1-2019

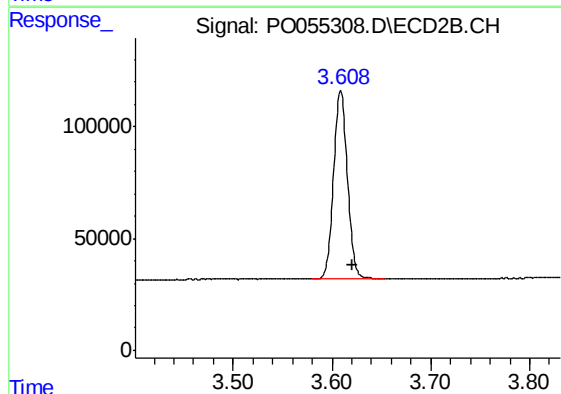


#1 Tetrachloro-m-xylene

R.T.: 3.609 min
Delta R.T.: -0.012 min
Response: 817477
Conc: 25.62 ng/ml

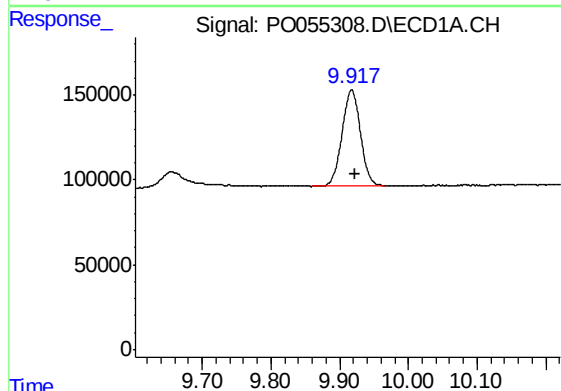


#2 Decachlorobiphenyl

R.T.: 9.917 min
Delta R.T.: -0.006 min
Response: 1049915
Conc: 21.30 ng/ml

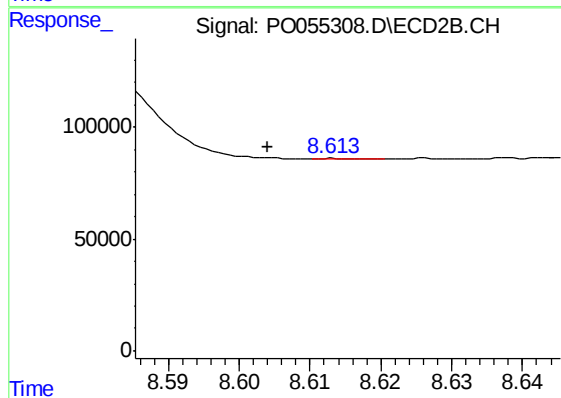

#2 Decachlorobiphenyl


R.T.: 8.613 min
Delta R.T.: 0.009 min
Response: 2409
Conc: 0.08 ng/ml

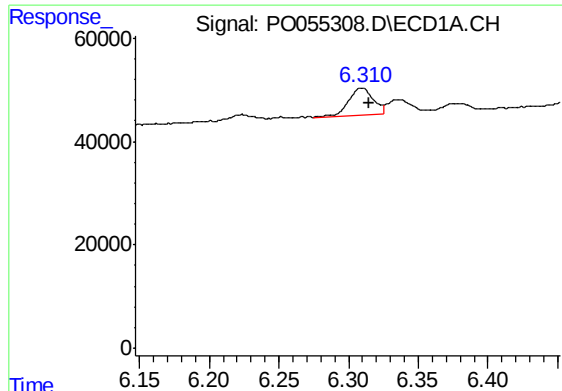

#26 AR-1254-1


R.T.: 6.310 min
Delta R.T.: -0.004 min
Response: 63301
Conc: 34.91 ng/ml

Instrument :
ECD_O
ClientSampleId :
MDL-MDL-WATER-03-QT1-2019

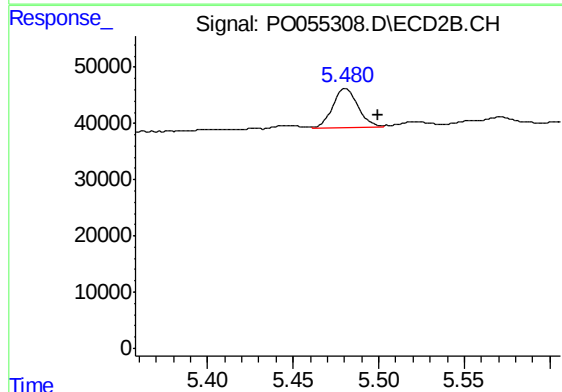


#26 AR-1254-1

R.T.: 5.480 min
Delta R.T.: -0.019 min
Response: 70769
Conc: 32.38 ng/ml

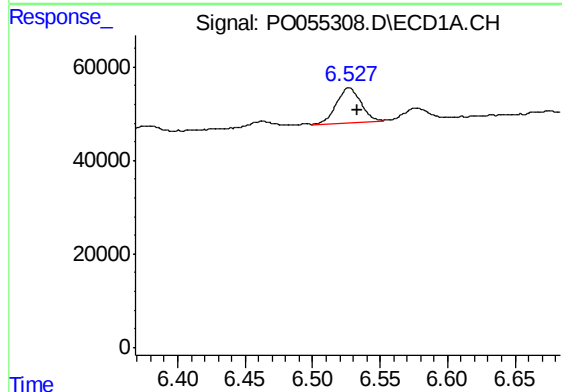


#27 AR-1254-2

R.T.: 6.527 min
Delta R.T.: -0.006 min
Response: 94055
Conc: 32.95 ng/ml

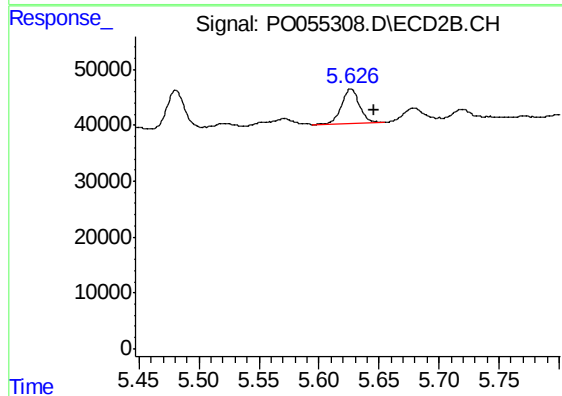

#27 AR-1254-2


R.T.: 5.626 min
Delta R.T.: -0.019 min
Response: 64232
Conc: 33.13 ng/ml

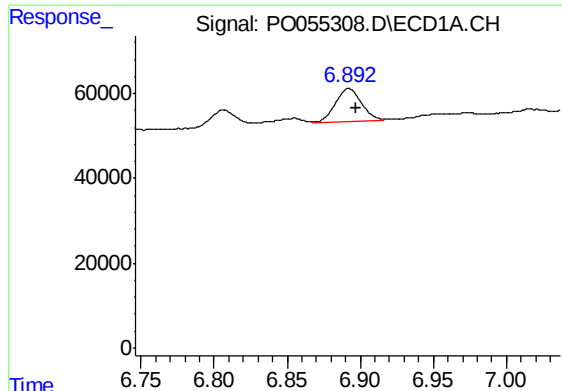

#28 AR-1254-3


R.T.: 6.892 min
Delta R.T.: -0.005 min
Response: 97494
Conc: 31.00 ng/ml

Instrument :
ECD_O
ClientSampleId :
MDL-MDL-WATER-03-QT1-2019

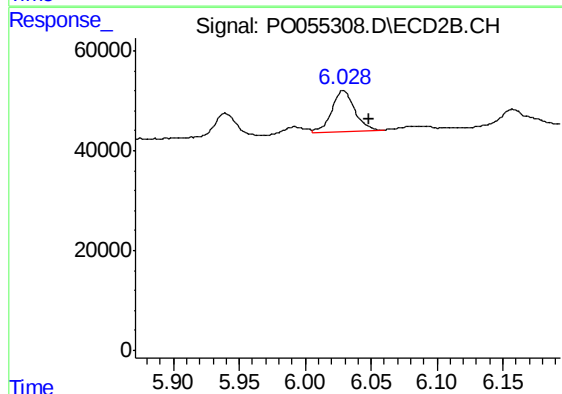


#28 AR-1254-3

R.T.: 6.029 min
Delta R.T.: -0.020 min
Response: 103240
Conc: 32.21 ng/ml

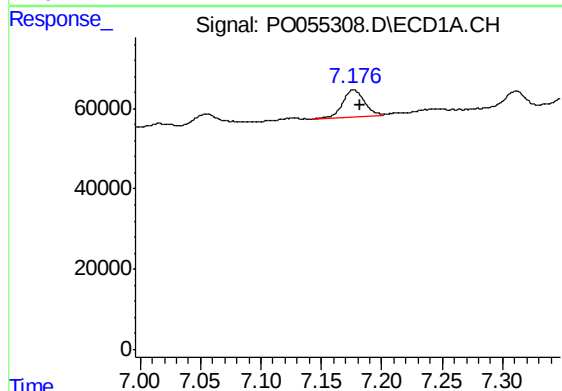


#29 AR-1254-4

R.T.: 7.177 min
Delta R.T.: -0.005 min
Response: 85029
Conc: 34.76 ng/ml

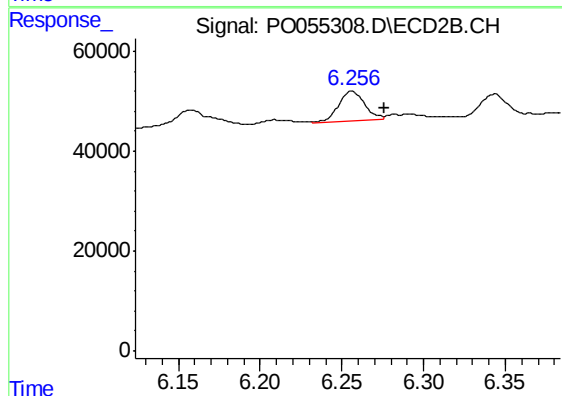

#29 AR-1254-4


R.T.: 6.256 min
Delta R.T.: -0.020 min
Response: 66787
Conc: 34.11 ng/ml m

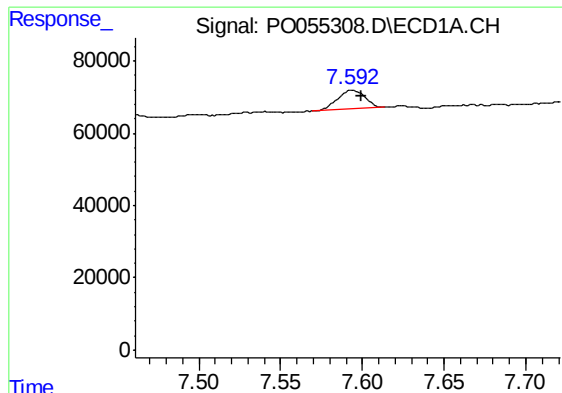

#30 AR-1254-5

R.T.: 7.592 min
Delta R.T.: -0.007 min
Response: 61976
Conc: 23.12 ng/ml m

Instrument :
ECD_O
ClientSampleId :
MDL-MDL-WATER-03-QT1-2019

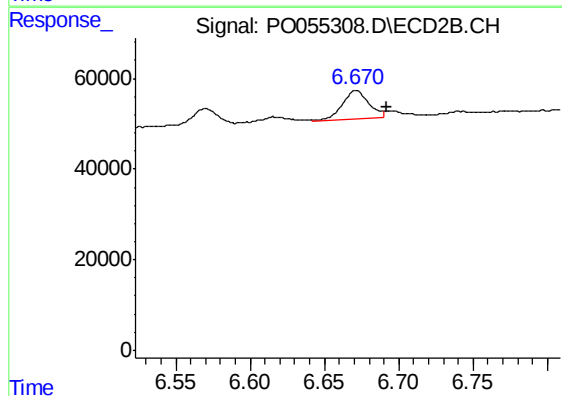

#30 AR-1254-5

R.T.: 6.670 min
Delta R.T.: -0.022 min
Response: 80675
Conc: 28.06 ng/ml m