

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\P0041519\
Data File : P0055318.D
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
Acq On : 15 Apr 2019 21:18
Operator : SM/SJ
Sample : K2389-01
Misc :
ALS Vial : 18 Sample Multiplier: 1

Instrument :
ECD_O
ClientSampleId :
CONCRETE

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Apr 16 12:04:13 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\P0032519.M
Quant Title : GC EXTRACTABLES
QLast Update : Mon Mar 25 17:22:26 2019
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	4.297	3.608	711729	735282	20.508	23.041
2) SA Decachlor...	9.912	8.574	704743	500712	14.296	15.722m

Target Compounds



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\P0041519\
Data File : P0055318.D
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
Acq On : 15 Apr 2019 21:18
Operator : SM/SJ
Sample : K2389-01
Misc :
ALS Vial : 18 Sample Multiplier: 1

Instrument :
ECD_O
ClientSampleId :
CONCRETE

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Apr 16 12:04:13 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\P0032519.M
Quant Title : GC EXTRACTABLES
QLast Update : Mon Mar 25 17:22:26 2019
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

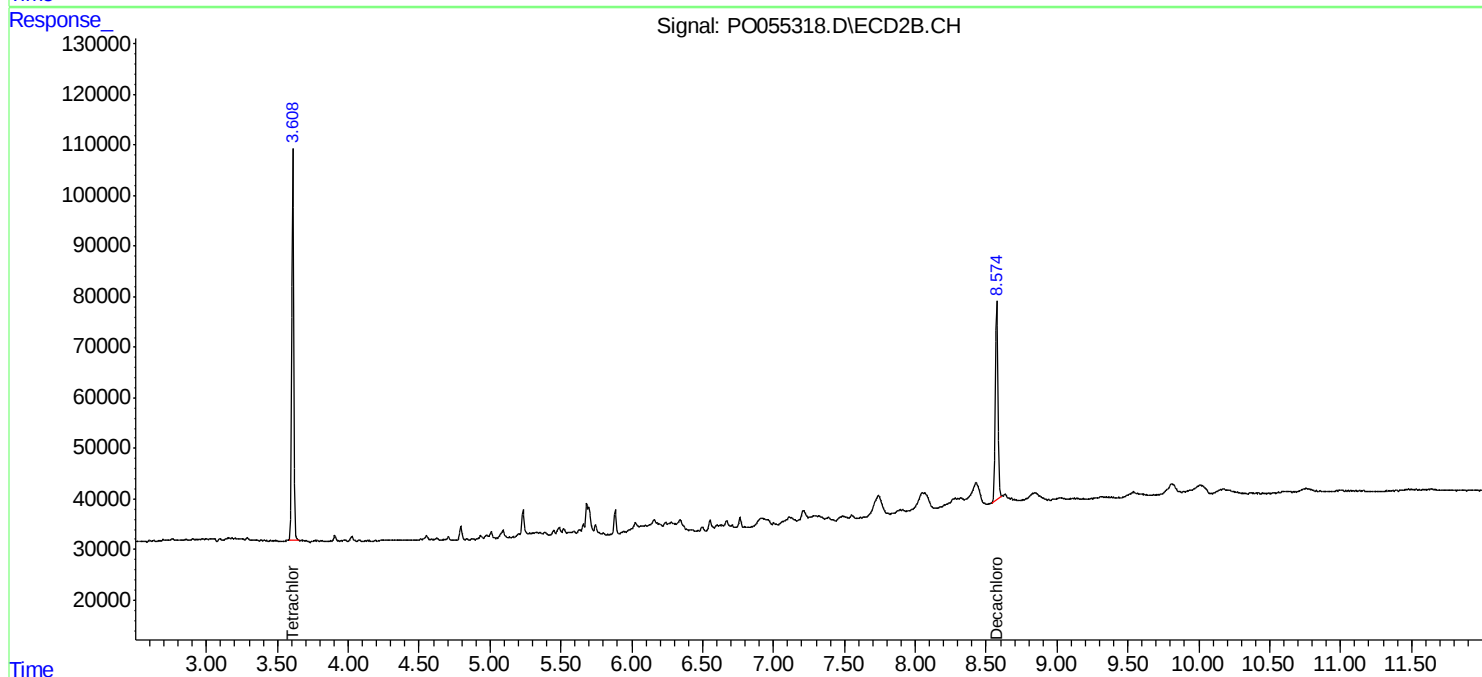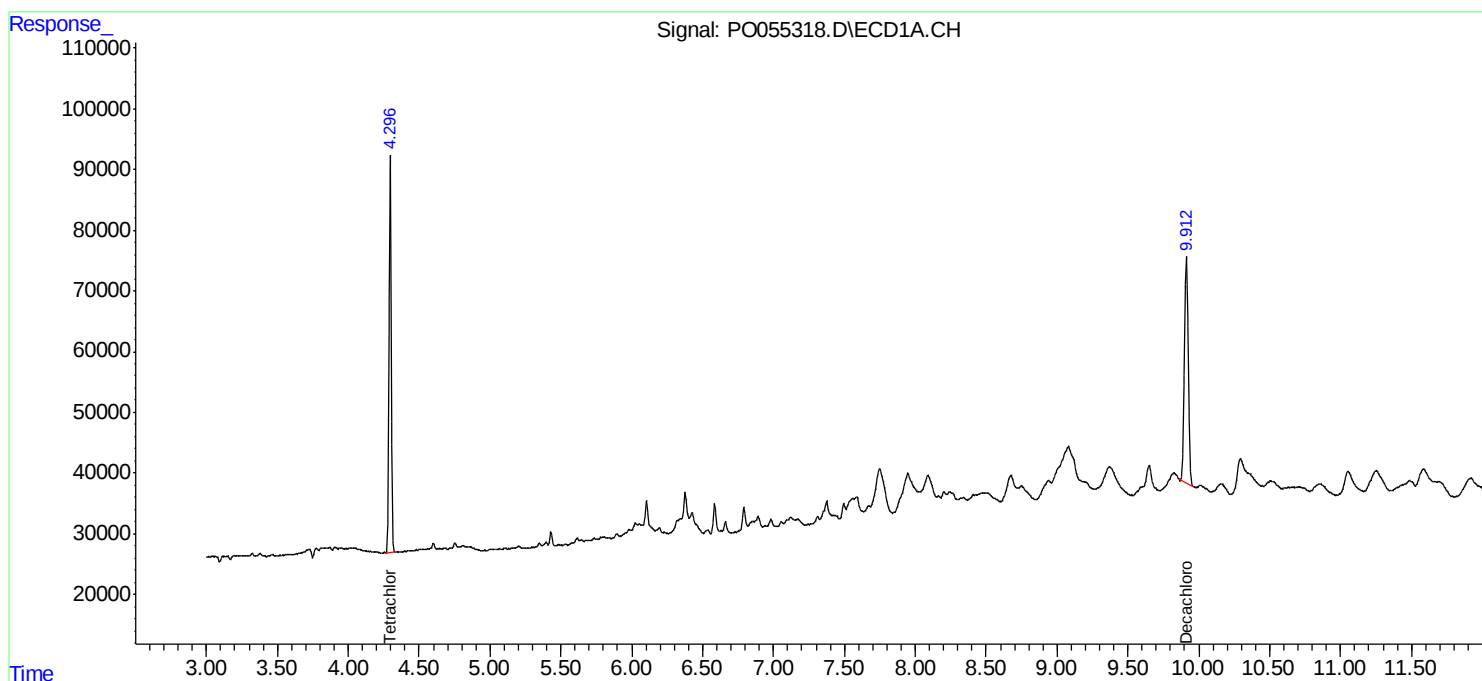


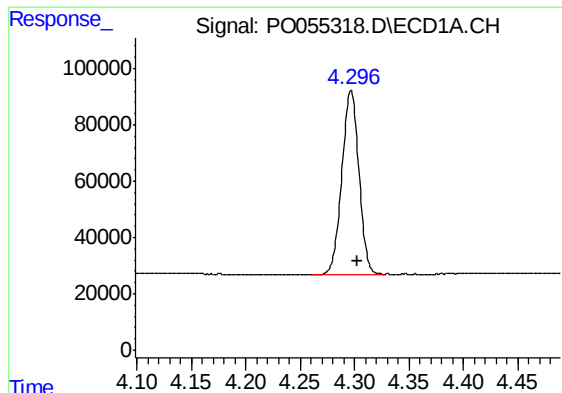

#1 Tetrachloro-m-xylene


R.T.: 4.297 min
Delta R.T.: -0.006 min
Response: 711729
Conc: 20.51 ng/ml

Instrument :
ECD_O
ClientSampleId :
CONCRETE

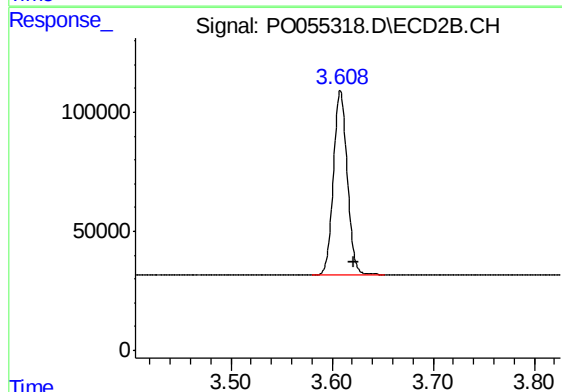


#1 Tetrachloro-m-xylene

R.T.: 3.608 min
Delta R.T.: -0.012 min
Response: 735282
Conc: 23.04 ng/ml

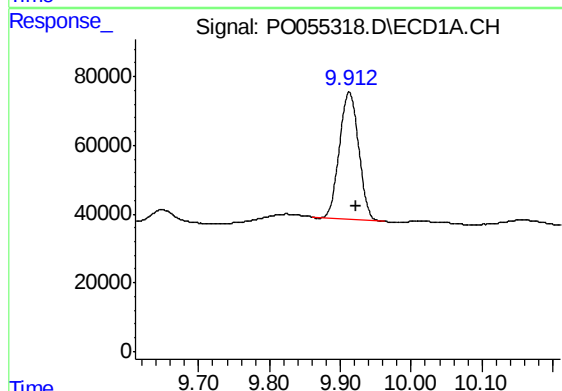

#2 Decachlorobiphenyl

R.T.: 9.912 min
Delta R.T.: -0.011 min
Response: 704743
Conc: 14.30 ng/ml

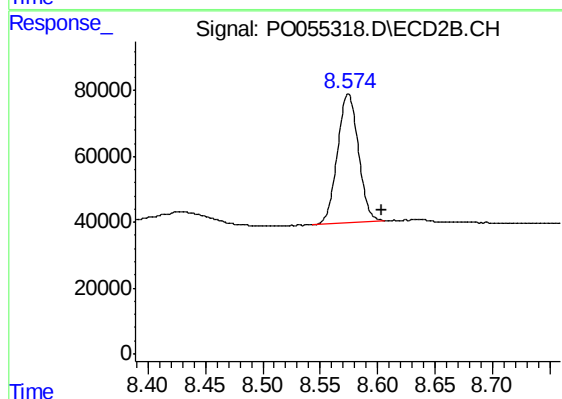

#2 Decachlorobiphenyl

R.T.: 8.574 min
Delta R.T.: -0.030 min
Response: 500712
Conc: 15.72 ng/ml m