

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\P0041519\
 Data File : P0055333.D
 Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
 Acq On : 16 Apr 2019 1:32
 Operator : SM/SJ
 Sample : K2407-03
 Misc :
 ALS Vial : 31 Sample Multiplier: 1

Instrument :
 ECD_O
 ClientSampleId :
 TP-11-S

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Apr 16 07:56:56 2019
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\P0032519.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Mon Mar 25 17:22:26 2019
 Response via : Initial Calibration
 Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	4.295	3.608	700162	684668	20.175	21.455
2) SA Decachlor...	9.912	8.573	738183	518155	14.974	16.270

Target Compounds



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\P0041519\
Data File : P0055333.D
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
Acq On : 16 Apr 2019 1:32
Operator : SM/SJ
Sample : K2407-03
Misc :
ALS Vial : 31 Sample Multiplier: 1

Instrument :
ECD_O
ClientSampleId :
TP-11-S

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Apr 16 07:56:56 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\P0032519.M
Quant Title : GC EXTRACTABLES
QLast Update : Mon Mar 25 17:22:26 2019
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

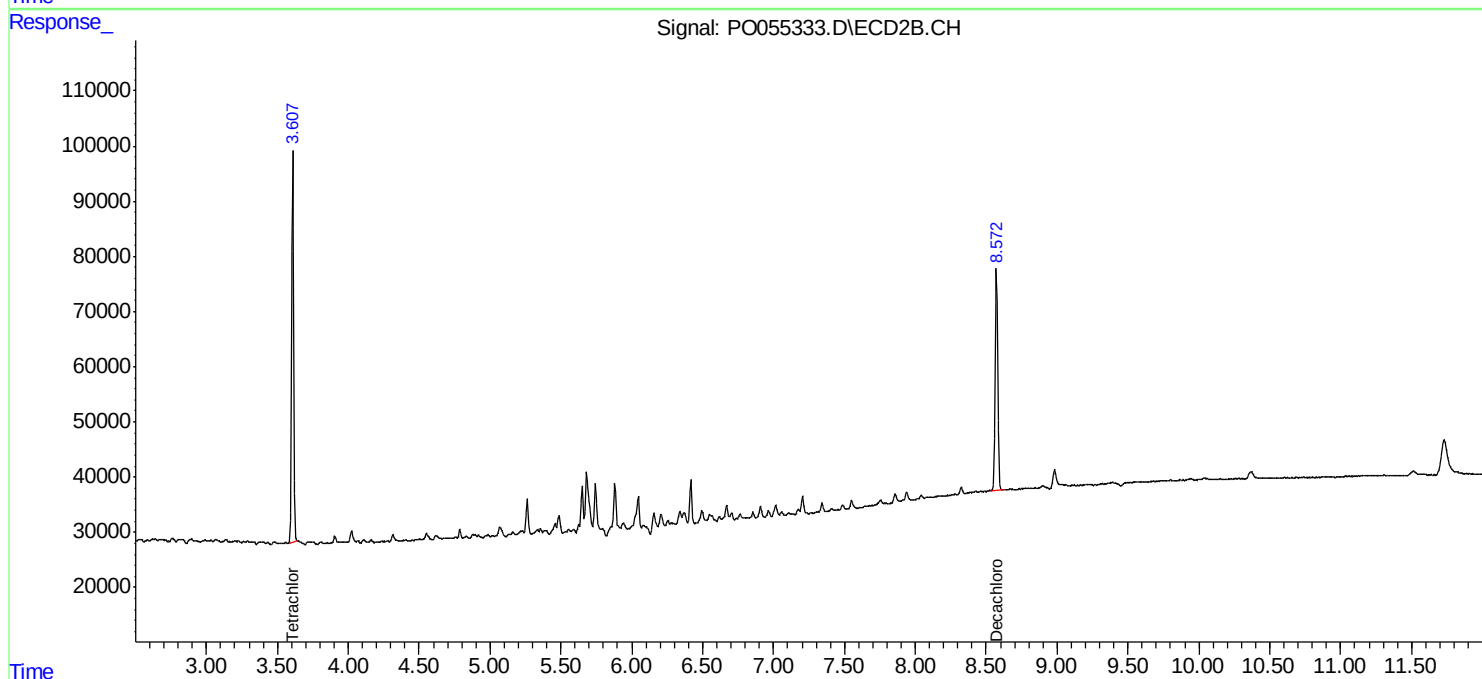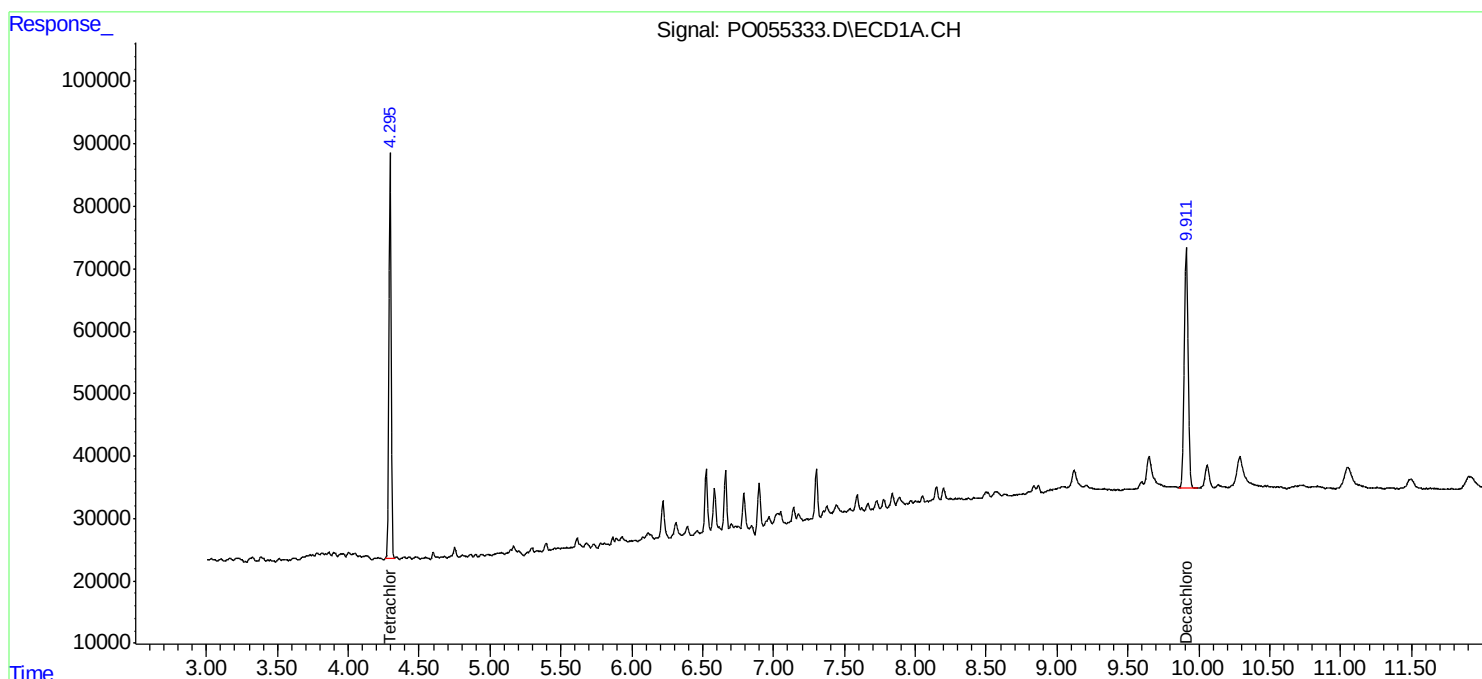


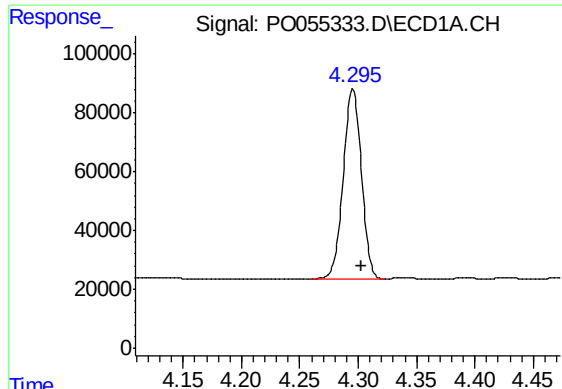

#1 Tetrachloro-m-xylene


R.T.: 4.295 min
Delta R.T.: -0.008 min
Response: 700162
Conc: 20.17 ng/ml

Instrument :
ECD_O
ClientSampleId :
TP-11-S

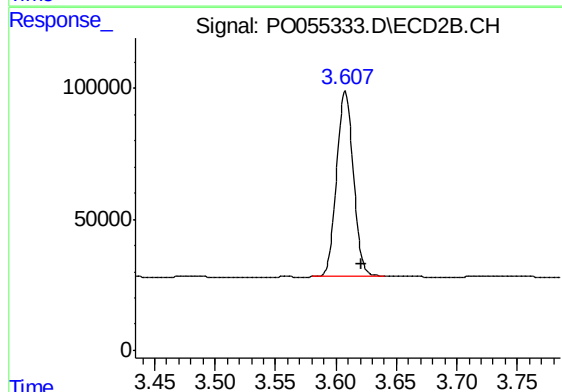


#1 Tetrachloro-m-xylene

R.T.: 3.608 min
Delta R.T.: -0.013 min
Response: 684668
Conc: 21.45 ng/ml

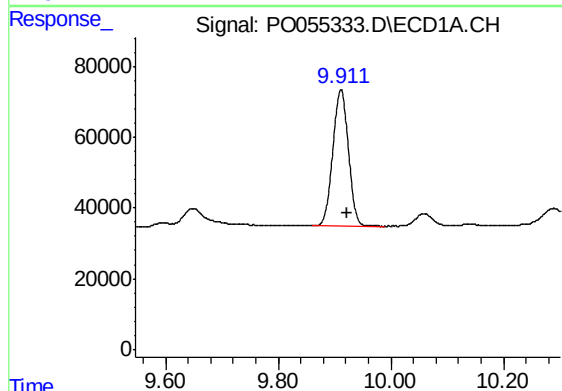

#2 Decachlorobiphenyl

R.T.: 9.912 min
Delta R.T.: -0.012 min
Response: 738183
Conc: 14.97 ng/ml

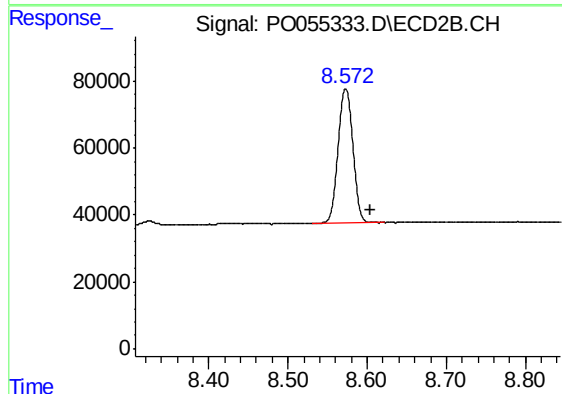

#2 Decachlorobiphenyl

R.T.: 8.573 min
Delta R.T.: -0.031 min
Response: 518155
Conc: 16.27 ng/ml