

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\P0041520\
 Data File : P0067851.D
 Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
 Acq On : 15 Apr 2020 20:31
 Operator : DD\AJ
 Sample : L2255-05
 Misc :
 ALS Vial : 25 Sample Multiplier: 1

Instrument :
 ECD_O
 ClientSampleId :

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Apr 16 03:25:24 2020
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\P0040120.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Fri Apr 03 16:04:09 2020
 Response via : Initial Calibration
 Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	0.000	3.939	0	614042	N.D.	18.320 #
2)	SA Decachlor...	0.000	9.223	0	476188	N.D.	11.517 #
Target Compounds							
29)	L6 AR-1254-4	0.000	6.940	0	41852	N.D.	17.361 #
32)	L7 AR-1260-2	0.000	6.940	0	41852	N.D.	16.299 #
38)	L8 AR-1262-3	0.000	8.154	0	55713	N.D.	28.346 #
39)	L8 AR-1262-4	0.000	8.229	0	50394	N.D.	14.701 #
41)	L9 AR-1268-1	0.000	8.154	0	55713	N.D.	10.354 #
42)	L9 AR-1268-2	0.000	8.229	0	50394	N.D.	10.206 #
43)	L9 AR-1268-3	0.000	8.395	0	183822	N.D.	43.857 #
45)	L9 AR-1268-5	0.000	8.984	0	26566	N.D.	2.060 #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\PO041520\
Data File : PO067851.D
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
Acq On : 15 Apr 2020 20:31
Operator : DD\AJ
Sample : L2255-05
Misc :
ALS Vial : 25 Sample Multiplier: 1

Instrument :
ECD_O
ClientSampleId :

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Apr 16 03:25:24 2020
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\PO040120.M
Quant Title : GC EXTRACTABLES
QLast Update : Fri Apr 03 16:04:09 2020
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

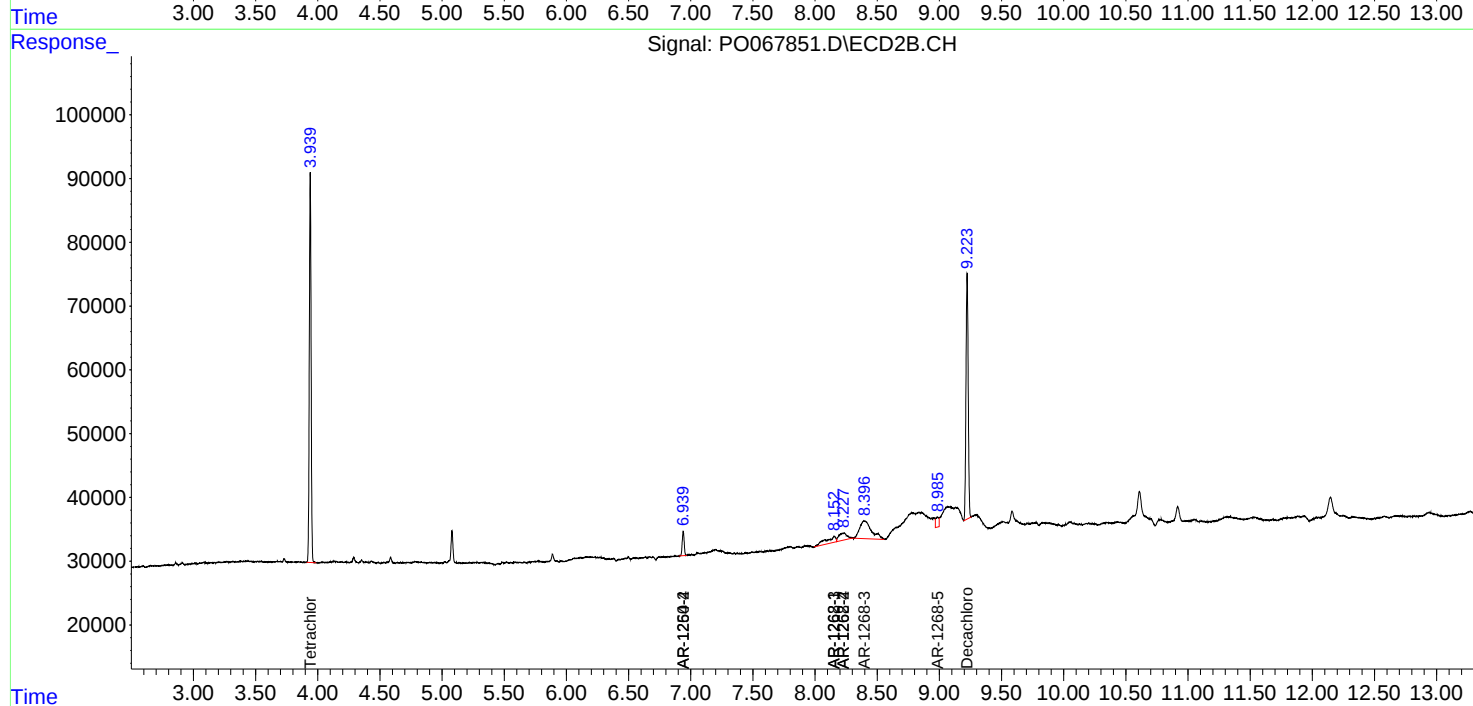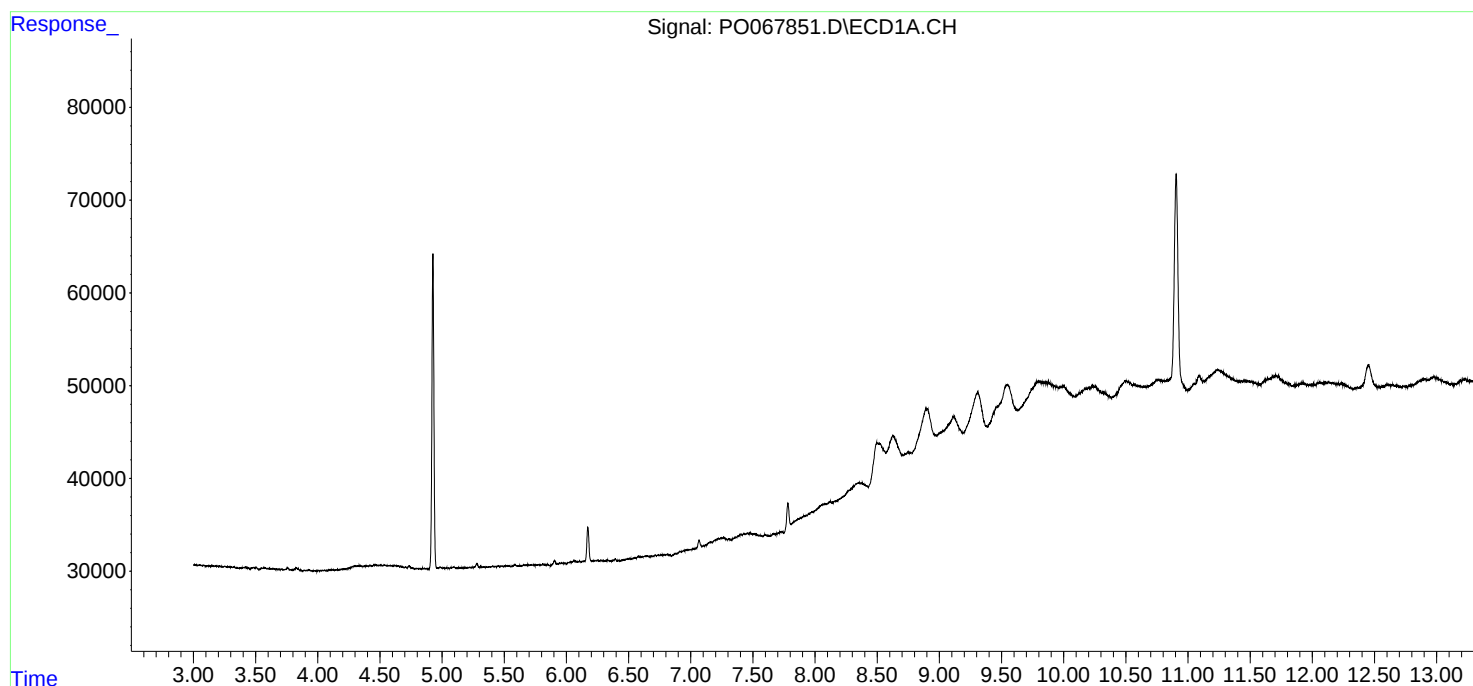


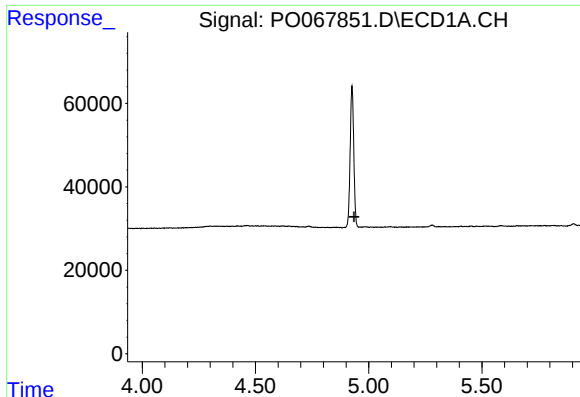

#1 Tetrachloro-m-xylene


R.T.: 0.000 min
Exp R.T.: 4.935 min
Response: 0
Conc: N.D.

Instrument :
ECD_O
ClientSampleId :

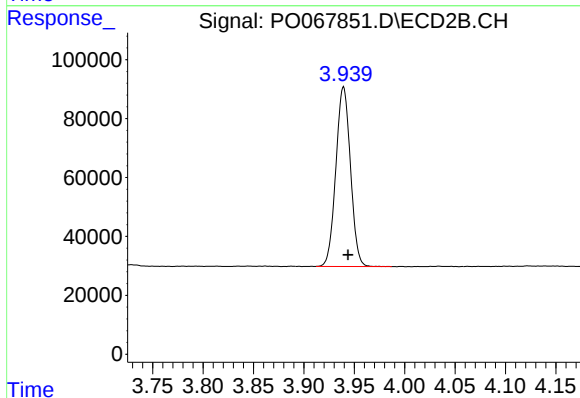


#1 Tetrachloro-m-xylene

R.T.: 3.939 min
Delta R.T.: -0.005 min
Response: 614042
Conc: 18.32 ng/ml

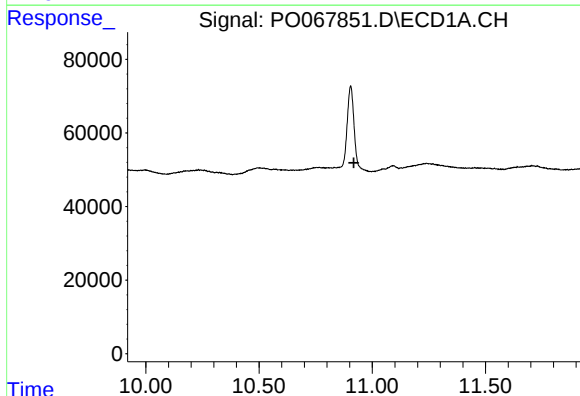


#2 Decachlorobiphenyl

R.T.: 0.000 min
Exp R.T.: 10.919 min
Response: 0
Conc: N.D.

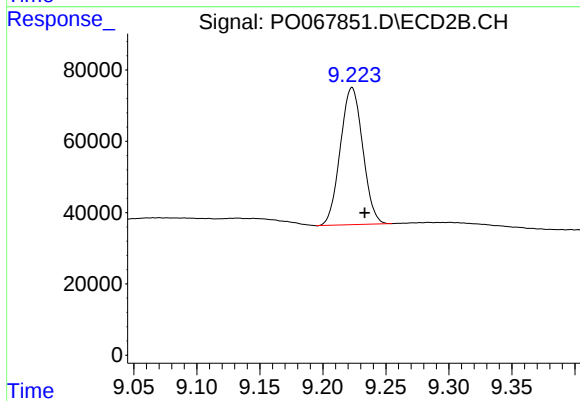

#2 Decachlorobiphenyl


R.T.: 9.223 min
Delta R.T.: -0.010 min
Response: 476188
Conc: 11.52 ng/ml

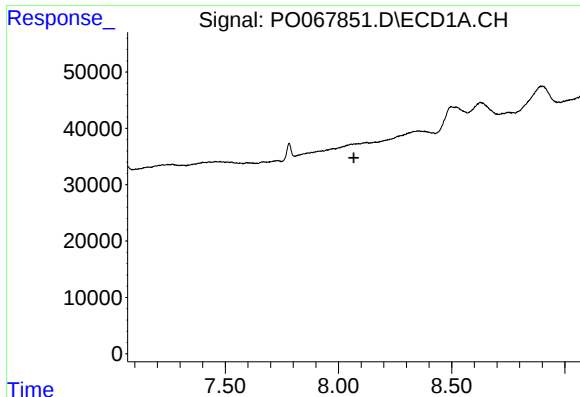

#29 AR-1254-4


R.T.: 0.000 min
Exp R.T.: 8.068 min
Response: 0
Conc: N.D.

Instrument :
ECD_O
ClientSampleId :

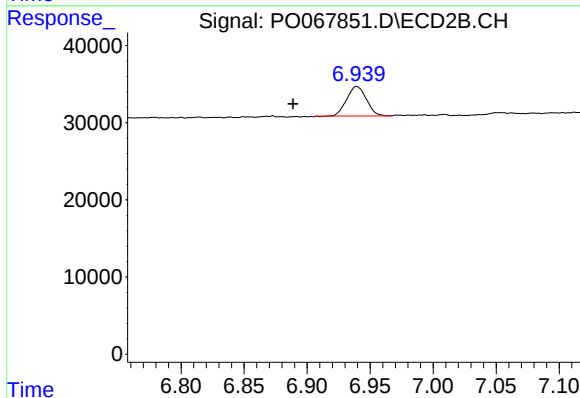


#29 AR-1254-4

R.T.: 6.940 min
Delta R.T.: 0.051 min
Response: 41852
Conc: 17.36 ng/ml

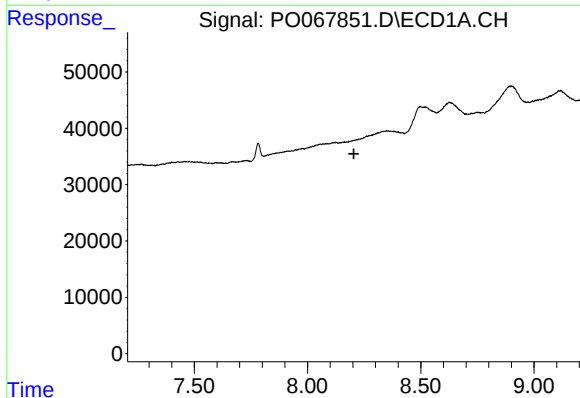


#32 AR-1260-2

R.T.: 0.000 min
Exp R.T.: 8.205 min
Response: 0
Conc: N.D.

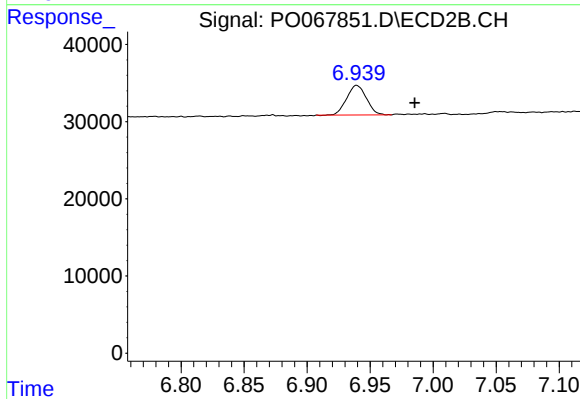

#32 AR-1260-2


R.T.: 6.940 min
Delta R.T.: -0.046 min
Response: 41852
Conc: 16.30 ng/ml

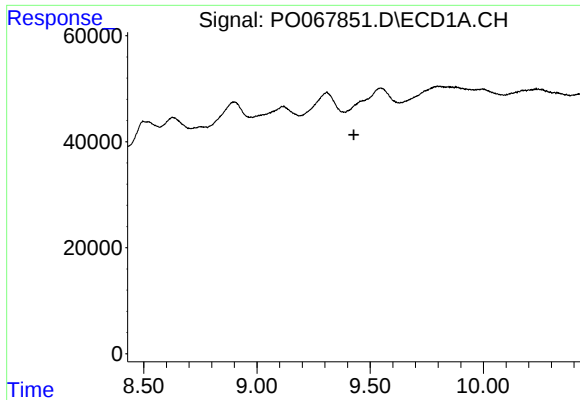

#38 AR-1262-3


R.T.: 0.000 min
Exp R.T.: 9.428 min
Response: 0
Conc: N.D.

Instrument :
ECD_O
ClientSampleId :

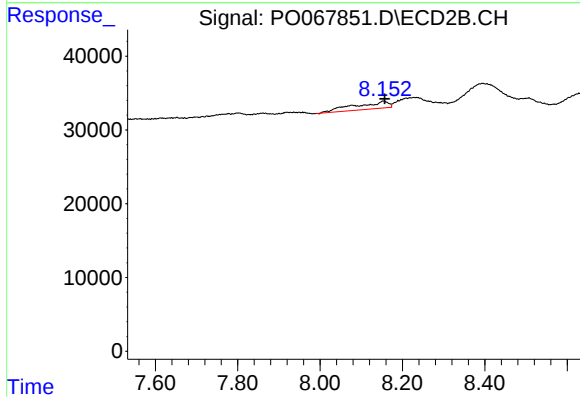


#38 AR-1262-3

R.T.: 8.154 min
Delta R.T.: -0.003 min
Response: 55713
Conc: 28.35 ng/ml

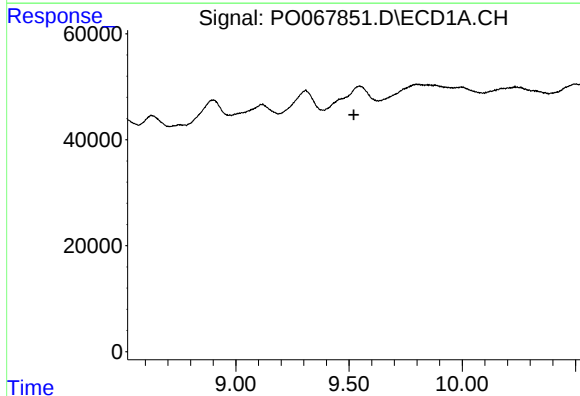


#39 AR-1262-4

R.T.: 0.000 min
Exp R.T.: 9.521 min
Response: 0
Conc: N.D.

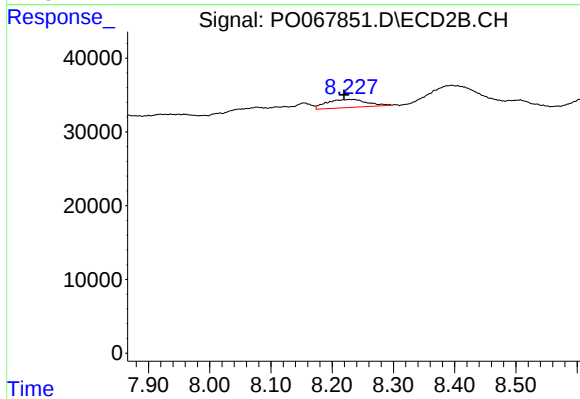

#39 AR-1262-4


R.T.: 8.229 min
Delta R.T.: 0.010 min
Response: 50394
Conc: 14.70 ng/ml

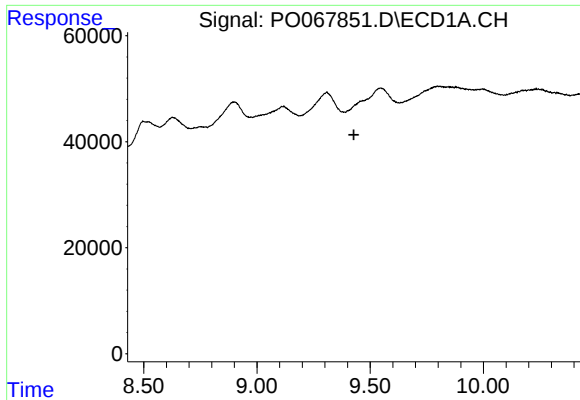

#41 AR-1268-1


R.T.: 0.000 min
Exp R.T.: 9.428 min
Response: 0
Conc: N.D.

Instrument :
ECD_O
ClientSampleId :

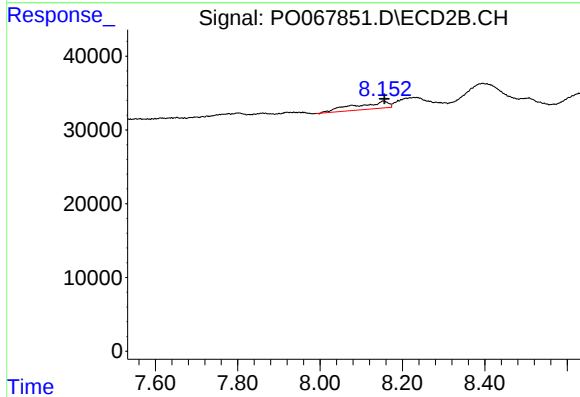


#41 AR-1268-1

R.T.: 8.154 min
Delta R.T.: -0.002 min
Response: 55713
Conc: 10.35 ng/ml

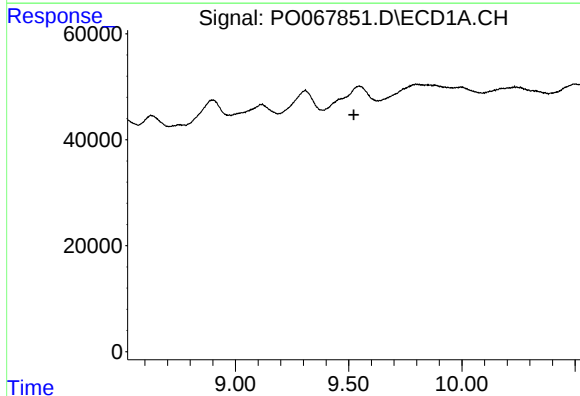


#42 AR-1268-2

R.T.: 0.000 min
Exp R.T.: 9.523 min
Response: 0
Conc: N.D.

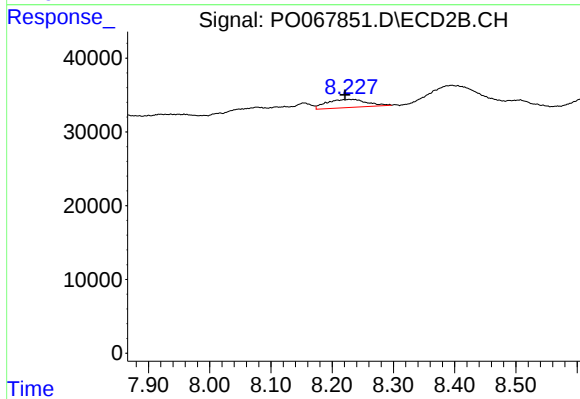

#42 AR-1268-2


R.T.: 8.229 min
Delta R.T.: 0.008 min
Response: 50394
Conc: 10.21 ng/ml

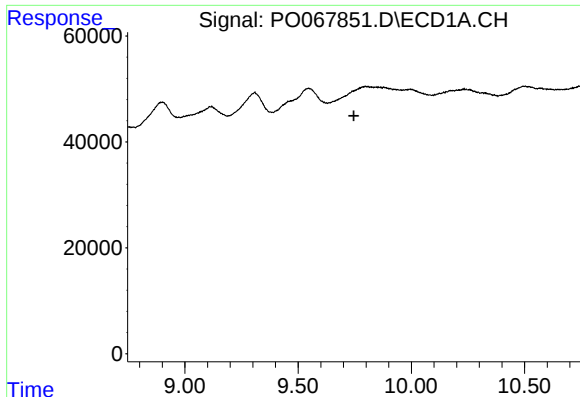

#43 AR-1268-3


R.T.: 0.000 min
Exp R.T.: 9.746 min
Response: 0
Conc: N.D.

Instrument :
ECD_O
ClientSampleId :

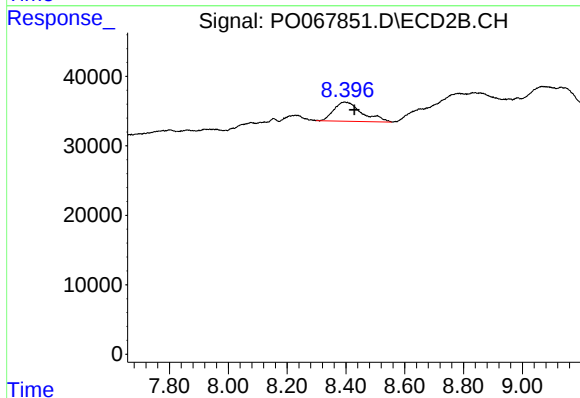


#43 AR-1268-3

R.T.: 8.395 min
Delta R.T.: -0.034 min
Response: 183822
Conc: 43.86 ng/ml

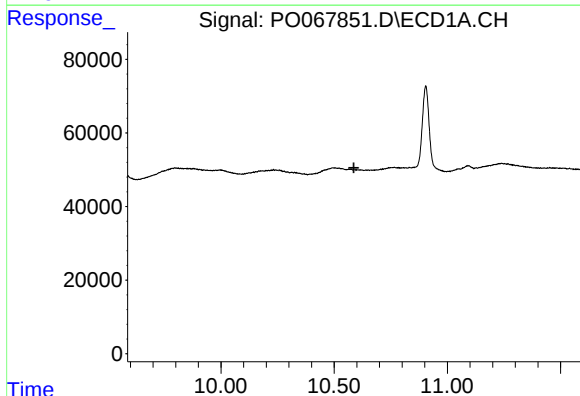

#45 AR-1268-5

R.T.: 0.000 min
Exp R.T.: 10.587 min
Response: 0
Conc: N.D.

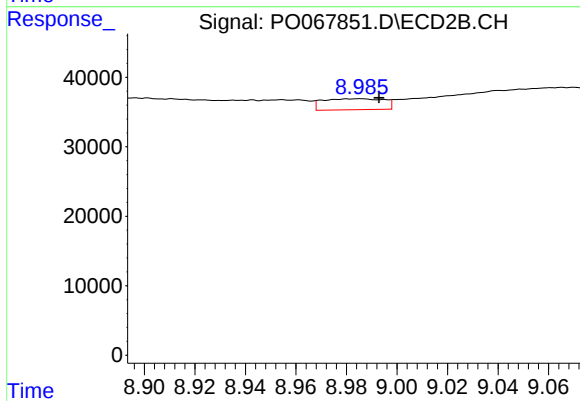

#45 AR-1268-5

R.T.: 8.984 min
Delta R.T.: -0.009 min
Response: 26566
Conc: 2.06 ng/ml