

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\P0041520\
 Data File : P0067836.D
 Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
 Acq On : 15 Apr 2020 12:10
 Operator : DD\AJ
 Sample : I.BLK
 Misc :
 ALS Vial : 2 Sample Multiplier: 1

Instrument :
 ECD_O
 ClientSampleId :
 I.BLK

Manual Integrations
 APPROVED

Sohil
 4/16/2020 9:02:33 AM

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Apr 15 12:36:40 2020
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\P0040120.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Fri Apr 03 16:04:09 2020
 Response via : Initial Calibration
 Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	4.924	3.939	574180	778469	24.111m	23.226
2) SA Decachlor...	10.900	9.223	765178	862556	22.476m	20.862

Target Compounds

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\P0041520\
Data File : P0067836.D
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
Acq On : 15 Apr 2020 12:10
Operator : DD\AJ
Sample : I.BLK
Misc :
ALS Vial : 2 Sample Multiplier: 1


Instrument :
ECD_O
ClientSampleId :
I.BLK


Manual Integrations
APPROVED

Sohil
4/16/2020 9:02:33 AM

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Apr 15 12:36:40 2020
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\P0040120.M
Quant Title : GC EXTRACTABLES
QLast Update : Fri Apr 03 16:04:09 2020
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

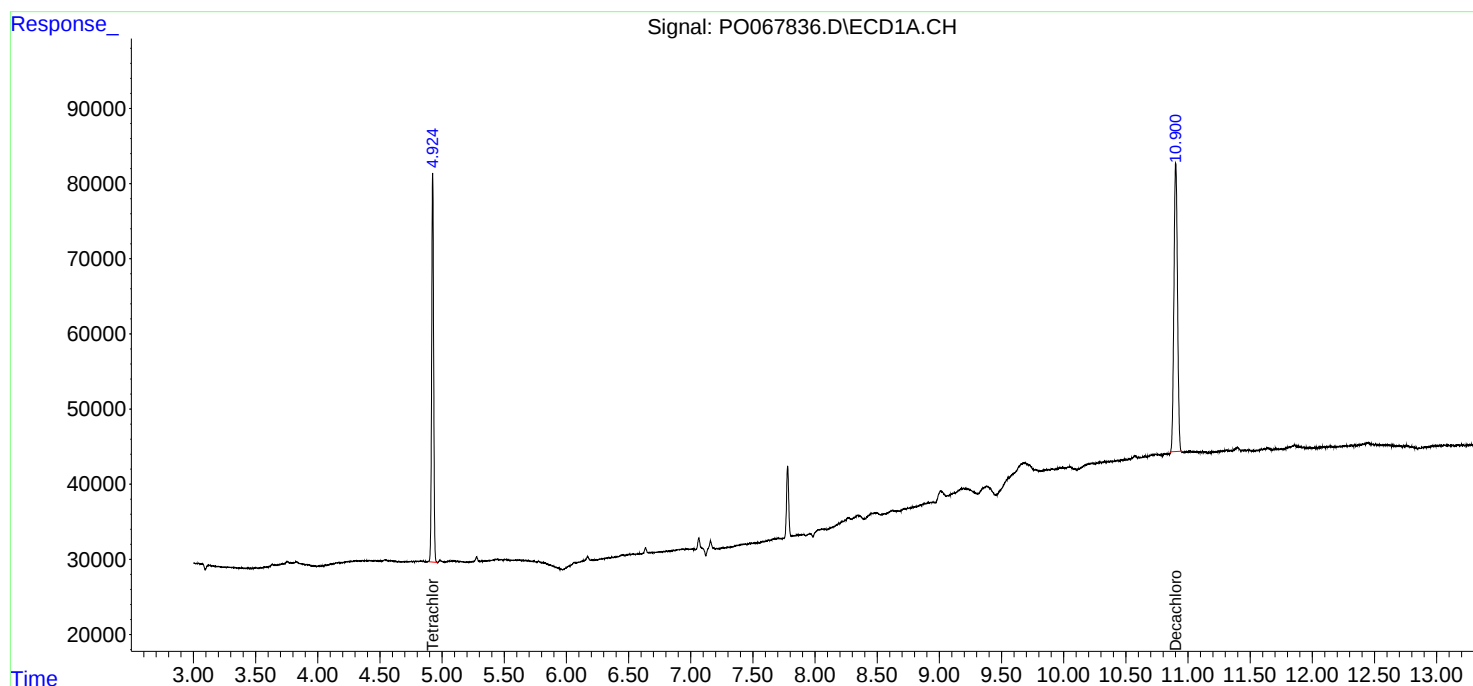

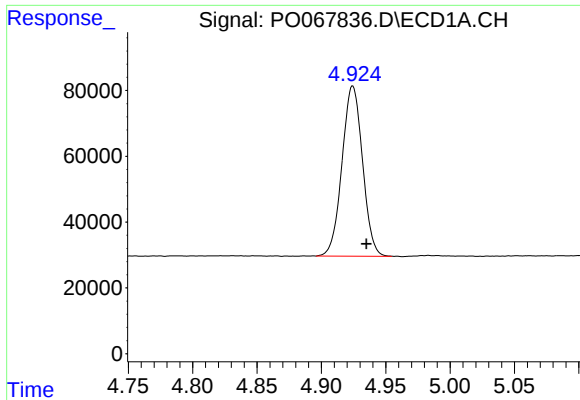


#1 Tetrachloro-m-xylene

R.T.: 4.924 min
Delta R.T.: -0.011 min
Response: 574180
Conc: 24.11 ng/ml m

Instrument :
ECD_O
ClientSampleId :
I.BLK


Manual Integrations
APPROVED

Sohil
4/16/2020 9:02:33 AM

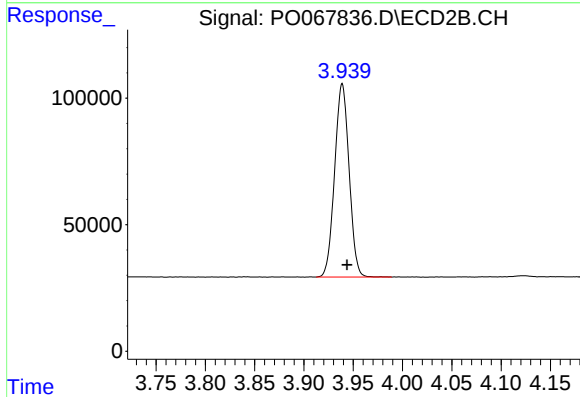


#1 Tetrachloro-m-xylene

R.T.: 3.939 min
Delta R.T.: -0.005 min
Response: 778469
Conc: 23.23 ng/ml

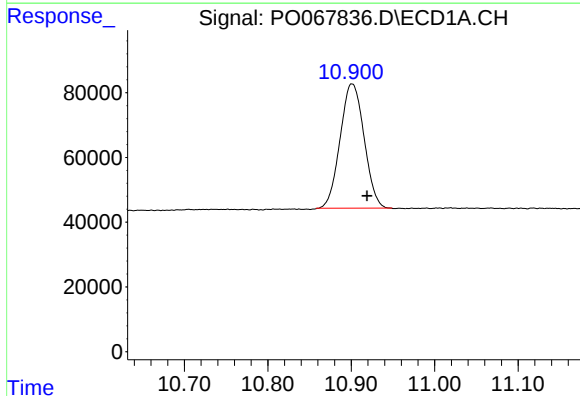

#2 Decachlorobiphenyl

R.T.: 10.900 min
Delta R.T.: -0.019 min
Response: 765178
Conc: 22.48 ng/ml m

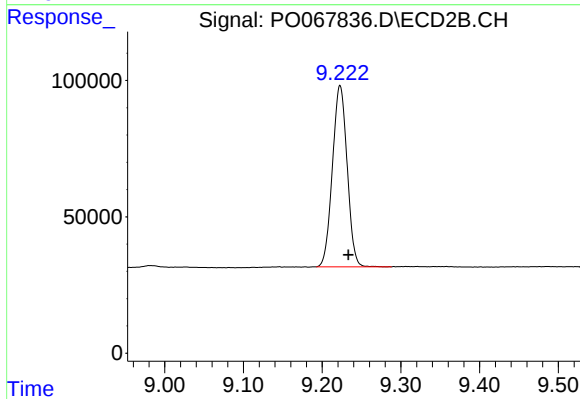

#2 Decachlorobiphenyl

R.T.: 9.223 min
Delta R.T.: -0.010 min
Response: 862556
Conc: 20.86 ng/ml