

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\P0041619\
 Data File : P0055371.D
 Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
 Acq On : 16 Apr 2019 19:11
 Operator : SM/SJ
 Sample : K2423-09
 Misc :
 ALS Vial : 13 Sample Multiplier: 1

Instrument :
 ECD_O
 ClientSampleId :

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Apr 17 00:59:48 2019
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\P0032519.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Mon Mar 25 17:22:26 2019
 Response via : Initial Calibration
 Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	4.293	3.605	726813	702889	20.943	22.026
2)	SA Decachlor...	9.908	8.569	745519	531965	15.123	16.703
Target Compounds							
9)	L2 AR-1221-2	4.598	3.906	11954	14171	35.249	47.271 #
10)	L2 AR-1221-3	0.000	4.034	0	15943	N.D.	17.296 #
11)	L3 AR-1232-1	0.000	4.034	0	15943	N.D.	21.261 #
28)	L6 AR-1254-3	6.896	0.000	11441	0	3.638	N.D. #
29)	L6 AR-1254-4	0.000	6.330	0	7948	N.D.	4.059 #
32)	L7 AR-1260-2	7.372	6.330	5288	7948	1.704	2.887 #
45)	L9 AR-1268-5	9.637	0.000	15061	0	0.914	N.D. #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\P0041619\
Data File : P0055371.D
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
Acq On : 16 Apr 2019 19:11
Operator : SM/SJ
Sample : K2423-09
Misc :
ALS Vial : 13 Sample Multiplier: 1

Instrument :
ECD_O
ClientSampleId :

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Apr 17 00:59:48 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\P0032519.M
Quant Title : GC EXTRACTABLES
QLast Update : Mon Mar 25 17:22:26 2019
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

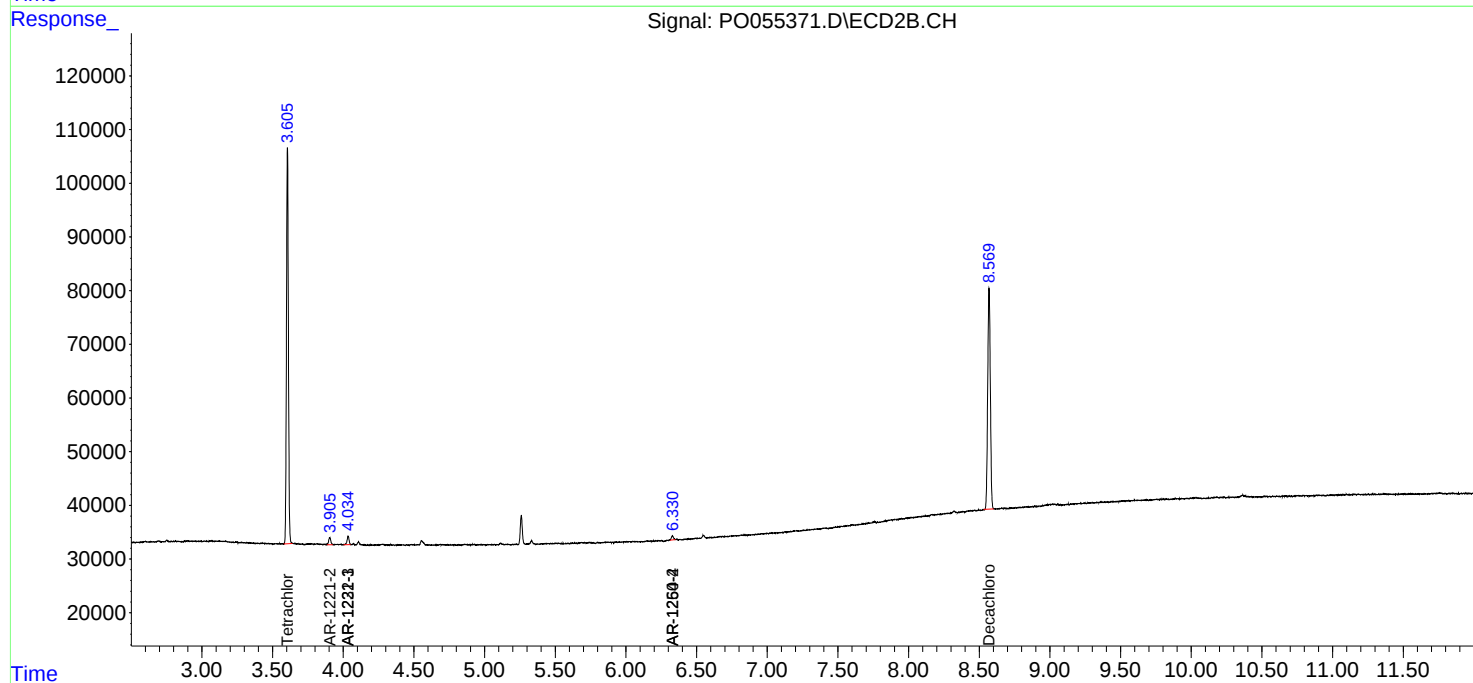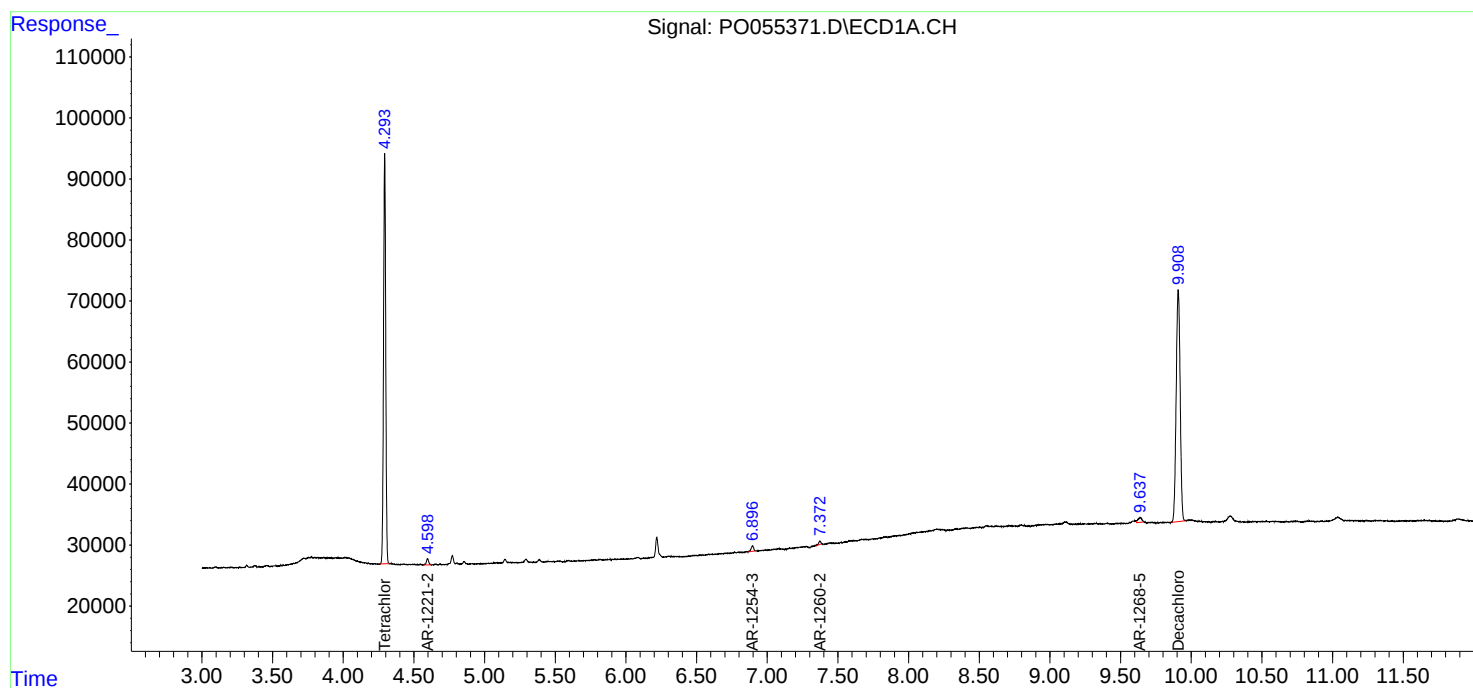


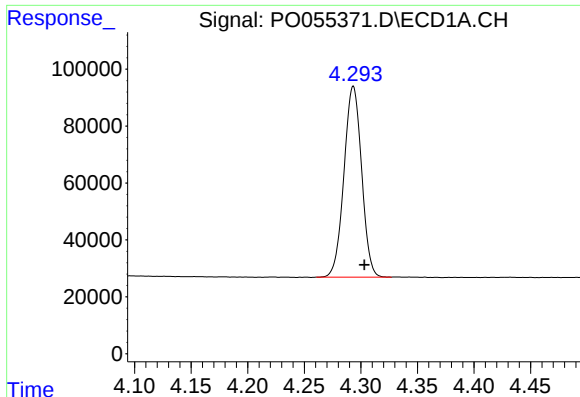

#1 Tetrachloro-m-xylene


R.T.: 4.293 min
Delta R.T.: -0.010 min
Response: 726813
Conc: 20.94 ng/ml

Instrument :
ECD_O
ClientSampleId :

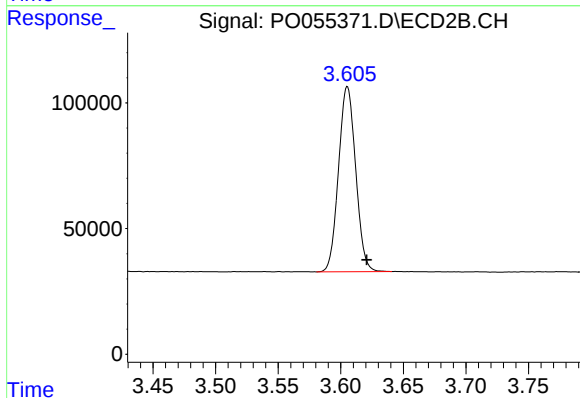


#1 Tetrachloro-m-xylene

R.T.: 3.605 min
Delta R.T.: -0.016 min
Response: 702889
Conc: 22.03 ng/ml

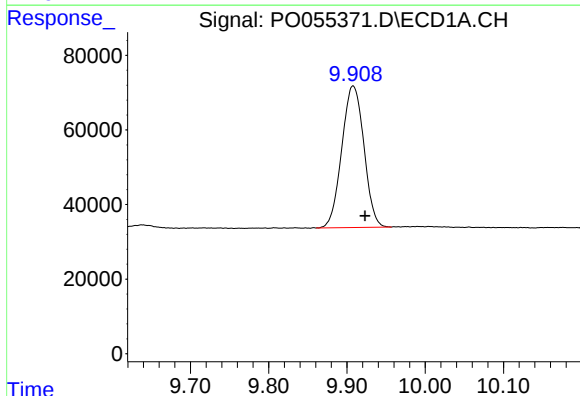


#2 Decachlorobiphenyl

R.T.: 9.908 min
Delta R.T.: -0.015 min
Response: 745519
Conc: 15.12 ng/ml

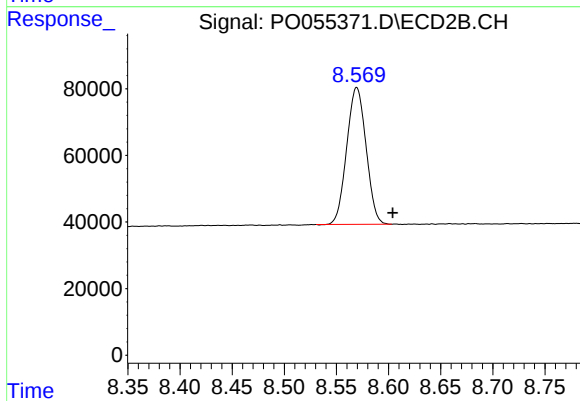

#2 Decachlorobiphenyl


R.T.: 8.569 min
Delta R.T.: -0.035 min
Response: 531965
Conc: 16.70 ng/ml

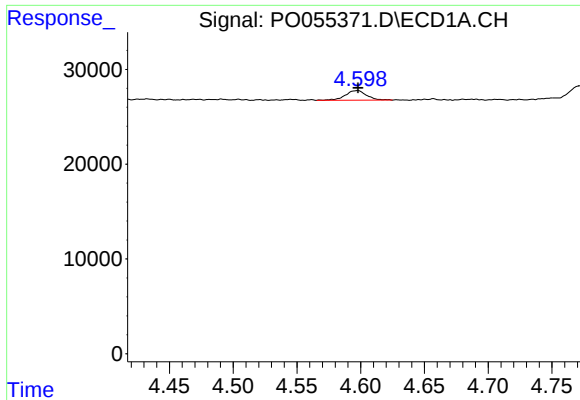

#9 AR-1221-2


R.T.: 4.598 min
Delta R.T.: 0.000 min
Response: 11954
Conc: 35.25 ng/ml

Instrument :
ECD_O
ClientSampleId :

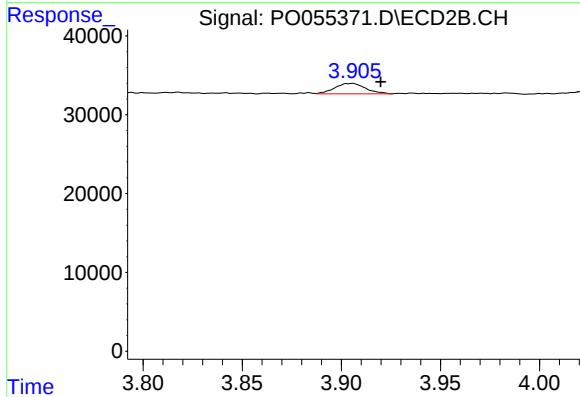


#9 AR-1221-2

R.T.: 3.906 min
Delta R.T.: -0.014 min
Response: 14171
Conc: 47.27 ng/ml

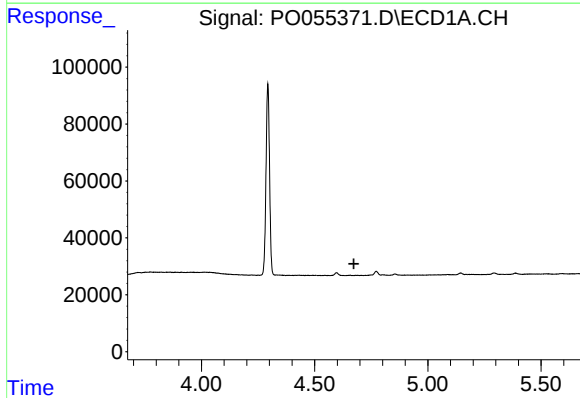


#10 AR-1221-3

R.T.: 0.000 min
Exp R.T. : 4.673 min
Response: 0
Conc: N.D.

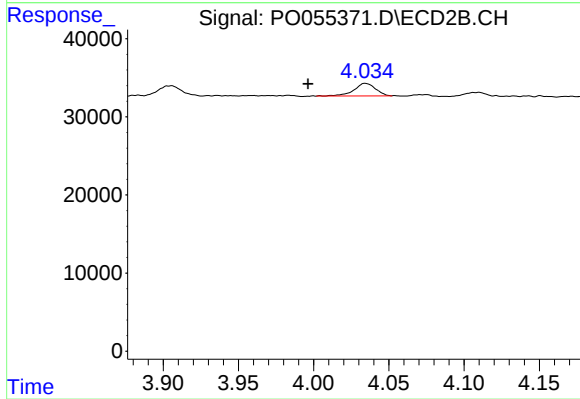

#10 AR-1221-3


R.T.: 4.034 min
Delta R.T.: 0.038 min
Response: 15943
Conc: 17.30 ng/ml

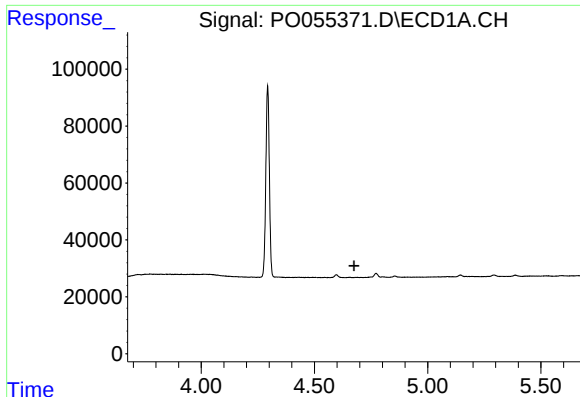

#11 AR-1232-1


R.T.: 0.000 min
Exp R.T.: 4.675 min
Response: 0
Conc: N.D.

Instrument :
ECD_O
ClientSampleId :

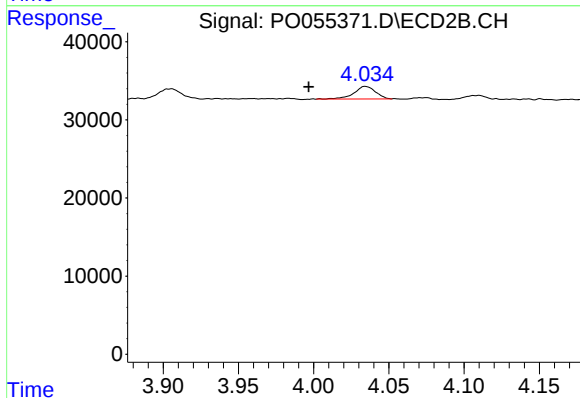


#11 AR-1232-1

R.T.: 4.034 min
Delta R.T.: 0.038 min
Response: 15943
Conc: 21.26 ng/ml

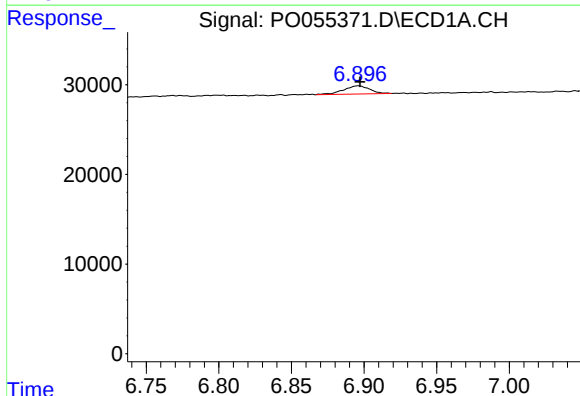


#28 AR-1254-3

R.T.: 6.896 min
Delta R.T.: -0.001 min
Response: 11441
Conc: 3.64 ng/ml

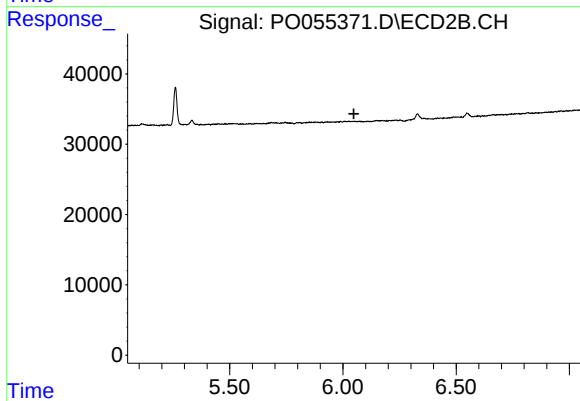

#28 AR-1254-3


R.T.: 0.000 min
Exp R.T.: 6.049 min
Response: 0
Conc: N.D.

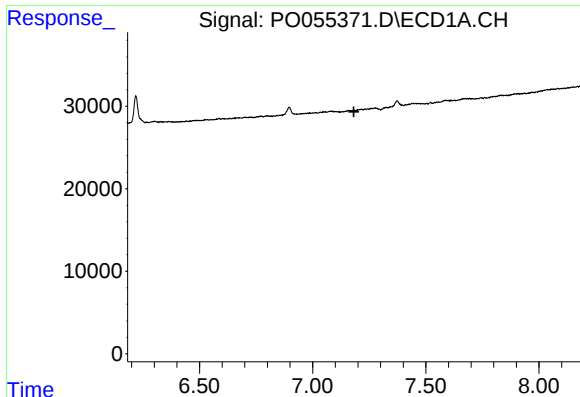

#29 AR-1254-4


R.T.: 0.000 min
Exp R.T.: 7.182 min
Response: 0
Conc: N.D.

Instrument :
ECD_O
ClientSampleId :

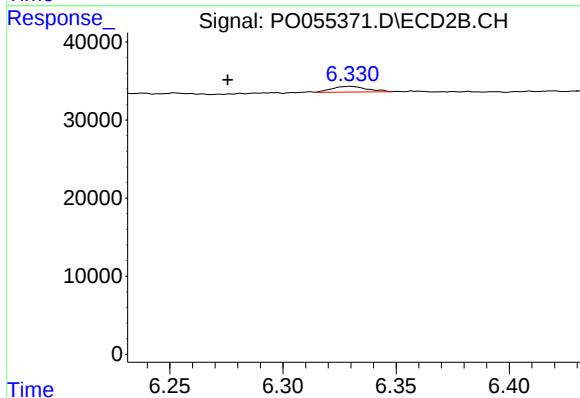


#29 AR-1254-4

R.T.: 6.330 min
Delta R.T.: 0.054 min
Response: 7948
Conc: 4.06 ng/ml

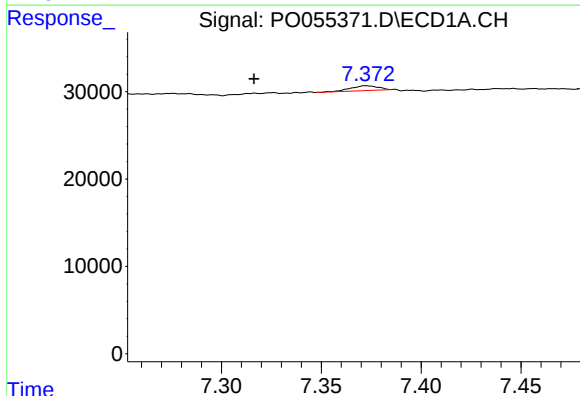


#32 AR-1260-2

R.T.: 7.372 min
Delta R.T.: 0.056 min
Response: 5288
Conc: 1.70 ng/ml

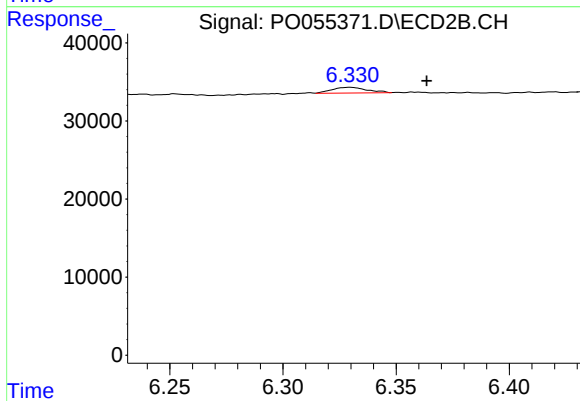

#32 AR-1260-2


R.T.: 6.330 min
Delta R.T.: -0.034 min
Response: 7948
Conc: 2.89 ng/ml

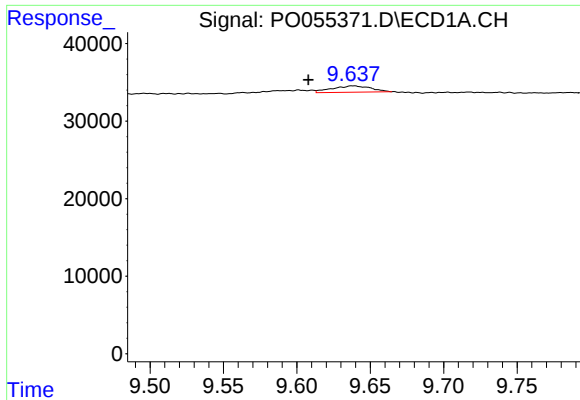

#45 AR-1268-5

R.T.: 9.637 min
Delta R.T.: 0.029 min
Response: 15061
Conc: 0.91 ng/ml

Instrument :
ECD_O
ClientSampleId :

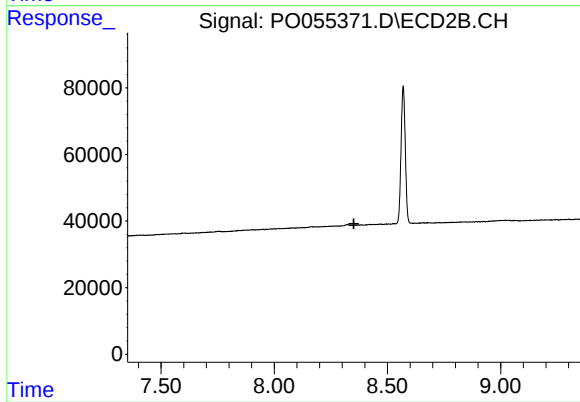

#45 AR-1268-5

R.T.: 0.000 min
Exp R.T. : 8.352 min
Response: 0
Conc: N.D.