

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\P0041619\
 Data File : P0055345.D
 Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
 Acq On : 16 Apr 2019 10:39
 Operator : SM/SJ
 Sample : K1560-09
 Misc : AR1221 MDL 25PPB
 ALS Vial : 4 Sample Multiplier: 1

Instrument :
 ECD_O
 ClientSampleId :
 MDL-MDL-WATER-03-QT1-2019

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Apr 17 00:47:16 2019
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\P0032519.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Mon Mar 25 17:22:26 2019
 Response via : Initial Calibration
 Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	4.300	3.605	492369	427828	14.187	13.406
2) SA Decachlor...	9.919	8.573	815895	551169	16.550	17.306
Target Compounds						
8) L2 AR-1221-1	4.512	3.816	16888	13629	38.683	35.054
9) L2 AR-1221-2	4.597	3.903	16382	14085	48.307	46.983
10) L2 AR-1221-3	4.672	3.977	43711	36058	42.080	39.118



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\P0041619\
Data File : P0055345.D
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
Acq On : 16 Apr 2019 10:39
Operator : SM/SJ
Sample : K1560-09
Misc : AR1221 MDL 25PPB
ALS Vial : 4 Sample Multiplier: 1

Instrument :
ECD_O
ClientSampleId :
MDL-MDL-WATER-03-QT1-2019

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Apr 17 00:47:16 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\P0032519.M
Quant Title : GC EXTRACTABLES
QLast Update : Mon Mar 25 17:22:26 2019
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

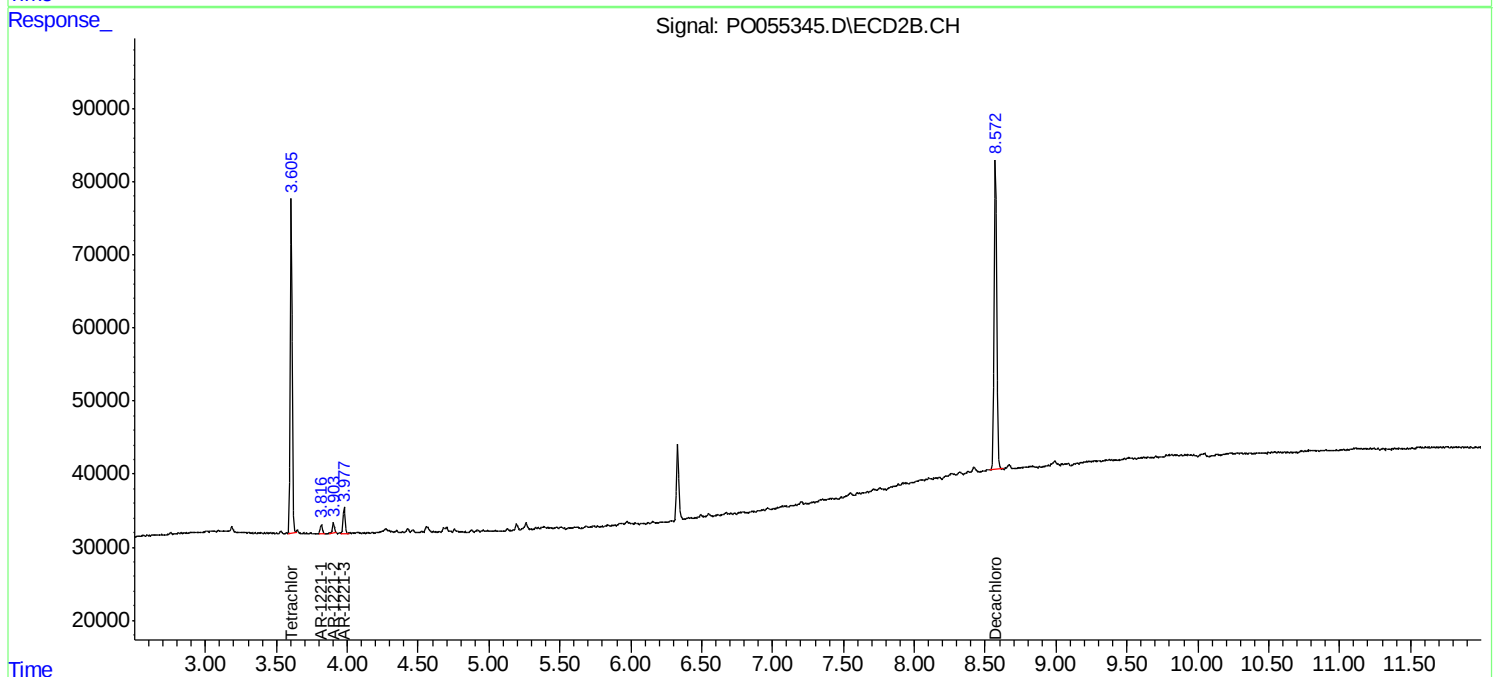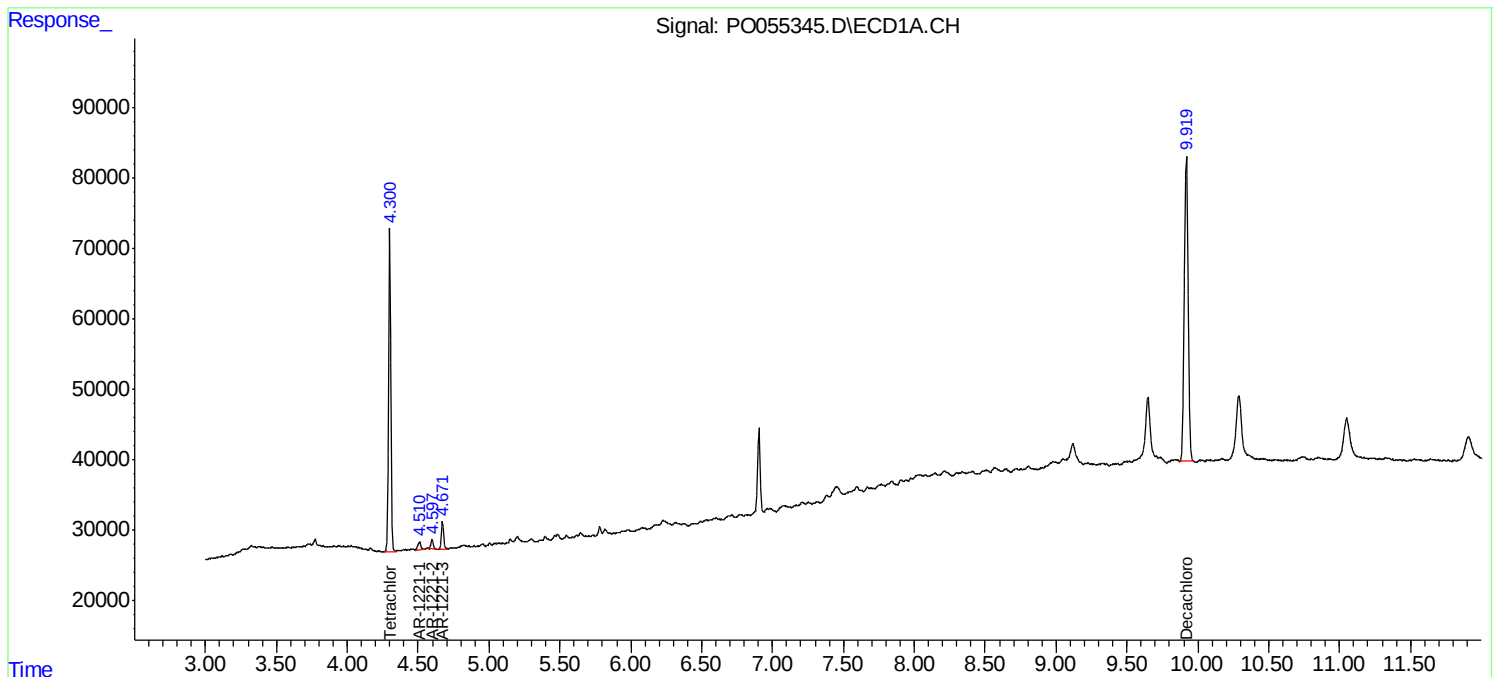


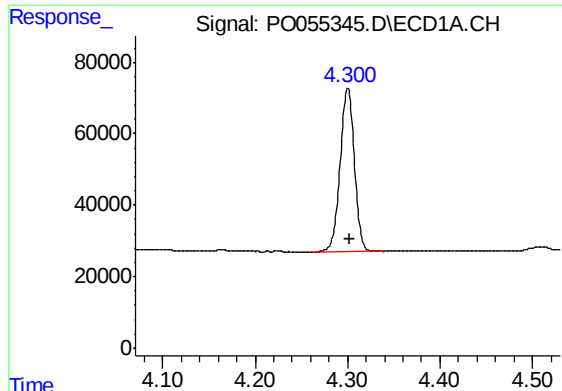

#1 Tetrachloro-m-xylene


R.T.: 4.300 min
Delta R.T.: -0.003 min
Response: 492369
Conc: 14.19 ng/ml

Instrument :
ECD_O
ClientSampleId :
MDL-MDL-WATER-03-QT1-2019

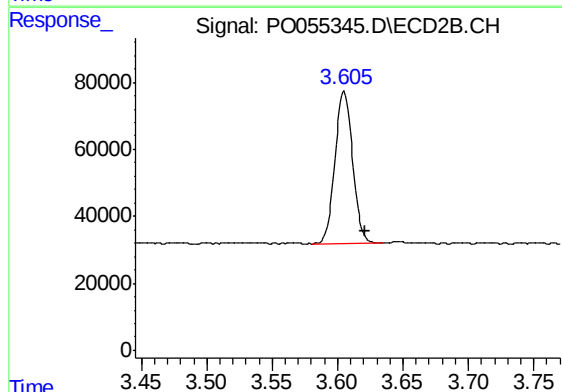


#1 Tetrachloro-m-xylene

R.T.: 3.605 min
Delta R.T.: -0.016 min
Response: 427828
Conc: 13.41 ng/ml

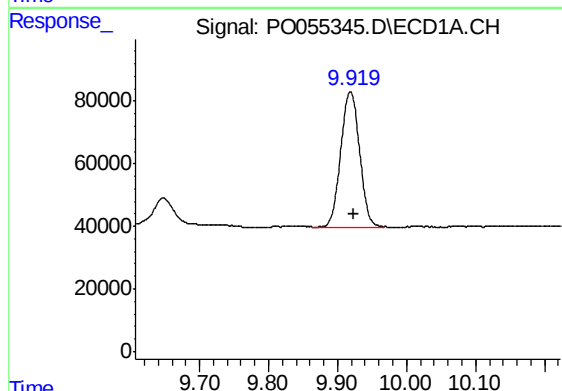


#2 Decachlorobiphenyl

R.T.: 9.919 min
Delta R.T.: -0.004 min
Response: 815895
Conc: 16.55 ng/ml

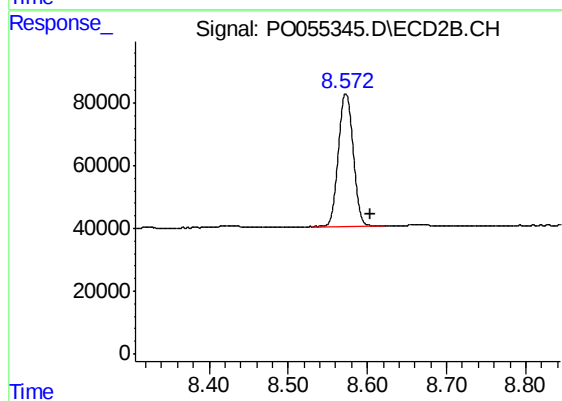

#2 Decachlorobiphenyl


R.T.: 8.573 min
Delta R.T.: -0.031 min
Response: 551169
Conc: 17.31 ng/ml

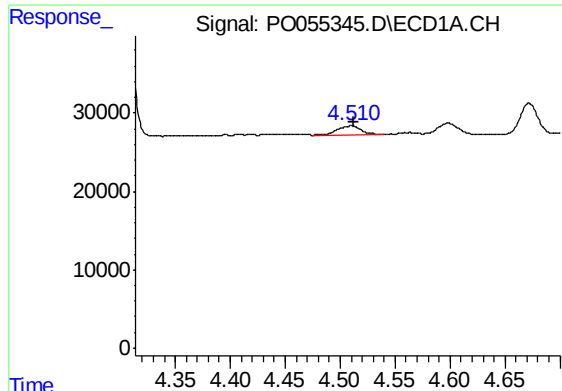

#8 AR-1221-1


R.T.: 4.512 min
Delta R.T.: 0.000 min
Response: 16888
Conc: 38.68 ng/ml

Instrument :
ECD_O
ClientSampleId :
MDL-MDL-WATER-03-QT1-2019

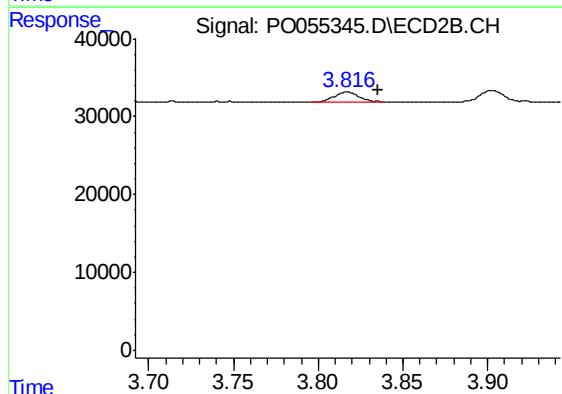


#8 AR-1221-1

R.T.: 3.816 min
Delta R.T.: -0.019 min
Response: 13629
Conc: 35.05 ng/ml

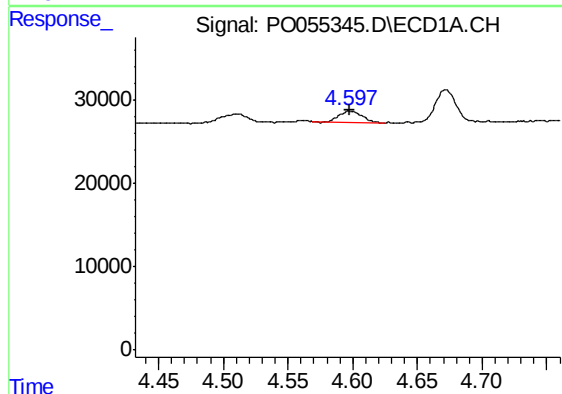


#9 AR-1221-2

R.T.: 4.597 min
Delta R.T.: 0.000 min
Response: 16382
Conc: 48.31 ng/ml

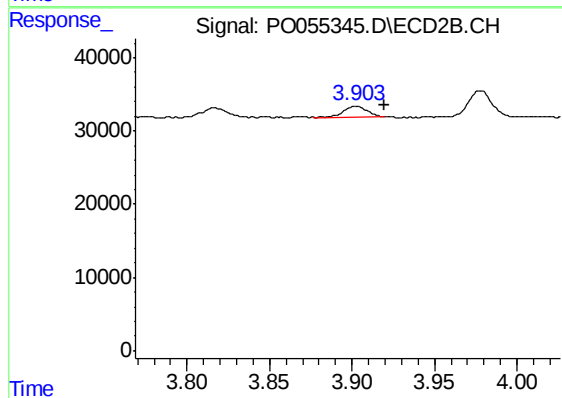

#9 AR-1221-2


R.T.: 3.903 min
Delta R.T.: -0.017 min
Response: 14085
Conc: 46.98 ng/ml

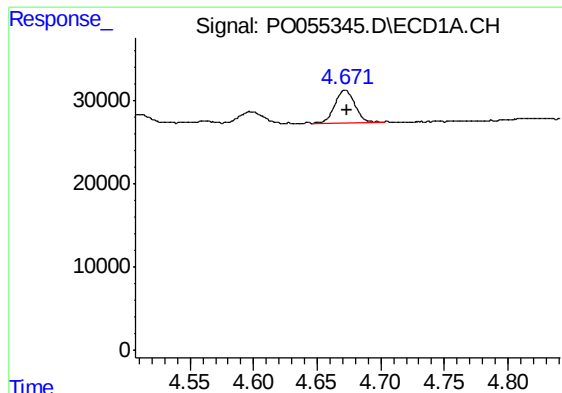

#10 AR-1221-3

R.T.: 4.672 min
Delta R.T.: -0.002 min
Response: 43711
Conc: 42.08 ng/ml

Instrument :
ECD_O
ClientSampleId :
MDL-MDL-WATER-03-QT1-2019

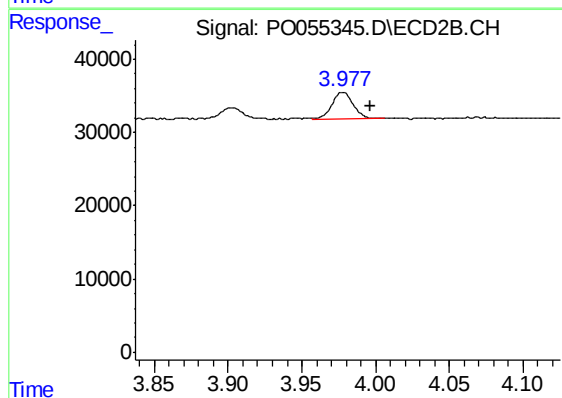

#10 AR-1221-3

R.T.: 3.977 min
Delta R.T.: -0.019 min
Response: 36058
Conc: 39.12 ng/ml