

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\P0041619\
 Data File : P0055365.D
 Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
 Acq On : 16 Apr 2019 17:29
 Operator : SM/SJ
 Sample : K2411-07
 Misc :
 ALS Vial : 7 Sample Multiplier: 1

Instrument :
 ECD_O
 ClientSampleId :
 TP-14-S

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Apr 17 00:57:02 2019
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\P0032519.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Mon Mar 25 17:22:26 2019
 Response via : Initial Calibration
 Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	4.294	3.606	722905	718554	20.830	22.516
2) SA Decachlor...	9.909	8.571	873525	590879	17.719	18.553

Target Compounds



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\P0041619\
Data File : P0055365.D
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
Acq On : 16 Apr 2019 17:29
Operator : SM/SJ
Sample : K2411-07
Misc :
ALS Vial : 7 Sample Multiplier: 1

Instrument :
ECD_O
ClientSampleId :
TP-14-S

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Apr 17 00:57:02 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\P0032519.M
Quant Title : GC EXTRACTABLES
QLast Update : Mon Mar 25 17:22:26 2019
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

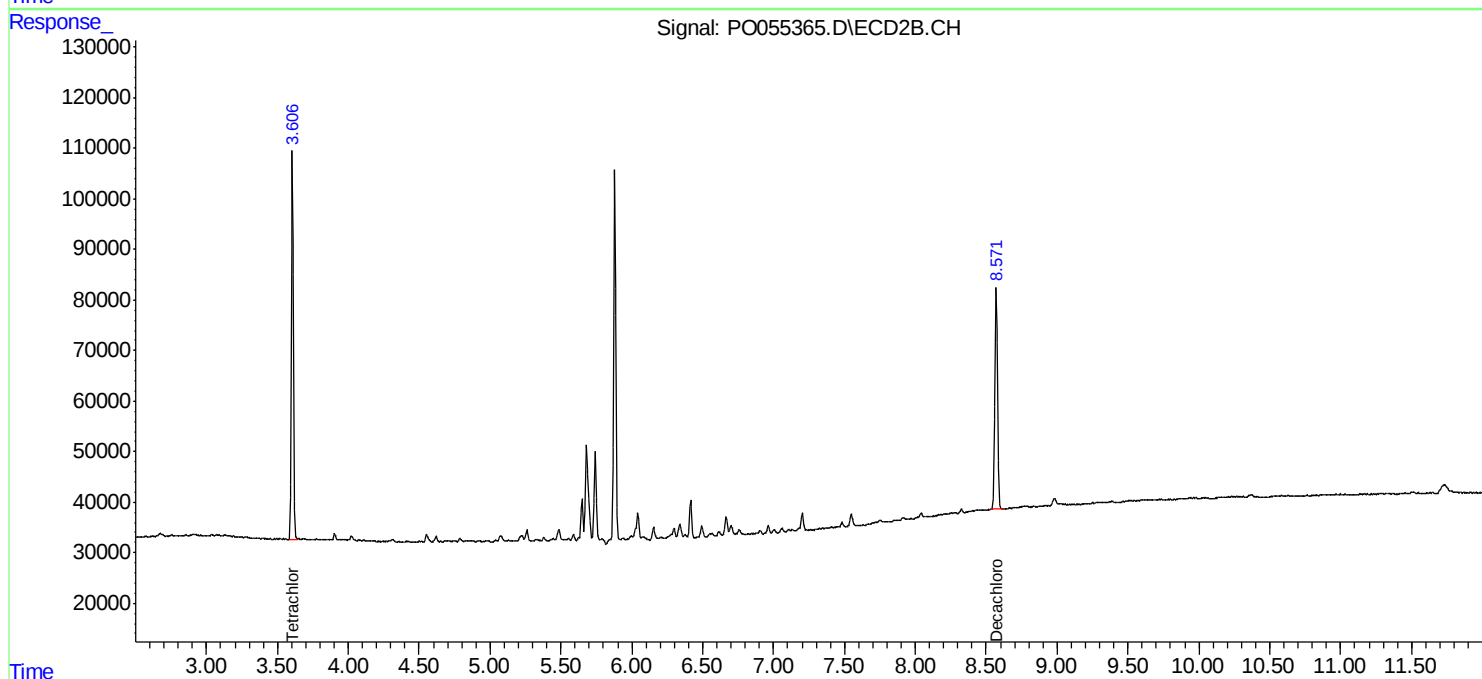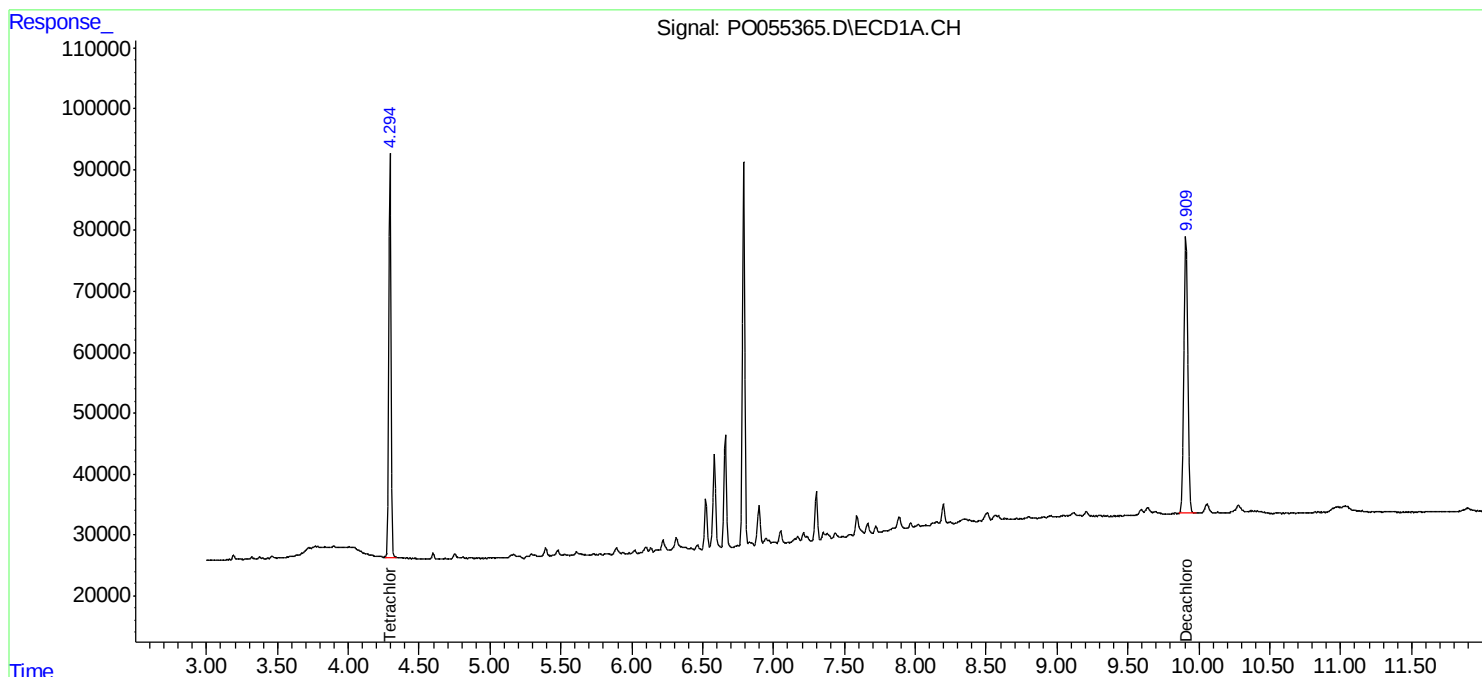


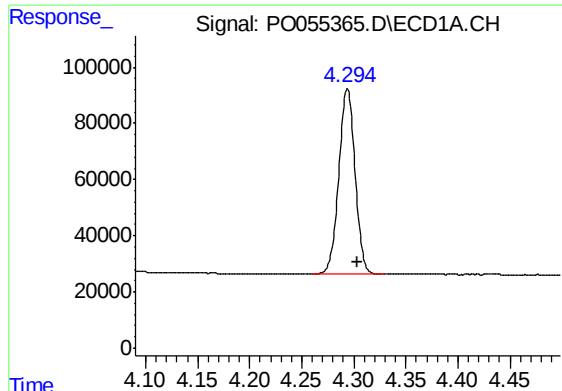

#1 Tetrachloro-m-xylene


R.T.: 4.294 min
Delta R.T.: -0.009 min
Response: 722905
Conc: 20.83 ng/ml

Instrument :
ECD_O
ClientSampleId :
TP-14-S

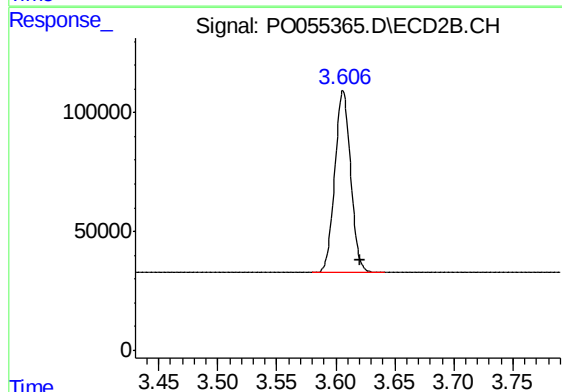


#1 Tetrachloro-m-xylene

R.T.: 3.606 min
Delta R.T.: -0.015 min
Response: 718554
Conc: 22.52 ng/ml

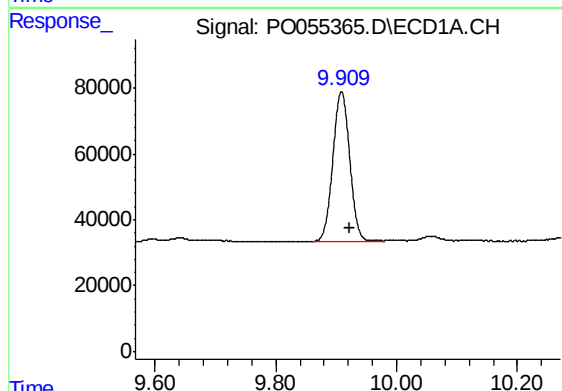

#2 Decachlorobiphenyl

R.T.: 9.909 min
Delta R.T.: -0.014 min
Response: 873525
Conc: 17.72 ng/ml

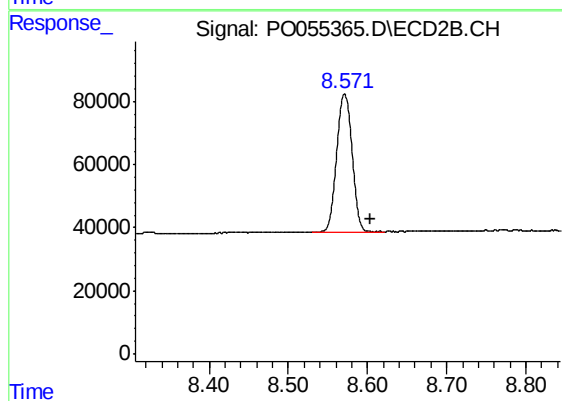

#2 Decachlorobiphenyl

R.T.: 8.571 min
Delta R.T.: -0.033 min
Response: 590879
Conc: 18.55 ng/ml