

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\P0041619\
 Data File : P0055379.D
 Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
 Acq On : 16 Apr 2019 21:27
 Operator : SM/SJ
 Sample : K2423-13
 Misc :
 ALS Vial : 19 Sample Multiplier: 1

Instrument :
 ECD_O
 ClientSampleId :
 TP4-A

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Apr 17 01:02:54 2019
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\P0032519.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Mon Mar 25 17:22:26 2019
 Response via : Initial Calibration
 Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	4.293	3.604	529771	510167	15.265	15.986
2)	SA Decachlor...	9.905	8.569	615886	448932	12.493	14.096

Target Compounds



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\PO041619\
Data File : PO055379.D
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
Acq On : 16 Apr 2019 21:27
Operator : SM/SJ
Sample : K2423-13
Misc :
ALS Vial : 19 Sample Multiplier: 1

Instrument :
ECD_O
ClientSampleId :
TP4-A

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Apr 17 01:02:54 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\PO032519.M
Quant Title : GC EXTRACTABLES
QLast Update : Mon Mar 25 17:22:26 2019
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

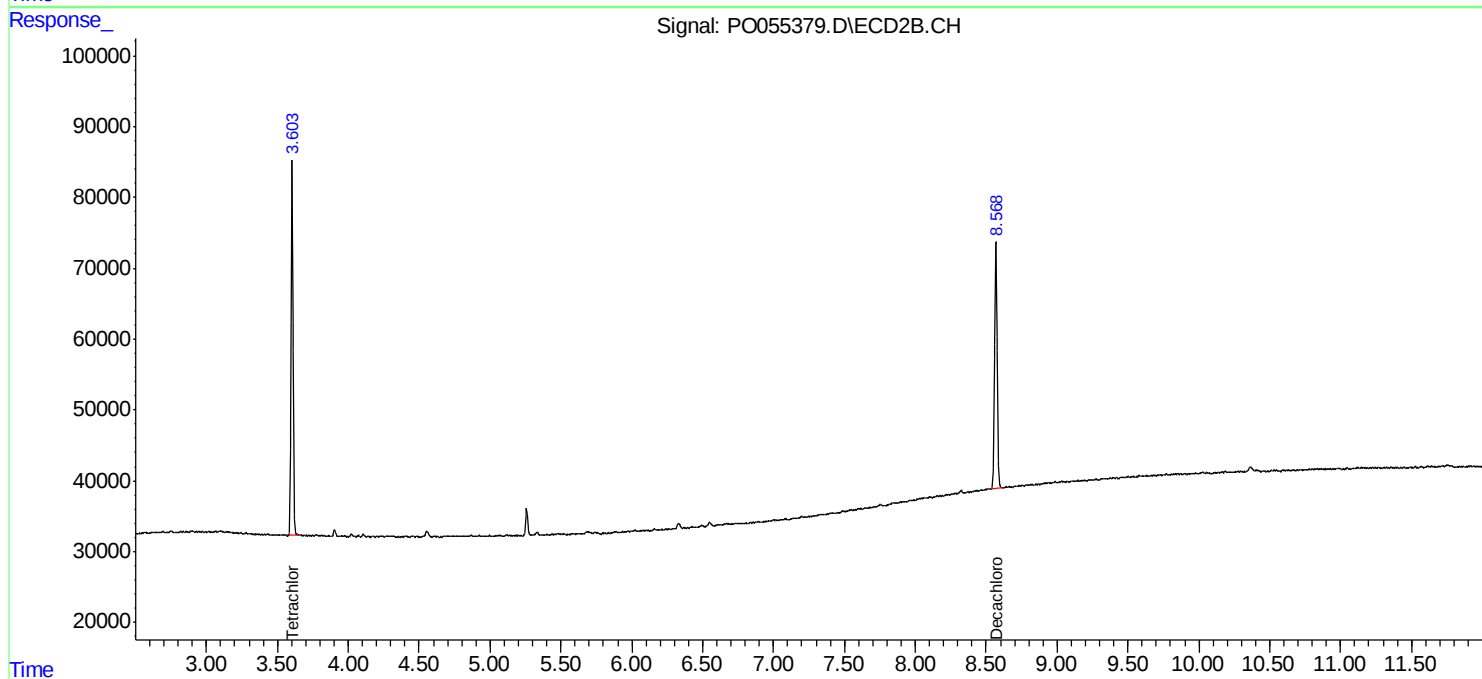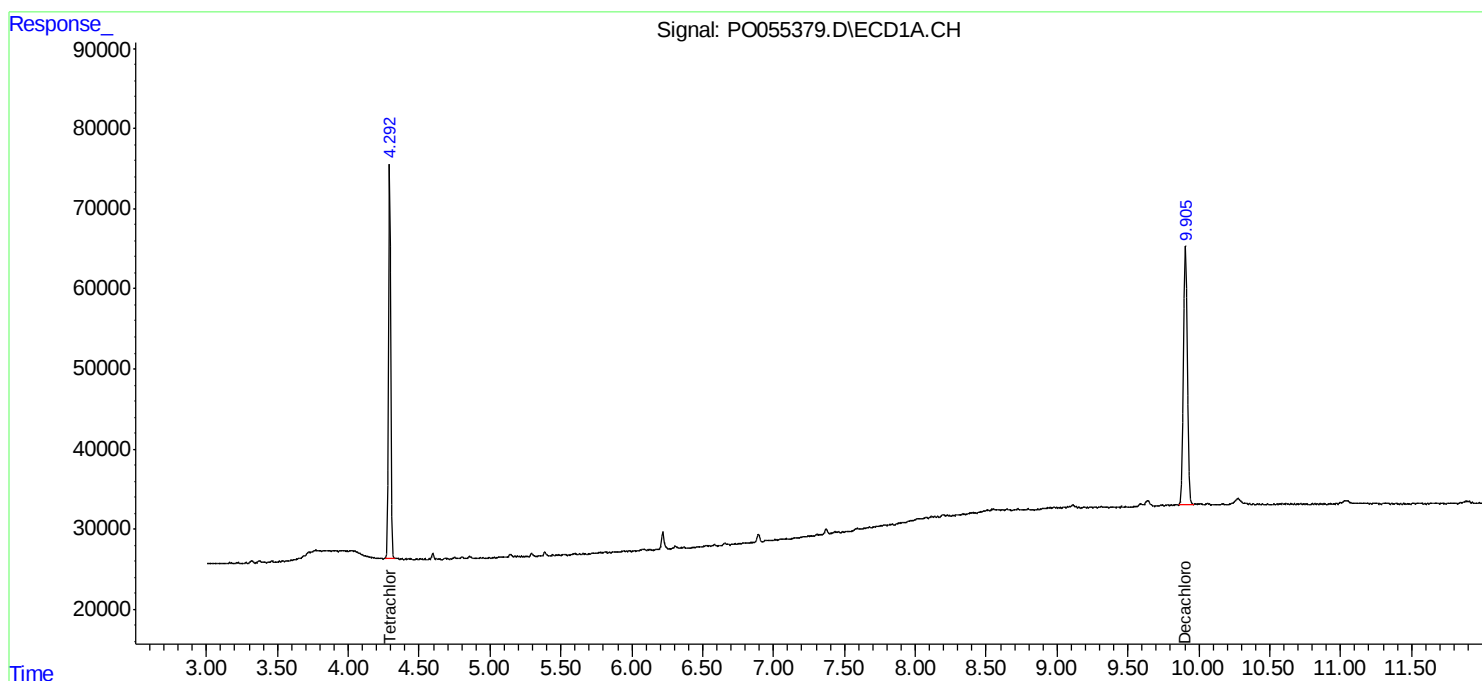


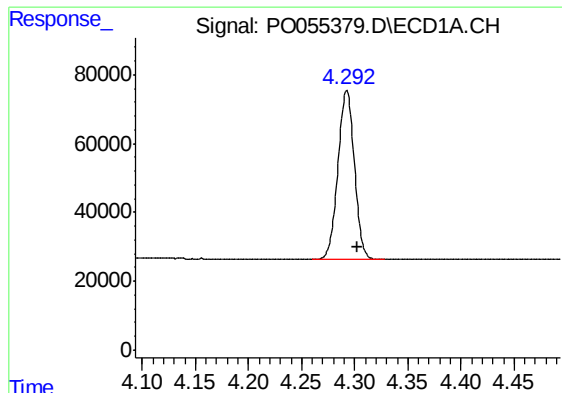

#1 Tetrachloro-m-xylene


R.T.: 4.293 min
Delta R.T.: -0.010 min
Response: 529771
Conc: 15.26 ng/ml

Instrument :
ECD_O
ClientSampleId :
TP4-A

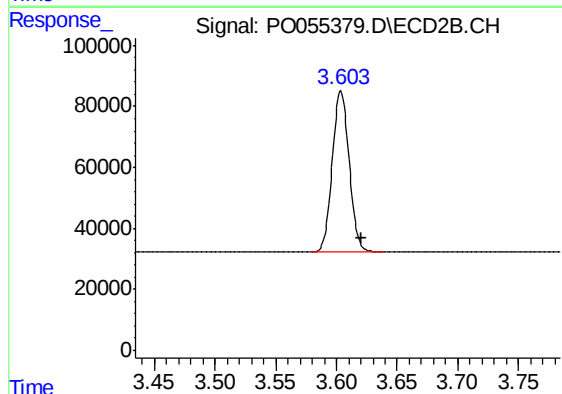


#1 Tetrachloro-m-xylene

R.T.: 3.604 min
Delta R.T.: -0.017 min
Response: 510167
Conc: 15.99 ng/ml

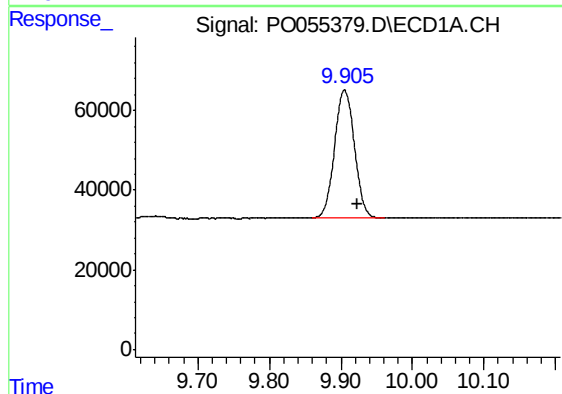

#2 Decachlorobiphenyl

R.T.: 9.905 min
Delta R.T.: -0.018 min
Response: 615886
Conc: 12.49 ng/ml

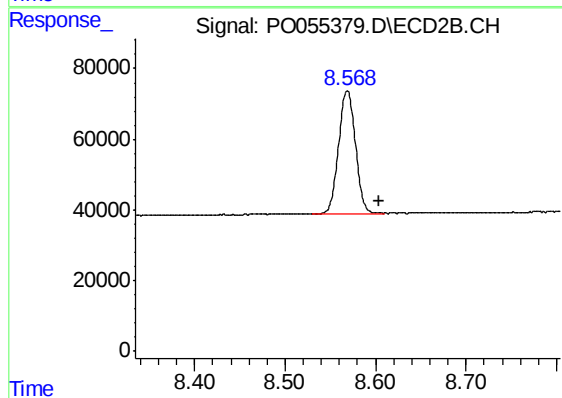

#2 Decachlorobiphenyl

R.T.: 8.569 min
Delta R.T.: -0.035 min
Response: 448932
Conc: 14.10 ng/ml