

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\P0041620\
 Data File : P0067879.D
 Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
 Acq On : 16 Apr 2020 16:13
 Operator : DD\AJ
 Sample : I.BLK
 Misc :
 ALS Vial : 2 Sample Multiplier: 1

Instrument :
 ECD_O
 ClientSampleId :
 I.BLK

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Apr 16 17:11:12 2020
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\P0040120.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Fri Apr 03 16:04:09 2020
 Response via : Initial Calibration
 Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	4.916	3.936	418207	833335	17.561	24.863 #
2)	SA Decachlor...	10.890	9.219	405326	885707	11.906	21.422 #
Target Compounds							
24)	L5 AR-1248-4	7.151	0.000	30301	0	32.117	N.D. #
26)	L6 AR-1254-1	7.151	0.000	30301	0	24.533	N.D. #
28)	L6 AR-1254-3	7.771	0.000	26048	0	12.553	N.D. #
29)	L6 AR-1254-4	0.000	6.936	0	45970	N.D.	19.069 #
32)	L7 AR-1260-2	0.000	6.936	0	45970	N.D.	17.903 #
33)	L7 AR-1260-3	8.597	0.000	303211	0	232.616	N.D. #
34)	L7 AR-1260-4	8.836	0.000	387829	0	252.361	N.D. #
36)	L8 AR-1262-1	8.597	0.000	303211	0	180.863	N.D. #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\P0041620\
Data File : P0067879.D
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
Acq On : 16 Apr 2020 16:13
Operator : DD\AJ
Sample : I.BLK
Misc :
ALS Vial : 2 Sample Multiplier: 1

Instrument :
ECD_O
ClientSampled :
I.BLK

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Apr 16 17:11:12 2020
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\P0040120.M
Quant Title : GC EXTRACTABLES
QLast Update : Fri Apr 03 16:04:09 2020
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

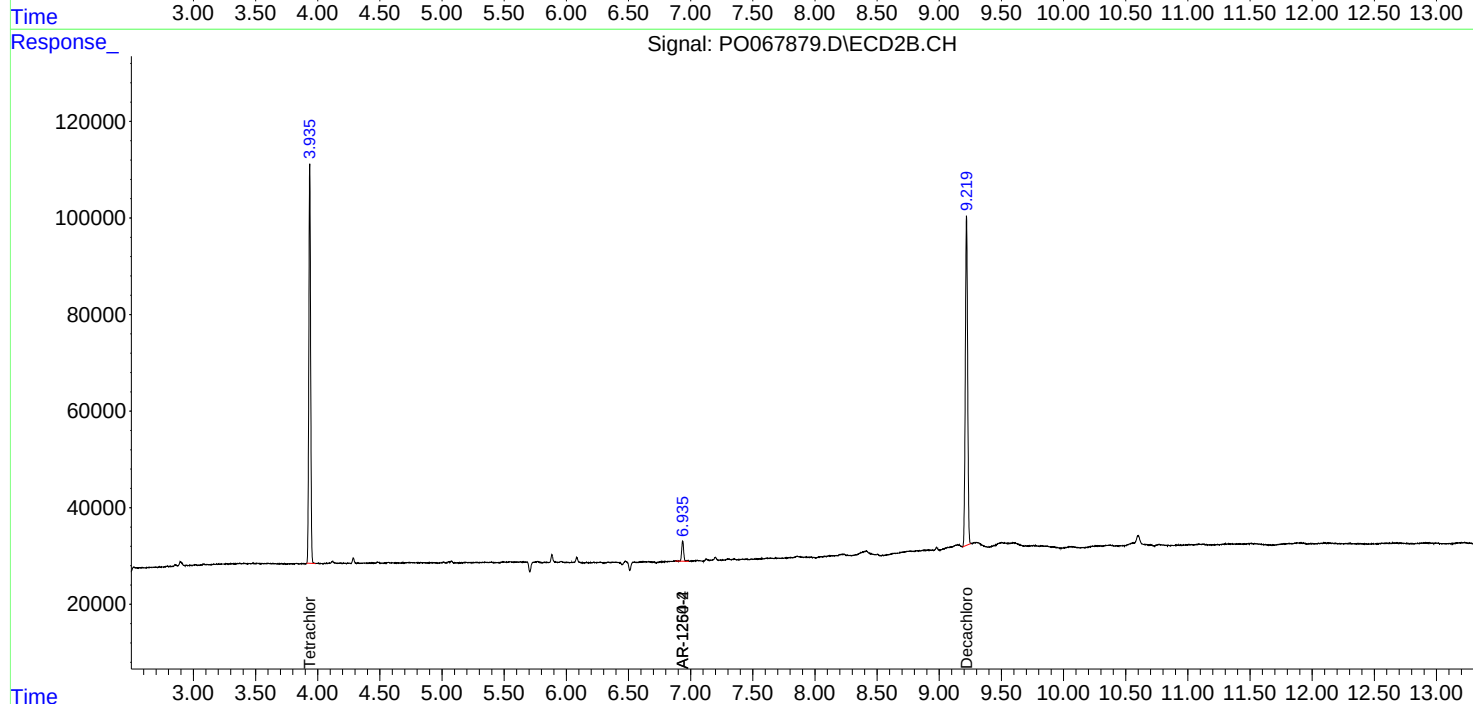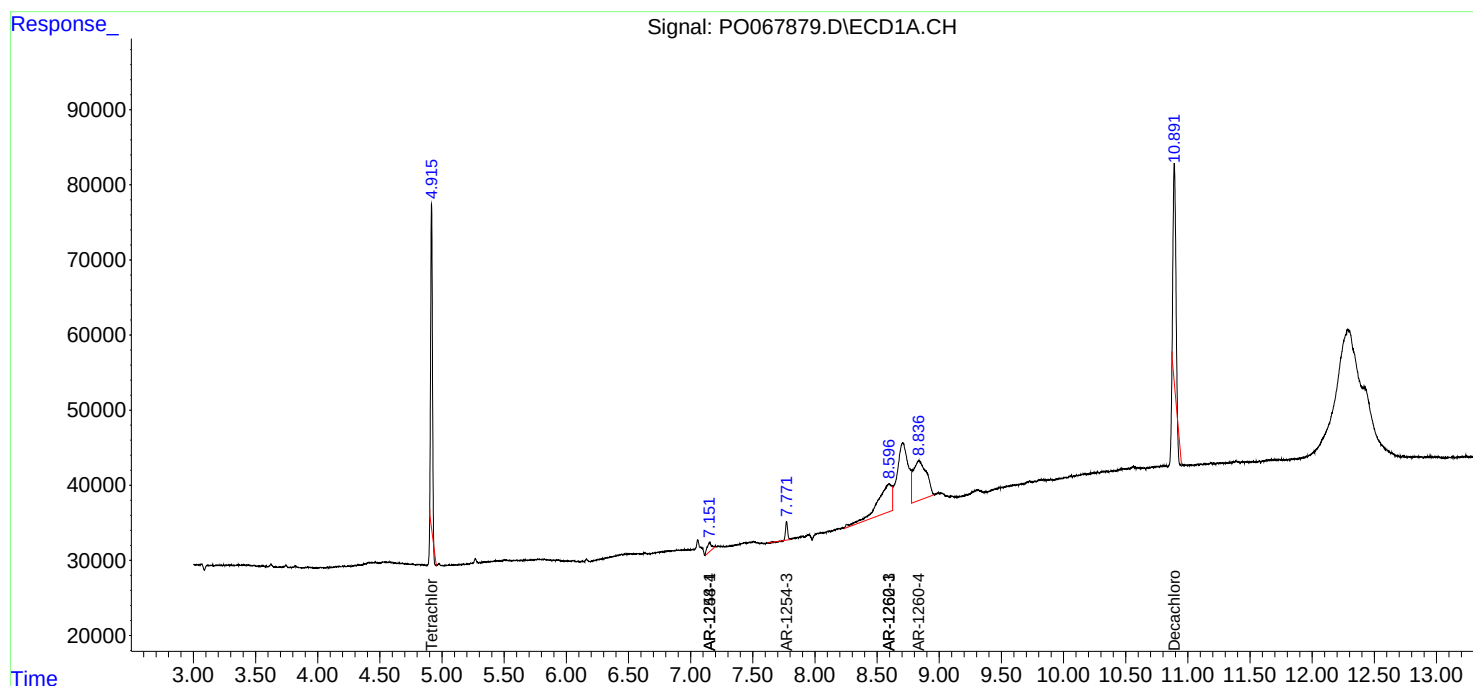


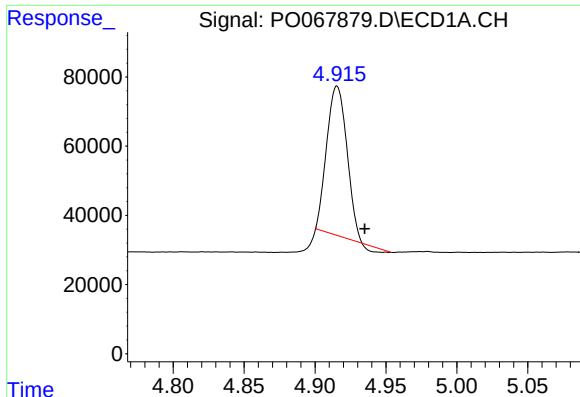

#1 Tetrachloro-m-xylene


R.T.: 4.916 min
Delta R.T.: -0.019 min
Response: 418207
Conc: 17.56 ng/ml

Instrument :
ECD_O
ClientSampleId :
I.BLK

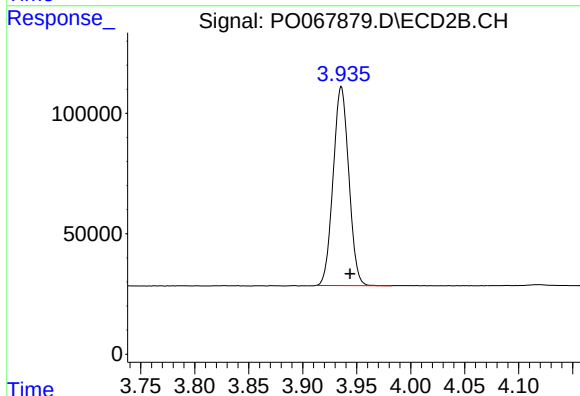


#1 Tetrachloro-m-xylene

R.T.: 3.936 min
Delta R.T.: -0.008 min
Response: 833335
Conc: 24.86 ng/ml

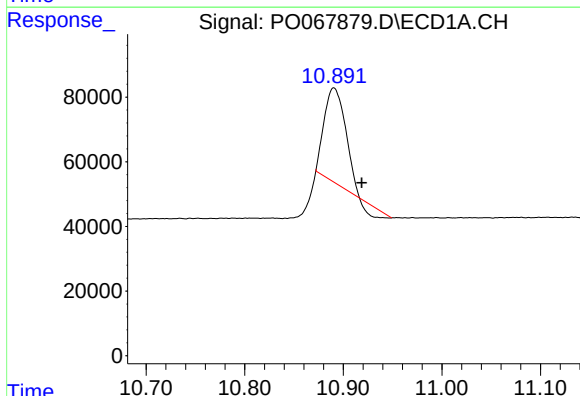


#2 Decachlorobiphenyl

R.T.: 10.890 min
Delta R.T.: -0.028 min
Response: 405326
Conc: 11.91 ng/ml

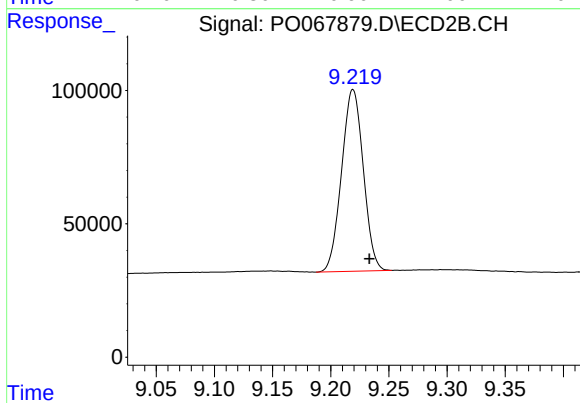

#2 Decachlorobiphenyl


R.T.: 9.219 min
Delta R.T.: -0.014 min
Response: 885707
Conc: 21.42 ng/ml

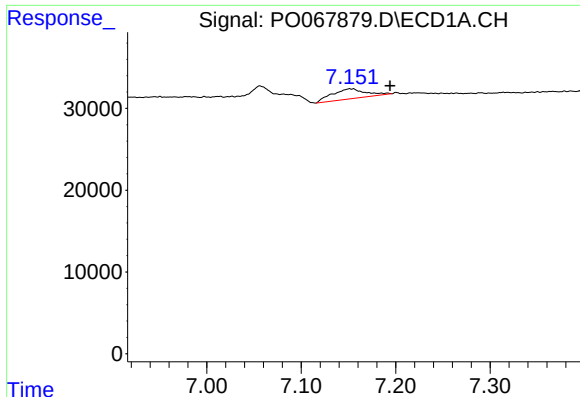

#24 AR-1248-4


R.T.: 7.151 min
Delta R.T.: -0.043 min
Response: 30301
Conc: 32.12 ng/ml

Instrument :
ECD_O
ClientSampleId :
I.BLK

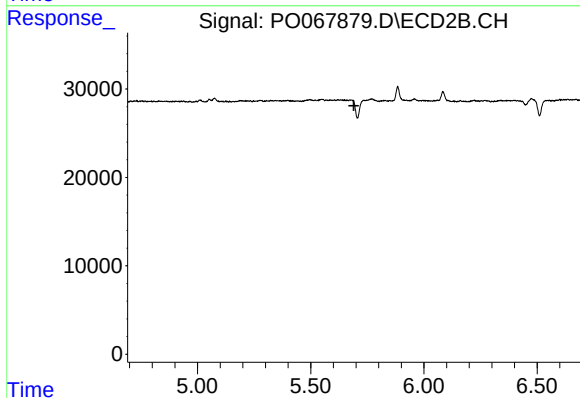


#24 AR-1248-4

R.T.: 0.000 min
Exp R.T. : 5.690 min
Response: 0
Conc: N.D.

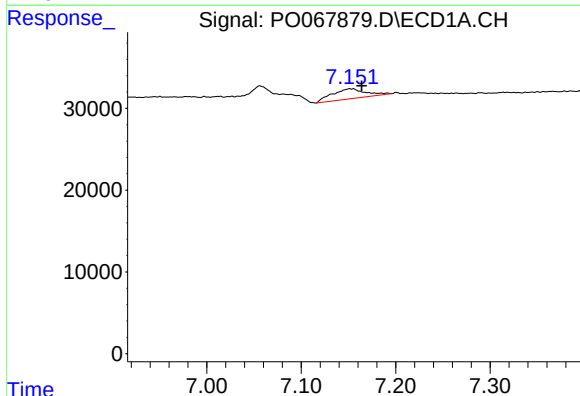


#26 AR-1254-1

R.T.: 7.151 min
Delta R.T.: -0.013 min
Response: 30301
Conc: 24.53 ng/ml

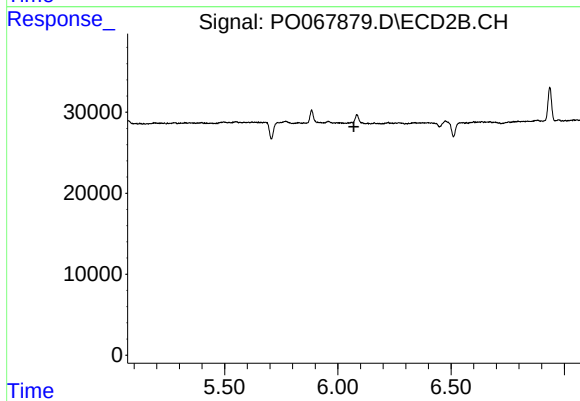

#26 AR-1254-1


R.T.: 0.000 min
Exp R.T. : 6.071 min
Response: 0
Conc: N.D.

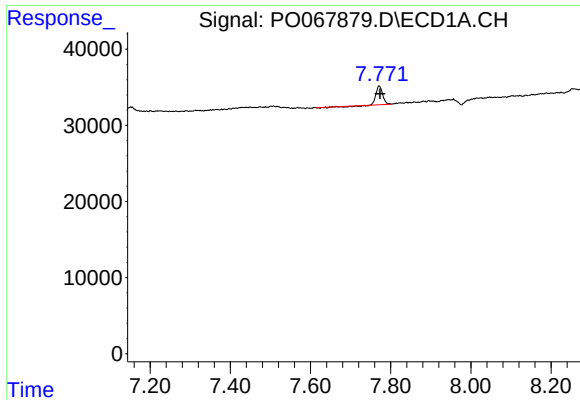

#28 AR-1254-3


R.T.: 7.771 min
Delta R.T.: -0.002 min
Response: 26048
Conc: 12.55 ng/ml

Instrument :
ECD_O
ClientSampleId :
I.BLK

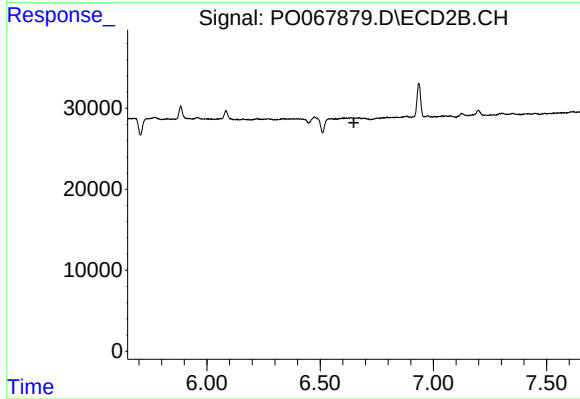


#28 AR-1254-3

R.T.: 0.000 min
Exp R.T. : 6.649 min
Response: 0
Conc: N.D.

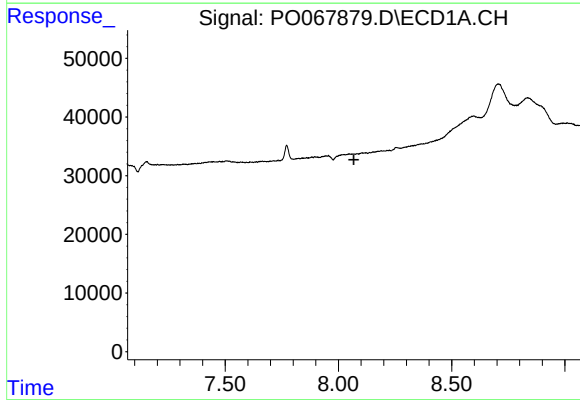


#29 AR-1254-4

R.T.: 0.000 min
Exp R.T. : 8.068 min
Response: 0
Conc: N.D.

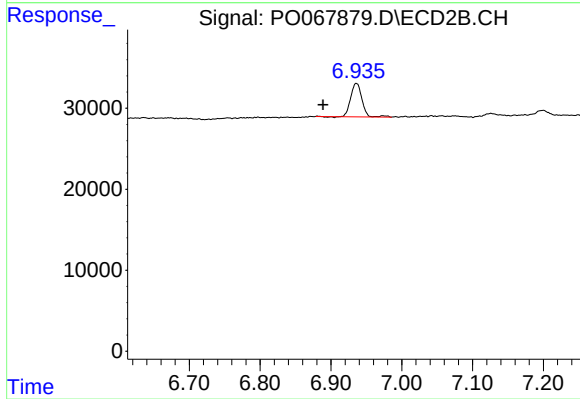

#29 AR-1254-4


R.T.: 6.936 min
Delta R.T.: 0.047 min
Response: 45970
Conc: 19.07 ng/ml

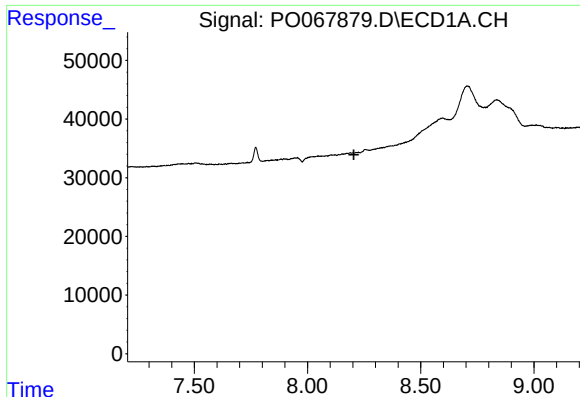

#32 AR-1260-2


R.T.: 0.000 min
Exp R.T.: 8.205 min
Response: 0
Conc: N.D.

Instrument :
ECD_O
ClientSampleId :
I.BLK

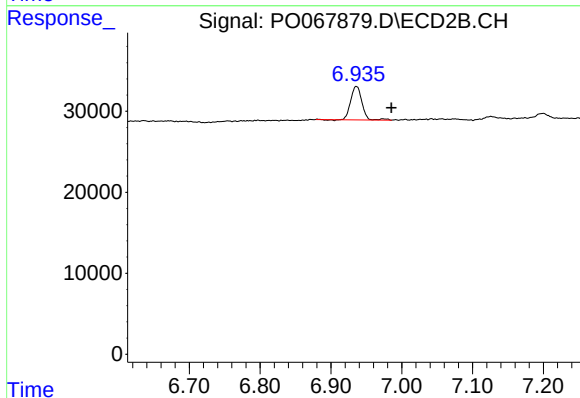


#32 AR-1260-2

R.T.: 6.936 min
Delta R.T.: -0.049 min
Response: 45970
Conc: 17.90 ng/ml

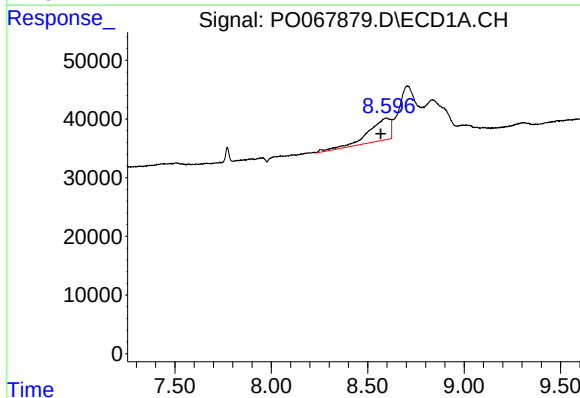


#33 AR-1260-3

R.T.: 8.597 min
Delta R.T.: 0.030 min
Response: 303211
Conc: 232.62 ng/ml

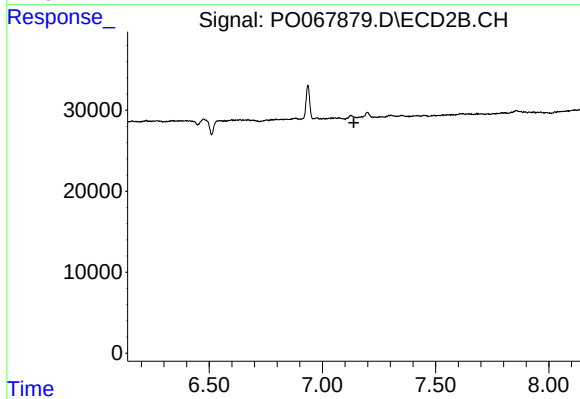

#33 AR-1260-3


R.T.: 0.000 min
Exp R.T.: 7.139 min
Response: 0
Conc: N.D.

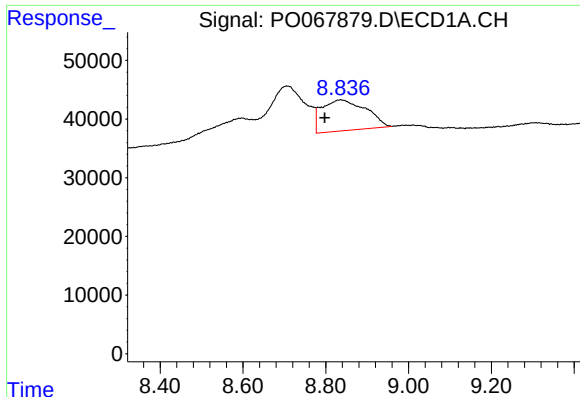

#34 AR-1260-4


R.T.: 8.836 min
Delta R.T.: 0.038 min
Response: 387829
Conc: 252.36 ng/ml

Instrument :
ECD_O
ClientSampleId :
I.BLK

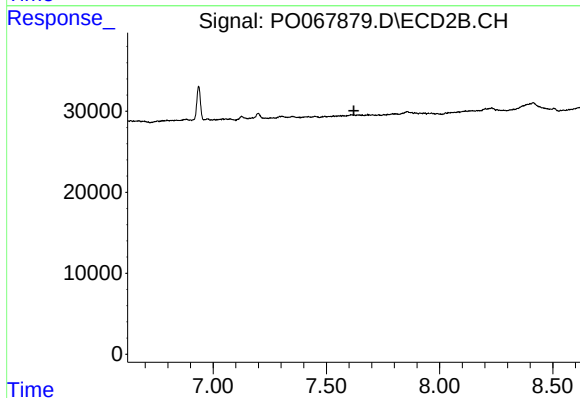


#34 AR-1260-4

R.T.: 0.000 min
Exp R.T. : 7.621 min
Response: 0
Conc: N.D.

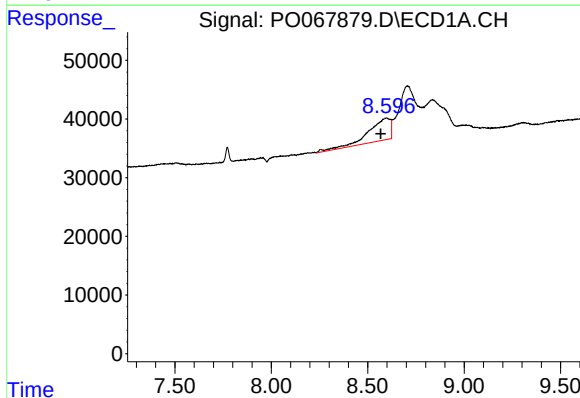

#36 AR-1262-1

R.T.: 8.597 min
Delta R.T.: 0.030 min
Response: 303211
Conc: 180.86 ng/ml

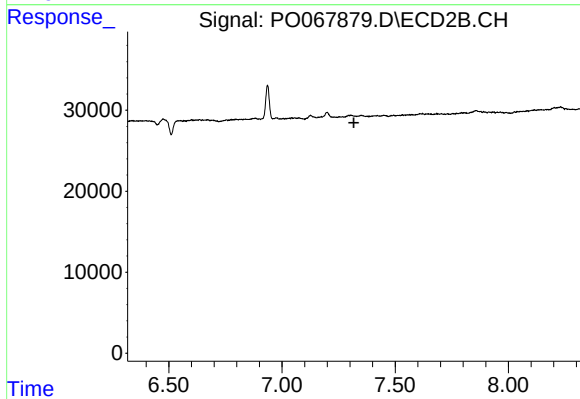

#36 AR-1262-1

R.T.: 0.000 min
Exp R.T. : 7.317 min
Response: 0
Conc: N.D.