

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\P0041620\
 Data File : P0067874.D
 Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
 Acq On : 16 Apr 2020 14:00
 Operator : DD\AJ
 Sample : L2245-22
 Misc :
 ALS Vial : 17 Sample Multiplier: 1

Instrument :
 ECD_O
 ClientSampleId :
 TP-21A

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Apr 16 15:21:25 2020
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\P0040120.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Fri Apr 03 16:04:09 2020
 Response via : Initial Calibration
 Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	4.924	3.939	28117	47630	1.181	1.421
2) SA Decachlor...	10.898	9.221	110047	135267	3.233	3.272

Target Compounds



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\P0041620\
Data File : P0067874.D
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
Acq On : 16 Apr 2020 14:00
Operator : DD\AJ
Sample : L2245-22
Misc :
ALS Vial : 17 Sample Multiplier: 1

Instrument :
ECD_O
ClientSampleId :
TP-21A

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Apr 16 15:21:25 2020
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\P0040120.M
Quant Title : GC EXTRACTABLES
QLast Update : Fri Apr 03 16:04:09 2020
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

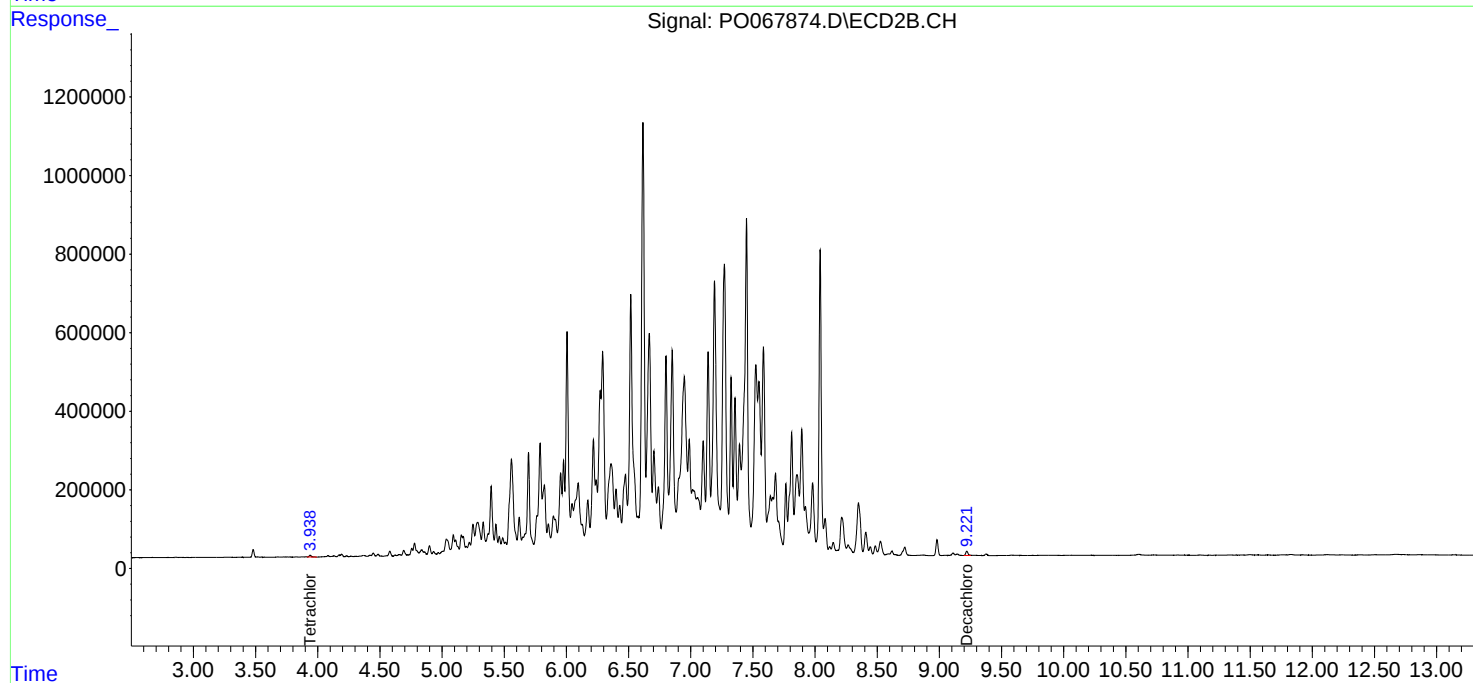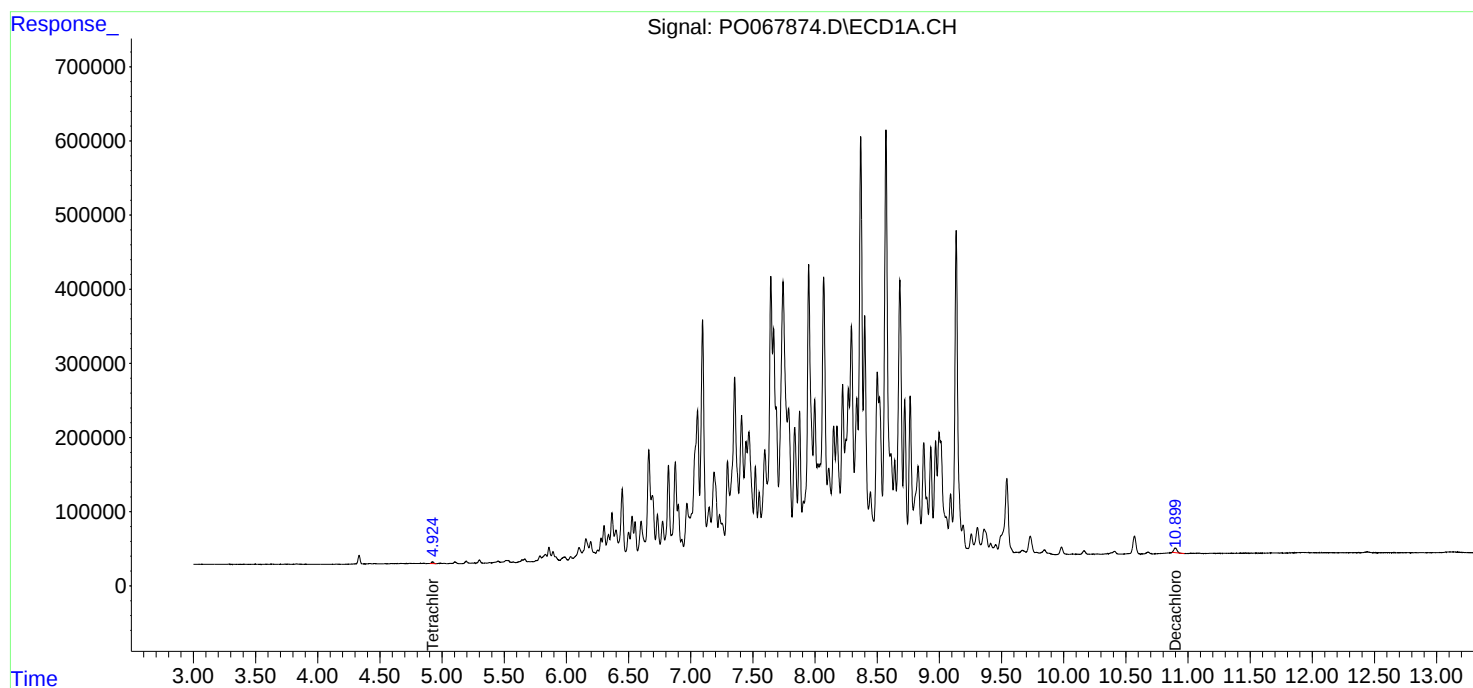


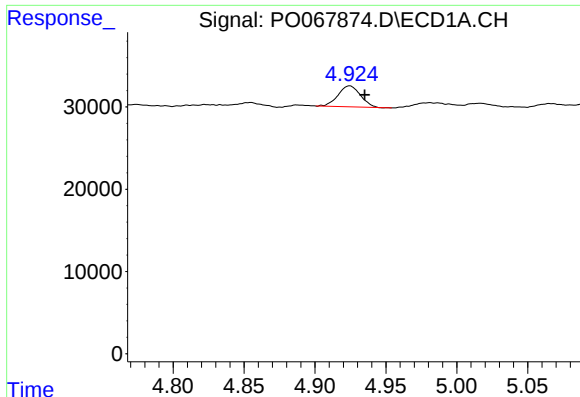

#1 Tetrachloro-m-xylene


R.T.: 4.924 min
Delta R.T.: -0.011 min
Response: 28117
Conc: 1.18 ng/ml

Instrument :
ECD_O
ClientSampleId :
TP-21A

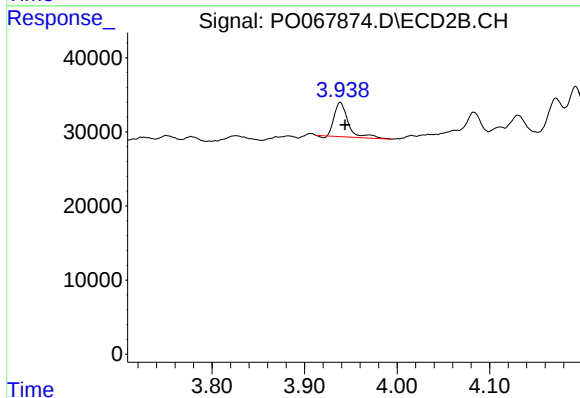


#1 Tetrachloro-m-xylene

R.T.: 3.939 min
Delta R.T.: -0.005 min
Response: 47630
Conc: 1.42 ng/ml

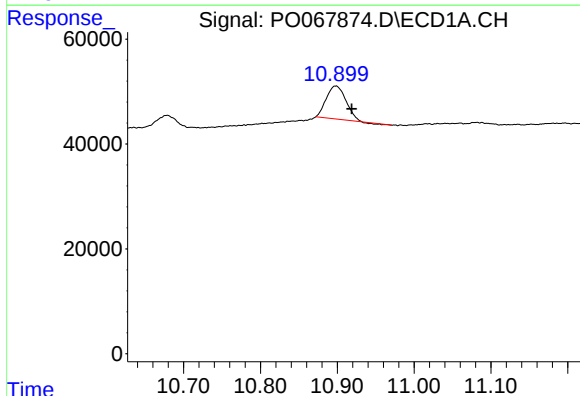

#2 Decachlorobiphenyl

R.T.: 10.898 min
Delta R.T.: -0.021 min
Response: 110047
Conc: 3.23 ng/ml

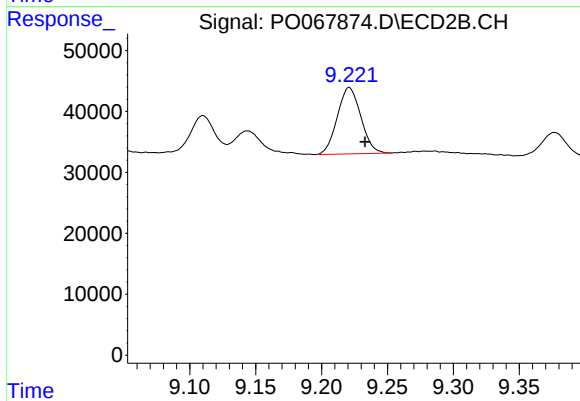

#2 Decachlorobiphenyl

R.T.: 9.221 min
Delta R.T.: -0.012 min
Response: 135267
Conc: 3.27 ng/ml