

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\P0041719\
 Data File : P0055405.D
 Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
 Acq On : 17 Apr 2019 19:12
 Operator : SM/SJ
 Sample : K2434-01
 Misc :
 ALS Vial : 13 Sample Multiplier: 1

Instrument :
 ECD_O
 ClientSampleId :
 RO-288

Manual Integrations
 APPROVED

mohammad
 4/19/2019 1:23:30 PM

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Apr 18 00:56:23 2019
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\P0032519.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Mon Mar 25 17:22:26 2019
 Response via : Initial Calibration
 Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	4.293	3.604	455072	480961	13.113	15.071
2) SA Decachlor...	9.906	8.567	430455	314239	8.732	9.867m

Target Compounds

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\P0041719\
Data File : P0055405.D
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
Acq On : 17 Apr 2019 19:12
Operator : SM/SJ
Sample : K2434-01
Misc :
ALS Vial : 13 Sample Multiplier: 1



Instrument :
ECD_O
ClientSampleId :
RO-288


Manual Integrations
APPROVED

mohammad
4/19/2019 1:23:30 PM

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Apr 18 00:56:23 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\P0032519.M
Quant Title : GC EXTRACTABLES
QLast Update : Mon Mar 25 17:22:26 2019
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

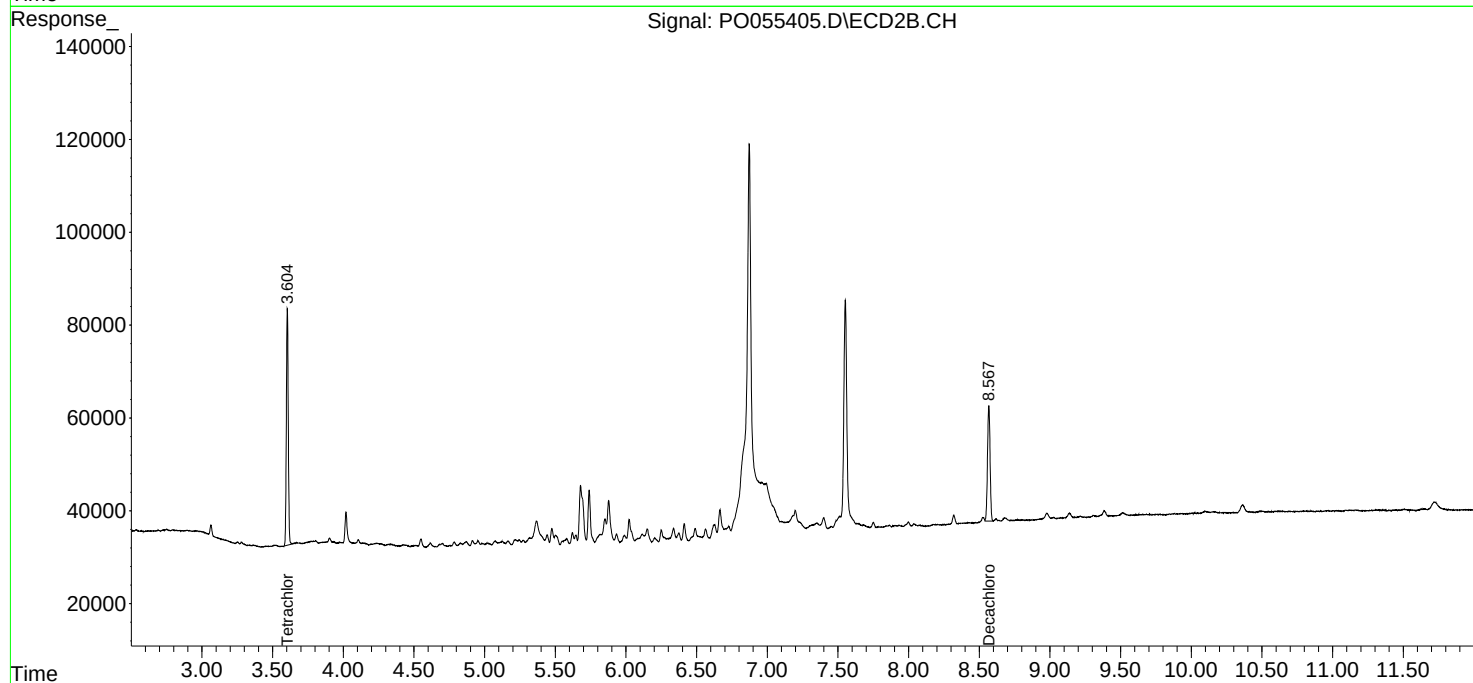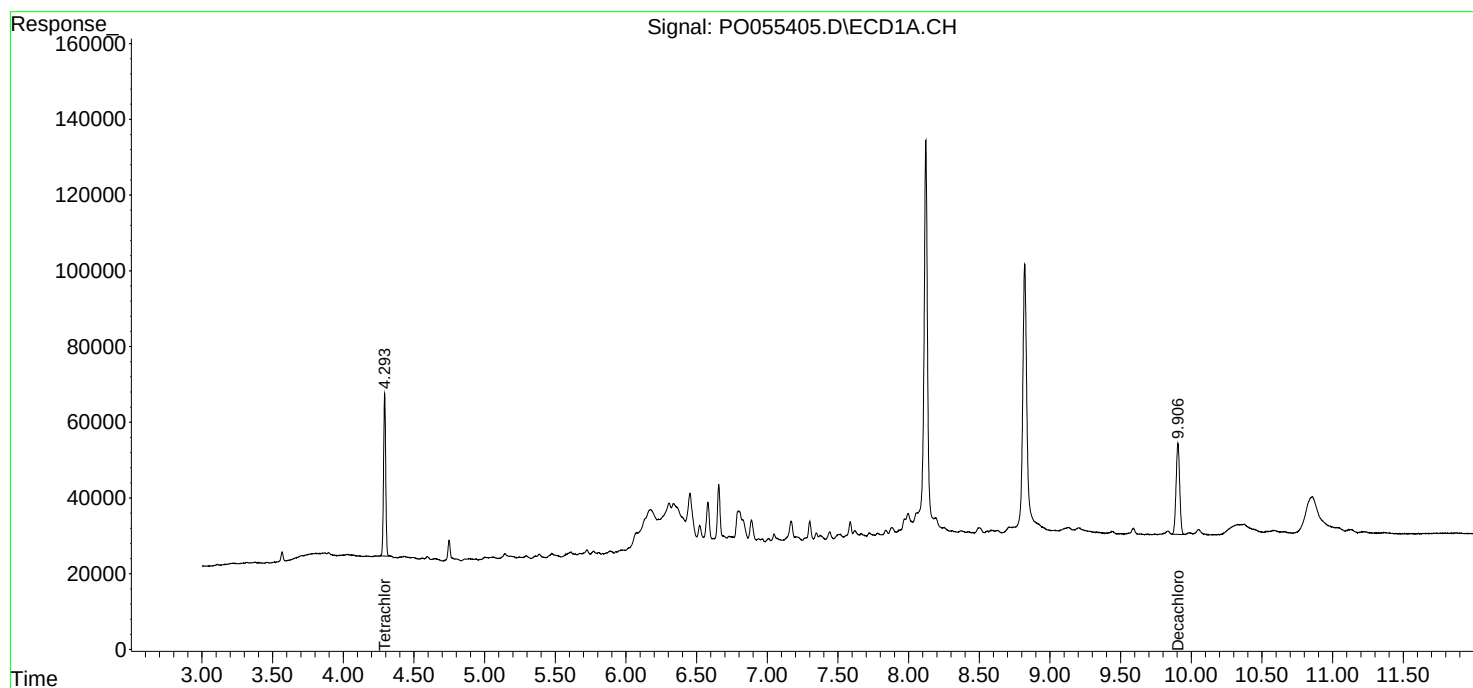

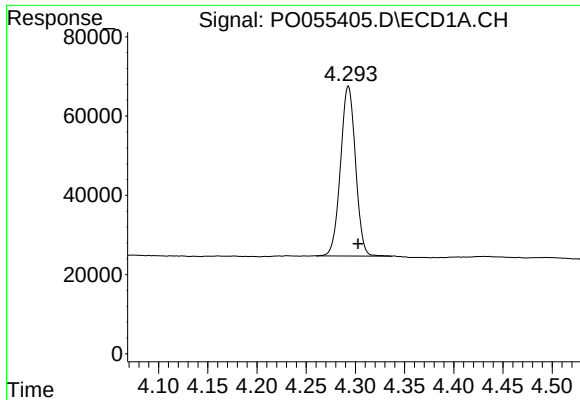


#1 Tetrachloro-m-xylene

R.T.: 4.293 min
Delta R.T.: -0.010 min
Response: 455072
Conc: 13.11 ng/ml

Instrument :
ECD_O
ClientSampleId :
RO-288


Manual Integrations
APPROVED

mohammad
4/19/2019 1:23:30 PM

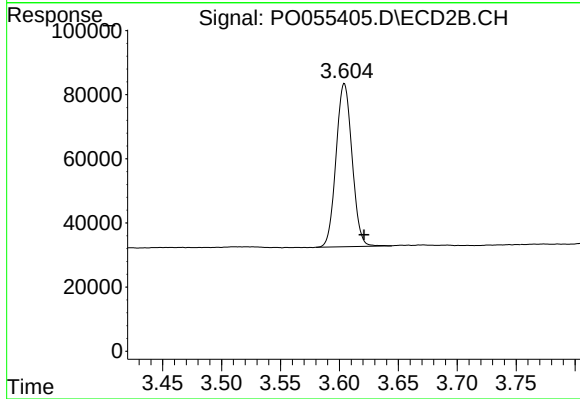


#1 Tetrachloro-m-xylene

R.T.: 3.604 min
Delta R.T.: -0.017 min
Response: 480961
Conc: 15.07 ng/ml

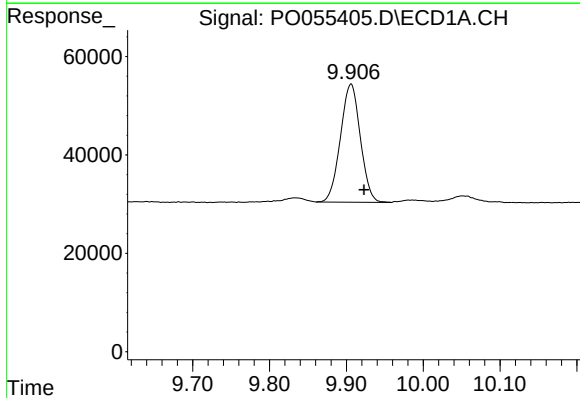

#2 Decachlorobiphenyl

R.T.: 9.906 min
Delta R.T.: -0.017 min
Response: 430455
Conc: 8.73 ng/ml

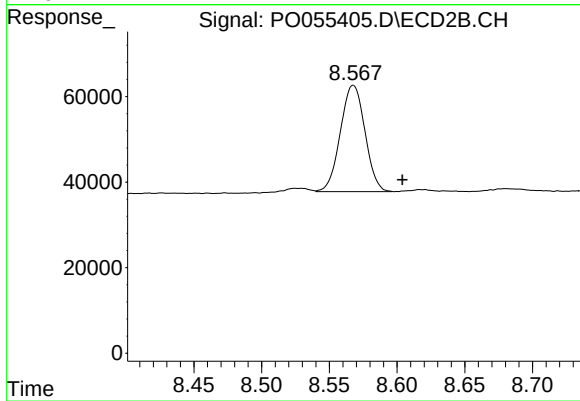

#2 Decachlorobiphenyl

R.T.: 8.567 min
Delta R.T.: -0.037 min
Response: 314239
Conc: 9.87 ng/ml m