

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\P0041719\
 Data File : P0055414.D
 Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
 Acq On : 17 Apr 2019 21:45
 Operator : SM/SJ
 Sample : K2437-01
 Misc :
 ALS Vial : 20 Sample Multiplier: 1

Instrument :
 ECD_O
 ClientSampleId :
 FK-PS-01-046

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Apr 18 01:00:53 2019
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\P0032519.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Mon Mar 25 17:22:26 2019
 Response via : Initial Calibration
 Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	4.291	3.603	704017	722581	20.286	22.643
2) SA Decachlor...	9.903	8.565	506346	378191	10.271	11.875

Target Compounds



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\P0041719\
Data File : P0055414.D
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
Acq On : 17 Apr 2019 21:45
Operator : SM/SJ
Sample : K2437-01
Misc :
ALS Vial : 20 Sample Multiplier: 1

Instrument :
ECD_O
ClientSampleId :
FK-PS-01-046

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Apr 18 01:00:53 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\P0032519.M
Quant Title : GC EXTRACTABLES
QLast Update : Mon Mar 25 17:22:26 2019
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

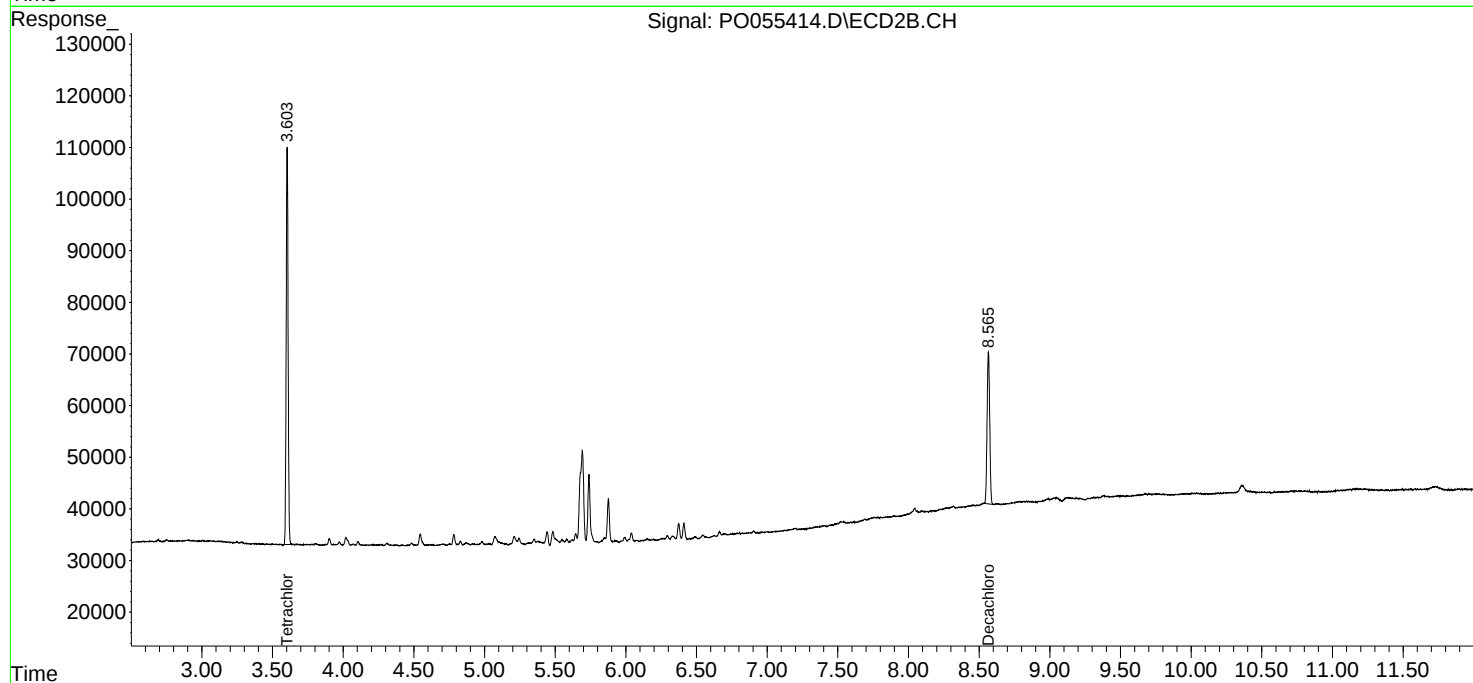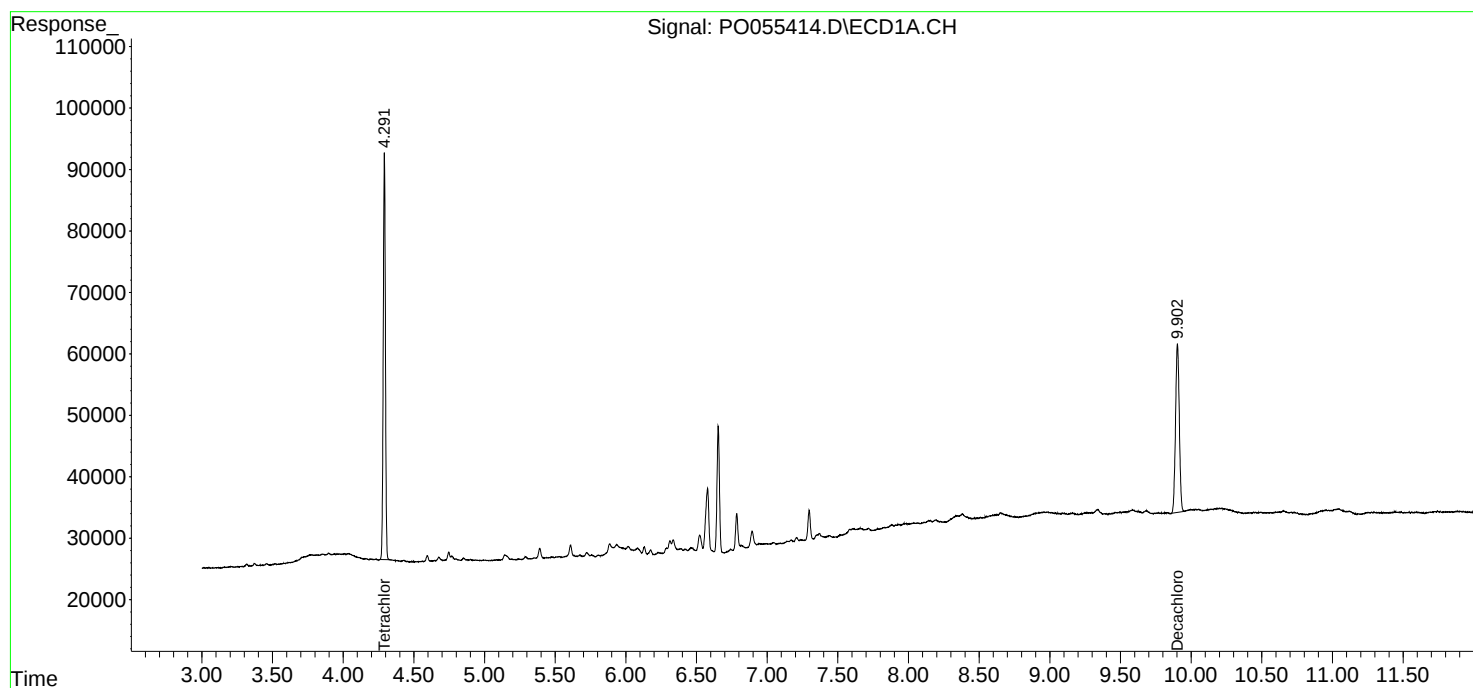


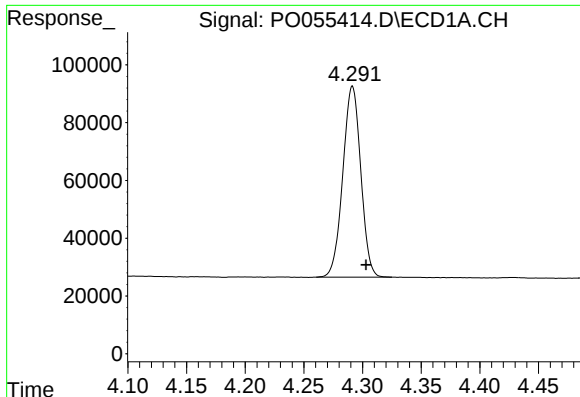

#1 Tetrachloro-m-xylene


R.T.: 4.291 min
Delta R.T.: -0.012 min
Response: 704017
Conc: 20.29 ng/ml

Instrument :
ECD_O
ClientSampleId :
FK-PS-01-046

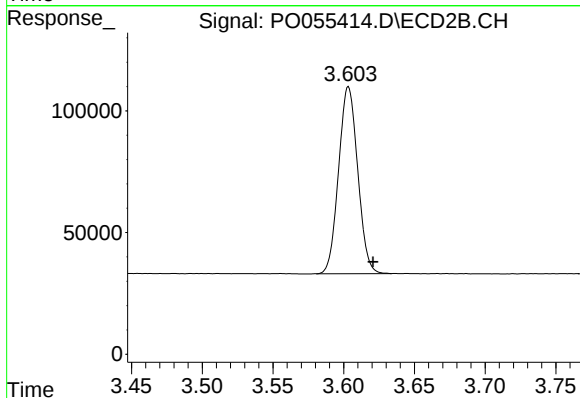


#1 Tetrachloro-m-xylene

R.T.: 3.603 min
Delta R.T.: -0.018 min
Response: 722581
Conc: 22.64 ng/ml

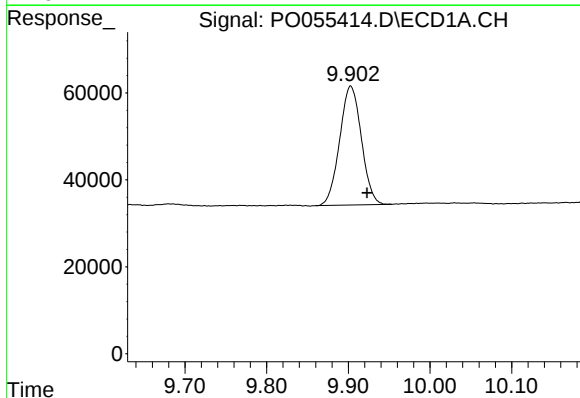

#2 Decachlorobiphenyl

R.T.: 9.903 min
Delta R.T.: -0.020 min
Response: 506346
Conc: 10.27 ng/ml

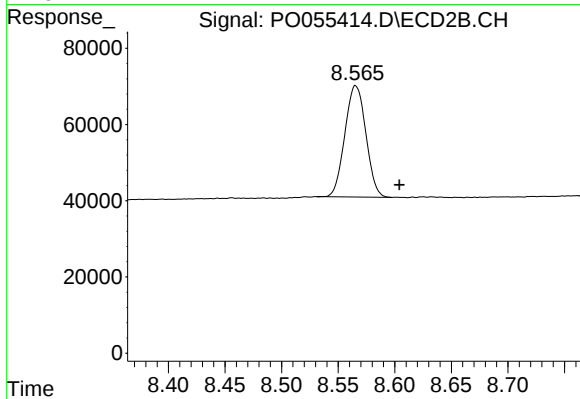

#2 Decachlorobiphenyl

R.T.: 8.565 min
Delta R.T.: -0.039 min
Response: 378191
Conc: 11.87 ng/ml