

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\P0041720\
 Data File : P0067899.D
 Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
 Acq On : 17 Apr 2020 10:13
 Operator : DD\AJ
 Sample : L2261-03
 Misc :
 ALS Vial : 8 Sample Multiplier: 1

Instrument :
 ECD_O
 ClientSampleId :
 NCQ-632

Manual Integrations
 APPROVED

Sohil
 4/20/2020 1:56:51 PM

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Apr 17 13:51:03 2020
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\P0040120.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Fri Apr 03 16:04:09 2020
 Response via : Initial Calibration
 Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	4.923	3.938	489975	684583	20.575	20.425m
2) SA Decachlor...	10.893	9.219	507049	585738	14.894m	14.167

Target Compounds

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\P0041720\
Data File : P0067899.D
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
Acq On : 17 Apr 2020 10:13
Operator : DD\AJ
Sample : L2261-03
Misc :
ALS Vial : 8 Sample Multiplier: 1



Instrument :
ECD_O
ClientSampleId :
NCQ-632


Manual Integrations
APPROVED

Sohil
4/20/2020 1:56:51 PM

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Apr 17 13:51:03 2020
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\P0040120.M
Quant Title : GC EXTRACTABLES
QLast Update : Fri Apr 03 16:04:09 2020
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

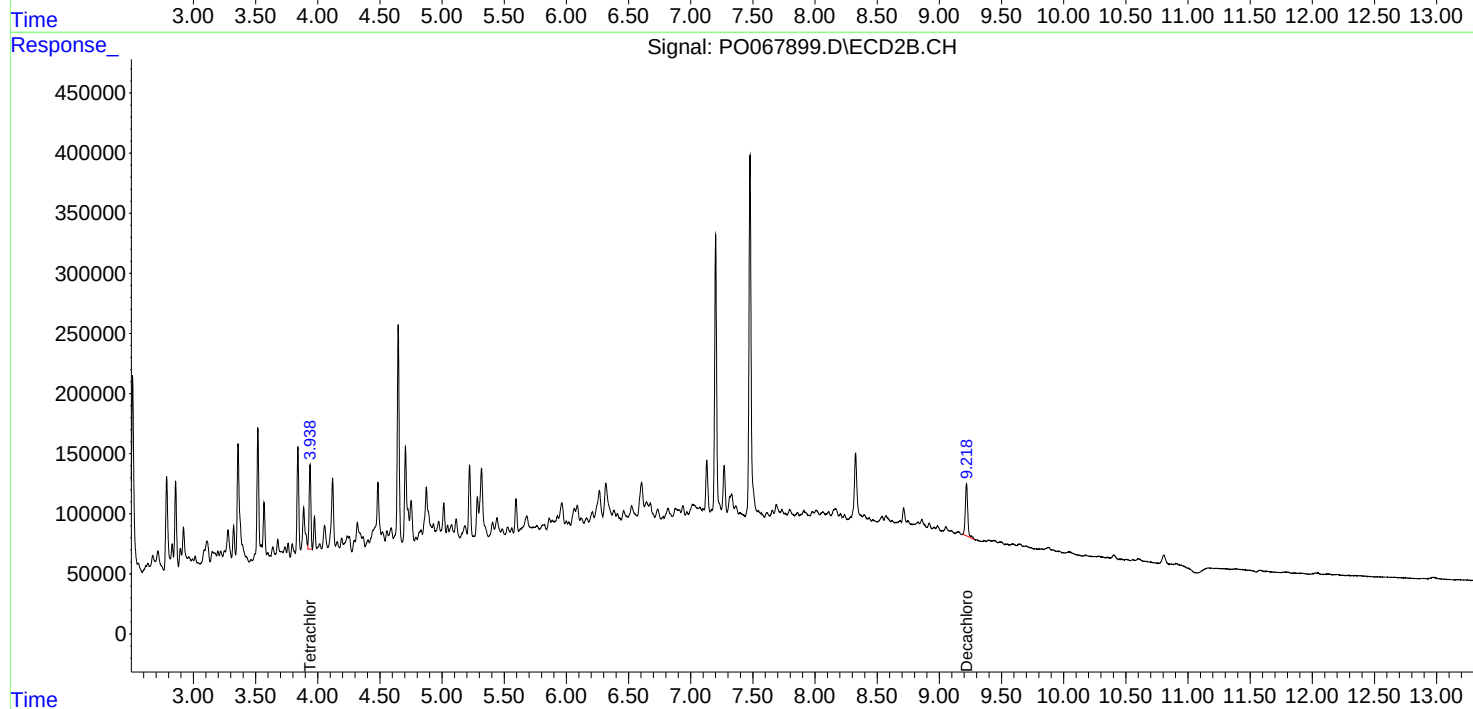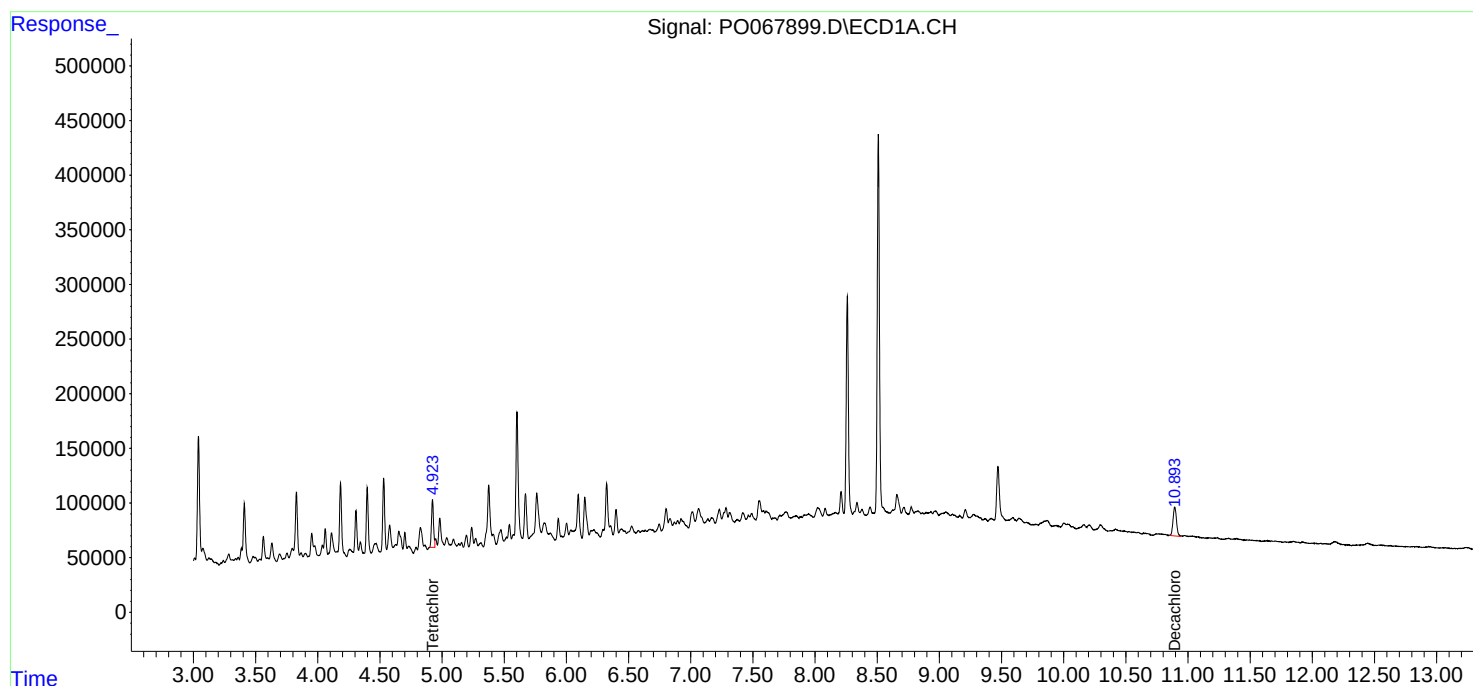

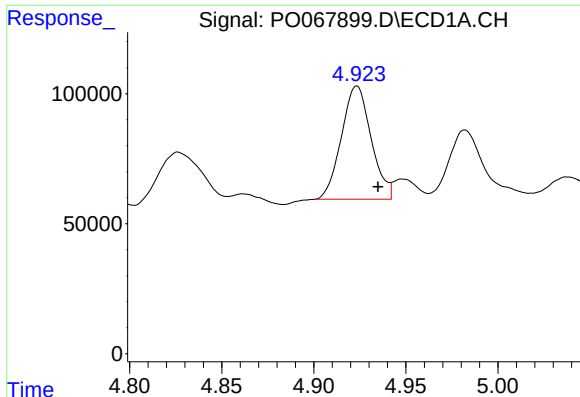


#1 Tetrachloro-m-xylene

R.T.: 4.923 min
Delta R.T.: -0.012 min
Response: 489975
Conc: 20.58 ng/ml

Instrument :
ECD_O
ClientSampleId :
NCQ-632


Manual Integrations
APPROVED

Sohil
4/20/2020 1:56:51 PM

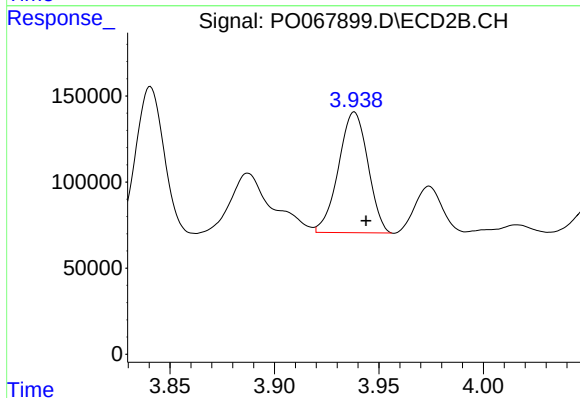


#1 Tetrachloro-m-xylene

R.T.: 3.938 min
Delta R.T.: -0.006 min
Response: 684583
Conc: 20.42 ng/ml m

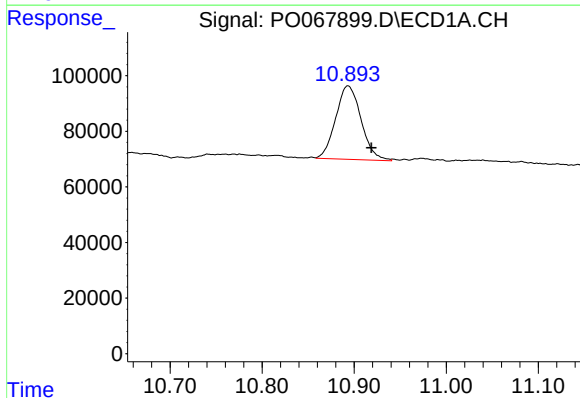

#2 Decachlorobiphenyl

R.T.: 10.893 min
Delta R.T.: -0.026 min
Response: 507049
Conc: 14.89 ng/ml m

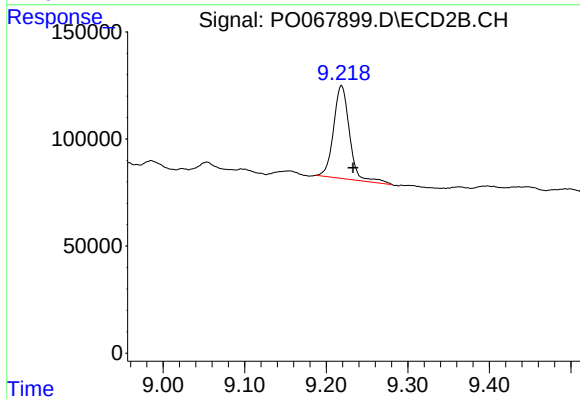

#2 Decachlorobiphenyl

R.T.: 9.219 min
Delta R.T.: -0.014 min
Response: 585738
Conc: 14.17 ng/ml