

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\P0041720\
 Data File : P0067902.D
 Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
 Acq On : 17 Apr 2020 13:01
 Operator : DD\AJ
 Sample : L2280-03 2X
 Misc :
 ALS Vial : 11 Sample Multiplier: 1

Instrument :
 ECD_O
 ClientSampleId :
 04-14-C-1-5

Manual Integrations
 APPROVED

Sohil
 4/20/2020 1:56:56 PM

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Apr 17 13:53:26 2020
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\P0040120.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Fri Apr 03 16:04:09 2020
 Response via : Initial Calibration
 Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	4.920	3.937	350911	569064	14.735m	16.978
2) SA Decachlor...	10.891	9.218	1094373	1229968	32.146m	29.748

Target Compounds

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\P0041720\
Data File : P0067902.D
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
Acq On : 17 Apr 2020 13:01
Operator : DD\AJ
Sample : L2280-03 2X
Misc :
ALS Vial : 11 Sample Multiplier: 1



Instrument :
ECD_O
ClientSampleId :
04-14-C-1-5


Manual Integrations
APPROVED

Sohil
4/20/2020 1:56:56 PM

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Apr 17 13:53:26 2020
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\P0040120.M
Quant Title : GC EXTRACTABLES
QLast Update : Fri Apr 03 16:04:09 2020
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

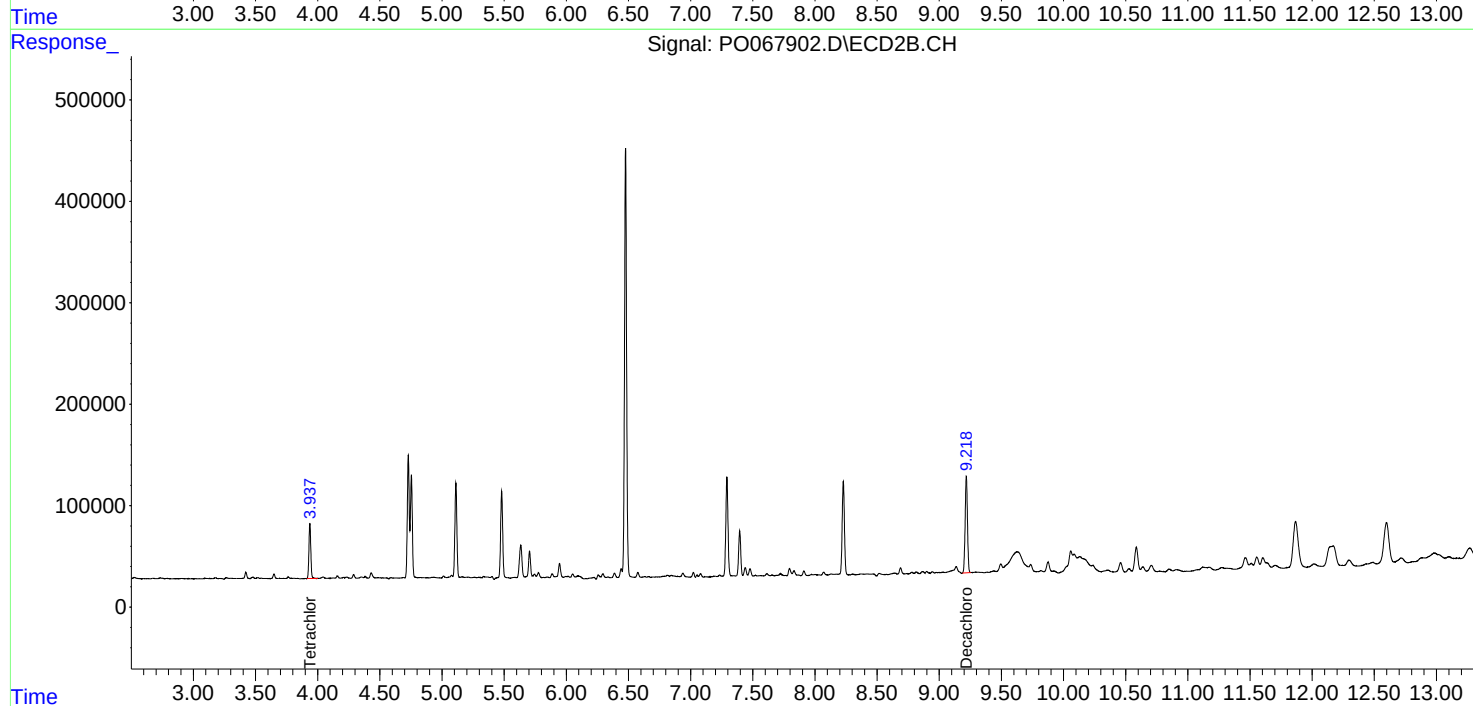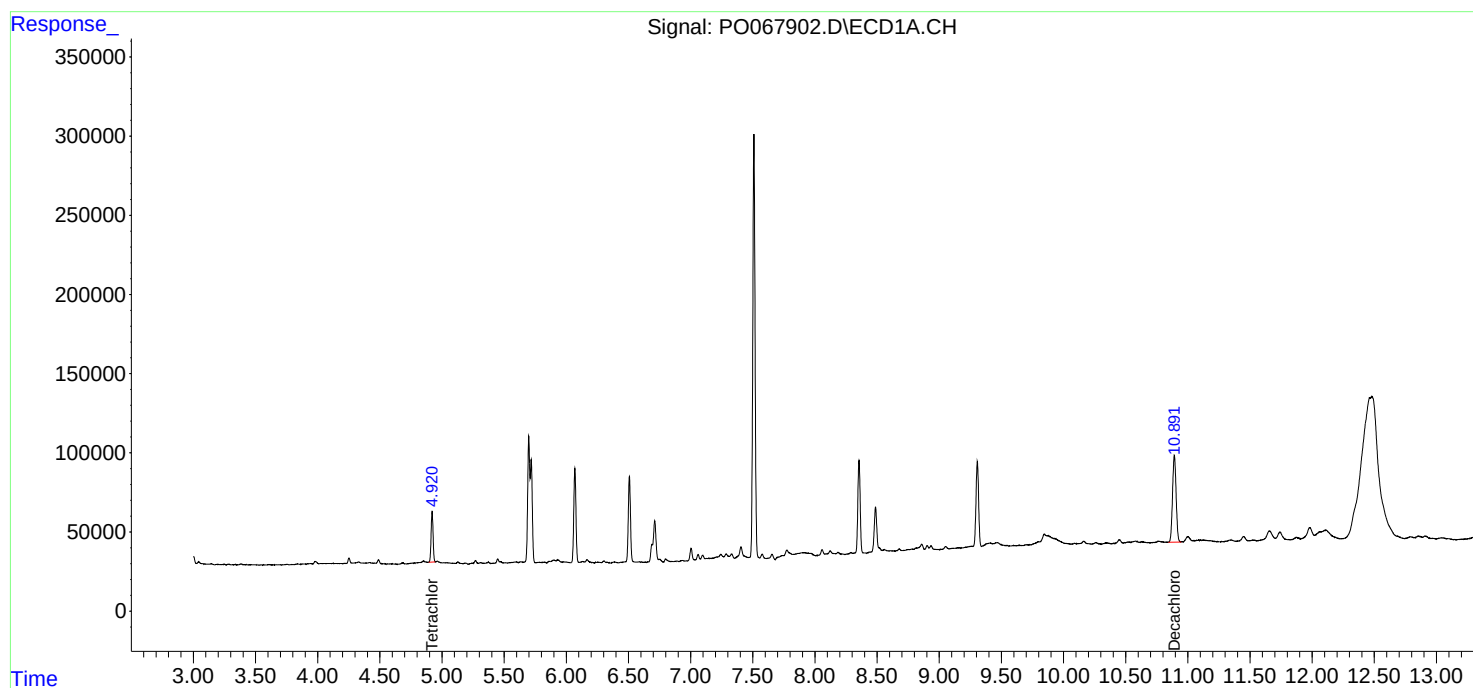

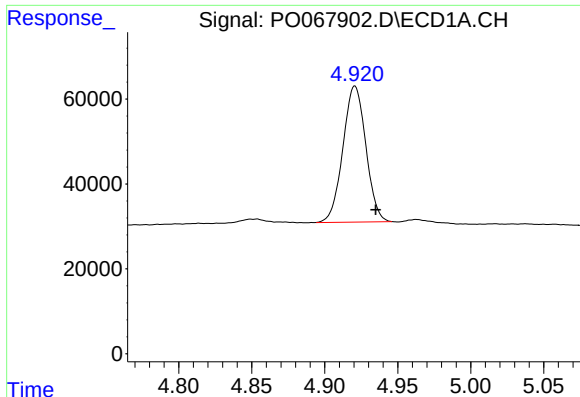


#1 Tetrachloro-m-xylene

R.T.: 4.920 min
Delta R.T.: -0.015 min
Response: 350911
Conc: 14.74 ng/ml m

Instrument :
ECD_O
ClientSampleId :
04-14-C-1-5


Manual Integrations
APPROVED

Sohil
4/20/2020 1:56:56 PM

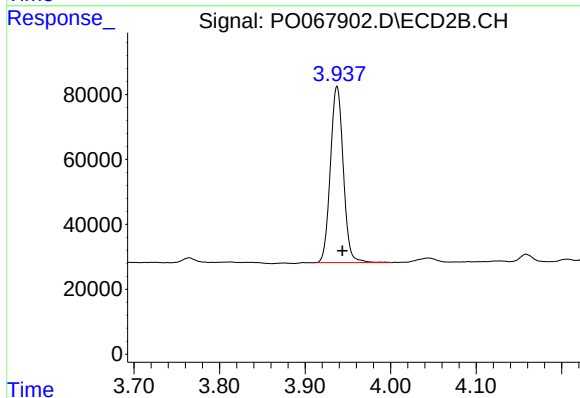


#1 Tetrachloro-m-xylene

R.T.: 3.937 min
Delta R.T.: -0.006 min
Response: 569064
Conc: 16.98 ng/ml

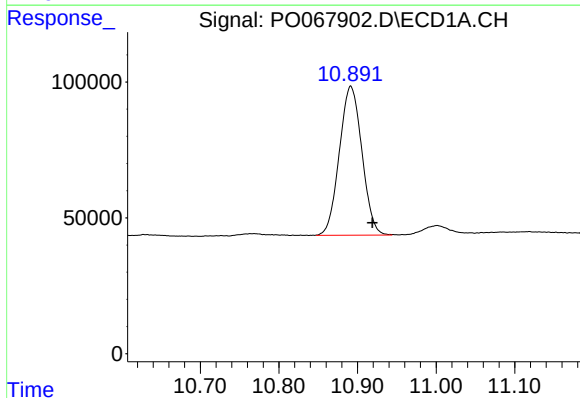

#2 Decachlorobiphenyl

R.T.: 10.891 min
Delta R.T.: -0.028 min
Response: 1094373
Conc: 32.15 ng/ml m

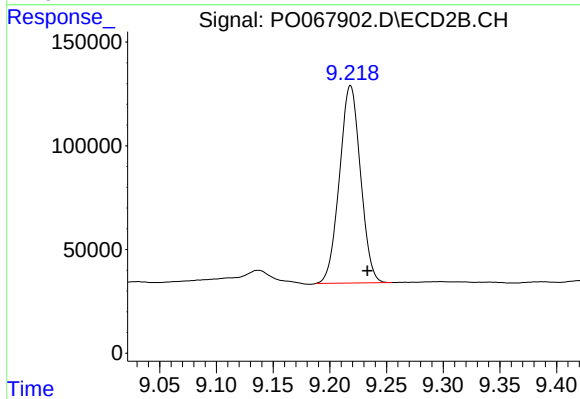

#2 Decachlorobiphenyl

R.T.: 9.218 min
Delta R.T.: -0.015 min
Response: 1229968
Conc: 29.75 ng/ml