

Data Path : P:\HPCHEM1\ECD_0\Data\P0041818\
 Data File : P0043992.D
 Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
 Acq On : 18 Apr 2018 15:28
 Operator : SM/UA
 Sample : J2387-11
 Misc :
 ALS Vial : 6 Sample Multiplier: 1

Instrument :
 ECD_O
 ClientSampleId :
 20180244-AMEND-COMP-A

Manual Integrations
 APPROVED

UGO
 4/19/2018 4:09:17 PM

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Apr 19 00:31:11 2018
 Quant Method : P:\HPCHEM1\ECD_0\methods\P0040418.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Wed Apr 04 15:17:57 2018
 Response via : Initial Calibration
 Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	4.063	3.318	4227609	5418105	23.780m	20.165
2) SA Decachlor...	9.421	8.078	4049264	5202881	22.470m	22.193m

Target Compounds

 (f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : P:\HPCHEM1\ECD_0\Data\P0041818\
Data File : P0043992.D
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
Acq On : 18 Apr 2018 15:28
Operator : SM/UA
Sample : J2387-11
Misc :
ALS Vial : 6 Sample Multiplier: 1



Instrument :
ECD_O
ClientSampleId :
20180244-AMEND-COMP-A


Manual Integrations
APPROVED

UGO
4/19/2018 4:09:17 PM

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Apr 19 00:31:11 2018
Quant Method : P:\HPCHEM1\ECD_0\methods\P0040418.M
Quant Title : GC EXTRACTABLES
QLast Update : Wed Apr 04 15:17:57 2018
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

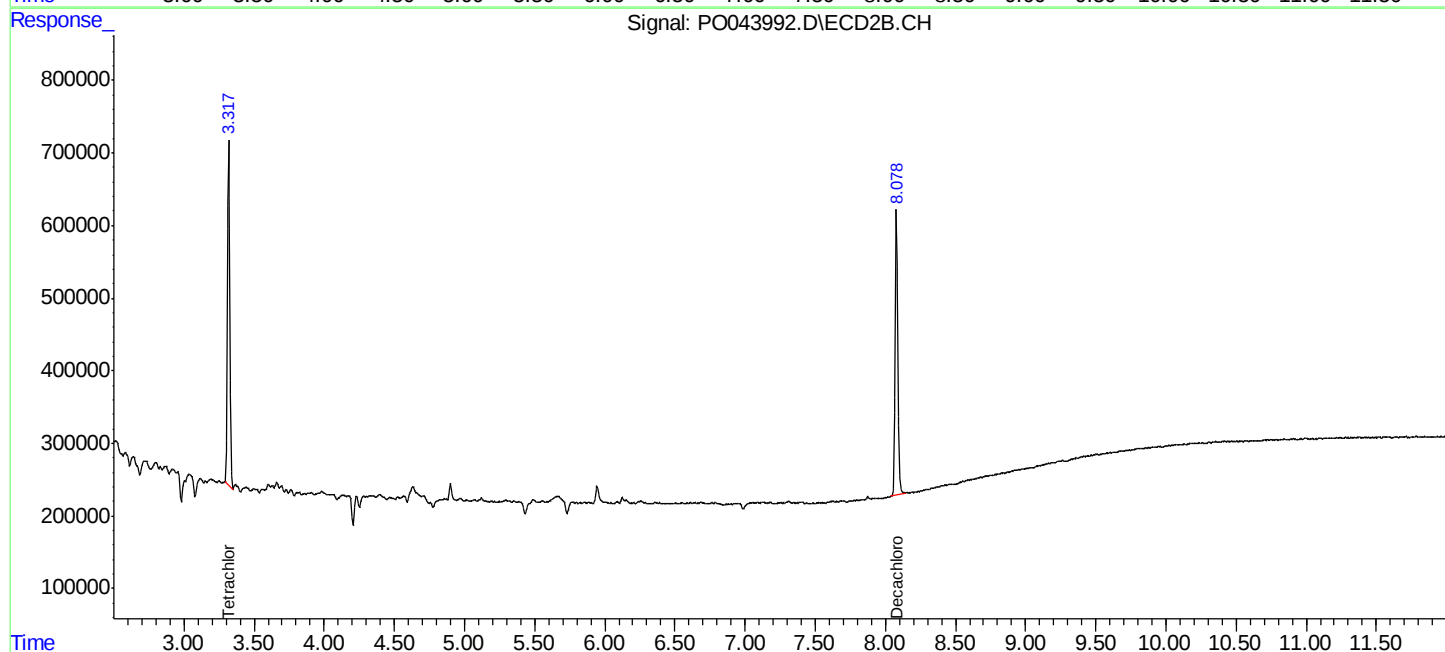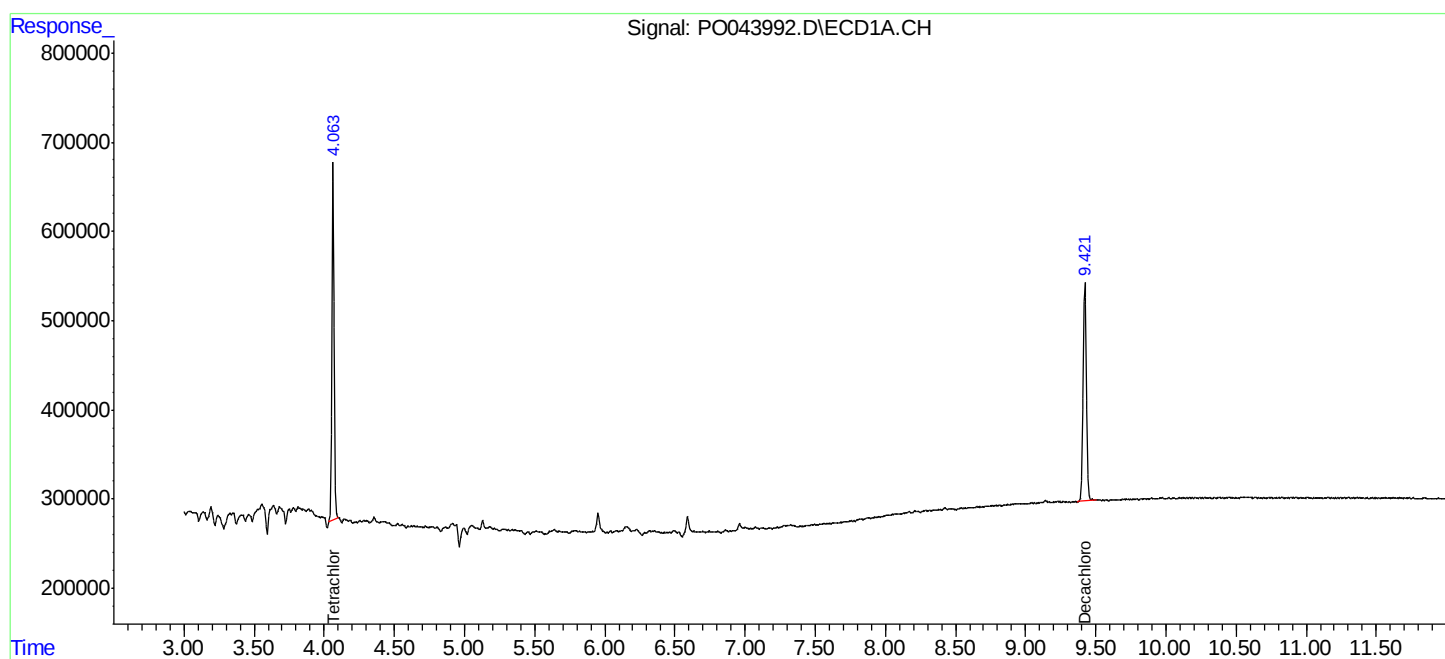

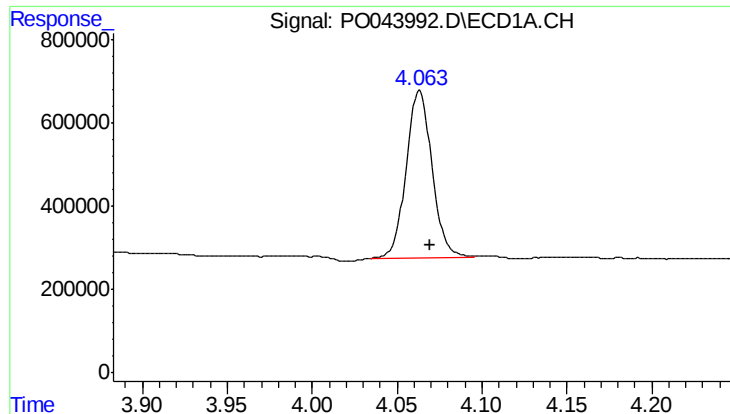


#1 Tetrachloro-m-xylene

R.T.: 4.063 min
Delta R.T.: -0.007 min
Response: 4227609
Conc: 23.78 ng/ml

Instrument :
ECD_O
ClientSampleId :
20180244-AMEND-COMP-A


Manual Integrations
APPROVED

UGO
4/19/2018 4:09:17 PM

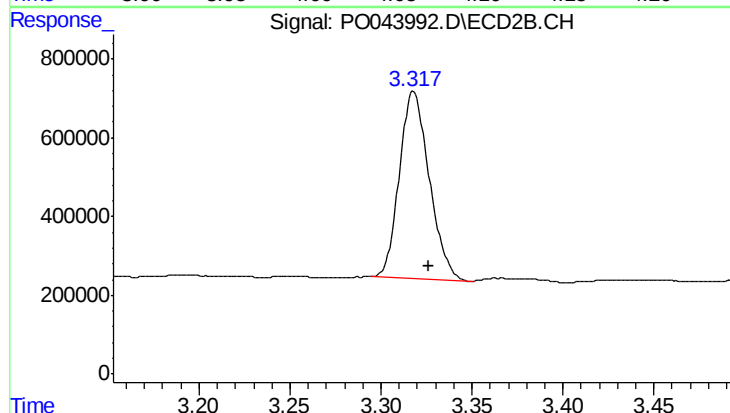


#1 Tetrachloro-m-xylene

R.T.: 3.318 min
Delta R.T.: -0.008 min
Response: 5418105
Conc: 20.17 ng/ml

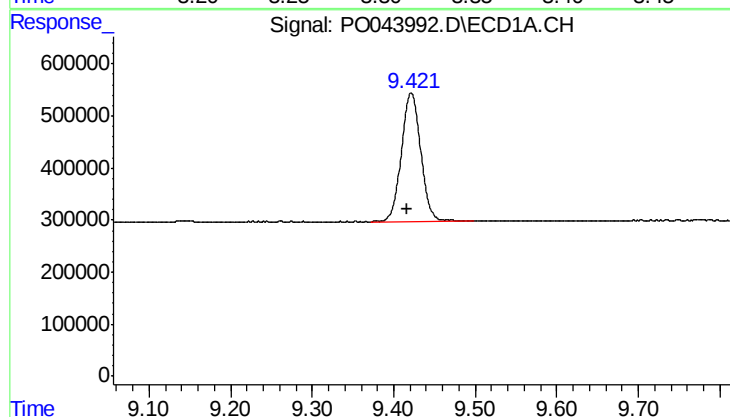

#2 Decachlorobiphenyl

R.T.: 9.421 min
Delta R.T.: 0.004 min
Response: 4049264
Conc: 22.47 ng/ml m

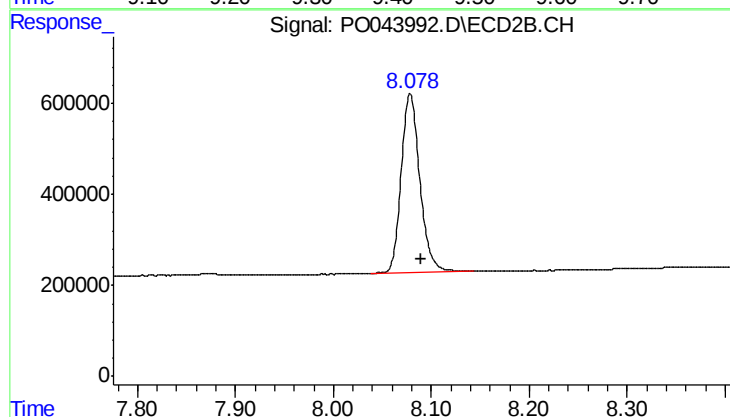

#2 Decachlorobiphenyl

R.T.: 8.078 min
Delta R.T.: -0.012 min
Response: 5202881
Conc: 22.19 ng/ml m