

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\P0041819\
 Data File : P0055427.D
 Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
 Acq On : 18 Apr 2019 11:11
 Operator : SM/SJ
 Sample : K2423-15RE
 Misc :
 ALS Vial : 4 Sample Multiplier: 1

Instrument :
 ECD_O
 ClientSampleId :

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Apr 18 11:26:23 2019
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\P0032519.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Mon Mar 25 17:22:26 2019
 Response via : Initial Calibration
 Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	4.301	3.602	767362	706675	22.111	22.144
2)	SA Decachlor...	9.917	8.568	1434806	1060539	29.105	33.300
Target Compounds							
8)	L2 AR-1221-1	0.000	3.900	0	11945	N.D.	30.722 #
9)	L2 AR-1221-2	4.605	3.900	11103	11945	32.741	39.843
10)	L2 AR-1221-3	4.605	0.000	11103	0	10.688	N.D. #
11)	L3 AR-1232-1	4.605	0.000	11103	0	12.896	N.D. #
12)	L3 AR-1232-2	5.153	0.000	12169	0	24.878	N.D. #
28)	L6 AR-1254-3	6.902	0.000	11880	0	3.778	N.D. #
29)	L6 AR-1254-4	0.000	6.330	0	12714	N.D.	6.494 #
32)	L7 AR-1260-2	7.380	6.330	-198	12714	N.D.	4.619 #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\PO041819\
Data File : PO055427.D
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
Acq On : 18 Apr 2019 11:11
Operator : SM/SJ
Sample : K2423-15RE
Misc :
ALS Vial : 4 Sample Multiplier: 1

Instrument :
ECD_O
ClientSampleId :

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Apr 18 11:26:23 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\PO032519.M
Quant Title : GC EXTRACTABLES
QLast Update : Mon Mar 25 17:22:26 2019
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

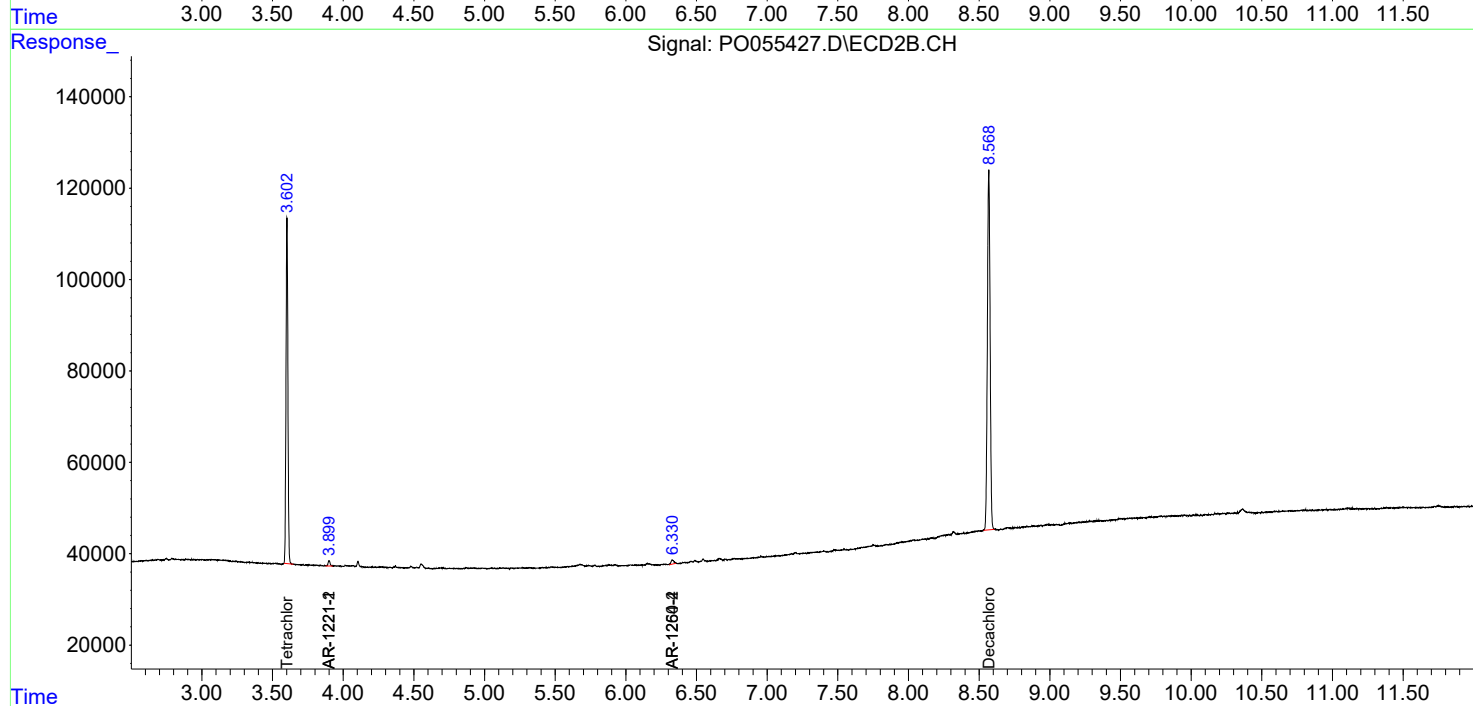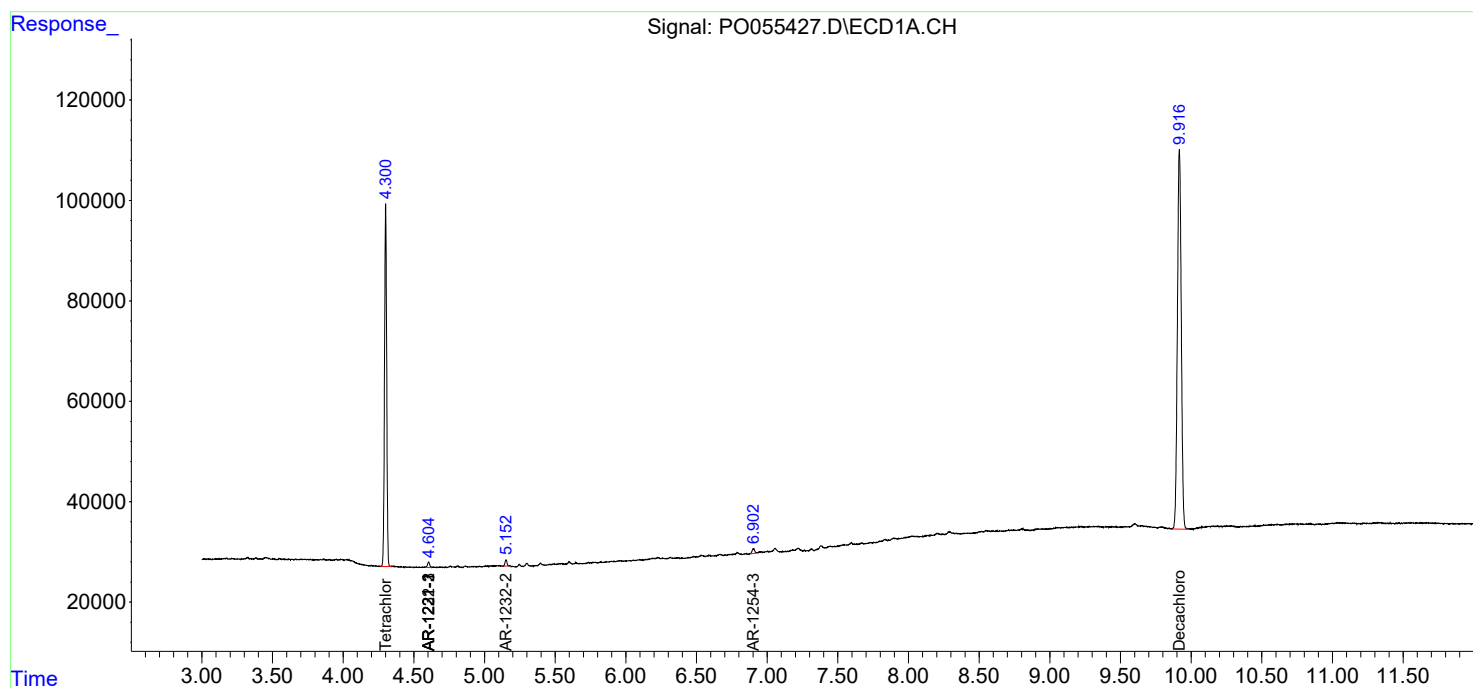


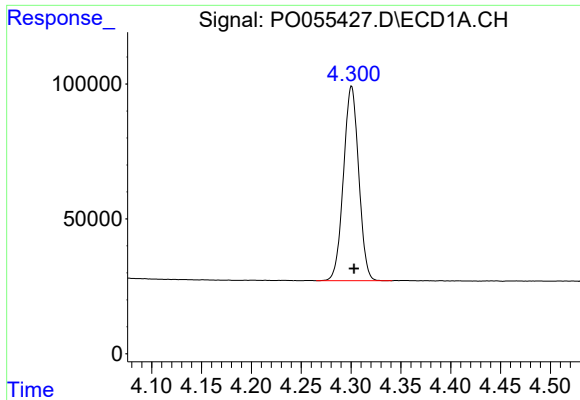

#1 Tetrachloro-m-xylene


R.T.: 4.301 min
Delta R.T.: -0.002 min
Response: 767362
Conc: 22.11 ng/ml

Instrument :
ECD_O
ClientSampleId :

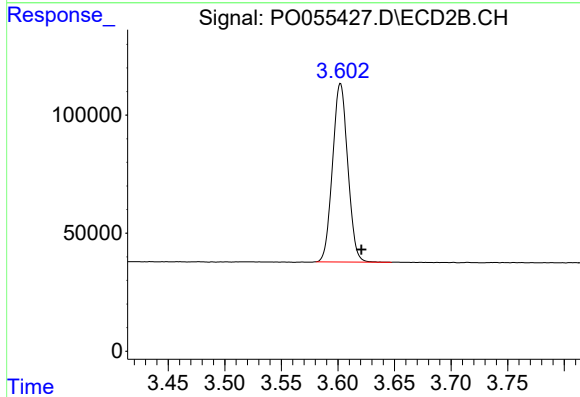


#1 Tetrachloro-m-xylene

R.T.: 3.602 min
Delta R.T.: -0.019 min
Response: 706675
Conc: 22.14 ng/ml

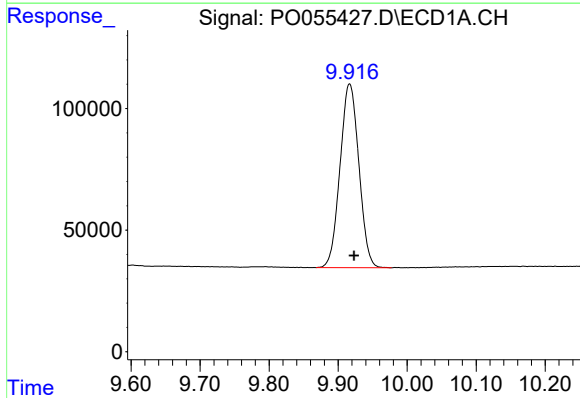


#2 Decachlorobiphenyl

R.T.: 9.917 min
Delta R.T.: -0.006 min
Response: 1434806
Conc: 29.11 ng/ml

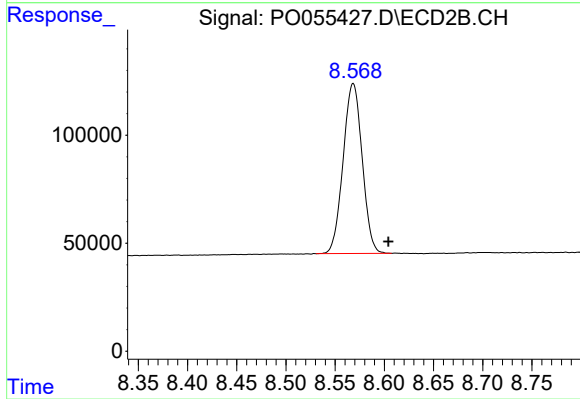

#2 Decachlorobiphenyl


R.T.: 8.568 min
Delta R.T.: -0.036 min
Response: 1060539
Conc: 33.30 ng/ml

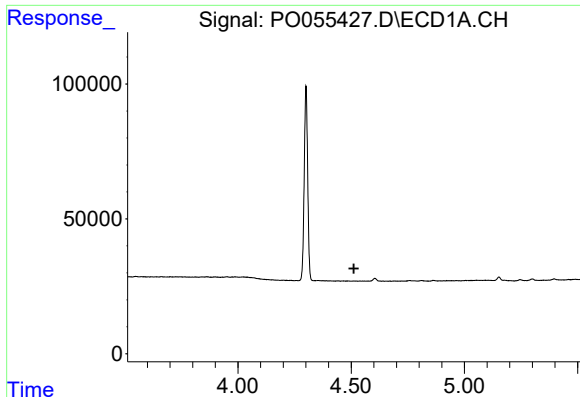

#8 AR-1221-1


R.T.: 0.000 min
Exp R.T.: 4.512 min
Response: 0
Conc: N.D.

Instrument :
ECD_O
ClientSampleId :

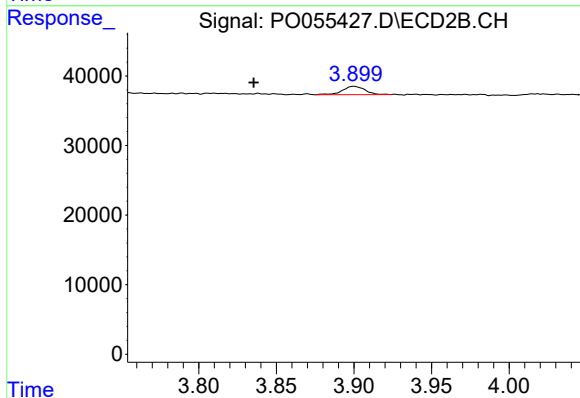


#8 AR-1221-1

R.T.: 3.900 min
Delta R.T.: 0.064 min
Response: 11945
Conc: 30.72 ng/ml

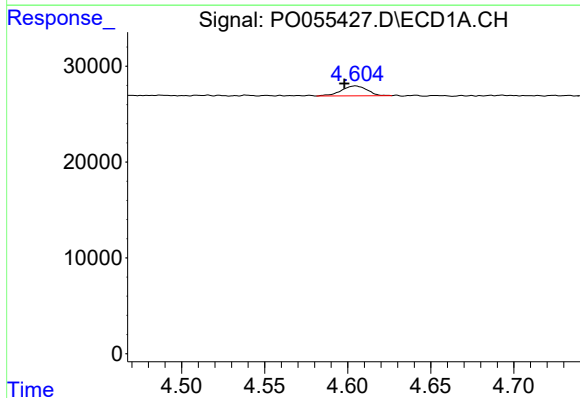


#9 AR-1221-2

R.T.: 4.605 min
Delta R.T.: 0.007 min
Response: 11103
Conc: 32.74 ng/ml

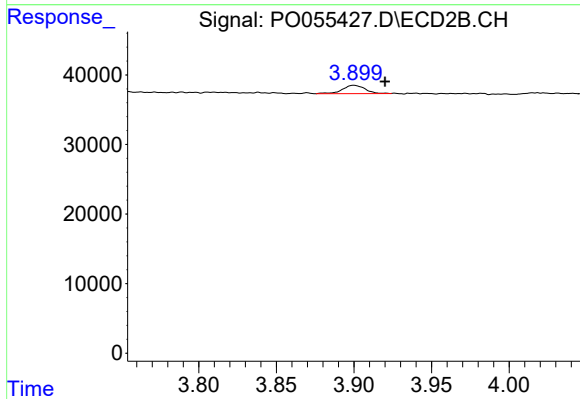

#9 AR-1221-2


R.T.: 3.900 min
Delta R.T.: -0.020 min
Response: 11945
Conc: 39.84 ng/ml

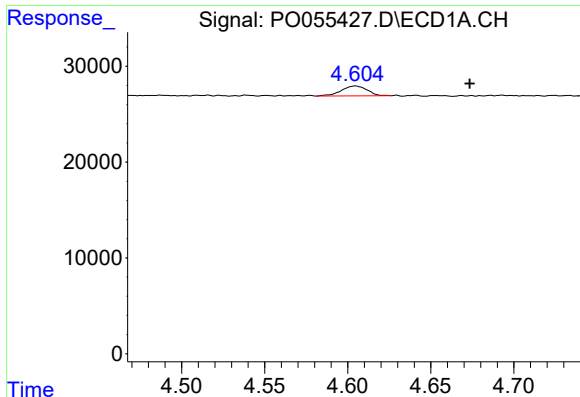

#10 AR-1221-3


R.T.: 4.605 min
Delta R.T.: -0.069 min
Response: 11103
Conc: 10.69 ng/ml

Instrument :
ECD_O
ClientSampleId :

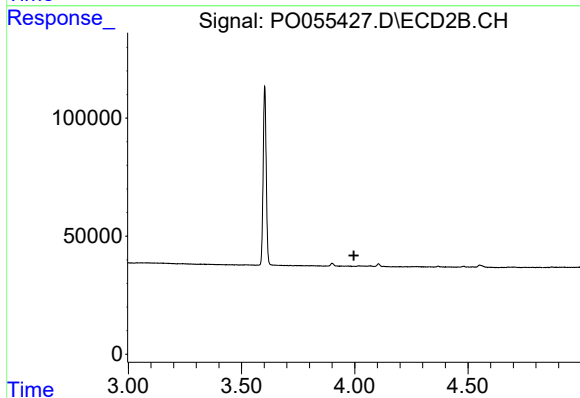


#10 AR-1221-3

R.T.: 0.000 min
Exp R.T. : 3.996 min
Response: 0
Conc: N.D.

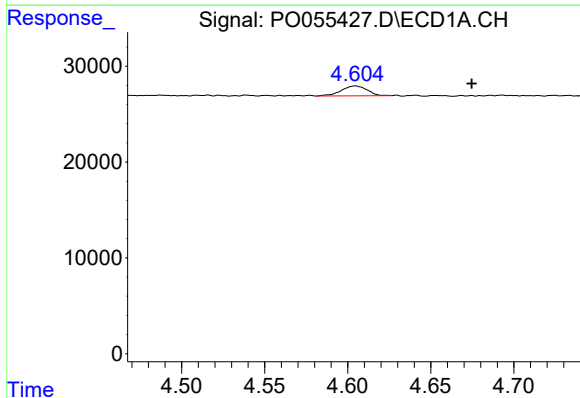


#11 AR-1232-1

R.T.: 4.605 min
Delta R.T.: -0.070 min
Response: 11103
Conc: 12.90 ng/ml

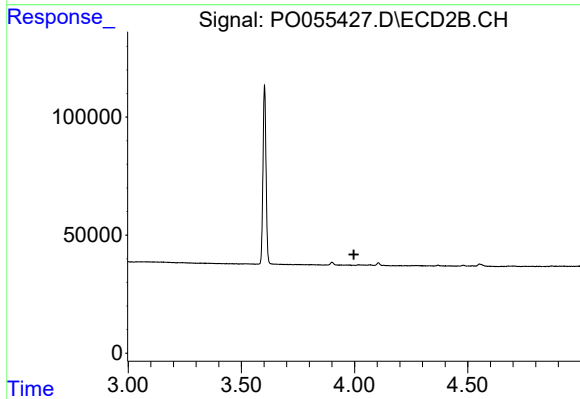

#11 AR-1232-1


R.T.: 0.000 min
Exp R.T. : 3.997 min
Response: 0
Conc: N.D.

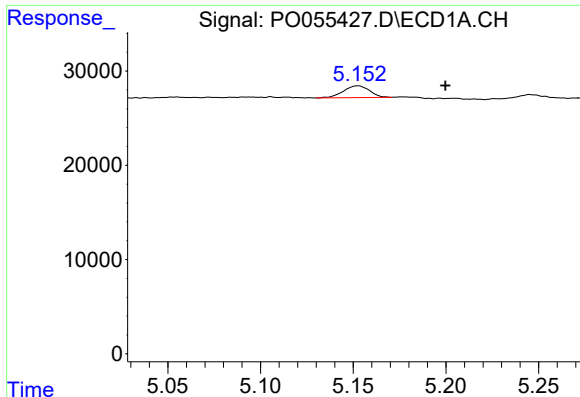

#12 AR-1232-2


R.T.: 5.153 min
Delta R.T.: -0.047 min
Response: 12169
Conc: 24.88 ng/ml

Instrument :
ECD_O
ClientSampleId :

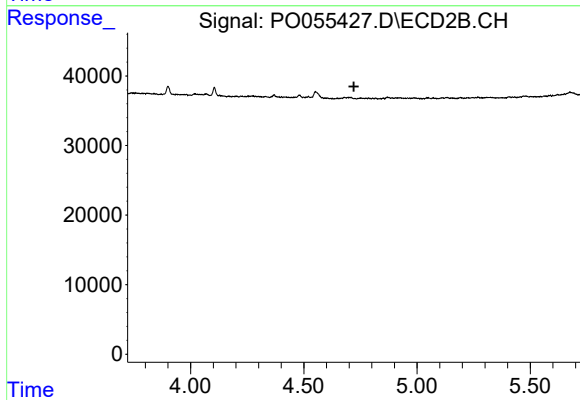


#12 AR-1232-2

R.T.: 0.000 min
Exp R.T. : 4.721 min
Response: 0
Conc: N.D.

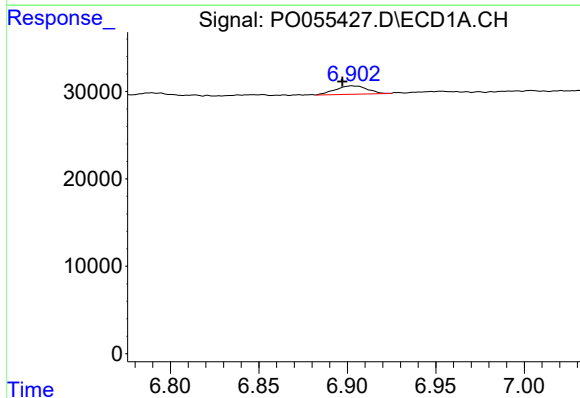


#28 AR-1254-3

R.T.: 6.902 min
Delta R.T.: 0.005 min
Response: 11880
Conc: 3.78 ng/ml

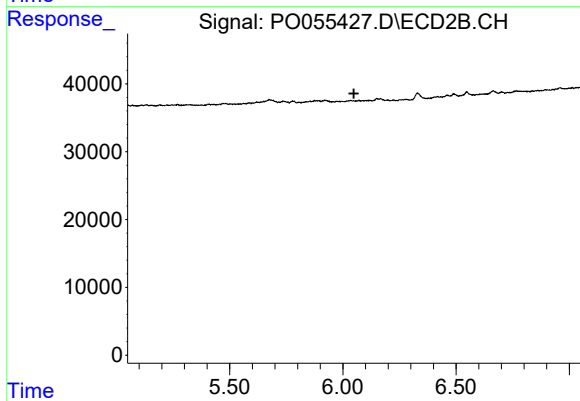

#28 AR-1254-3


R.T.: 0.000 min
Exp R.T. : 6.049 min
Response: 0
Conc: N.D.

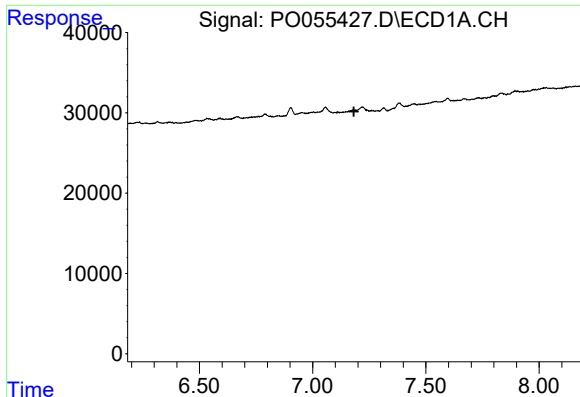

#29 AR-1254-4


R.T.: 0.000 min
Exp R.T.: 7.182 min
Response: 0
Conc: N.D.

Instrument :
ECD_O
ClientSampleId :

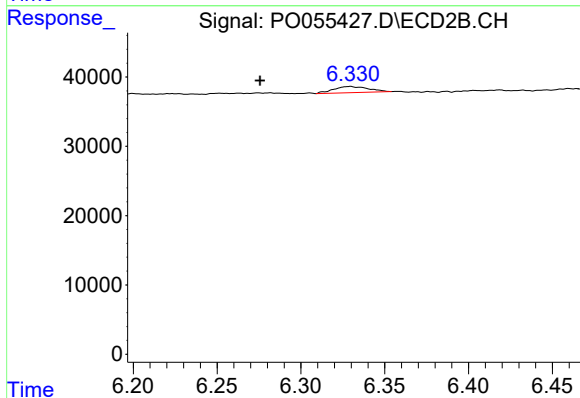


#29 AR-1254-4

R.T.: 6.330 min
Delta R.T.: 0.054 min
Response: 12714
Conc: 6.49 ng/ml

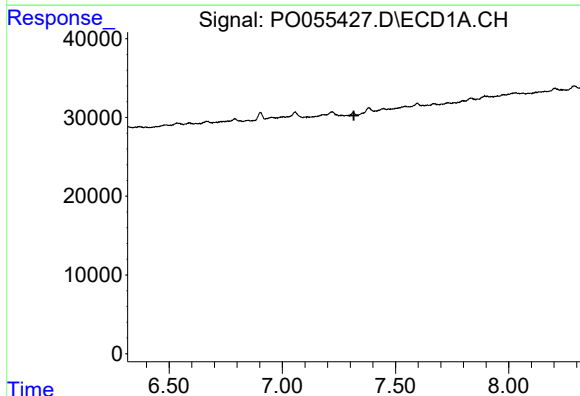

#32 AR-1260-2

R.T.: 7.380 min
Delta R.T.: 0.064 min
Response: -198
Conc: N.D.

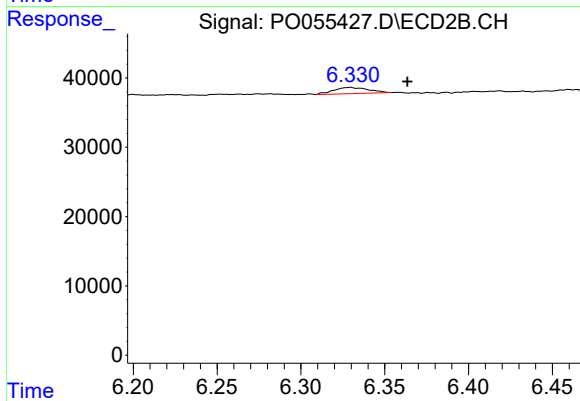

#32 AR-1260-2

R.T.: 6.330 min
Delta R.T.: -0.034 min
Response: 12714
Conc: 4.62 ng/ml