

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\P0041819\
 Data File : P0055434.D
 Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
 Acq On : 18 Apr 2019 13:10
 Operator : SM/SJ
 Sample : K2414-01RE
 Misc :
 ALS Vial : 11 Sample Multiplier: 1

Instrument :
 ECD_O
 ClientSampleId :
 FK-PS-01-044RE

Manual Integrations
 APPROVED

mohammad
 4/19/2019 2:42:31 PM

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Apr 19 00:46:22 2019
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\P0032519.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Mon Mar 25 17:22:26 2019
 Response via : Initial Calibration
 Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	4.289	3.601	500754	474298	14.429	14.862
2) SA Decachlor...	9.900	8.563	481700	374695	9.771m	11.765m

Target Compounds

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\P0041819\
Data File : P0055434.D
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
Acq On : 18 Apr 2019 13:10
Operator : SM/SJ
Sample : K2414-01RE
Misc :
ALS Vial : 11 Sample Multiplier: 1



Instrument :
ECD_O
ClientSampleId :
FK-PS-01-044RE


Manual Integrations
APPROVED

mohammad
4/19/2019 2:42:31 PM

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Apr 19 00:46:22 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\P0032519.M
Quant Title : GC EXTRACTABLES
QLast Update : Mon Mar 25 17:22:26 2019
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

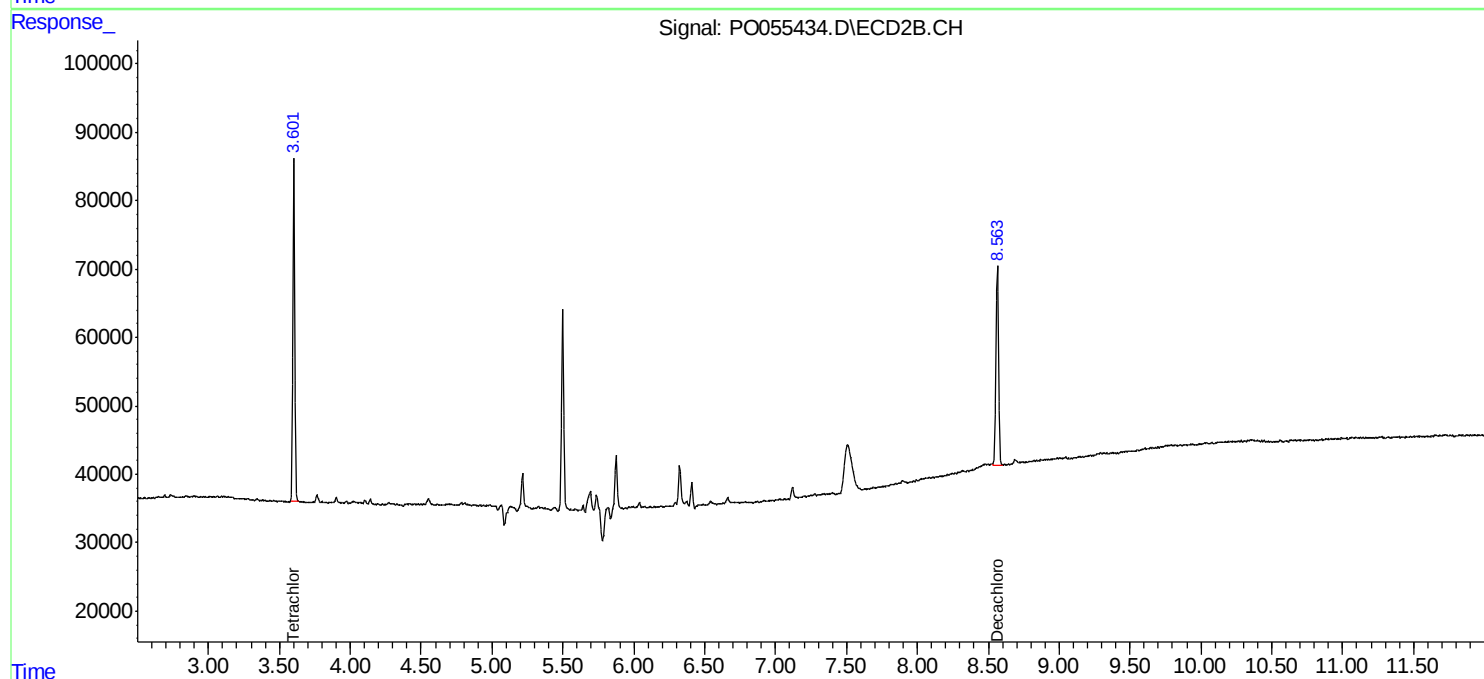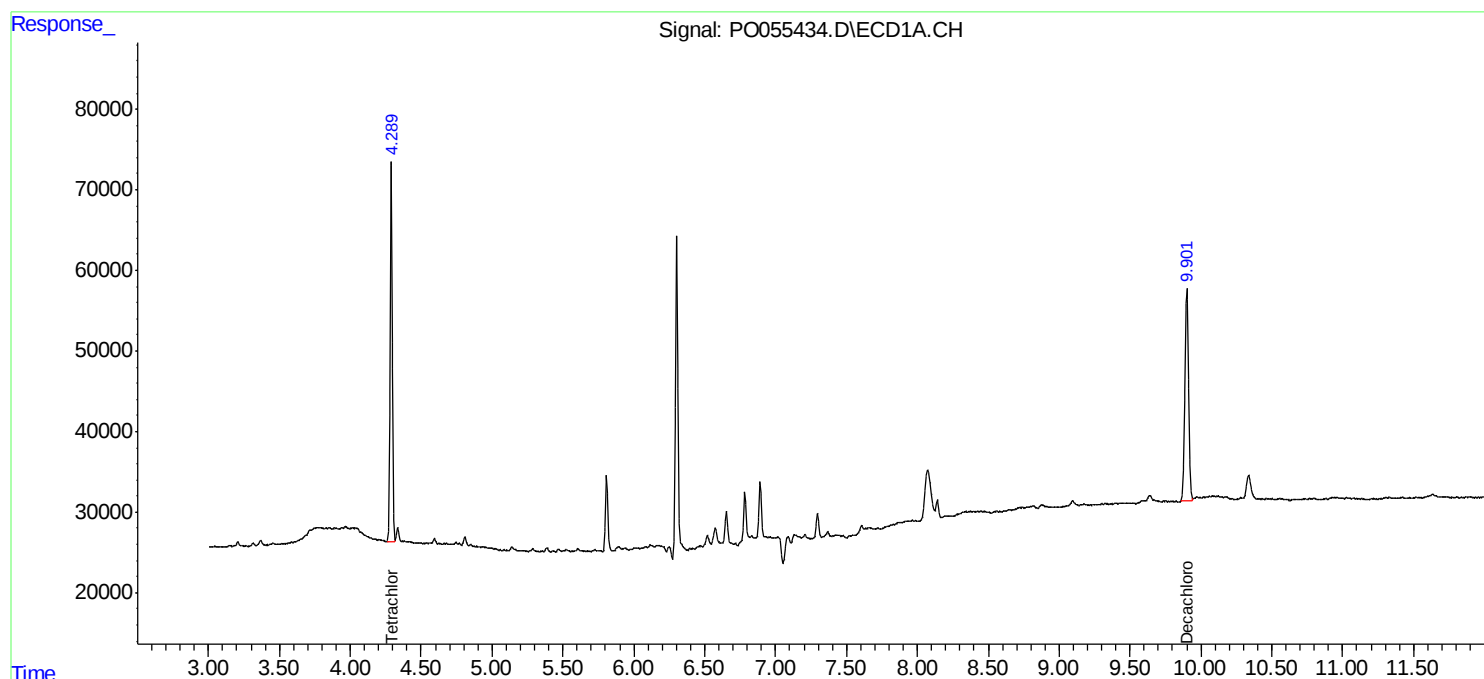

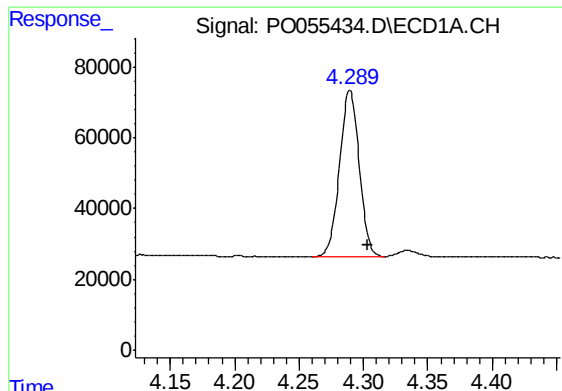


#1 Tetrachloro-m-xylene

R.T.: 4.289 min
Delta R.T.: -0.014 min
Response: 500754
Conc: 14.43 ng/ml

Instrument :
ECD_O
ClientSampleId :
FK-PS-01-044RE


Manual Integrations
APPROVED

mohammad
4/19/2019 2:42:31 PM

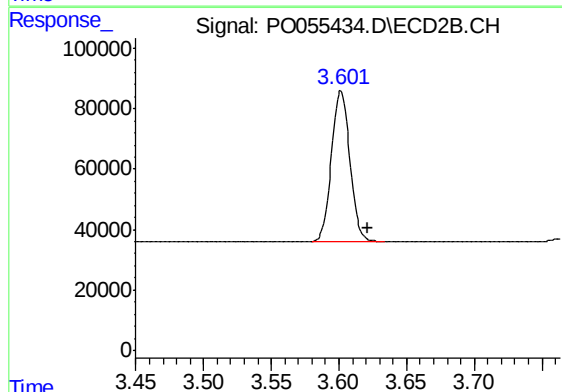


#1 Tetrachloro-m-xylene

R.T.: 3.601 min
Delta R.T.: -0.019 min
Response: 474298
Conc: 14.86 ng/ml

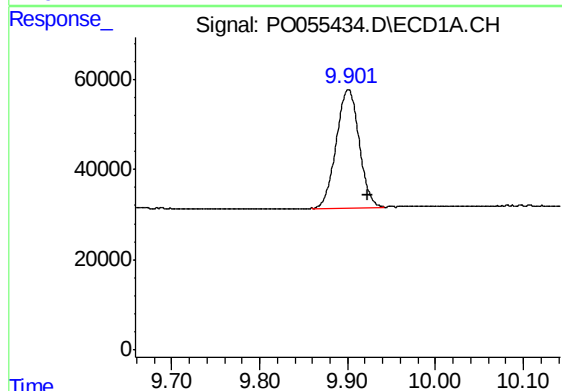

#2 Decachlorobiphenyl

R.T.: 9.900 min
Delta R.T.: -0.023 min
Response: 481700
Conc: 9.77 ng/ml m

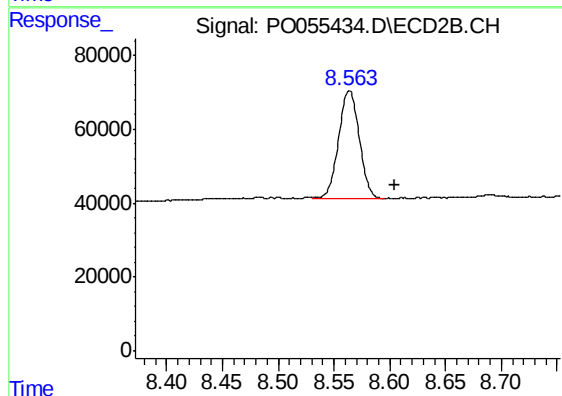

#2 Decachlorobiphenyl

R.T.: 8.563 min
Delta R.T.: -0.041 min
Response: 374695
Conc: 11.77 ng/ml m