

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\P0041819\
 Data File : P0055435.D
 Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
 Acq On : 18 Apr 2019 13:35
 Operator : SM/SJ
 Sample : K2417-01RE
 Misc :
 ALS Vial : 12 Sample Multiplier: 1

Instrument :
 ECD_O
 ClientSampleId :
 FK-PS-01-045RE

Manual Integrations
 APPROVED

mohammad
 4/19/2019 2:42:34 PM

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Apr 19 00:46:47 2019
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\P0032519.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Mon Mar 25 17:22:26 2019
 Response via : Initial Calibration
 Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	4.301	3.601	396575	377061	11.427	11.816
2) SA Decachlor...	9.917	8.568	266580	214126	5.408m	6.723m

Target Compounds

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\P0041819\
Data File : P0055435.D
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
Acq On : 18 Apr 2019 13:35
Operator : SM/SJ
Sample : K2417-01RE
Misc :
ALS Vial : 12 Sample Multiplier: 1



Instrument :
ECD_O
ClientSampleId :
FK-PS-01-045RE


Manual Integrations
APPROVED

mohammad
4/19/2019 2:42:34 PM

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Apr 19 00:46:47 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\P0032519.M
Quant Title : GC EXTRACTABLES
QLast Update : Mon Mar 25 17:22:26 2019
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

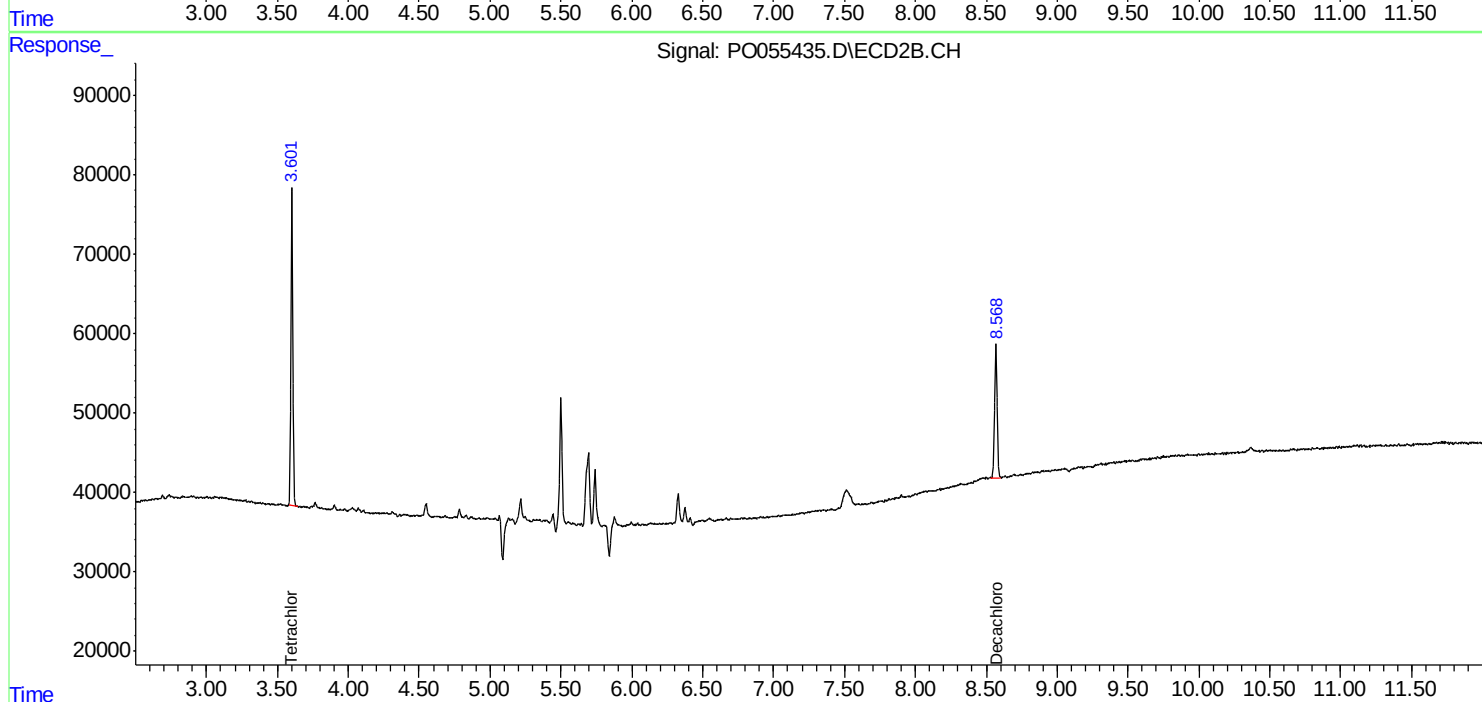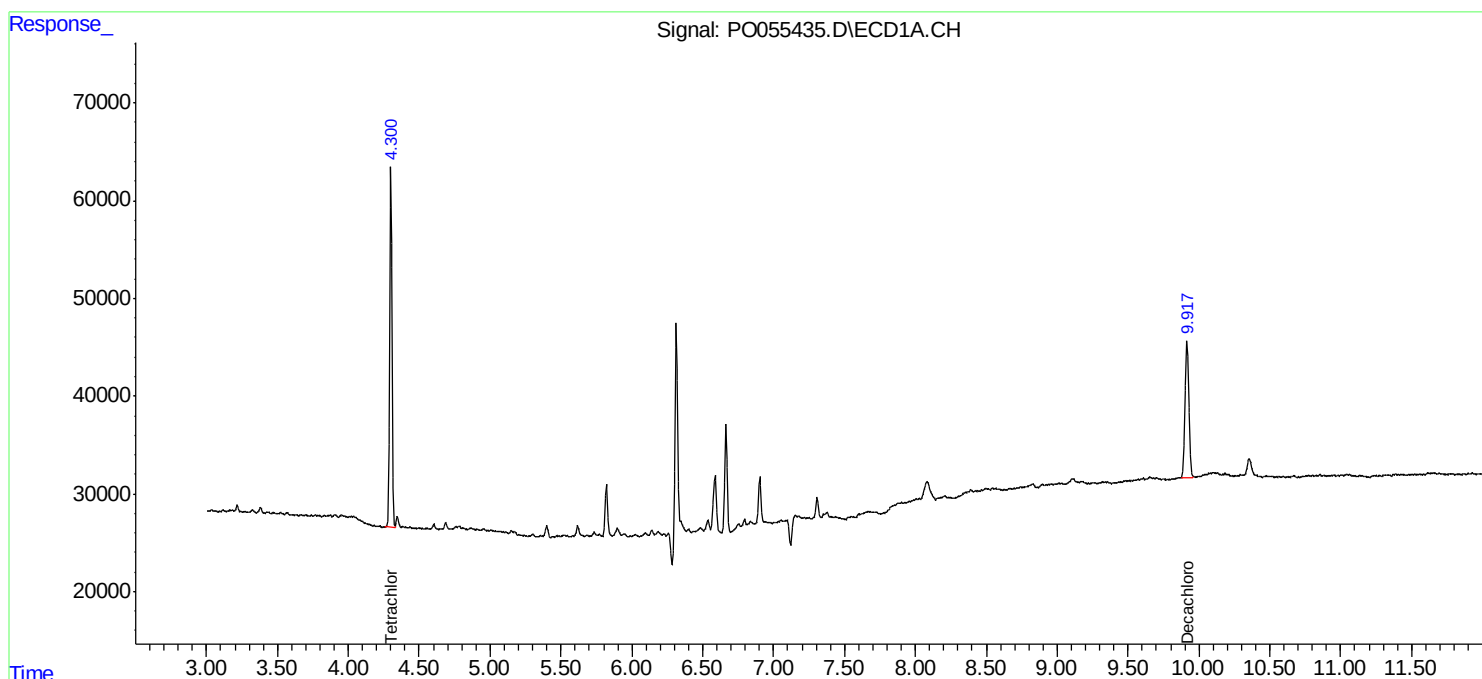

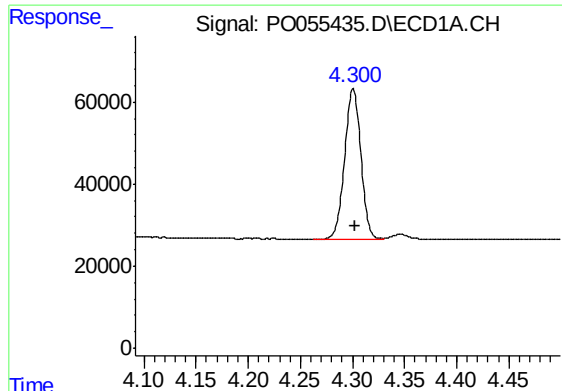


#1 Tetrachloro-m-xylene

R.T.: 4.301 min
Delta R.T.: -0.002 min
Response: 396575
Conc: 11.43 ng/ml

Instrument :
ECD_O
ClientSampleId :
FK-PS-01-045RE


Manual Integrations
APPROVED

mohammad
4/19/2019 2:42:34 PM

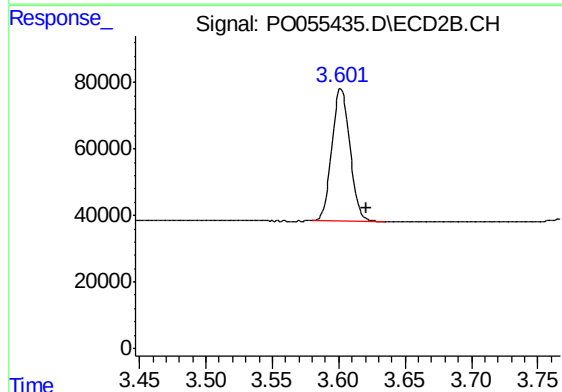


#1 Tetrachloro-m-xylene

R.T.: 3.601 min
Delta R.T.: -0.019 min
Response: 377061
Conc: 11.82 ng/ml

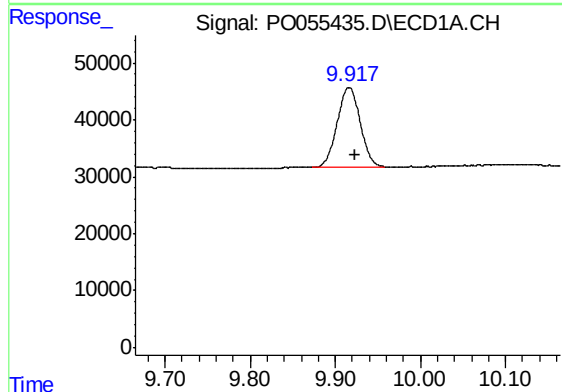

#2 Decachlorobiphenyl

R.T.: 9.917 min
Delta R.T.: -0.007 min
Response: 266580
Conc: 5.41 ng/ml m

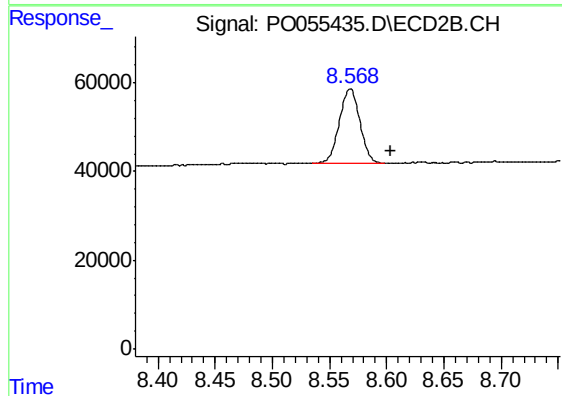

#2 Decachlorobiphenyl

R.T.: 8.568 min
Delta R.T.: -0.036 min
Response: 214126
Conc: 6.72 ng/ml m