

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\P0041919\
 Data File : P0055462.D
 Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
 Acq On : 19 Apr 2019 14:16
 Operator : SM/SJ
 Sample : I.BLK
 Misc :
 ALS Vial : 2 Sample Multiplier: 1

Instrument :
 ECD_O
 ClientSampleId :
 I.BLK

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Apr 19 22:49:10 2019
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\P0032519.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Mon Mar 25 17:22:26 2019
 Response via : Initial Calibration
 Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	4.292	3.603	736963	778472	21.235	24.394
2)	SA Decachlor...	9.906	8.596	821538	7151	16.665	0.225 #
Target Compounds							
7)	L1 AR-1016-5	5.936	0.000	907	0	0.679	N.D. #
8)	L2 AR-1221-1	0.000	3.902	0	9357	N.D.	24.066 #
9)	L2 AR-1221-2	4.597	3.902	10591	9357	31.230	31.211
23)	L5 AR-1248-3	5.936	0.000	907	0	0.568	N.D. #
24)	L5 AR-1248-4	6.305	0.000	8094	0	4.309	N.D. #
26)	L6 AR-1254-1	6.305	0.000	8094	0	4.464	N.D. #
27)	L6 AR-1254-2	6.475	0.000	12582	0	4.407	N.D. #
28)	L6 AR-1254-3	6.895	0.000	10821	0	3.441	N.D. #
29)	L6 AR-1254-4	0.000	6.329	0	7002	N.D.	3.576 #
32)	L7 AR-1260-2	0.000	6.329	0	7002	N.D.	2.544 #
35)	L7 AR-1260-5	8.200	7.199	8643	1159	1.558	0.242 #
37)	L8 AR-1262-2	8.200	7.199	8643	1159	1.459	0.236 #
39)	L8 AR-1262-4	8.624	0.000	1992	0	0.618	N.D. #
40)	L8 AR-1262-5	0.000	8.031	0	260	N.D.	0.161 #
42)	L9 AR-1268-2	8.624	0.000	1992	0	0.304	N.D. #
44)	L9 AR-1268-4	0.000	8.031	0	260	N.D.	0.140 #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\PO041919\
Data File : PO055462.D
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
Acq On : 19 Apr 2019 14:16
Operator : SM/SJ
Sample : I.BLK
Misc :
ALS Vial : 2 Sample Multiplier: 1

Instrument :
ECD_O
ClientSampleId :
I.BLK

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Apr 19 22:49:10 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\PO032519.M
Quant Title : GC EXTRACTABLES
QLast Update : Mon Mar 25 17:22:26 2019
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

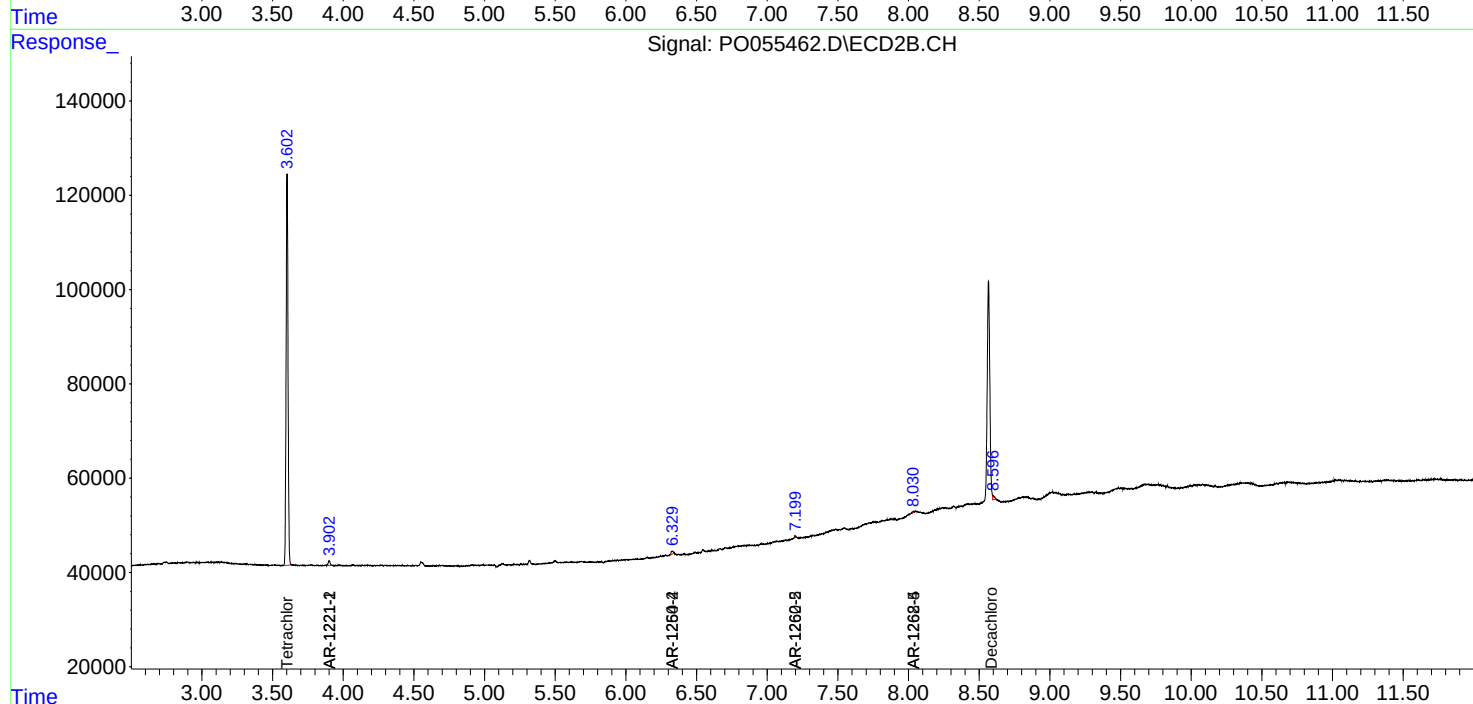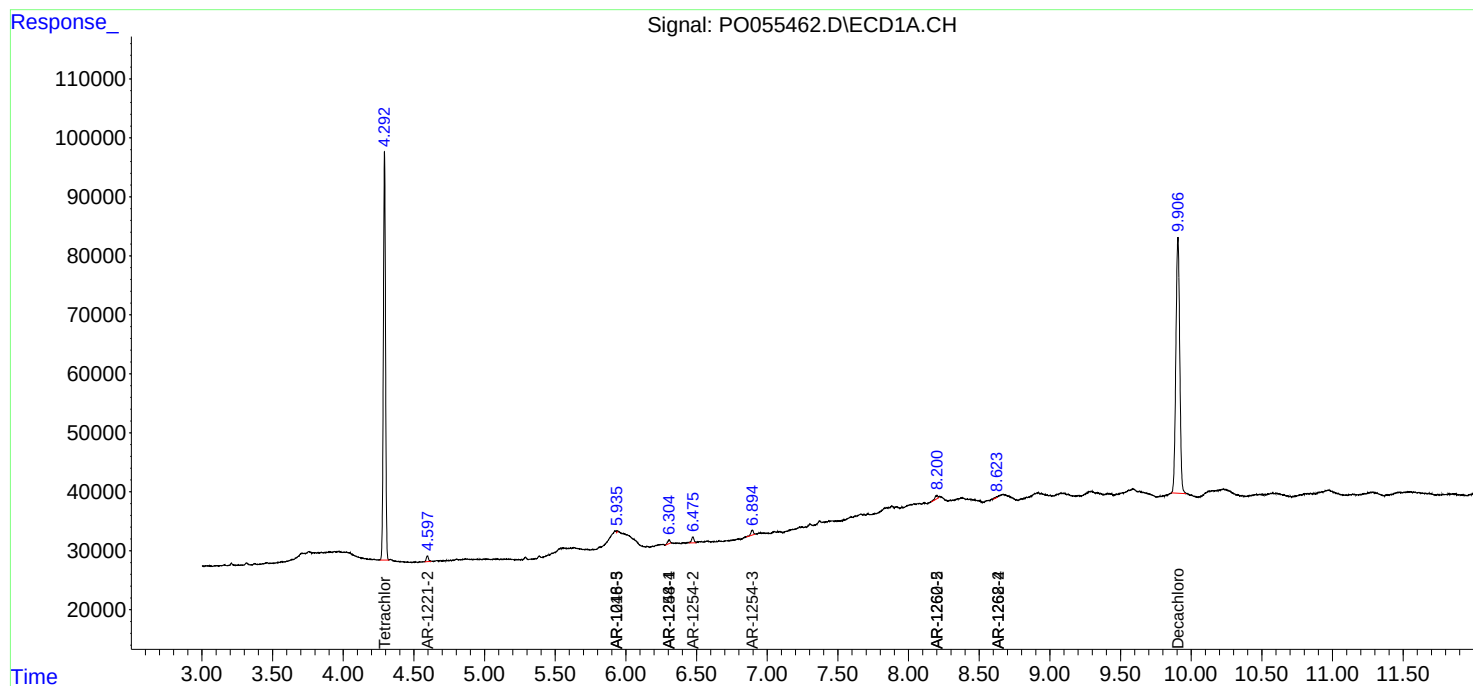


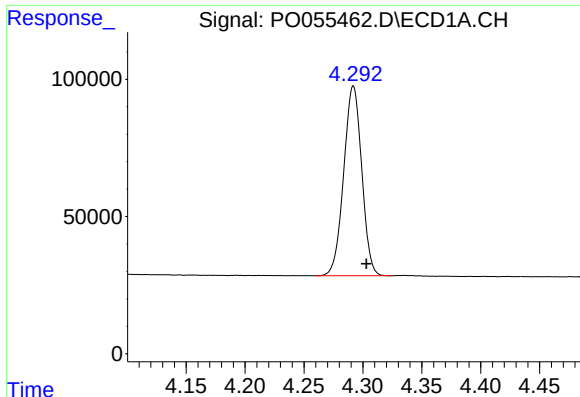

#1 Tetrachloro-m-xylene


R.T.: 4.292 min
Delta R.T.: -0.011 min
Response: 736963
Conc: 21.23 ng/ml

Instrument :
ECD_O
ClientSampleId :
I.BLK

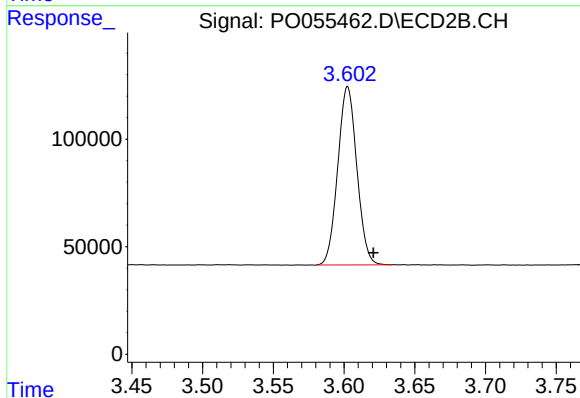


#1 Tetrachloro-m-xylene

R.T.: 3.603 min
Delta R.T.: -0.018 min
Response: 778472
Conc: 24.39 ng/ml

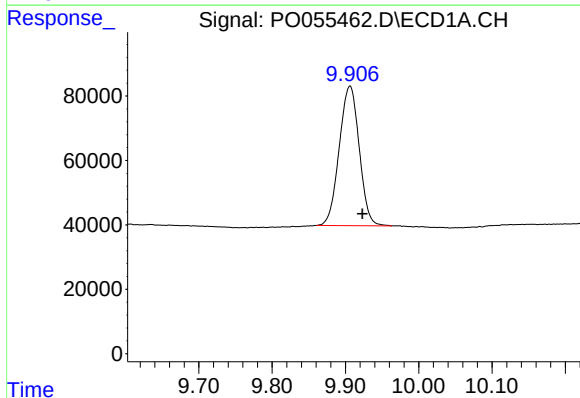


#2 Decachlorobiphenyl

R.T.: 9.906 min
Delta R.T.: -0.017 min
Response: 821538
Conc: 16.66 ng/ml

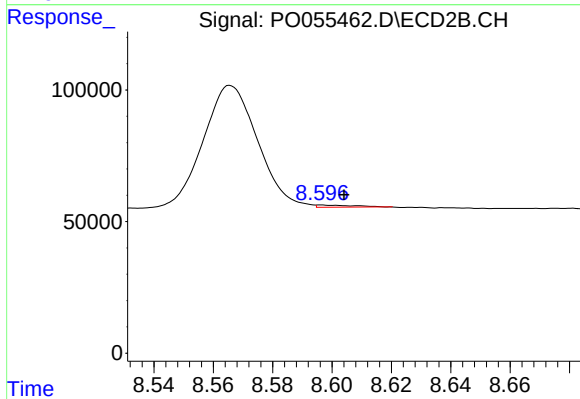

#2 Decachlorobiphenyl


R.T.: 8.596 min
Delta R.T.: -0.008 min
Response: 7151
Conc: 0.22 ng/ml

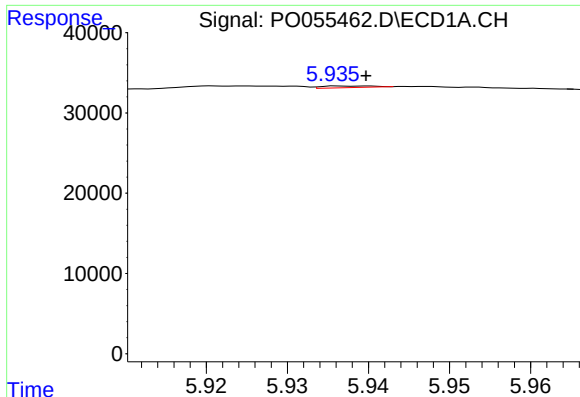

#7 AR-1016-5


R.T.: 5.936 min
Delta R.T.: -0.004 min
Response: 907
Conc: 0.68 ng/ml

Instrument :
ECD_O
ClientSampleId :
I.BLK

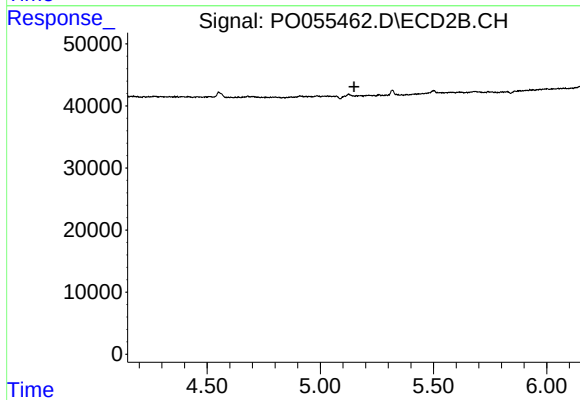


#7 AR-1016-5

R.T.: 0.000 min
Exp R.T. : 5.149 min
Response: 0
Conc: N.D.

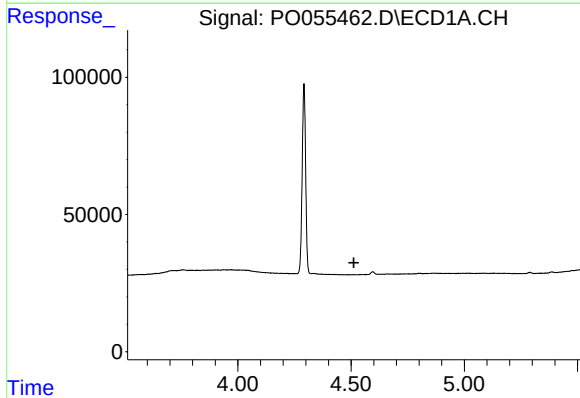


#8 AR-1221-1

R.T.: 0.000 min
Exp R.T. : 4.512 min
Response: 0
Conc: N.D.

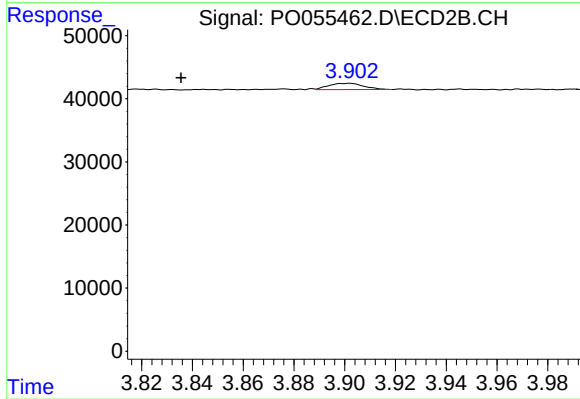

#8 AR-1221-1


R.T.: 3.902 min
Delta R.T.: 0.067 min
Response: 9357
Conc: 24.07 ng/ml

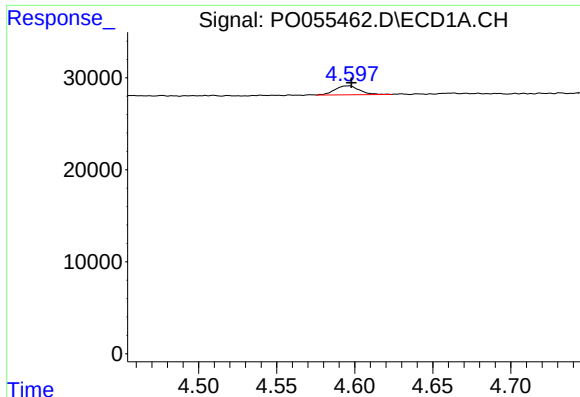

#9 AR-1221-2


R.T.: 4.597 min
Delta R.T.: -0.001 min
Response: 10591
Conc: 31.23 ng/ml

Instrument :
ECD_O
ClientSampleId :
I.BLK

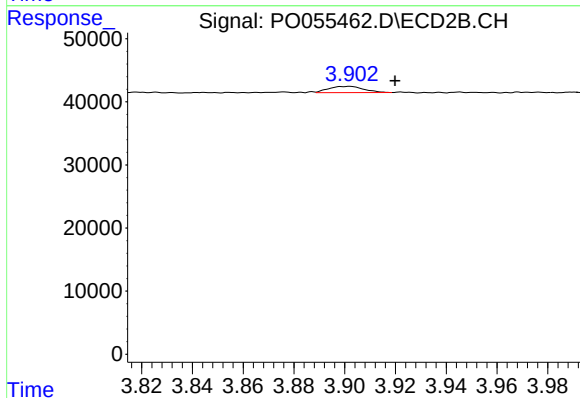


#9 AR-1221-2

R.T.: 3.902 min
Delta R.T.: -0.018 min
Response: 9357
Conc: 31.21 ng/ml

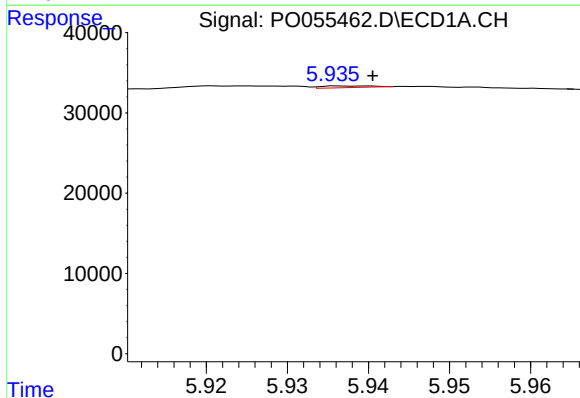


#23 AR-1248-3

R.T.: 5.936 min
Delta R.T.: -0.004 min
Response: 907
Conc: 0.57 ng/ml

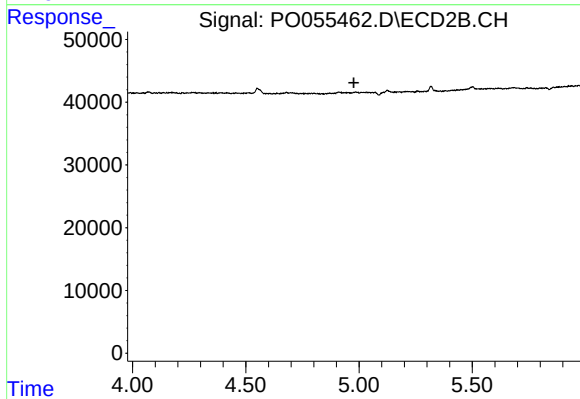

#23 AR-1248-3


R.T.: 0.000 min
Exp R.T.: 4.977 min
Response: 0
Conc: N.D.

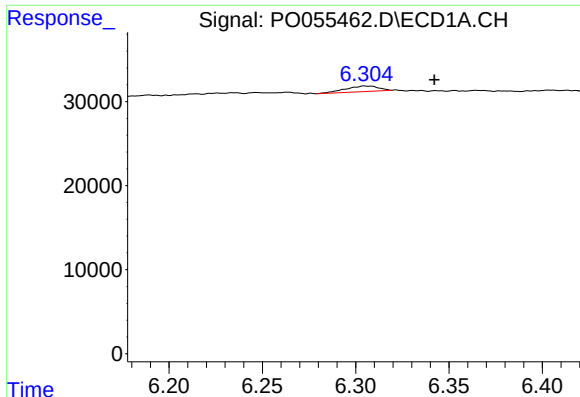

#24 AR-1248-4


R.T.: 6.305 min
Delta R.T.: -0.038 min
Response: 8094
Conc: 4.31 ng/ml

Instrument :
ECD_O
ClientSampleId :
I.BLK

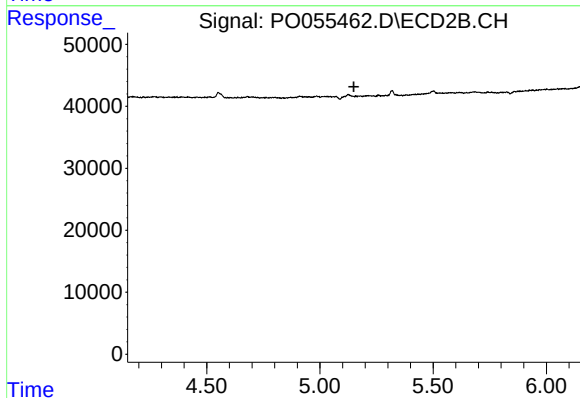


#24 AR-1248-4

R.T.: 0.000 min
Exp R.T. : 5.149 min
Response: 0
Conc: N.D.

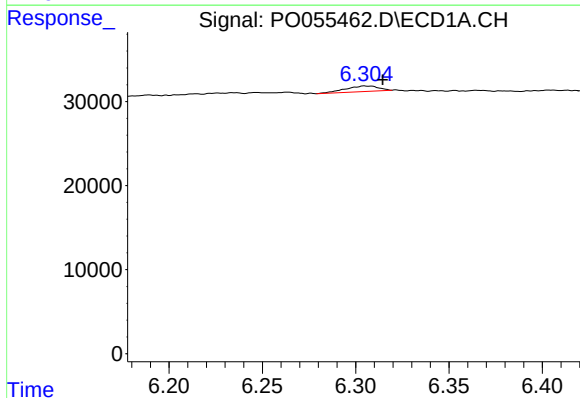


#26 AR-1254-1

R.T.: 6.305 min
Delta R.T.: -0.010 min
Response: 8094
Conc: 4.46 ng/ml

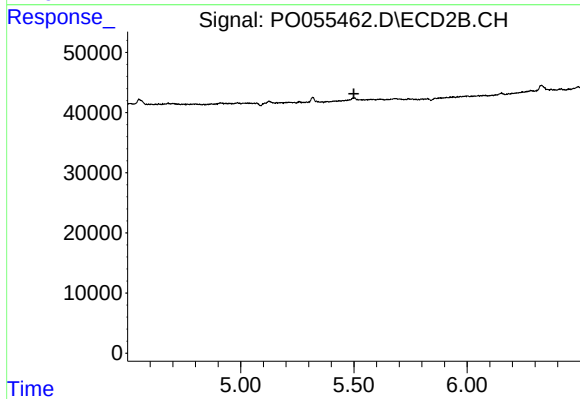

#26 AR-1254-1


R.T.: 0.000 min
Exp R.T. : 5.500 min
Response: 0
Conc: N.D.

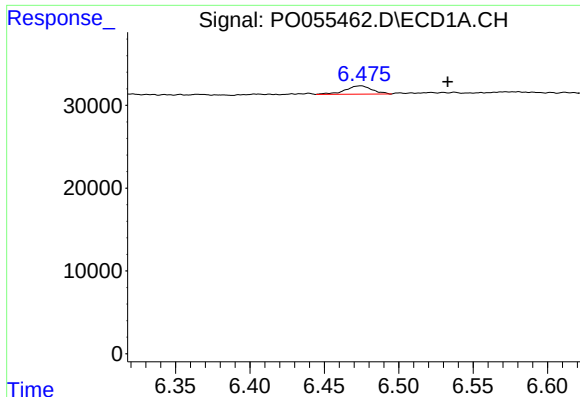

#27 AR-1254-2


R.T.: 6.475 min
Delta R.T.: -0.058 min
Response: 12582
Conc: 4.41 ng/ml

Instrument :
ECD_O
ClientSampleId :
I.BLK

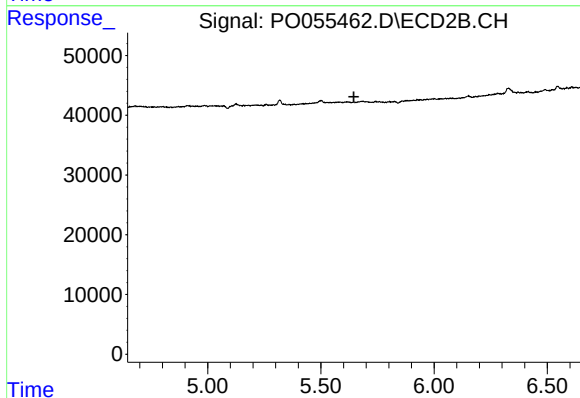


#27 AR-1254-2

R.T.: 0.000 min
Exp R.T. : 5.646 min
Response: 0
Conc: N.D.

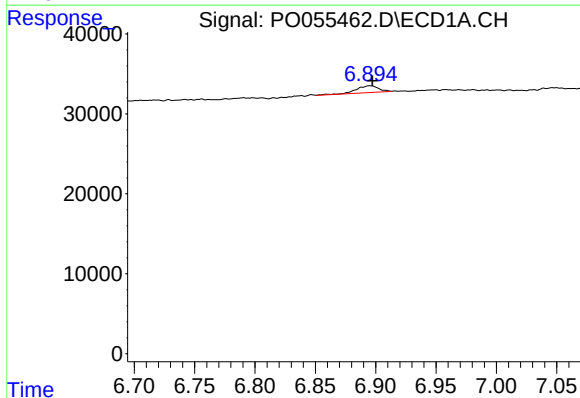


#28 AR-1254-3

R.T.: 6.895 min
Delta R.T.: -0.002 min
Response: 10821
Conc: 3.44 ng/ml

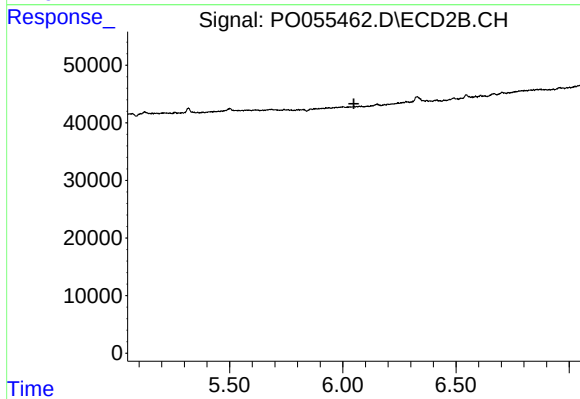

#28 AR-1254-3


R.T.: 0.000 min
Exp R.T. : 6.049 min
Response: 0
Conc: N.D.

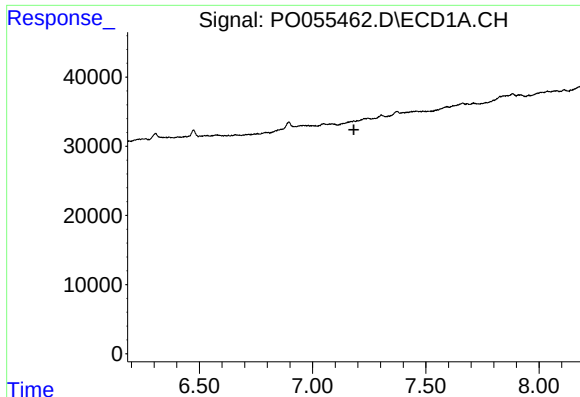

#29 AR-1254-4


R.T.: 0.000 min
Exp R.T.: 7.182 min
Response: 0
Conc: N.D.

Instrument :
ECD_O
ClientSampleId :
I.BLK

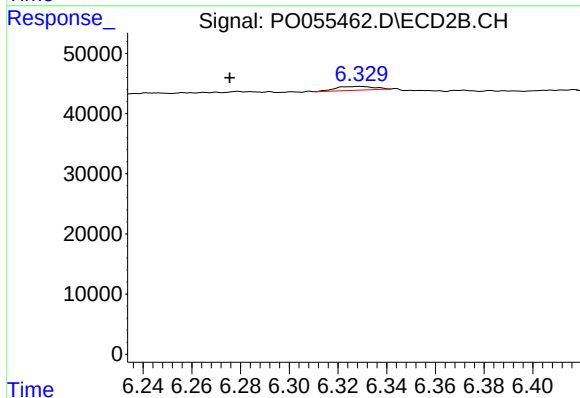


#29 AR-1254-4

R.T.: 6.329 min
Delta R.T.: 0.053 min
Response: 7002
Conc: 3.58 ng/ml

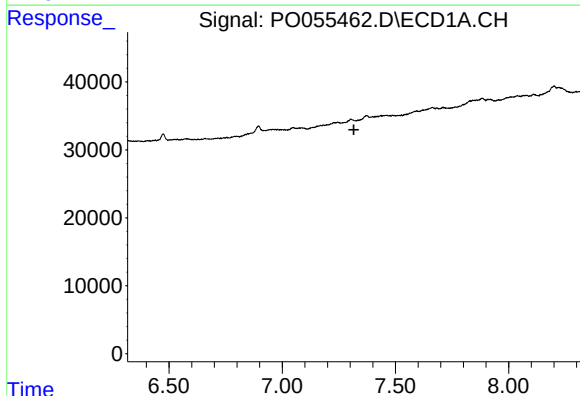


#32 AR-1260-2

R.T.: 0.000 min
Exp R.T.: 7.316 min
Response: 0
Conc: N.D.

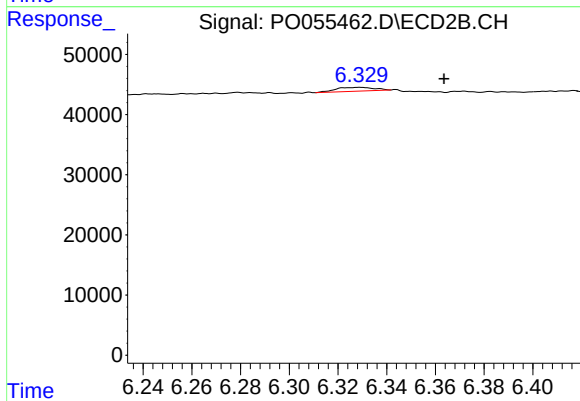

#32 AR-1260-2


R.T.: 6.329 min
Delta R.T.: -0.035 min
Response: 7002
Conc: 2.54 ng/ml

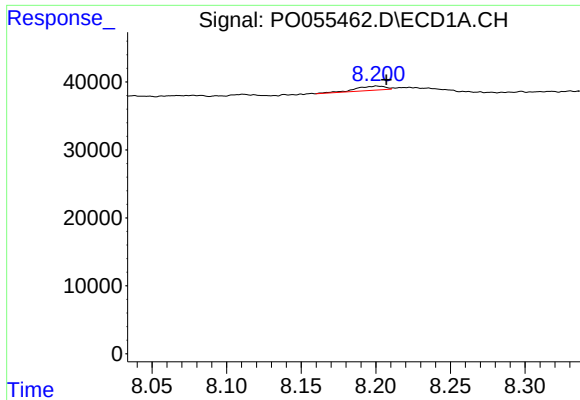

#35 AR-1260-5


R.T.: 8.200 min
Delta R.T.: -0.007 min
Response: 8643
Conc: 1.56 ng/ml

Instrument :
ECD_O
ClientSampleId :
I.BLK

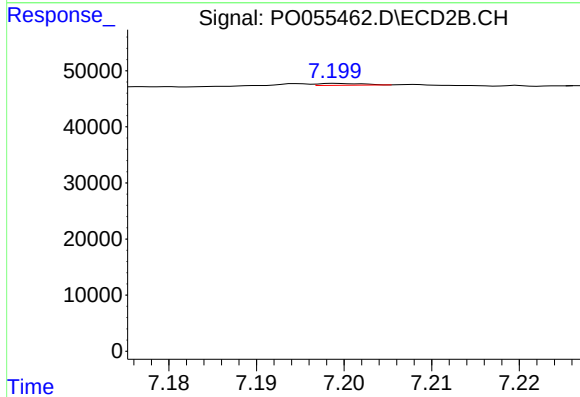


#35 AR-1260-5

R.T.: 7.199 min
Delta R.T.: -0.028 min
Response: 1159
Conc: 0.24 ng/ml

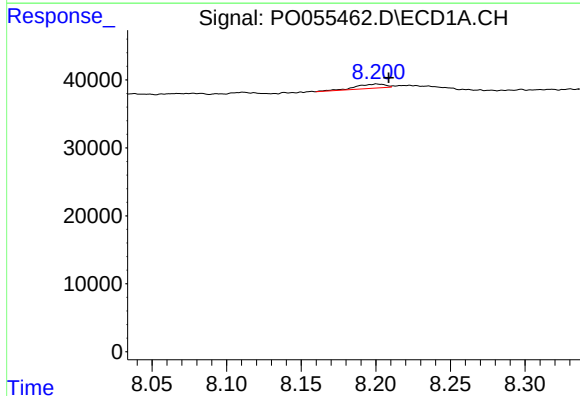


#37 AR-1262-2

R.T.: 8.200 min
Delta R.T.: -0.008 min
Response: 8643
Conc: 1.46 ng/ml

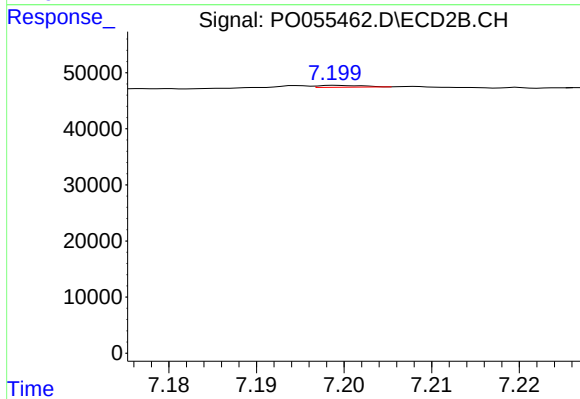

#37 AR-1262-2


R.T.: 7.199 min
Delta R.T.: -0.030 min
Response: 1159
Conc: 0.24 ng/ml

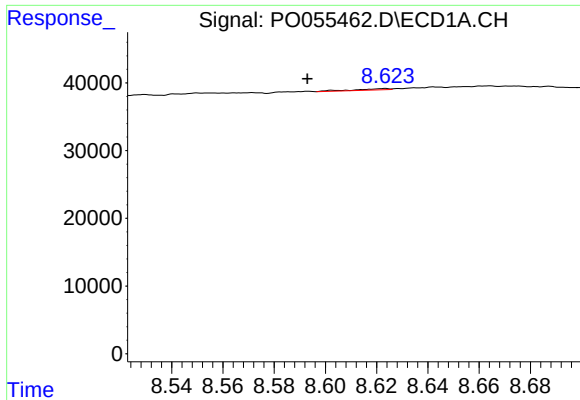

#39 AR-1262-4


R.T.: 8.624 min
Delta R.T.: 0.031 min
Response: 1992
Conc: 0.62 ng/ml

Instrument :
ECD_O
ClientSampleId :
I.BLK

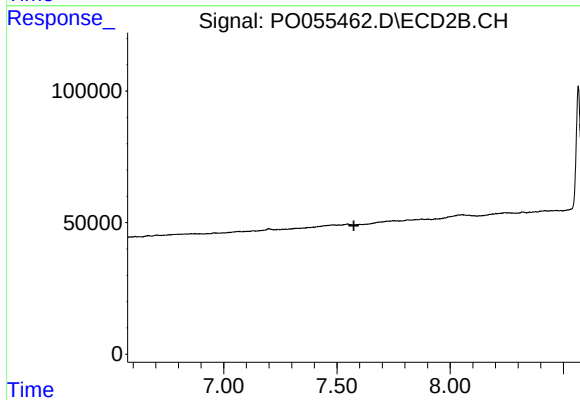


#39 AR-1262-4

R.T.: 0.000 min
Exp R.T. : 7.575 min
Response: 0
Conc: N.D.

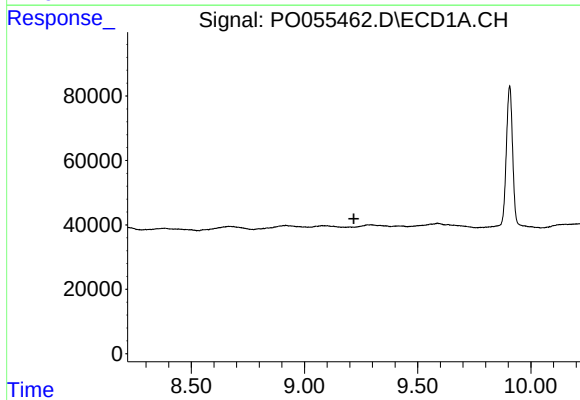


#40 AR-1262-5

R.T.: 0.000 min
Exp R.T. : 9.218 min
Response: 0
Conc: N.D.

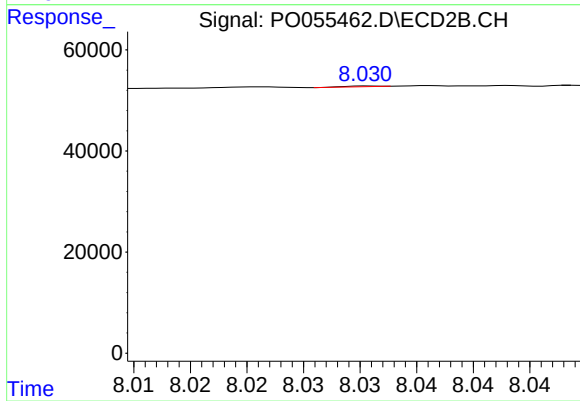

#40 AR-1262-5


R.T.: 8.031 min
Delta R.T.: -0.036 min
Response: 260
Conc: 0.16 ng/ml

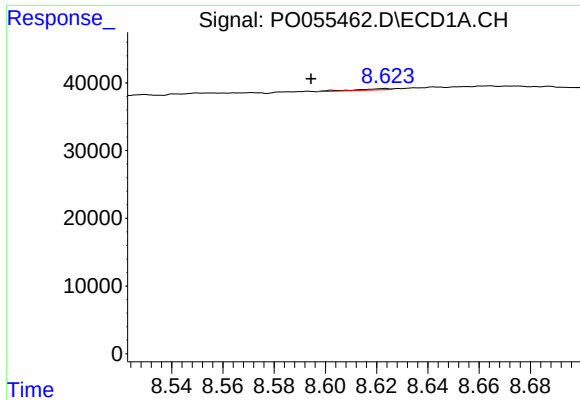

#42 AR-1268-2


R.T.: 8.624 min
Delta R.T.: 0.029 min
Response: 1992
Conc: 0.30 ng/ml

Instrument :
ECD_O
ClientSampleId :
I.BLK

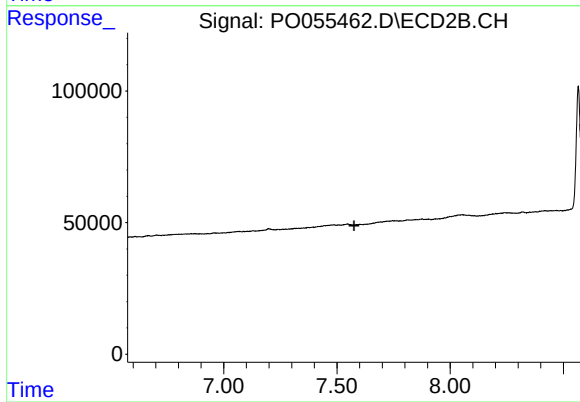


#42 AR-1268-2

R.T.: 0.000 min
Exp R.T. : 7.575 min
Response: 0
Conc: N.D.

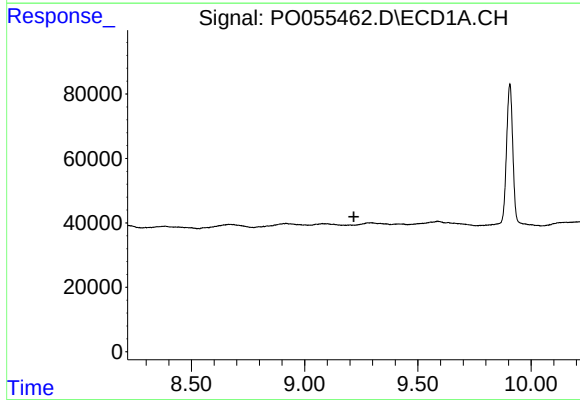

#44 AR-1268-4

R.T.: 0.000 min
Exp R.T. : 9.217 min
Response: 0
Conc: N.D.

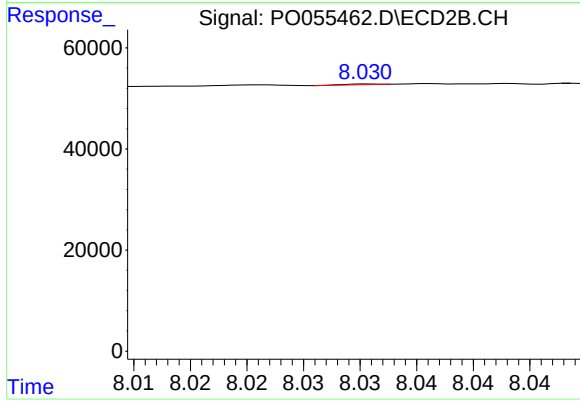

#44 AR-1268-4

R.T.: 8.031 min
Delta R.T.: -0.035 min
Response: 260
Conc: 0.14 ng/ml