

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\P0041919\
 Data File : P0055501.D
 Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
 Acq On : 20 Apr 2019 2:04
 Operator : SM/SJ
 Sample : K2482-01
 Misc :
 ALS Vial : 30 Sample Multiplier: 1

Instrument :
 ECD_O
 ClientSampleId :
 AU-041819

Manual Integrations
 APPROVED

Sohil
 4/23/2019 12:06:14 PM

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Apr 20 03:26:04 2019
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\P0032519.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Mon Mar 25 17:22:26 2019
 Response via : Initial Calibration
 Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	4.292	3.603	838402	916902	24.158	28.732m
2)	SA Decachlor...	9.905	8.565	646481	474766	13.114	14.907

Target Compounds

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\P0041919\
Data File : P0055501.D
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
Acq On : 20 Apr 2019 2:04
Operator : SM/SJ
Sample : K2482-01
Misc :
ALS Vial : 30 Sample Multiplier: 1



Instrument :
ECD_O
ClientSampleId :
AU-041819


Manual Integrations
APPROVED

Sohil
4/23/2019 12:06:14 PM

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Apr 20 03:26:04 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\P0032519.M
Quant Title : GC EXTRACTABLES
QLast Update : Mon Mar 25 17:22:26 2019
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

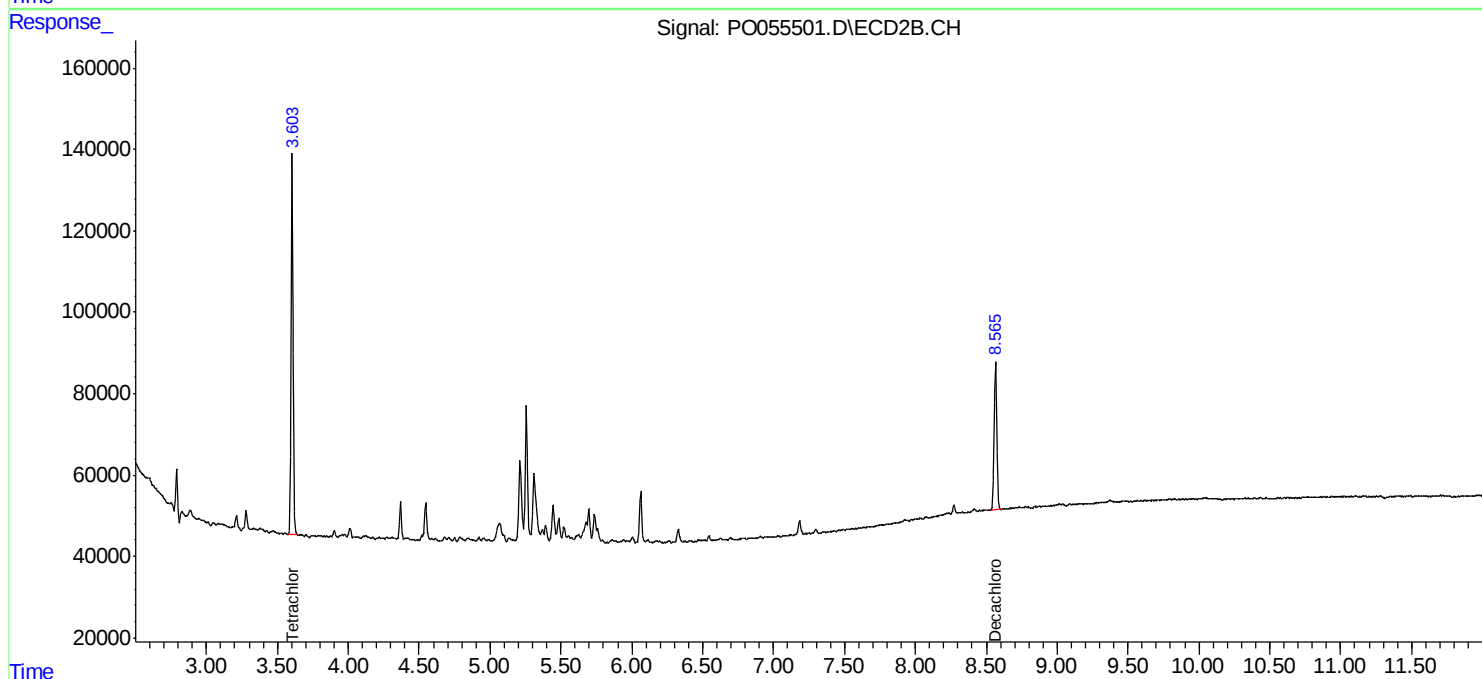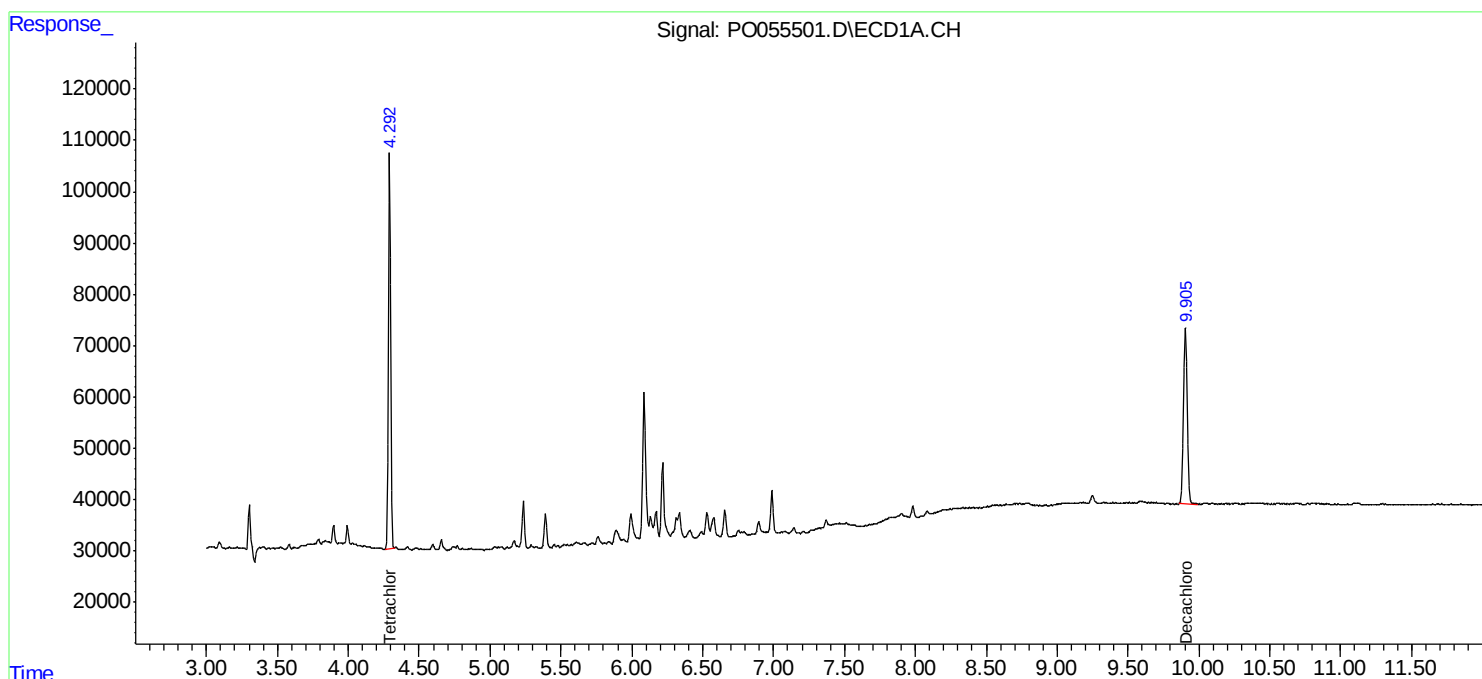

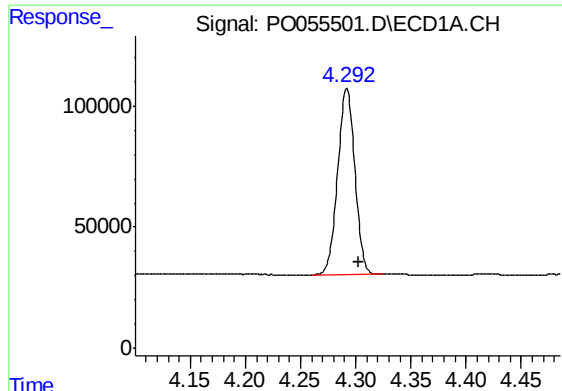


#1 Tetrachloro-m-xylene

R.T.: 4.292 min
Delta R.T.: -0.011 min
Response: 838402
Conc: 24.16 ng/ml

Instrument :
ECD_O
ClientSampleId :
AU-041819


Manual Integrations
APPROVED

Sohil
4/23/2019 12:06:14 PM

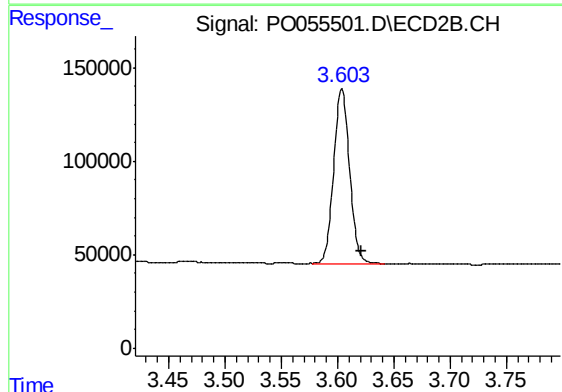


#1 Tetrachloro-m-xylene

R.T.: 3.603 min
Delta R.T.: -0.017 min
Response: 916902
Conc: 28.73 ng/ml m

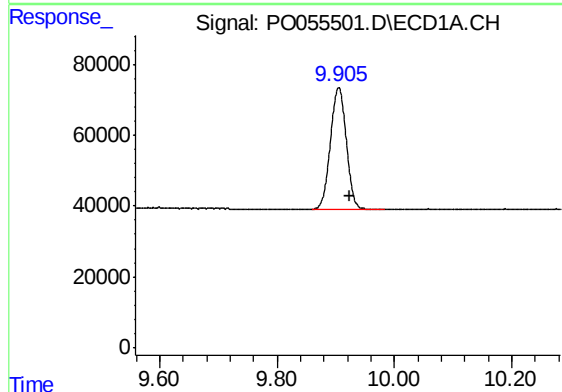

#2 Decachlorobiphenyl

R.T.: 9.905 min
Delta R.T.: -0.018 min
Response: 646481
Conc: 13.11 ng/ml

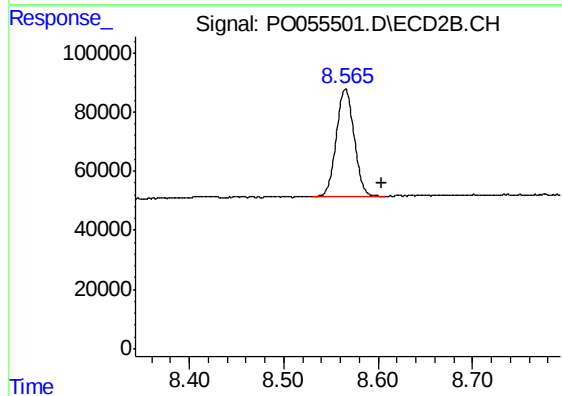

#2 Decachlorobiphenyl

R.T.: 8.565 min
Delta R.T.: -0.039 min
Response: 474766
Conc: 14.91 ng/ml