

Data Path : P:\HPCHEM1\ECD 0\Data\P0042018\
 Data File : P0044003.D
 Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
 Acq On : 20 Apr 2018 16:58
 Operator : SM/UA
 Sample : J2460-02
 Misc :
 ALS Vial : 7 Sample Multiplier: 1

Instrument :
 ECD_O
 ClientSampleId :
 MDP-B-1-18-20

Manual Integrations
 APPROVED

ugo
 4/23/2018 1:54:41 PM

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Apr 20 23:21:49 2018
 Quant Method : P:\HPCHEM1\ECD_0\methods\P0040418.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Wed Apr 04 15:17:57 2018
 Response via : Initial Calibration
 Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

ugo

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

4/23/2018 1:54:41 PM

Compound	RT#1	RT#2	Resp#1	Resp#2	nq/ml	nq/ml

System Monitoring Compounds						
1) SA Tetrachlo...	4.062	3.319	3175380	4703548	17.862	17.506
2) SA Decachlor...	9.411	8.074	1883798	2119184	10.453	9.039m

4/23/2018 1:54:41 PM

Target Compounds

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : P:\HPCHEM1\ECD 0\Data\P0042018\
Data File : P0044003.D
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
Acq On : 20 Apr 2018 16:58
Operator : SM/UA
Sample : J2460-02
Misc :
ALS Vial : 7 Sample Multiplier: 1

Instrument :
ECD_O
ClientSampled :
MDP-B-1-18-20



Manual Integrations
APPROVED


ugo
4/23/2018 1:54:41 PM

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Apr 20 23:21:49 2018
Quant Method : P:\HPCHEM1\ECD_0\methods\P0040418.M
Quant Title : GC EXTRACTABLES
QLast Update : Wed Apr 04 15:17:57 2018
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

4/23/2018 1:54:41 PM

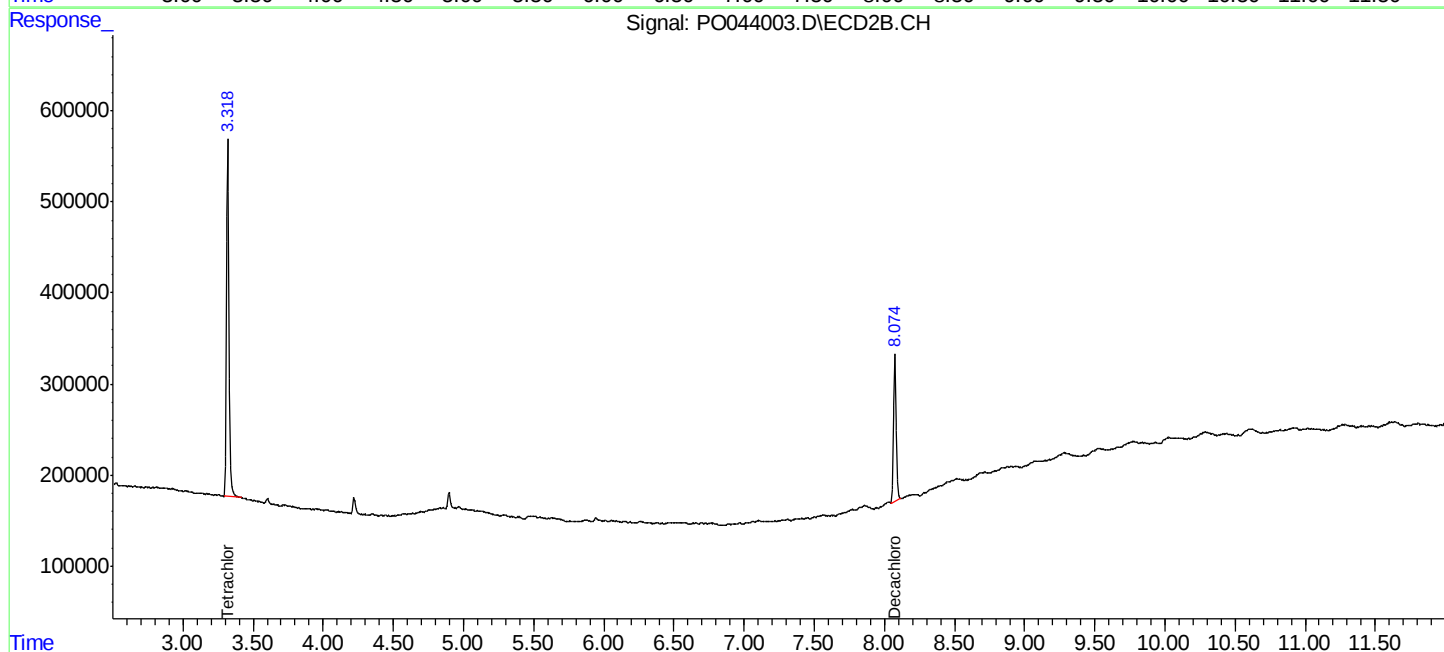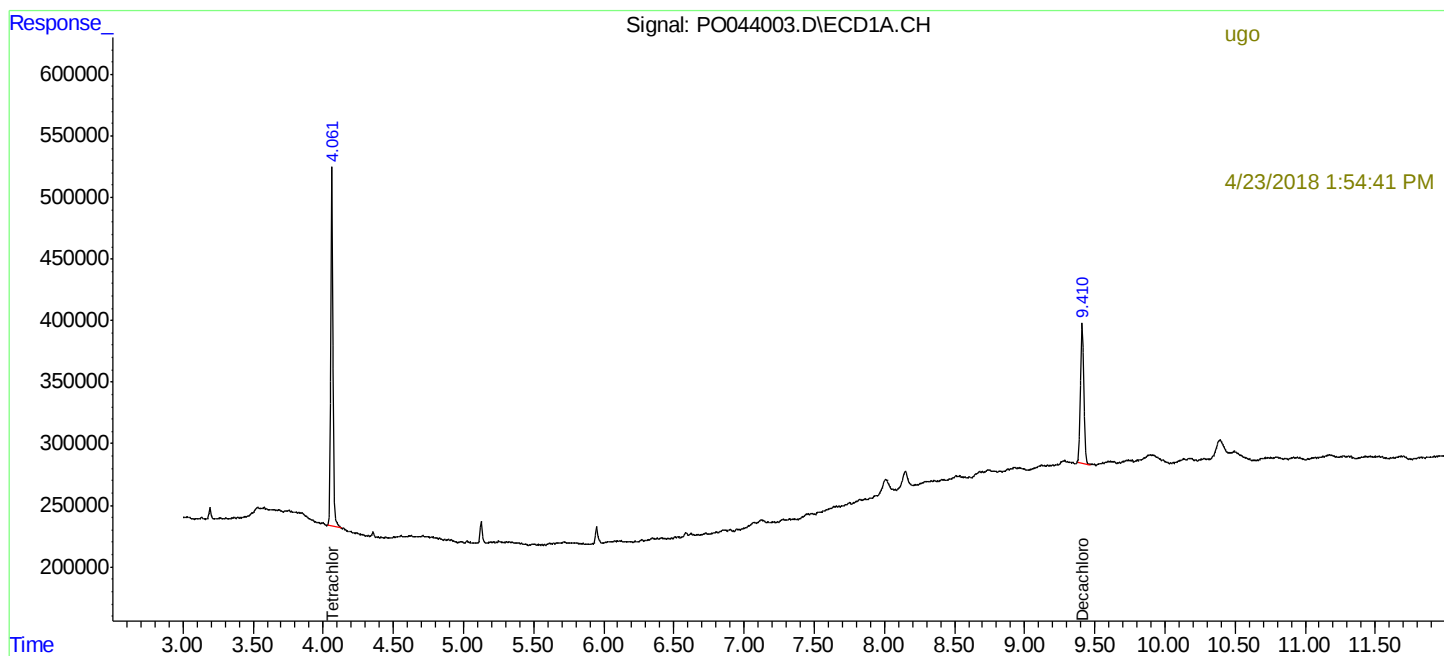

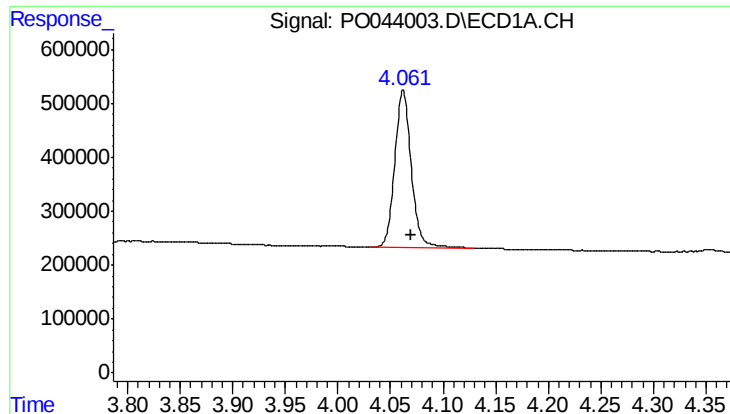


#1 Tetrachloro-m-xylene

R.T.: 4.062 min
Delta R.T.: -0.007 min
Response: 3175380
Conc: 17.86 ng/ml

Instrument :
ECD_O
ClientSampleId :
MDP-B-1-18-20

Manual Integrations
APPROVED

ugo
4/23/2018 1:54:41 PM

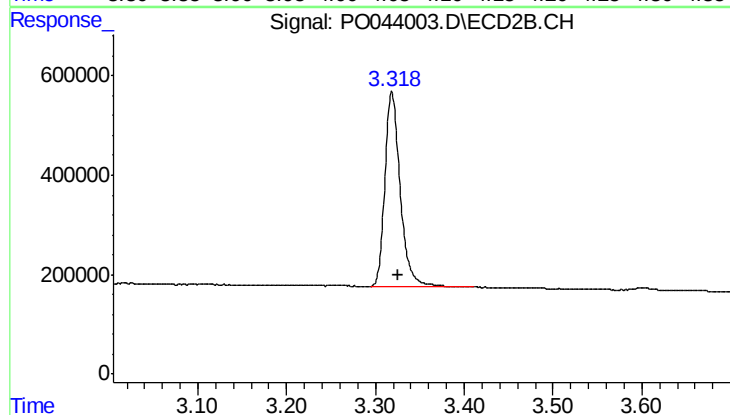


#1 Tetrachloro-m-xylene

R.T.: 3.319 min
Delta R.T.: -0.008 min
Response: 4703548
Conc: 17.51 ng/ml

ugo

4/23/2018 1:54:41 PM


ugo

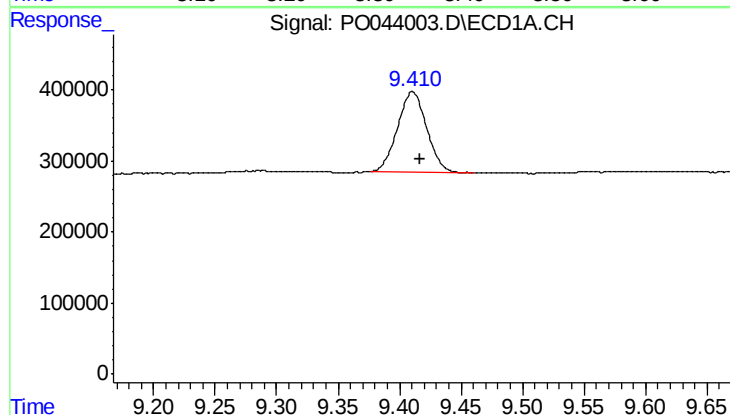

#2 Decachlorobiphenyl

R.T.: 9.411 min
Delta R.T.: -0.006 min
Response: 1883798
Conc: 10.45 ng/ml

4/23/2018 1:54:41 PM

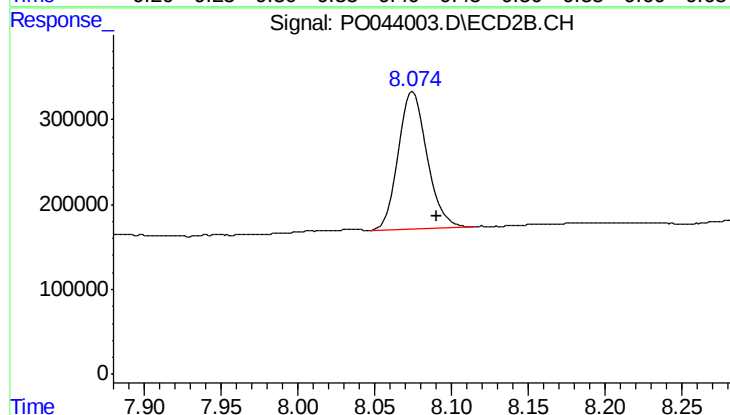

#2 Decachlorobiphenyl

R.T.: 8.074 min
Delta R.T.: -0.016 min
Response: 2119184
Conc: 9.04 ng/ml m