

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\P0042219\
 Data File : P0055505.D
 Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
 Acq On : 22 Apr 2019 12:24
 Operator : SM/SJ
 Sample : I.BLK
 Misc :
 ALS Vial : 2 Sample Multiplier: 1

Instrument :
 ECD_O
 ClientSampleId :
 I.BLK

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Apr 22 13:51:40 2019
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\P0032519.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Mon Mar 25 17:22:26 2019
 Response via : Initial Calibration
 Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	4.292	3.600	507228	489284	14.615	15.332
2) SA Decachlor...	9.901	8.562	655031	486264	13.287	15.268
Target Compounds						
28) L6 AR-1254-3	6.894	0.000	12721	0	4.045	N.D. #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\P0042219\
Data File : P0055505.D
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
Acq On : 22 Apr 2019 12:24
Operator : SM/SJ
Sample : I.BLK
Misc :
ALS Vial : 2 Sample Multiplier: 1

Instrument :
ECD_O
ClientSampleId :
I.BLK

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Apr 22 13:51:40 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\P0032519.M
Quant Title : GC EXTRACTABLES
QLast Update : Mon Mar 25 17:22:26 2019
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

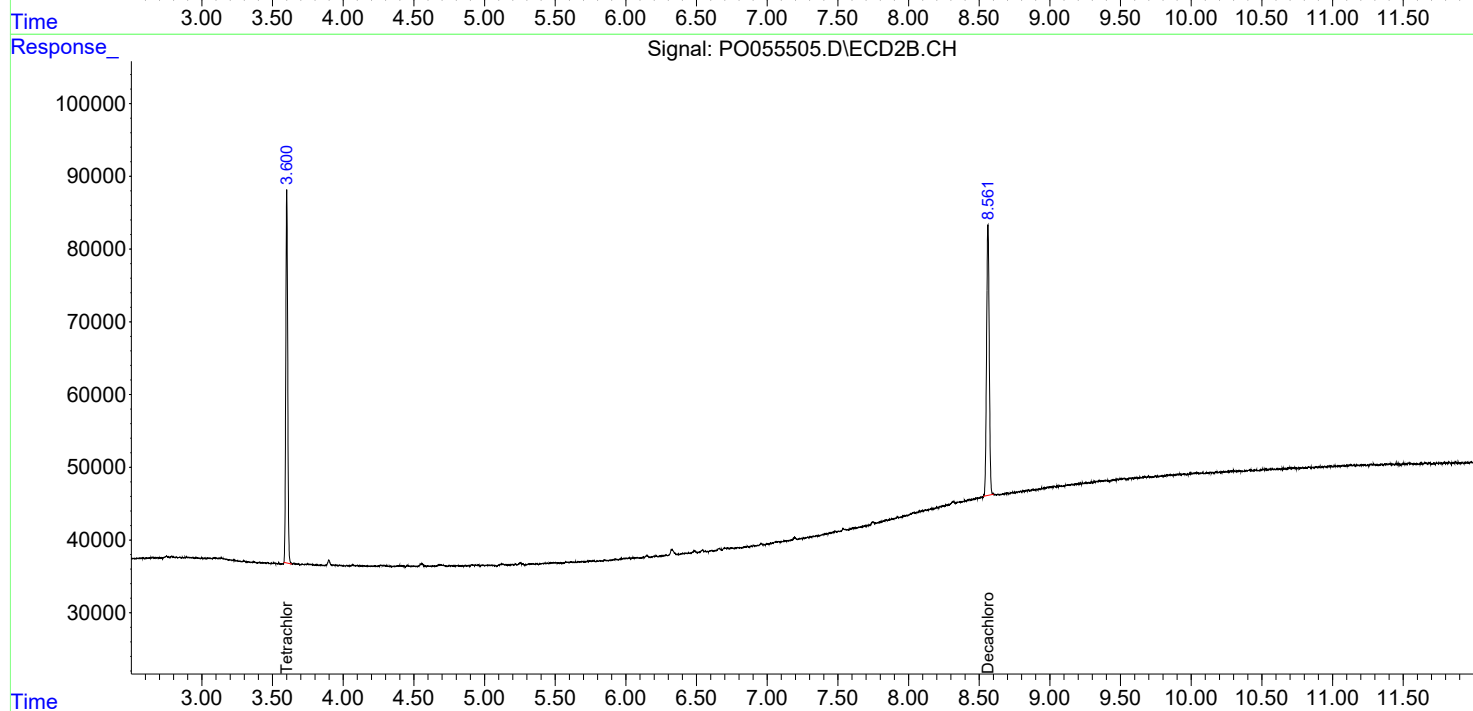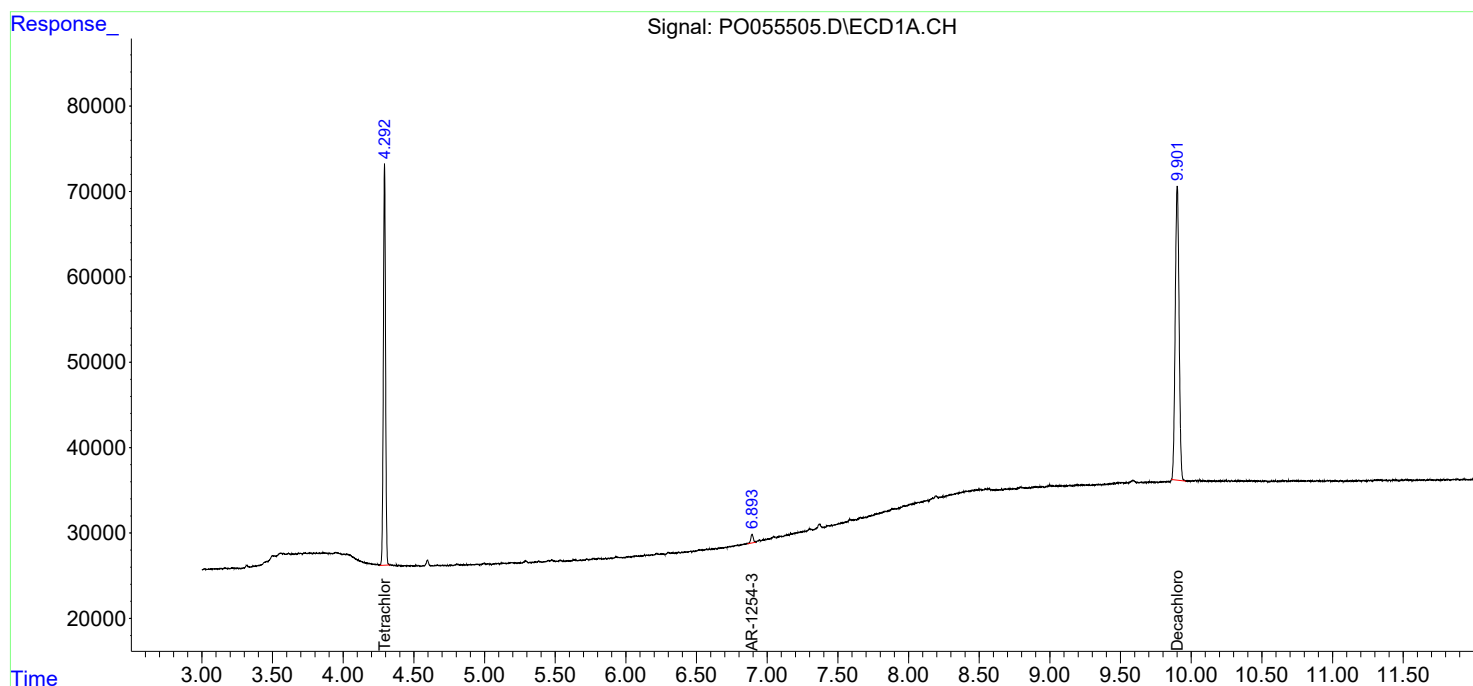


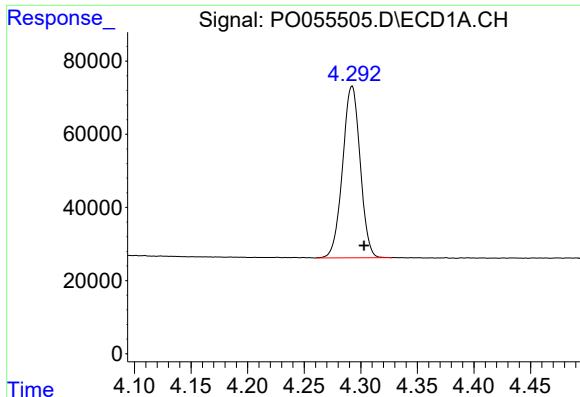

#1 Tetrachloro-m-xylene


R.T.: 4.292 min
Delta R.T.: -0.011 min
Response: 507228
Conc: 14.62 ng/ml

Instrument :
ECD_O
ClientSampleId :
I.BLK

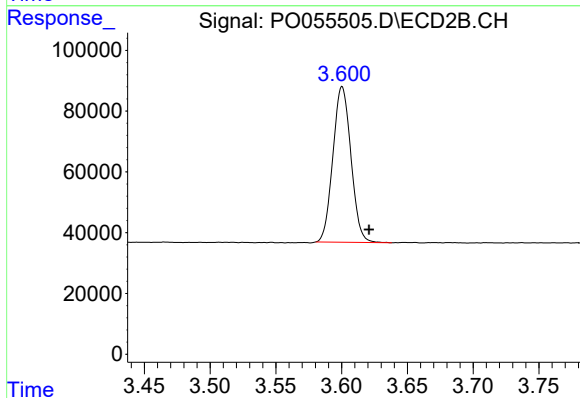


#1 Tetrachloro-m-xylene

R.T.: 3.600 min
Delta R.T.: -0.020 min
Response: 489284
Conc: 15.33 ng/ml

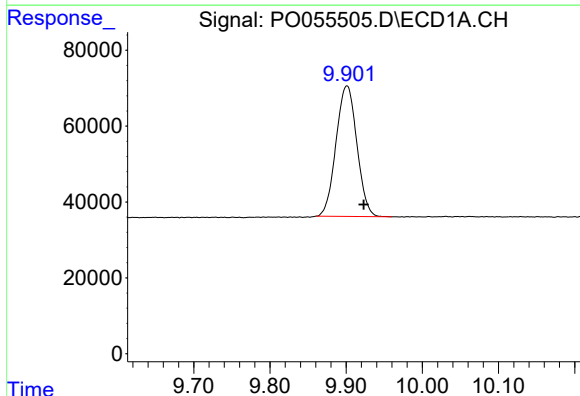


#2 Decachlorobiphenyl

R.T.: 9.901 min
Delta R.T.: -0.022 min
Response: 655031
Conc: 13.29 ng/ml

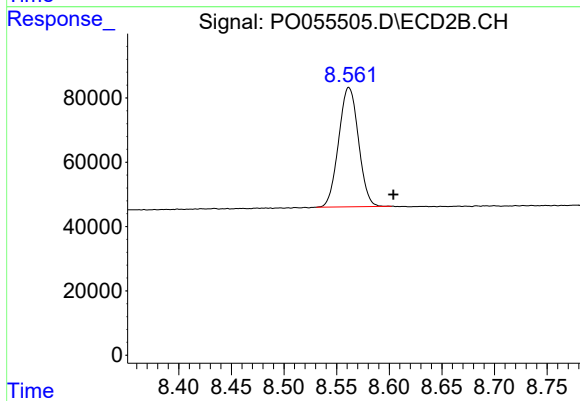

#2 Decachlorobiphenyl


R.T.: 8.562 min
Delta R.T.: -0.043 min
Response: 486264
Conc: 15.27 ng/ml

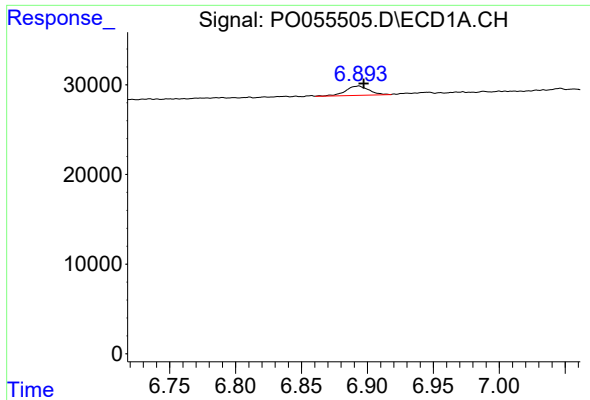

#28 AR-1254-3

R.T.: 6.894 min
Delta R.T.: -0.004 min
Response: 12721
Conc: 4.05 ng/ml

Instrument :
ECD_O
ClientSampleId :
I.BLK

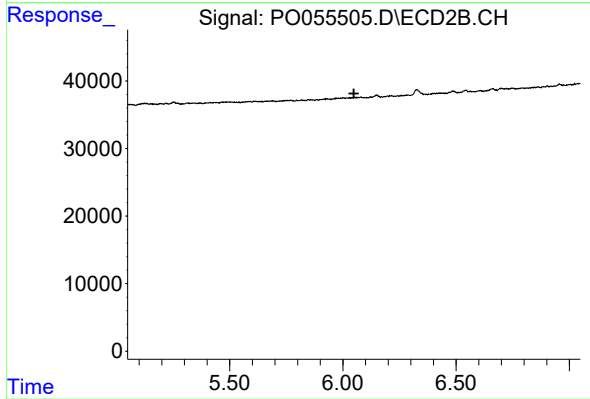

#28 AR-1254-3

R.T.: 0.000 min
Exp R.T. : 6.049 min
Response: 0
Conc: N.D.