

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\P0042219\
Data File : P0055508.D
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
Acq On : 22 Apr 2019 13:43
Operator : SM/SJ
Sample : K2442-07
Misc :
ALS Vial : 5 Sample Multiplier: 1

Instrument :
ECD_O
ClientSampleId :
TP-20-S

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Apr 22 14:03:45 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\P0032519.M
Quant Title : GC EXTRACTABLES
QLast Update : Mon Mar 25 17:22:26 2019
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	4.289	3.600	771288	765365	22.224	23.983
2)	SA Decachlor...	9.899	8.561	761614	558977	15.449	17.551

Target Compounds



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\P0042219\
Data File : P0055508.D
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
Acq On : 22 Apr 2019 13:43
Operator : SM/SJ
Sample : K2442-07
Misc :
ALS Vial : 5 Sample Multiplier: 1

Instrument :
ECD_O
ClientSampleId :
TP-20-S

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Apr 22 14:03:45 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\P0032519.M
Quant Title : GC EXTRACTABLES
QLast Update : Mon Mar 25 17:22:26 2019
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

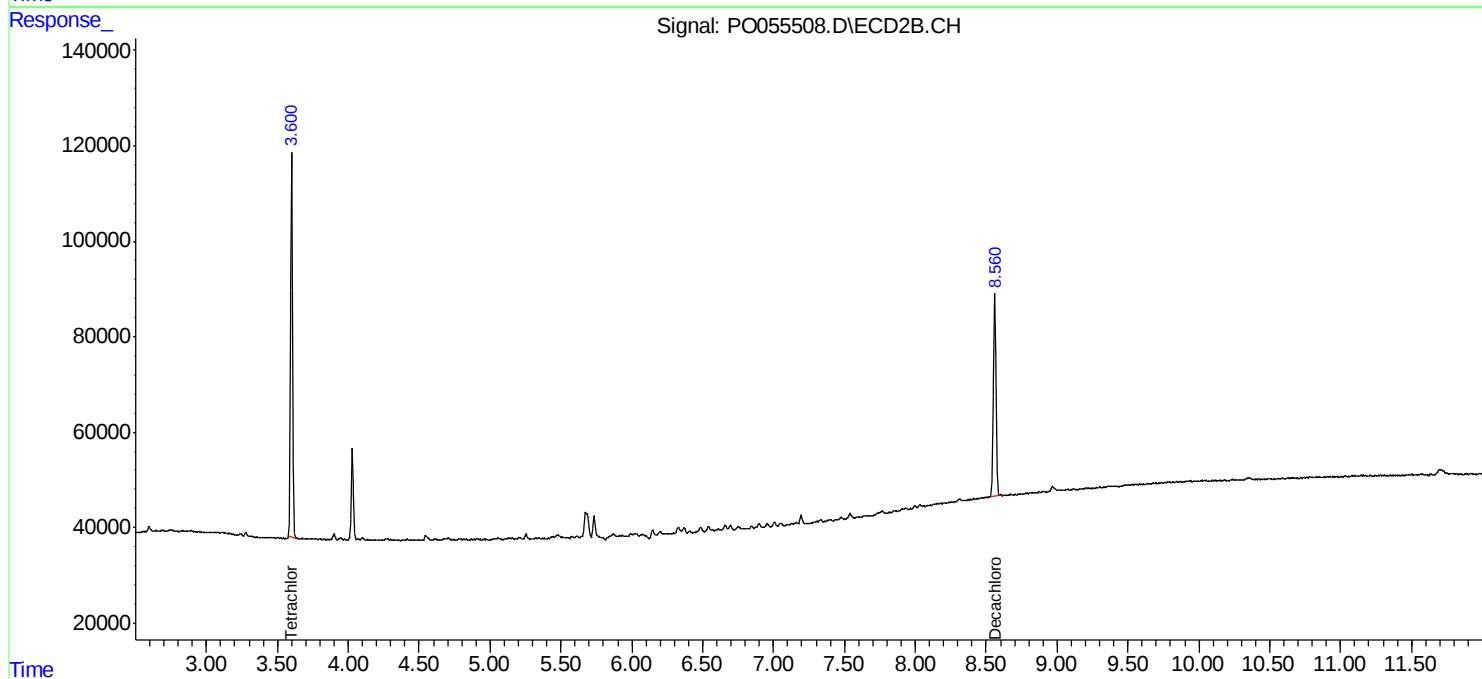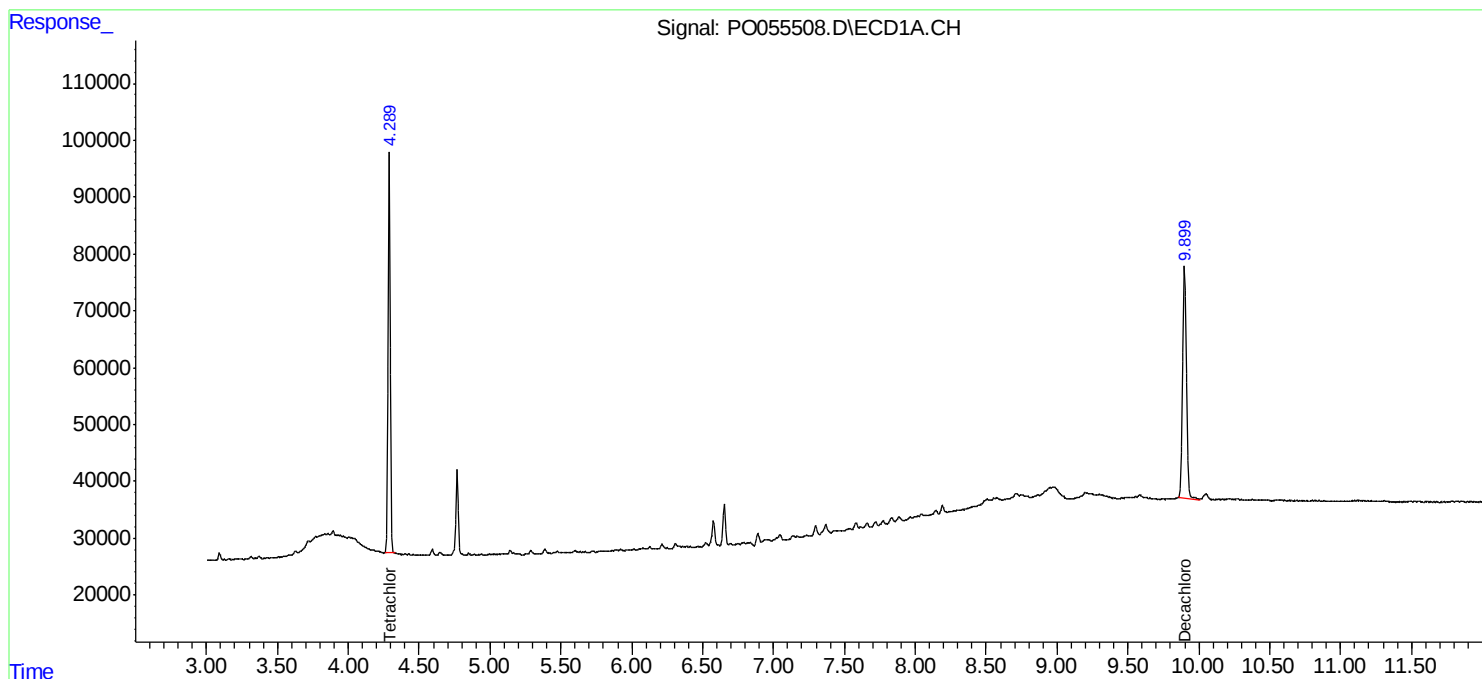


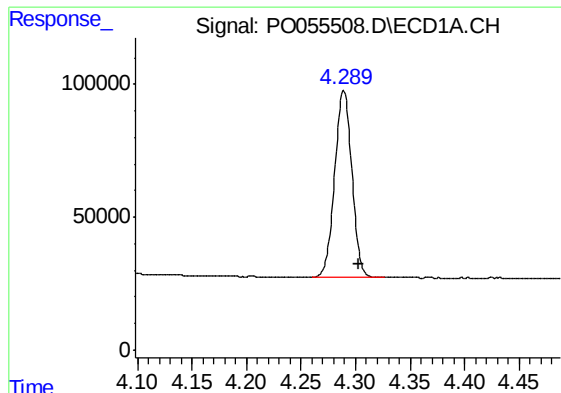

#1 Tetrachloro-m-xylene


R.T.: 4.289 min
Delta R.T.: -0.014 min
Response: 771288
Conc: 22.22 ng/ml

Instrument :
ECD_O
ClientSampleId :
TP-20-S

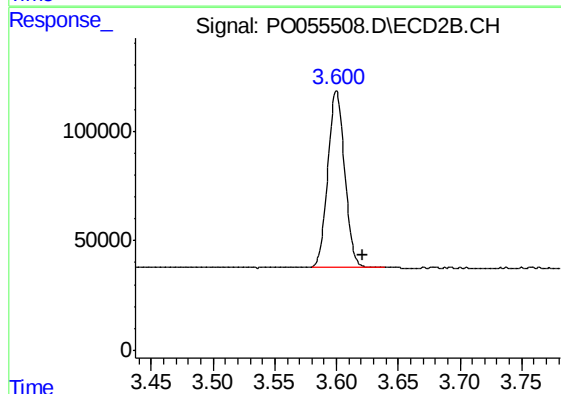


#1 Tetrachloro-m-xylene

R.T.: 3.600 min
Delta R.T.: -0.021 min
Response: 765365
Conc: 23.98 ng/ml

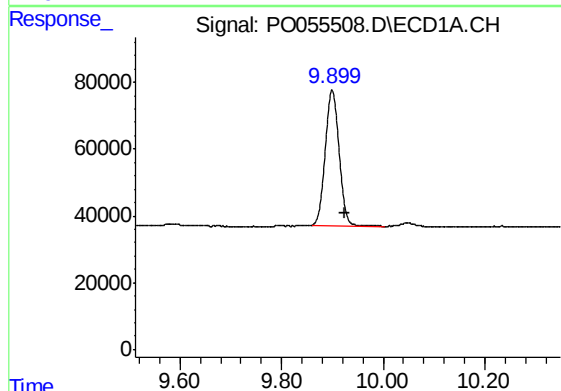

#2 Decachlorobiphenyl

R.T.: 9.899 min
Delta R.T.: -0.024 min
Response: 761614
Conc: 15.45 ng/ml

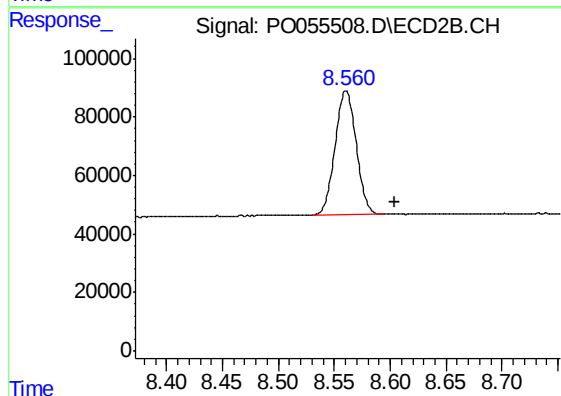

#2 Decachlorobiphenyl

R.T.: 8.561 min
Delta R.T.: -0.044 min
Response: 558977
Conc: 17.55 ng/ml