

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\P0042220\
 Data File : P0067985.D
 Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
 Acq On : 22 Apr 2020 15:19
 Operator : DD\AJ
 Sample : L2350-07
 Misc :
 ALS Vial : 25 Sample Multiplier: 1

Instrument :
 ECD_O
 ClientSampleId :
 TP-5-S

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Apr 22 16:09:07 2020
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\P0040120.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Fri Apr 03 16:04:09 2020
 Response via : Initial Calibration
 Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	4.918	3.936	479872	790150	20.151	23.575
2)	SA Decachlor...	10.891	9.217	690183	787591	20.273	19.049
Target Compounds							
27)	L6 AR-1254-2	7.436	6.269	20686	48688	10.518	21.348 #
34)	L7 AR-1260-4	0.000	7.608	0	14036	N.D.	6.678 #
38)	L8 AR-1262-3	9.407	8.142	28551	67637	13.721	34.413 #
39)	L8 AR-1262-4	9.501	8.206	27131	52275	17.146	15.250
41)	L9 AR-1268-1	9.407	8.142	28551	67637	7.727	12.570 #
42)	L9 AR-1268-2	9.501	8.206	27131	52275	7.828	10.587 #
43)	L9 AR-1268-3	0.000	8.414	0	33899	N.D.	8.088 #
45)	L9 AR-1268-5	10.561	8.977	65530	64698	6.609	5.017



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\P0042220\
Data File : P0067985.D
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
Acq On : 22 Apr 2020 15:19
Operator : DD\AJ
Sample : L2350-07
Misc :
ALS Vial : 25 Sample Multiplier: 1

Instrument :
ECD_O
ClientSampled :
TP-5-S

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Apr 22 16:09:07 2020
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\P0040120.M
Quant Title : GC EXTRACTABLES
QLast Update : Fri Apr 03 16:04:09 2020
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

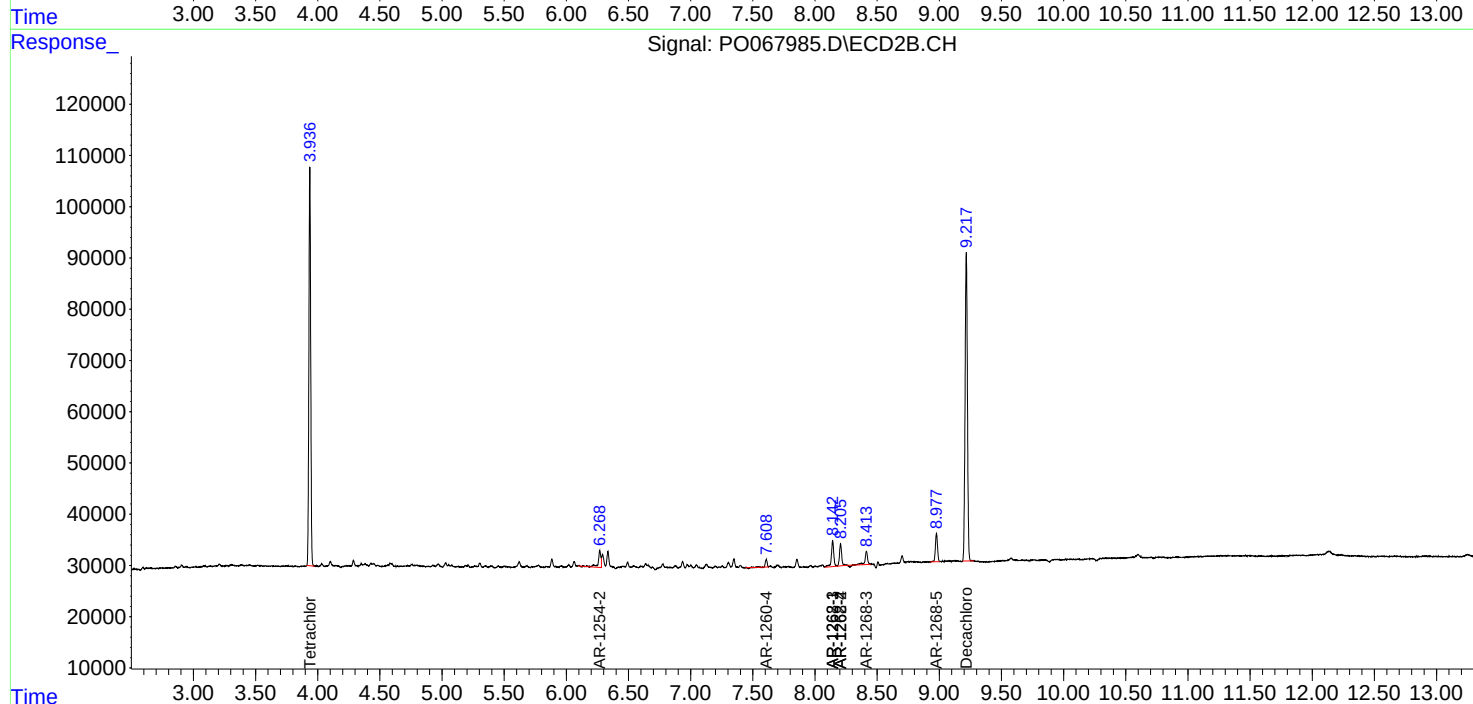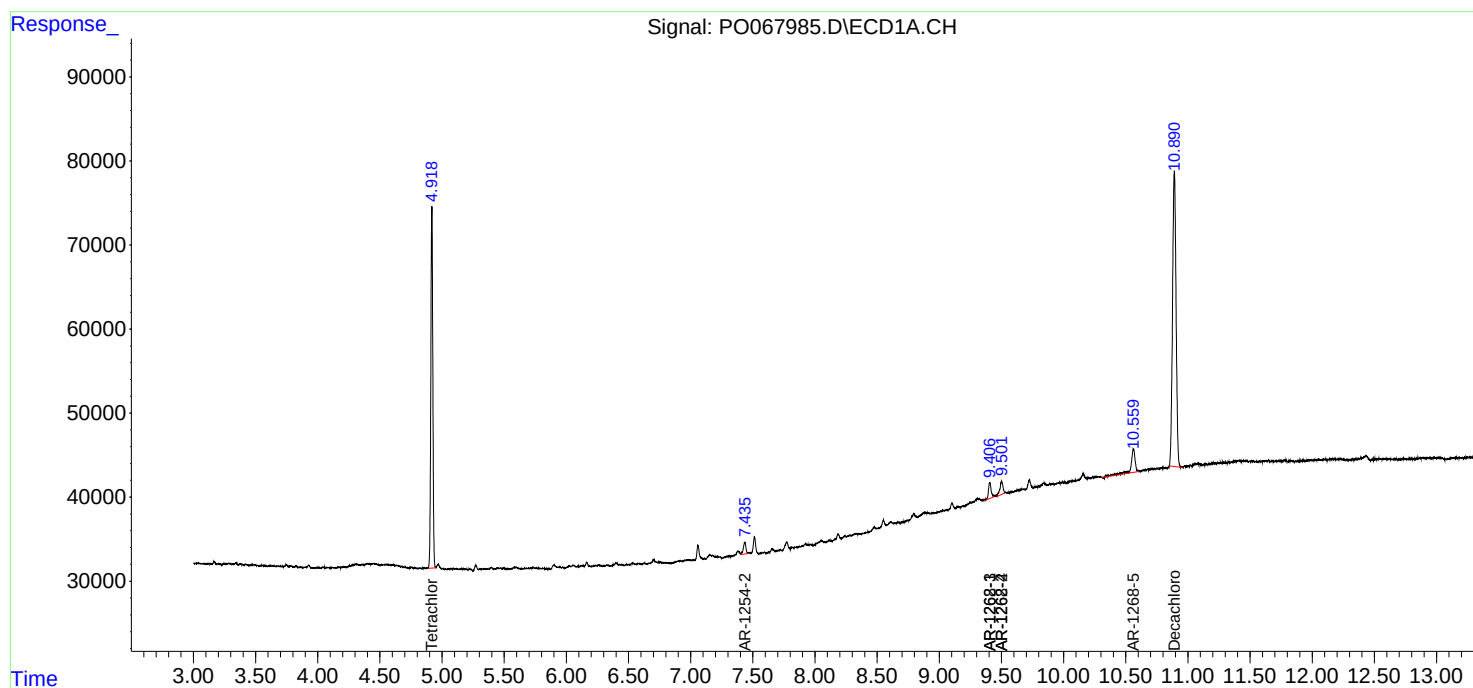


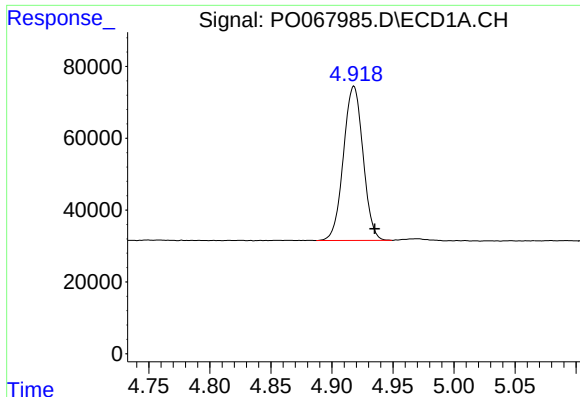

#1 Tetrachloro-m-xylene


R.T.: 4.918 min
Delta R.T.: -0.017 min
Response: 479872
Conc: 20.15 ng/ml

Instrument :
ECD_O
ClientSampleId :
TP-5-S

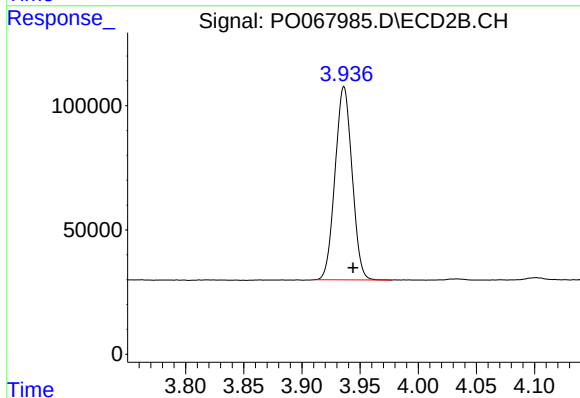


#1 Tetrachloro-m-xylene

R.T.: 3.936 min
Delta R.T.: -0.008 min
Response: 790150
Conc: 23.57 ng/ml

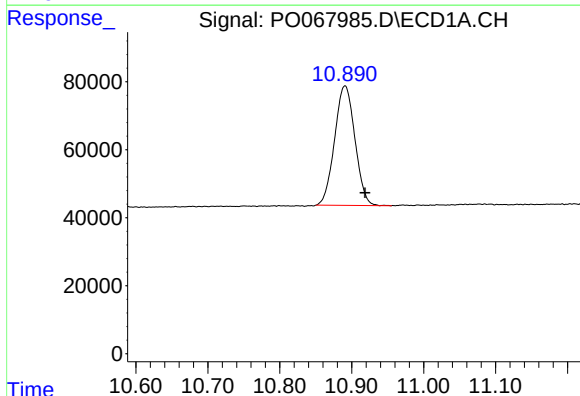


#2 Decachlorobiphenyl

R.T.: 10.891 min
Delta R.T.: -0.028 min
Response: 690183
Conc: 20.27 ng/ml

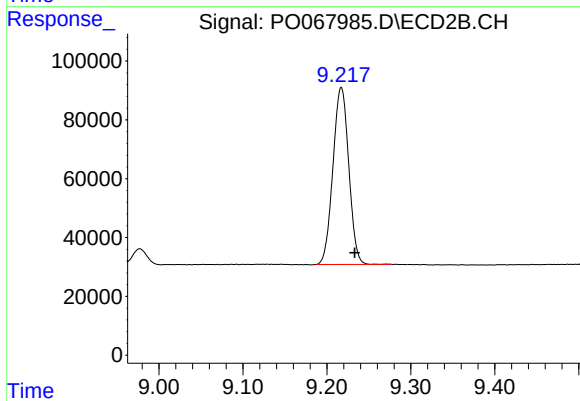

#2 Decachlorobiphenyl


R.T.: 9.217 min
Delta R.T.: -0.016 min
Response: 787591
Conc: 19.05 ng/ml

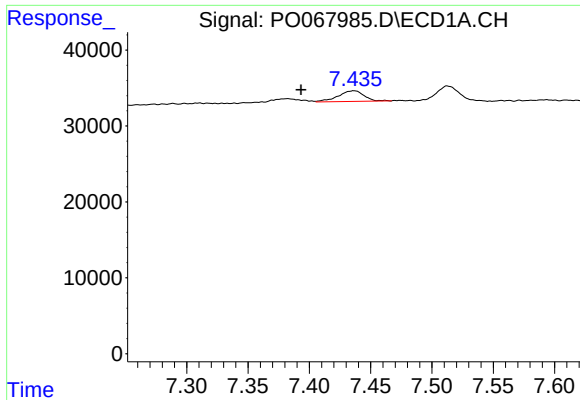

#27 AR-1254-2


R.T.: 7.436 min
Delta R.T.: 0.043 min
Response: 20686
Conc: 10.52 ng/ml

Instrument :
ECD_O
ClientSampleId :
TP-5-S

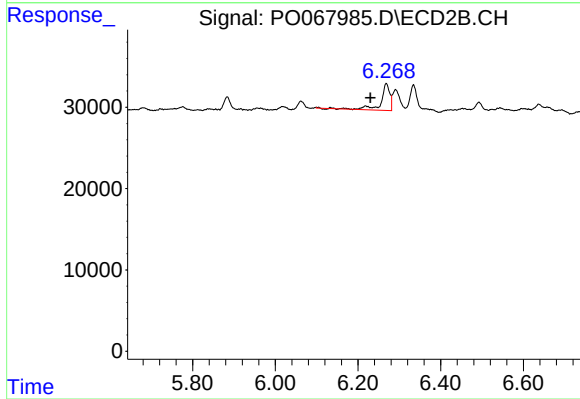


#27 AR-1254-2

R.T.: 6.269 min
Delta R.T.: 0.038 min
Response: 48688
Conc: 21.35 ng/ml

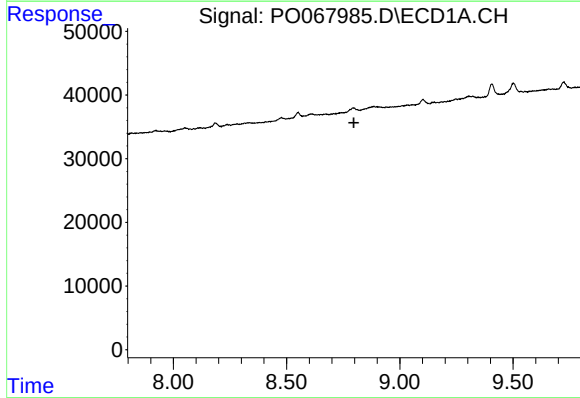


#34 AR-1260-4

R.T.: 0.000 min
Exp R.T. : 8.797 min
Response: 0
Conc: N.D.

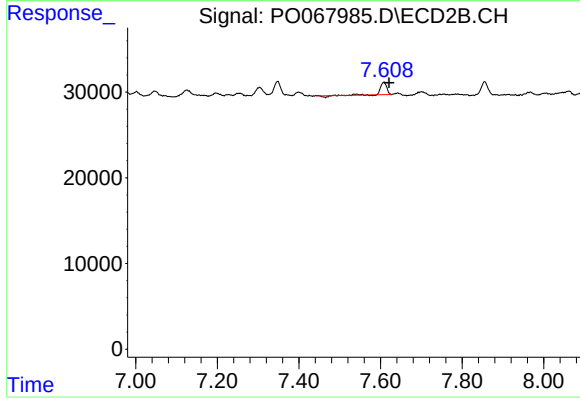

#34 AR-1260-4


R.T.: 7.608 min
Delta R.T.: -0.013 min
Response: 14036
Conc: 6.68 ng/ml

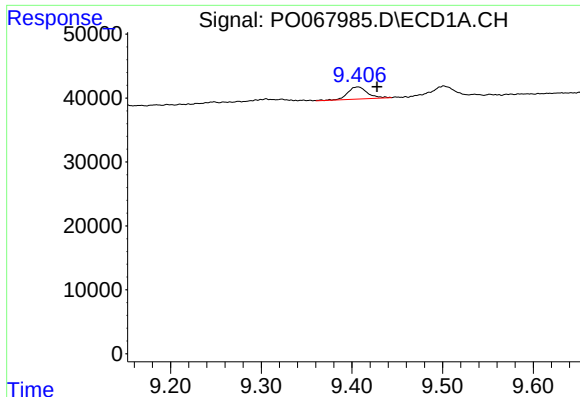

#38 AR-1262-3


R.T.: 9.407 min
Delta R.T.: -0.021 min
Response: 28551
Conc: 13.72 ng/ml

Instrument :
ECD_O
ClientSampleId :
TP-5-S

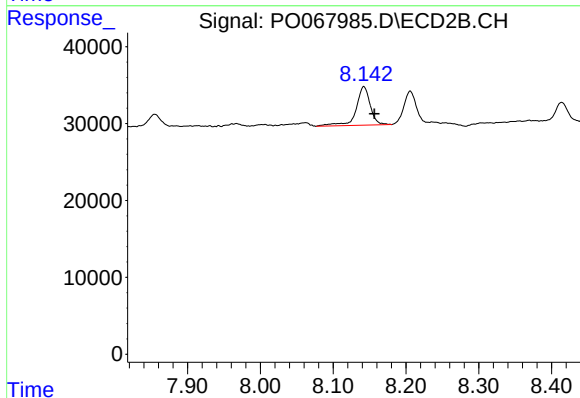


#38 AR-1262-3

R.T.: 8.142 min
Delta R.T.: -0.015 min
Response: 67637
Conc: 34.41 ng/ml

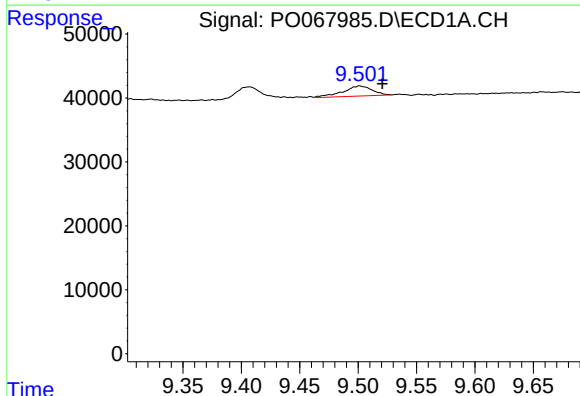


#39 AR-1262-4

R.T.: 9.501 min
Delta R.T.: -0.019 min
Response: 27131
Conc: 17.15 ng/ml

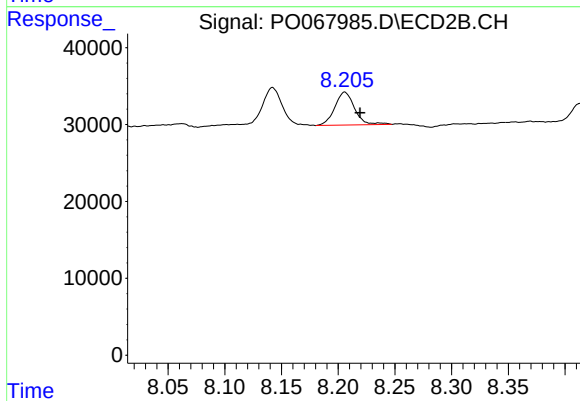

#39 AR-1262-4


R.T.: 8.206 min
Delta R.T.: -0.013 min
Response: 52275
Conc: 15.25 ng/ml

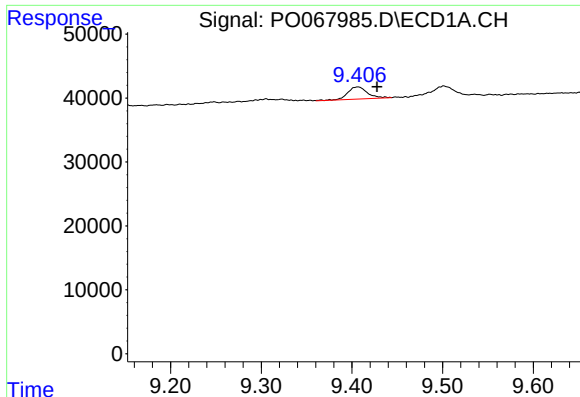

#41 AR-1268-1


R.T.: 9.407 min
Delta R.T.: -0.021 min
Response: 28551
Conc: 7.73 ng/ml

Instrument :
ECD_O
ClientSampleId :
TP-5-S

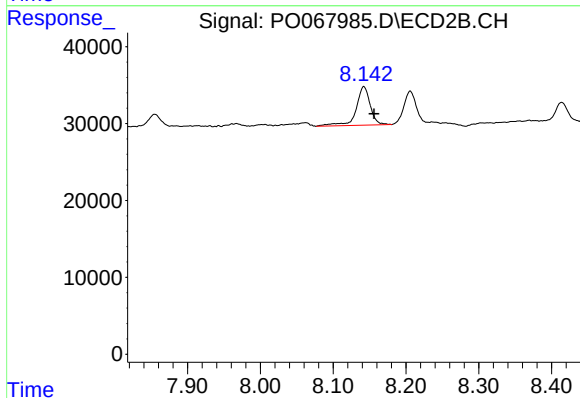


#41 AR-1268-1

R.T.: 8.142 min
Delta R.T.: -0.014 min
Response: 67637
Conc: 12.57 ng/ml

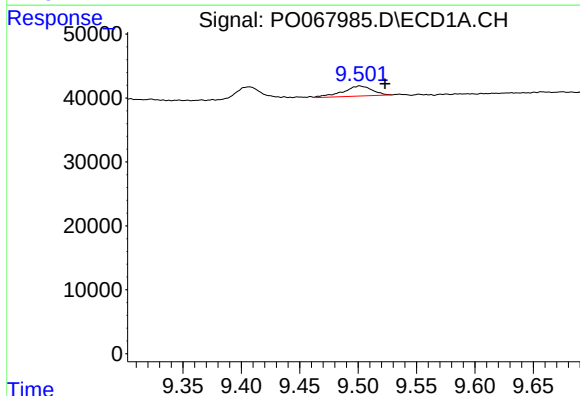


#42 AR-1268-2

R.T.: 9.501 min
Delta R.T.: -0.022 min
Response: 27131
Conc: 7.83 ng/ml

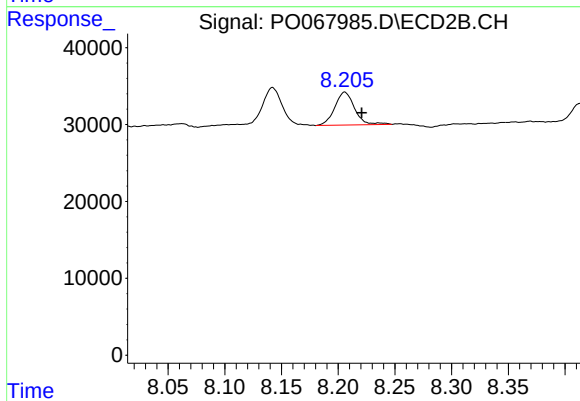

#42 AR-1268-2


R.T.: 8.206 min
Delta R.T.: -0.015 min
Response: 52275
Conc: 10.59 ng/ml

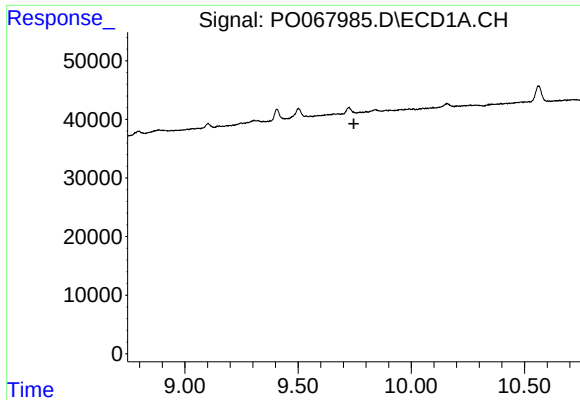

#43 AR-1268-3


R.T.: 0.000 min
Exp R.T.: 9.746 min
Response: 0
Conc: N.D.

Instrument :
ECD_O
ClientSampleId :
TP-5-S

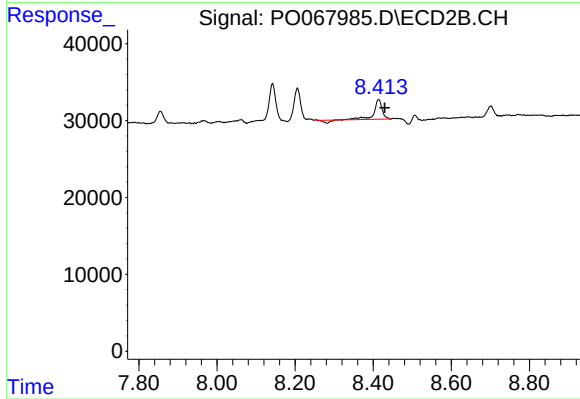


#43 AR-1268-3

R.T.: 8.414 min
Delta R.T.: -0.016 min
Response: 33899
Conc: 8.09 ng/ml

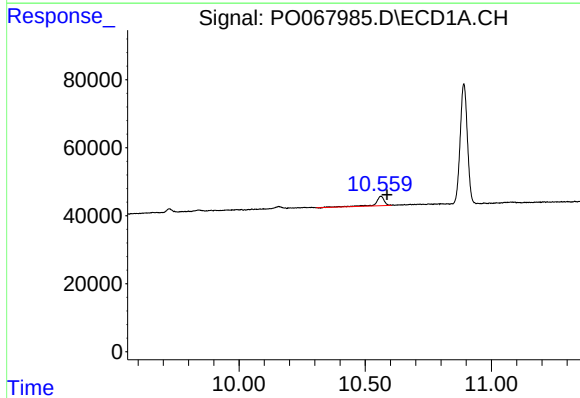

#45 AR-1268-5

R.T.: 10.561 min
Delta R.T.: -0.026 min
Response: 65530
Conc: 6.61 ng/ml

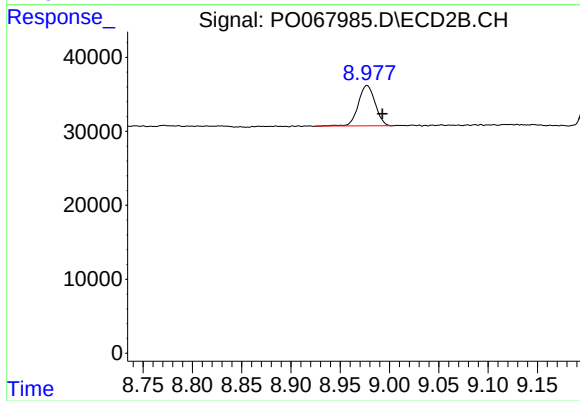

#45 AR-1268-5

R.T.: 8.977 min
Delta R.T.: -0.016 min
Response: 64698
Conc: 5.02 ng/ml