

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\P0042220\
Data File : P0067969.D
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
Acq On : 22 Apr 2020 10:27
Operator : DD\AJ
Sample : L2327-33
Misc :
ALS Vial : 11 Sample Multiplier: 1

Instrument :
ECD_O
ClientSampleId :
TP-6-S

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Apr 22 10:42:09 2020
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\P0040120.M
Quant Title : GC EXTRACTABLES
QLast Update : Fri Apr 03 16:04:09 2020
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	4.919	3.937	504031	804443	21.165	24.001
2) SA Decachlor...	10.891	9.218	714486	794423	20.987	19.214

Target Compounds



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\P0042220\
Data File : P0067969.D
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
Acq On : 22 Apr 2020 10:27
Operator : DD\AJ
Sample : L2327-33
Misc :
ALS Vial : 11 Sample Multiplier: 1

Instrument :
ECD_O
ClientSampleId :
TP-6-S

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Apr 22 10:42:09 2020
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\P0040120.M
Quant Title : GC EXTRACTABLES
QLast Update : Fri Apr 03 16:04:09 2020
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

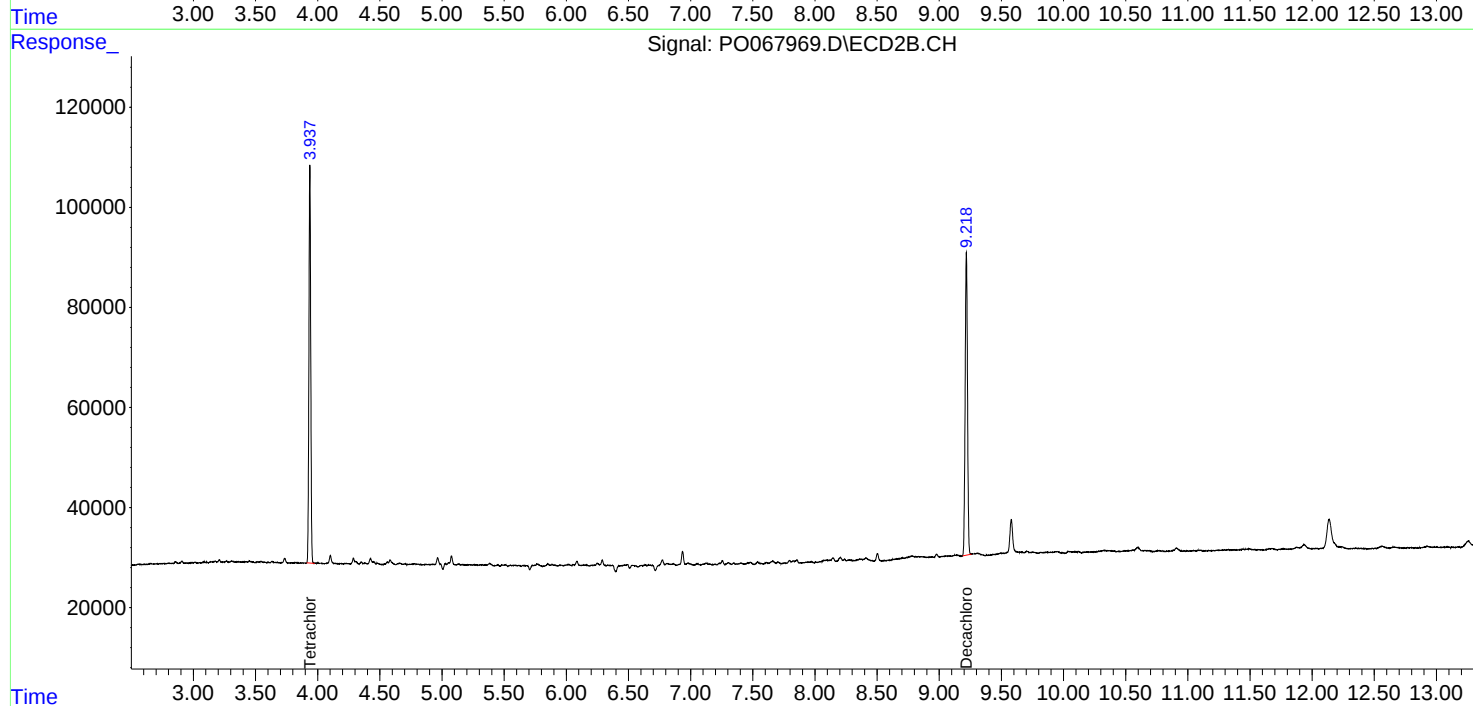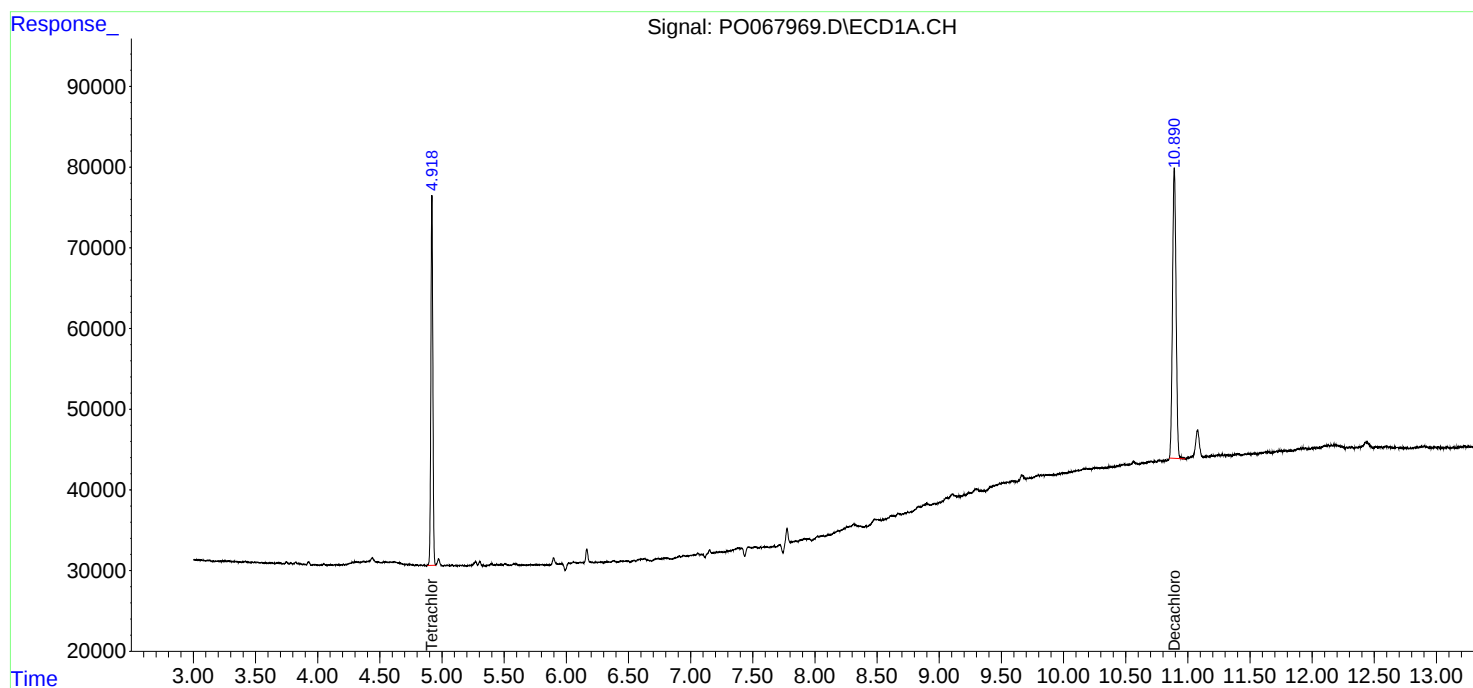


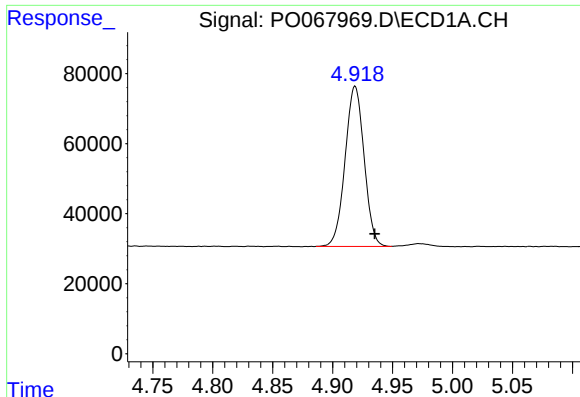

#1 Tetrachloro-m-xylene


R.T.: 4.919 min
Delta R.T.: -0.016 min
Response: 504031
Conc: 21.17 ng/ml

Instrument :
ECD_O
ClientSampleId :
TP-6-S

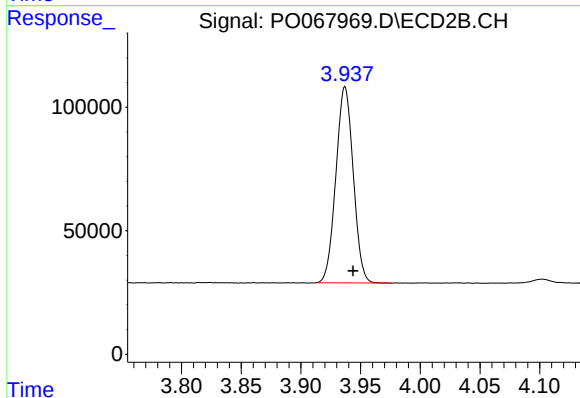


#1 Tetrachloro-m-xylene

R.T.: 3.937 min
Delta R.T.: -0.007 min
Response: 804443
Conc: 24.00 ng/ml

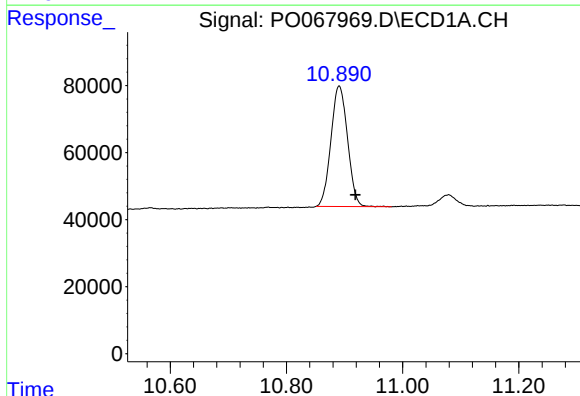

#2 Decachlorobiphenyl

R.T.: 10.891 min
Delta R.T.: -0.028 min
Response: 714486
Conc: 20.99 ng/ml

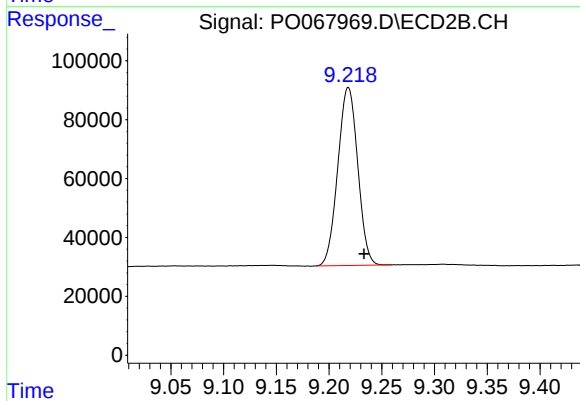

#2 Decachlorobiphenyl

R.T.: 9.218 min
Delta R.T.: -0.015 min
Response: 794423
Conc: 19.21 ng/ml