

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\P0042220\
 Data File : P0067985.D
 Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
 Acq On : 22 Apr 2020 15:19
 Operator : DD\AJ
 Sample : L2350-07
 Misc :
 ALS Vial : 25 Sample Multiplier: 1

Instrument :
 ECD_O
 ClientSampleId :
 TP-5-S

Manual Integrations
 APPROVED

Sohil
 4/23/2020 9:52:00 AM

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Apr 22 16:09:07 2020
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\P0040120.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Fri Apr 03 16:04:09 2020
 Response via : Initial Calibration
 Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	4.918	3.936	479872	790150	20.151	23.575
2) SA Decachlor...	10.890	9.217	697066	787591	20.476m	19.049

Target Compounds

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\P0042220\
Data File : P0067985.D
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
Acq On : 22 Apr 2020 15:19
Operator : DD\AJ
Sample : L2350-07
Misc :
ALS Vial : 25 Sample Multiplier: 1



Instrument :
ECD_O
ClientSampleId :
TP-5-S


Manual Integrations
APPROVED

Sohil
4/23/2020 9:52:00 AM

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Apr 22 16:09:07 2020
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\P0040120.M
Quant Title : GC EXTRACTABLES
QLast Update : Fri Apr 03 16:04:09 2020
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

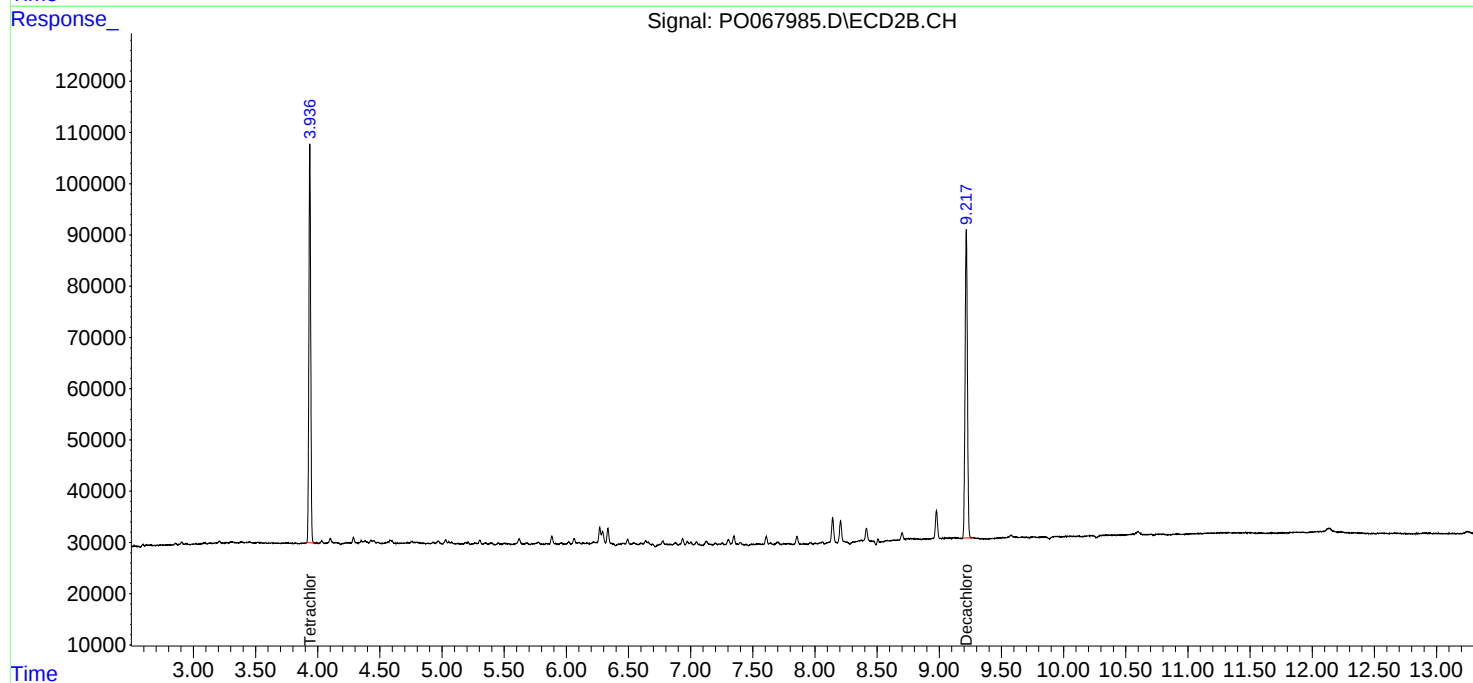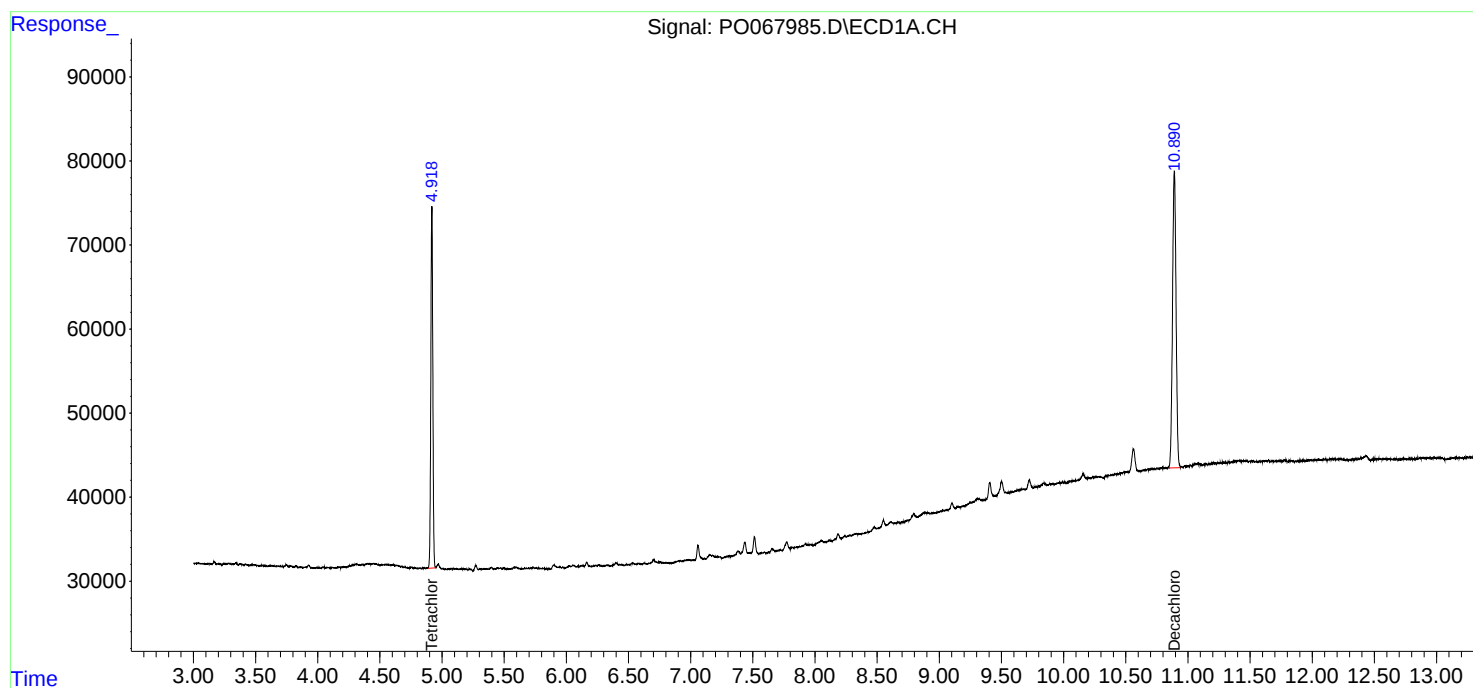

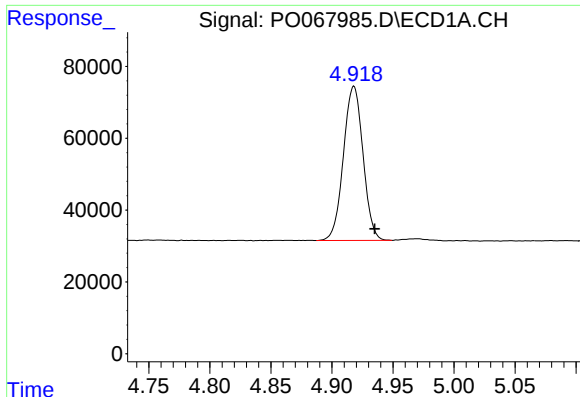


#1 Tetrachloro-m-xylene

R.T.: 4.918 min
Delta R.T.: -0.017 min
Response: 479872
Conc: 20.15 ng/ml

Instrument :
ECD_O
ClientSampleId :
TP-5-S


Manual Integrations
APPROVED

Sohil
4/23/2020 9:52:00 AM

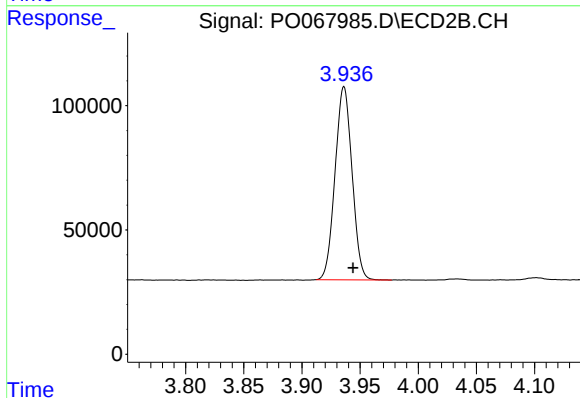


#1 Tetrachloro-m-xylene

R.T.: 3.936 min
Delta R.T.: -0.008 min
Response: 790150
Conc: 23.57 ng/ml

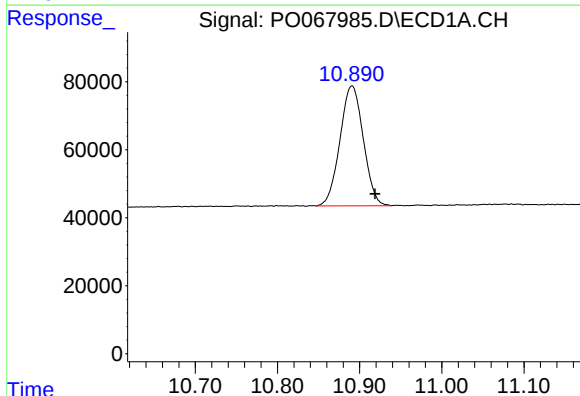

#2 Decachlorobiphenyl

R.T.: 10.890 min
Delta R.T.: -0.028 min
Response: 697066
Conc: 20.48 ng/ml m

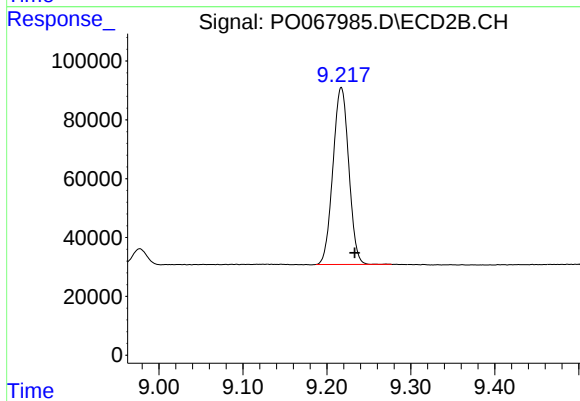

#2 Decachlorobiphenyl

R.T.: 9.217 min
Delta R.T.: -0.016 min
Response: 787591
Conc: 19.05 ng/ml