

Data Path : P:\HPCHEM1\ECD 0\Data\P0042318\
 Data File : P0044028.D
 Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
 Acq On : 23 Apr 2018 11:54
 Operator : SM/UA
 Sample : J2490-01
 Misc :
 ALS Vial : 12 Sample Multiplier: 1

Instrument :
 ECD_O
 ClientSampleId :
 MDP-B-3-0-6

Manual Integrations
 APPROVED

ugo
 4/24/2018 3:35:06 PM

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Apr 24 01:31:43 2018
 Quant Method : P:\HPCHEM1\ECD_0\methods\P0040418.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Wed Apr 04 15:17:57 2018
 Response via : Initial Calibration
 Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	4.062	3.319	4635732	6270380	26.076	23.337
2) SA Decachlor...	9.411	8.072	3964644	2758852	22.000m	11.768m#

Target Compounds

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : P:\HPCHEM1\ECD 0\Data\PO042318\
Data File : PO044028.D
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
Acq On : 23 Apr 2018 11:54
Operator : SM/UA
Sample : J2490-01
Misc :
ALS Vial : 12 Sample Multiplier: 1



Instrument :
ECD_O
ClientSampleId :
MDP-B-3-0-6


Manual Integrations
APPROVED

ugo
4/24/2018 3:35:06 PM

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Apr 24 01:31:43 2018
Quant Method : P:\HPCHEM1\ECD_0\methods\PO040418.M
Quant Title : GC EXTRACTABLES
QLast Update : Wed Apr 04 15:17:57 2018
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Ini. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

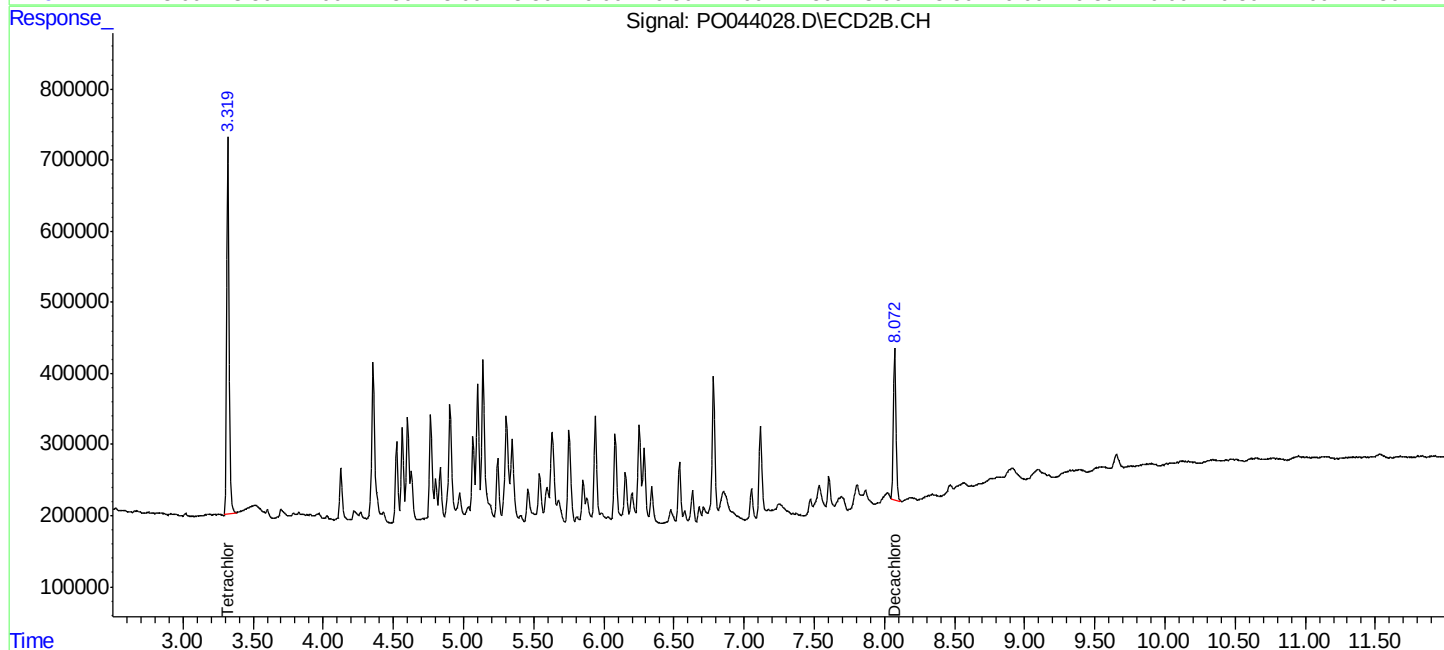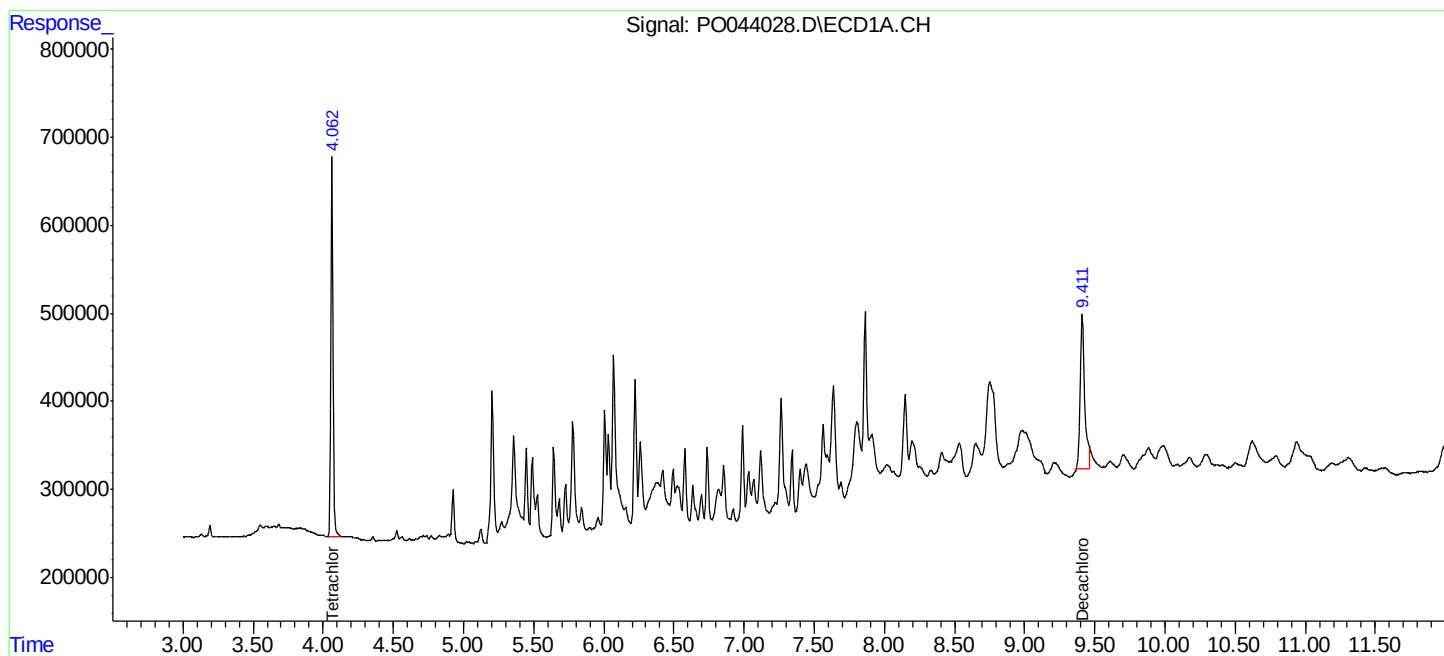

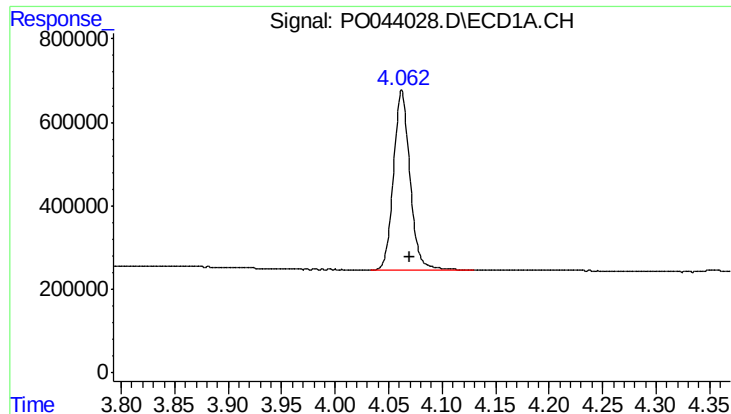


#1 Tetrachloro-m-xylene

R.T.: 4.062 min
Delta R.T.: -0.007 min
Response: 4635732
Conc: 26.08 ng/ml

Instrument :
ECD_O
ClientSampleId :
MDP-B-3-0-6


Manual Integrations
APPROVED

ugo
4/24/2018 3:35:06 PM

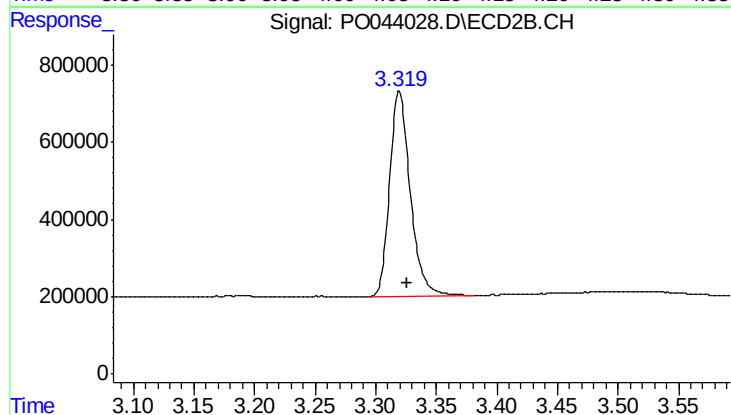


#1 Tetrachloro-m-xylene

R.T.: 3.319 min
Delta R.T.: -0.007 min
Response: 6270380
Conc: 23.34 ng/ml

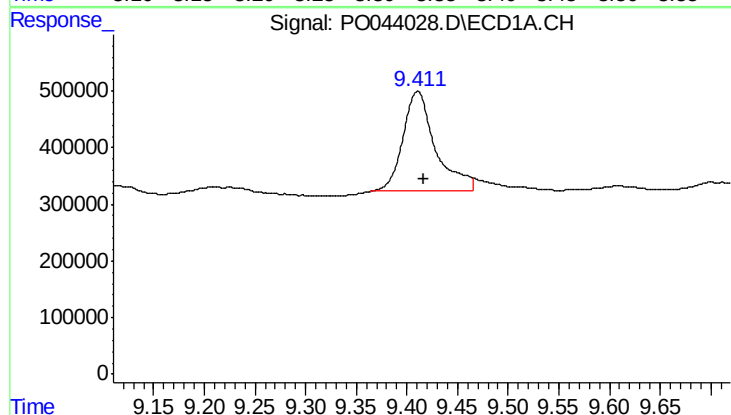

#2 Decachlorobiphenyl

R.T.: 9.411 min
Delta R.T.: -0.006 min
Response: 3964644
Conc: 22.00 ng/ml m

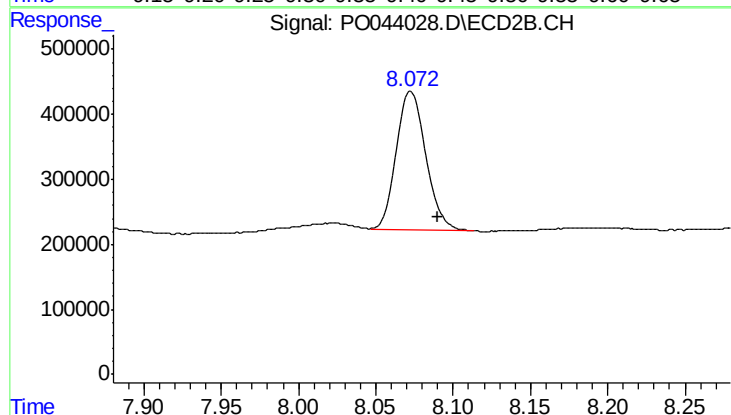

#2 Decachlorobiphenyl

R.T.: 8.072 min
Delta R.T.: -0.018 min
Response: 2758852
Conc: 11.77 ng/ml m