

Data Path : P:\HPCHEM1\ECD_0\Data\P0042418\
Data File : P0044080.D
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
Acq On : 25 Apr 2018 00:08
Operator : SM/UA
Sample : J2518-05
Misc :
ALS Vial : 31 Sample Multiplier: 1

Instrument :
ECD_O
ClientSampleId :
SF-UST

Manual Integrations
APPROVED

ugo
4/26/2018 1:57:51 PM

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Apr 25 07:03:02 2018
Quant Method : P:\HPCHEM1\ECD_0\methods\P0042418.M
Quant Title : GC EXTRACTABLES
QLast Update : Wed Apr 25 02:21:54 2018
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	4.047	3.304	10851573	12405900	24.549m	21.486m
2)	SA Decachlor...	9.397	8.066	8727010	9872198	18.894	16.318

Target Compounds

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : P:\HPCHEM1\ECD_0\Data\P0042418\
Data File : P0044080.D
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
Acq On : 25 Apr 2018 00:08
Operator : SM/UA
Sample : J2518-05
Misc :
ALS Vial : 31 Sample Multiplier: 1



Instrument :
ECD_O
ClientSampleId :
SF-UST


Manual Integrations
APPROVED

ugo
4/26/2018 1:57:51 PM

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Apr 25 07:03:02 2018
Quant Method : P:\HPCHEM1\ECD_0\methods\P0042418.M
Quant Title : GC EXTRACTABLES
QLast Update : Wed Apr 25 02:21:54 2018
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

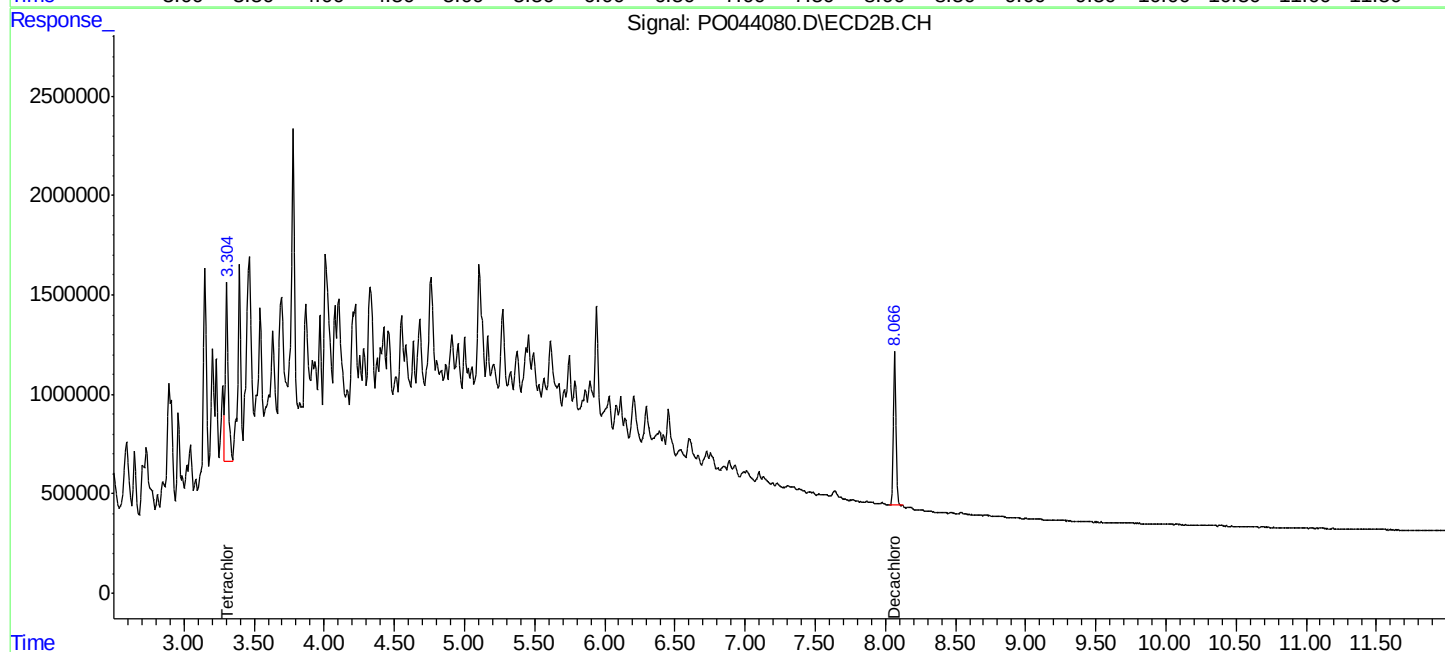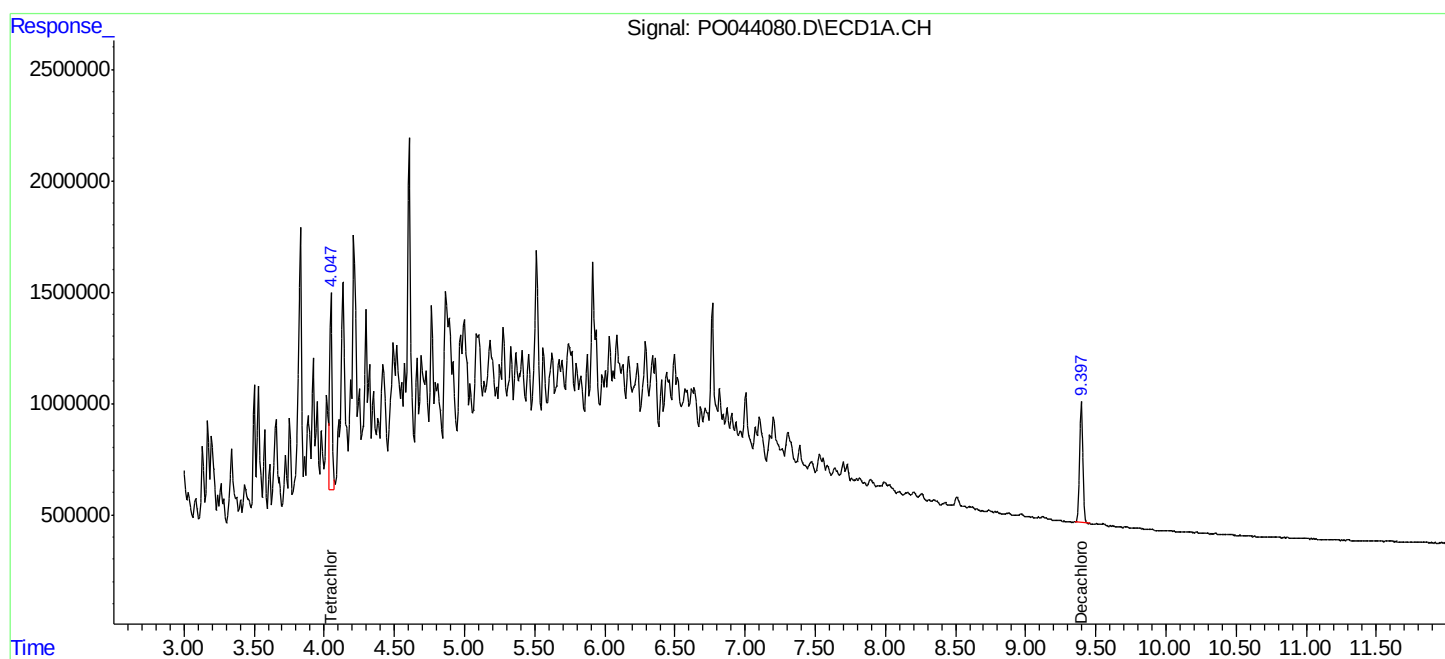

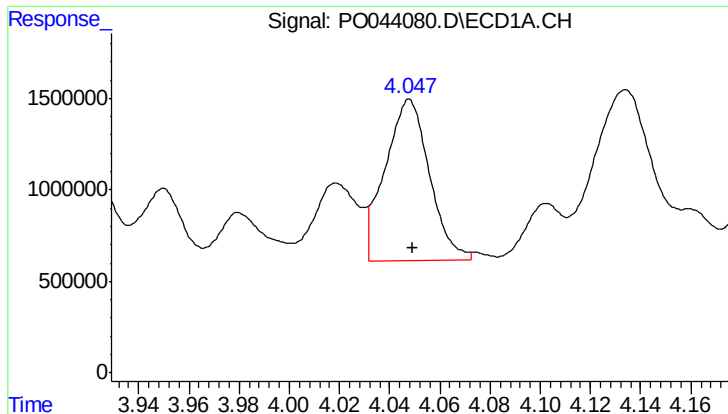


#1 Tetrachloro-m-xylene

R.T.: 4.047 min
Delta R.T.: -0.002 min
Response: 10851573
Conc: 24.55 ng/ml

Instrument :
ECD_O
ClientSampleId :
SF-UST


Manual Integrations
APPROVED

ugo
4/26/2018 1:57:51 PM

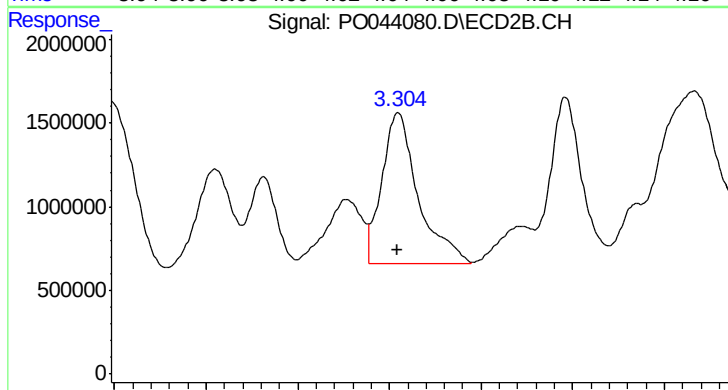


#1 Tetrachloro-m-xylene

R.T.: 3.304 min
Delta R.T.: 0.000 min
Response: 12405900
Conc: 21.49 ng/ml m

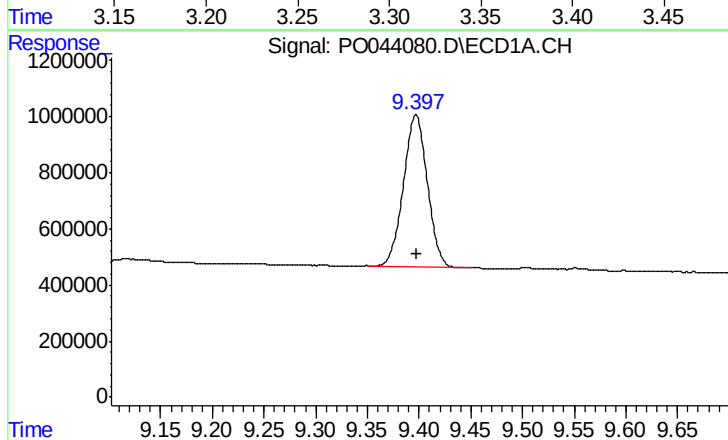

#2 Decachlorobiphenyl

R.T.: 9.397 min
Delta R.T.: -0.001 min
Response: 8727010
Conc: 18.89 ng/ml

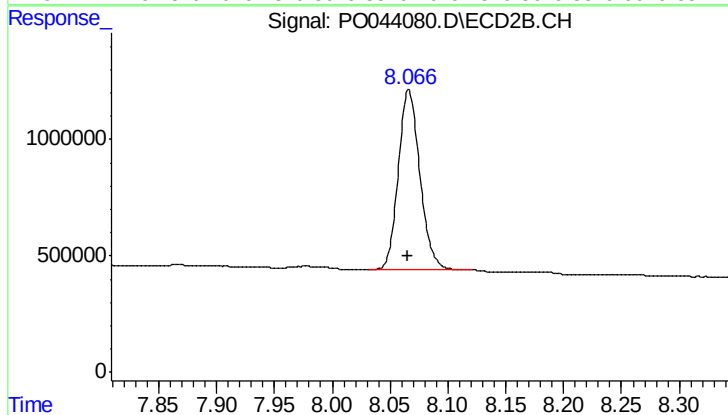

#2 Decachlorobiphenyl

R.T.: 8.066 min
Delta R.T.: 0.001 min
Response: 9872198
Conc: 16.32 ng/ml