

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\P0042420\
 Data File : P0068044.D
 Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
 Acq On : 24 Apr 2020 14:42
 Operator : DD\AJ
 Sample : L2118-01
 Misc :
 ALS Vial : 21 Sample Multiplier: 1

Instrument :
 ECD_O
 ClientSampleId :
 EO-02-042320

Manual Integrations
 APPROVED

Sohil
 4/27/2020 3:04:17 PM

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Apr 24 15:10:00 2020
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\P0040120.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Fri Apr 03 16:04:09 2020
 Response via : Initial Calibration
 Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	4.917	3.938	587078	806504	24.653	24.062
2) SA Decachlor...	10.888	9.218	609222	612247	17.895m	14.808

Target Compounds

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\P0042420\
Data File : P0068044.D
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
Acq On : 24 Apr 2020 14:42
Operator : DD\AJ
Sample : L2118-01
Misc :
ALS Vial : 21 Sample Multiplier: 1



Instrument :
ECD_O
ClientSampleId :
EO-02-042320


Manual Integrations
APPROVED

Sohil
4/27/2020 3:04:17 PM

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Apr 24 15:10:00 2020
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\P0040120.M
Quant Title : GC EXTRACTABLES
QLast Update : Fri Apr 03 16:04:09 2020
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

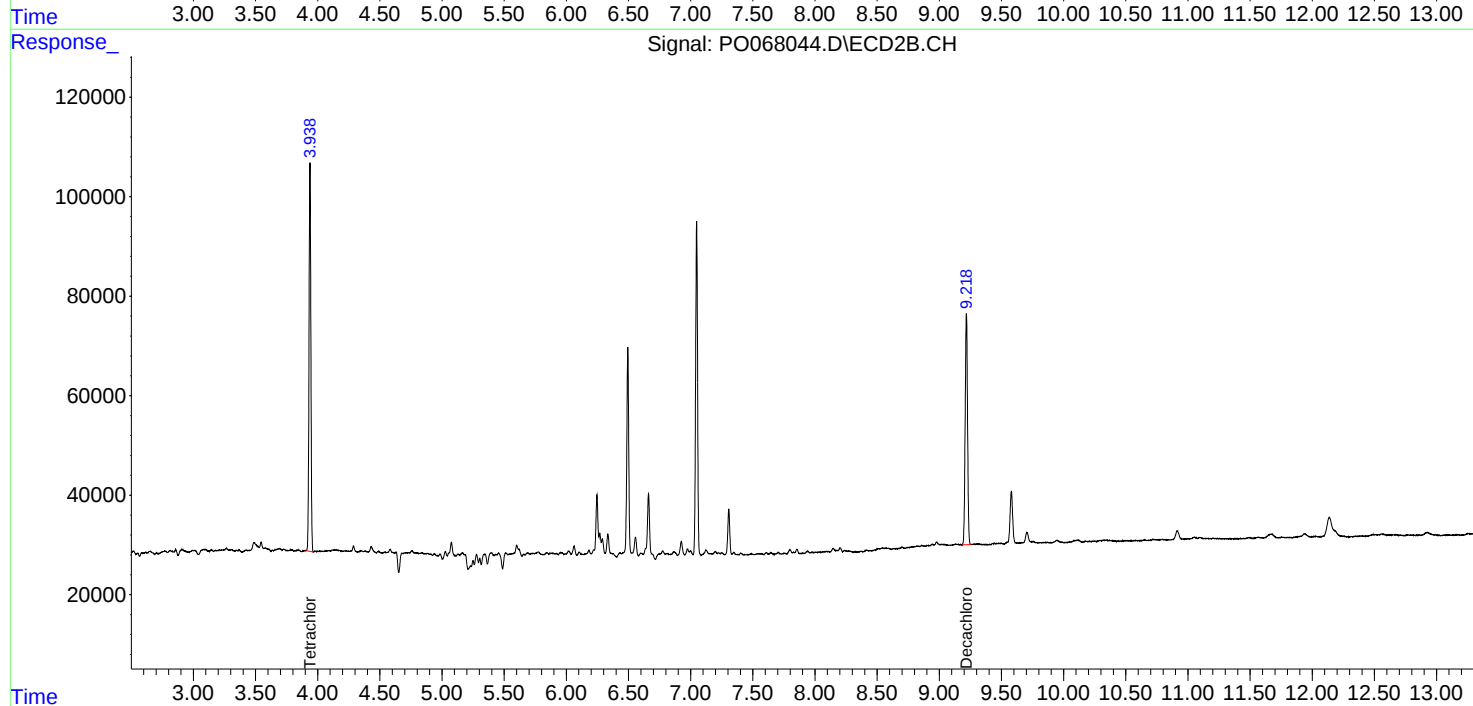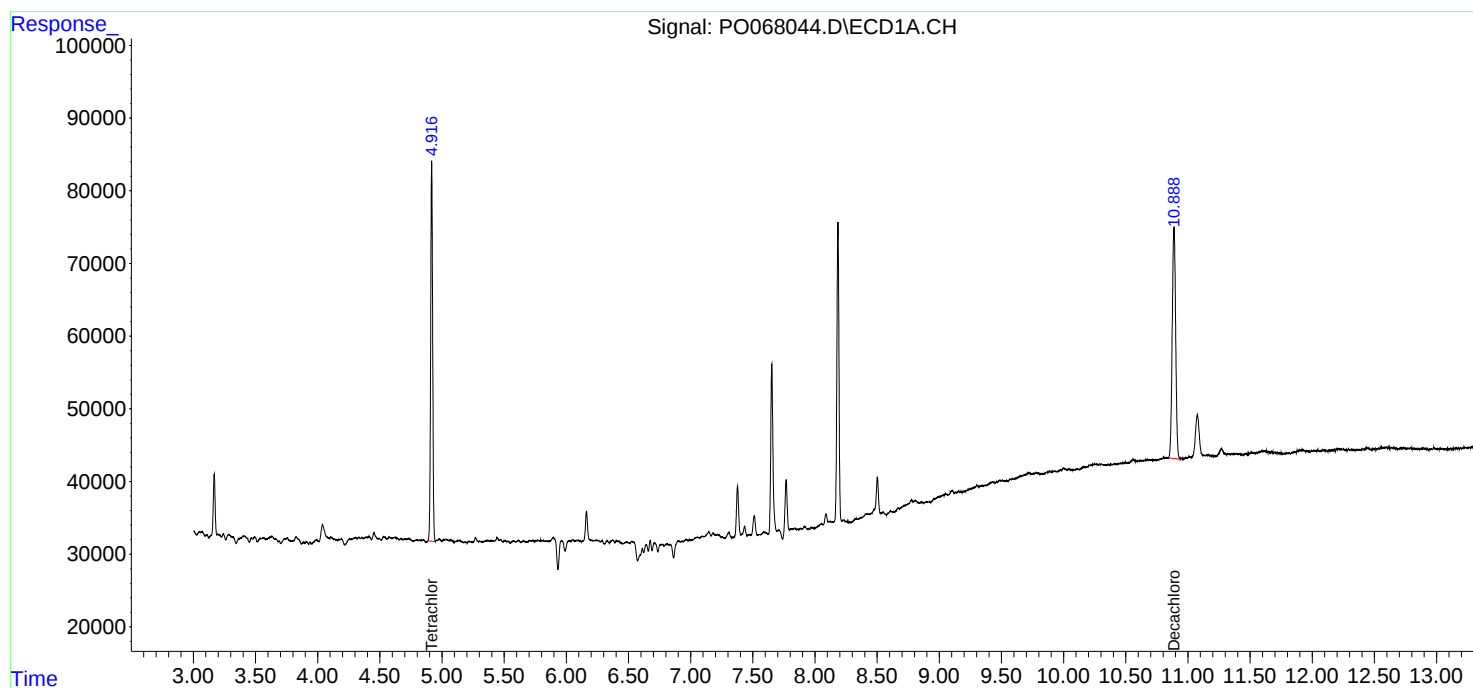

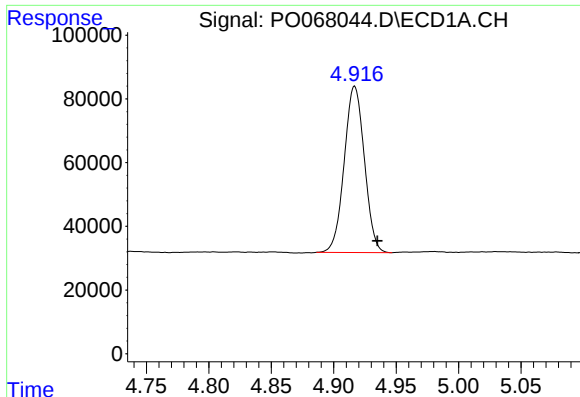


#1 Tetrachloro-m-xylene

R.T.: 4.917 min
Delta R.T.: -0.018 min
Response: 587078
Conc: 24.65 ng/ml

Instrument :
ECD_O
ClientSampleId :
EO-02-042320


Manual Integrations
APPROVED

Sohil
4/27/2020 3:04:17 PM

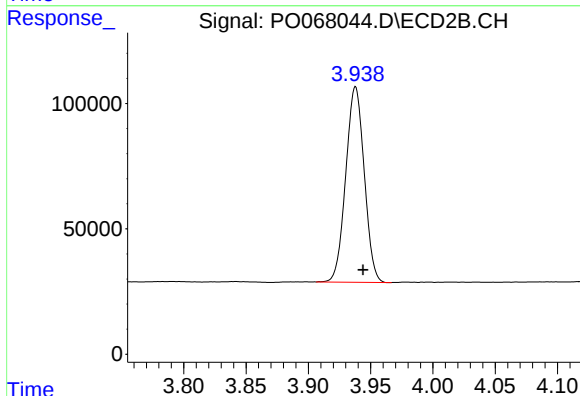


#1 Tetrachloro-m-xylene

R.T.: 3.938 min
Delta R.T.: -0.006 min
Response: 806504
Conc: 24.06 ng/ml

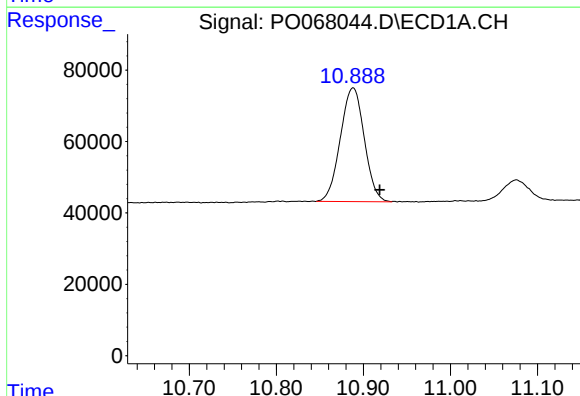

#2 Decachlorobiphenyl

R.T.: 10.888 min
Delta R.T.: -0.031 min
Response: 609222
Conc: 17.90 ng/ml m

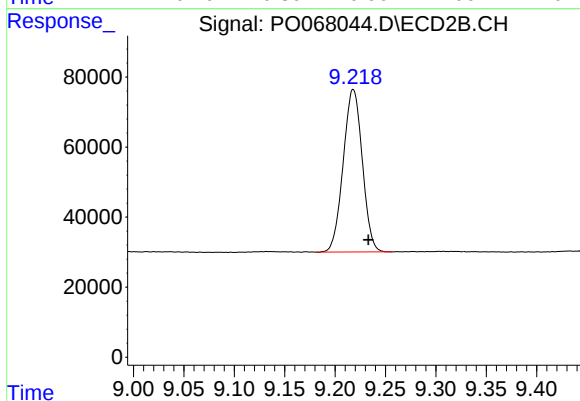

#2 Decachlorobiphenyl

R.T.: 9.218 min
Delta R.T.: -0.015 min
Response: 612247
Conc: 14.81 ng/ml