

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\P0042519\
 Data File : P0055659.D
 Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
 Acq On : 25 Apr 2019 15:06
 Operator : SM/SJ
 Sample : K2540-01
 Misc :
 ALS Vial : 5 Sample Multiplier: 1

Instrument :
 ECD_O
 ClientSampleId :
 FK-SF-03-007-A

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Apr 26 00:44:55 2019
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\P0042419.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Thu Apr 25 01:58:33 2019
 Response via : Initial Calibration
 Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	4.286	3.598	736987	731131	29.086	30.023
2)	SA Decachlor...	9.895	8.557	698492	454717	16.277	14.793
Target Compounds							
3)	L1 AR-1016-1	5.447	4.671	5881	8146	4.735	7.061 #
4)	L1 AR-1016-2	5.470	4.700	18477	194288	10.781	124.716 #
5)	L1 AR-1016-3	5.537	4.864	12084	52744	10.831	60.665 #
6)	L1 AR-1016-4	5.651	4.907	73602	33894	79.819	48.202 #
7)	L1 AR-1016-5	5.927	5.131	68918	144248	69.829	152.410 #
9)	L2 AR-1221-2	0.000	3.896	0	12800	N.D.	56.199 #
10)	L2 AR-1221-3	4.672	3.965	12436	15065	15.342	20.604 #
11)	L3 AR-1232-1	4.672	3.965	12436	15065	18.693	25.374 #
12)	L3 AR-1232-2	5.186	4.700	24626	194288	63.528	267.449 #
13)	L3 AR-1232-3	5.470	4.864	18477	52744	23.972	130.831 #
14)	L3 AR-1232-4	5.651	4.929	73602	14122	178.205	41.089 #
15)	L3 AR-1232-5	5.720	5.131	33855	144248	99.746	358.333 #
16)	L4 AR-1242-1	5.447	4.671	5881	8146	5.970	8.833 #
17)	L4 AR-1242-2	5.470	4.700	18477	194288	13.476	156.885 #
18)	L4 AR-1242-3	5.537	4.864	12084	52744	13.451	73.904 #
19)	L4 AR-1242-4	5.651	4.929	73602	14122	99.966	20.618 #
20)	L4 AR-1242-5	6.385	5.475	116514	402663	126.181	402.478 #
21)	L5 AR-1248-1	5.447	4.671	5881	8146	8.147	11.789 #
22)	L5 AR-1248-2	5.720	4.907	33855	33894	32.182	38.021
23)	L5 AR-1248-3	5.927	4.929	68918	14122	58.116	15.397 #
24)	L5 AR-1248-4	6.340	5.131	169049	144248	119.050	124.936
25)	L5 AR-1248-5	6.340	5.511	169049	63420	123.186	51.281 #
26)	L6 AR-1254-1	6.308	5.475	344606	402663	223.240	198.931
27)	L6 AR-1254-2	6.521	5.613	330422	95146	133.900	52.367 #
28)	L6 AR-1254-3	6.887	6.014	235123	67998	84.127	22.109 #
29)	L6 AR-1254-4	7.164	6.240	95931	37748	43.079	17.661 #
30)	L6 AR-1254-5	7.581	6.655	134543	216429	53.667	73.869 #
31)	L7 AR-1260-1	7.042	6.142	83863	74770	40.822	38.570
32)	L7 AR-1260-2	7.293	6.327	454433	127646	179.247	49.050 #
33)	L7 AR-1260-3	7.655	6.481	52522	83379	25.565	36.663 #
34)	L7 AR-1260-4	7.877	6.950	82881	48795	34.718	24.305 #
35)	L7 AR-1260-5	8.189	7.190	112340	114255	24.354	22.985
36)	L8 AR-1262-1	7.655	6.691	52522	65631	17.066	19.195
37)	L8 AR-1262-2	8.189	7.190	112340	114255	20.453	20.169
38)	L8 AR-1262-3	8.502	7.473	115006	31758	30.097	13.659 #
39)	L8 AR-1262-4	8.569	7.535	22731	89819	7.889	22.895 #
40)	L8 AR-1262-5	9.194	8.028	20808	29500	10.735	16.654 #
41)	L9 AR-1268-1	8.502	7.473	115006	31758	18.192	4.870 #
42)	L9 AR-1268-2	8.569	7.535	22731	89819	3.932	16.075 #

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\P0042519\
 Data File : P0055659.D
 Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
 Acq On : 25 Apr 2019 15:06
 Operator : SM/SJ
 Sample : K2540-01
 Misc :
 ALS Vial : 5 Sample Multiplier: 1

Instrument :
 ECD_O
 ClientSampleId :
 FK-SF-03-007-A

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Apr 26 00:44:55 2019
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\P0042419.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Thu Apr 25 01:58:33 2019
 Response via : Initial Calibration
 Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml
43) L9	AR-1268-3	0.000	7.742	0	13398	N.D.	2.881 #
44) L9	AR-1268-4	9.194	8.028	20808	29500	9.734	15.280 #
45) L9	AR-1268-5	9.582	8.310	39648	21336	2.750	1.778 #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\PO042519\
Data File : PO055659.D
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
Acq On : 25 Apr 2019 15:06
Operator : SM/SJ
Sample : K2540-01
Misc :
ALS Vial : 5 Sample Multiplier: 1

Instrument :
ECD_O
ClientSampleId :
FK-SF-03-007-A

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Apr 26 00:44:55 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\PO042419.M
Quant Title : GC EXTRACTABLES
QLast Update : Thu Apr 25 01:58:33 2019
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

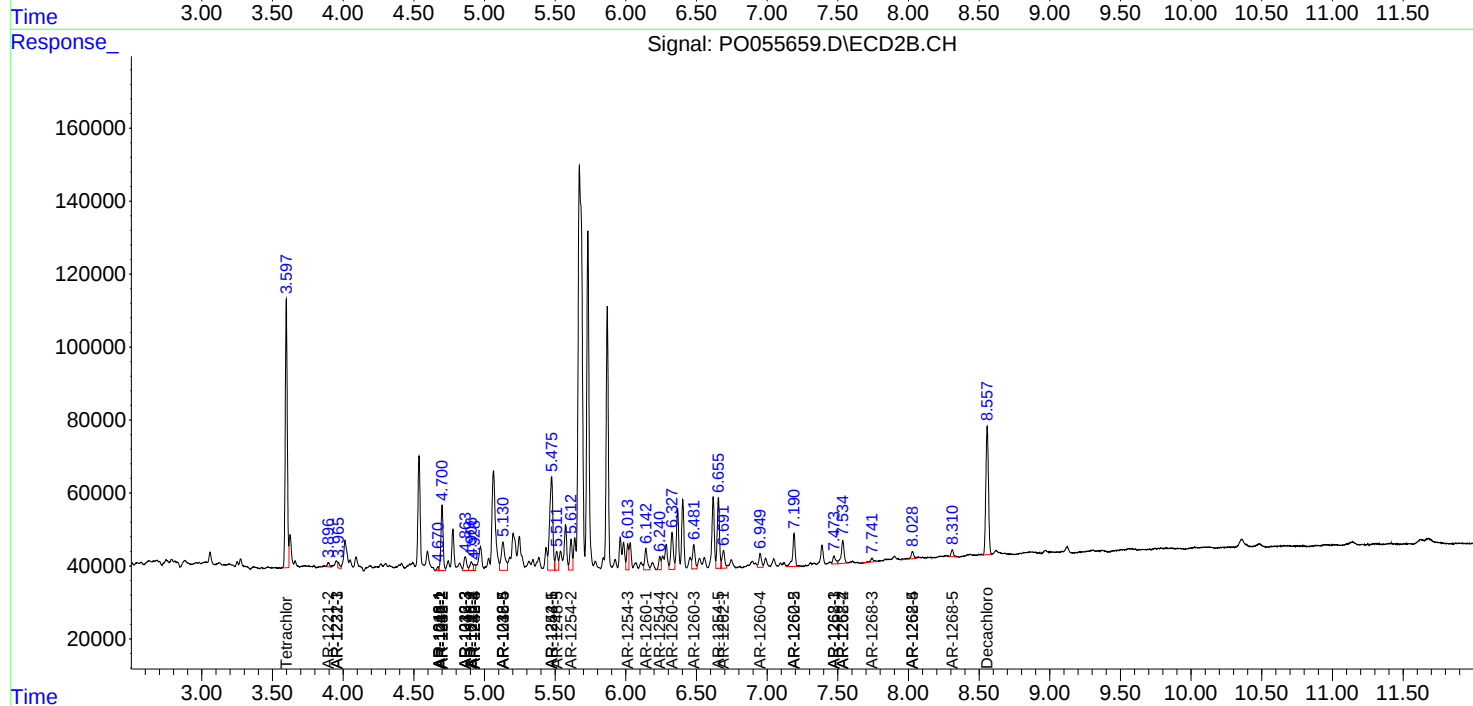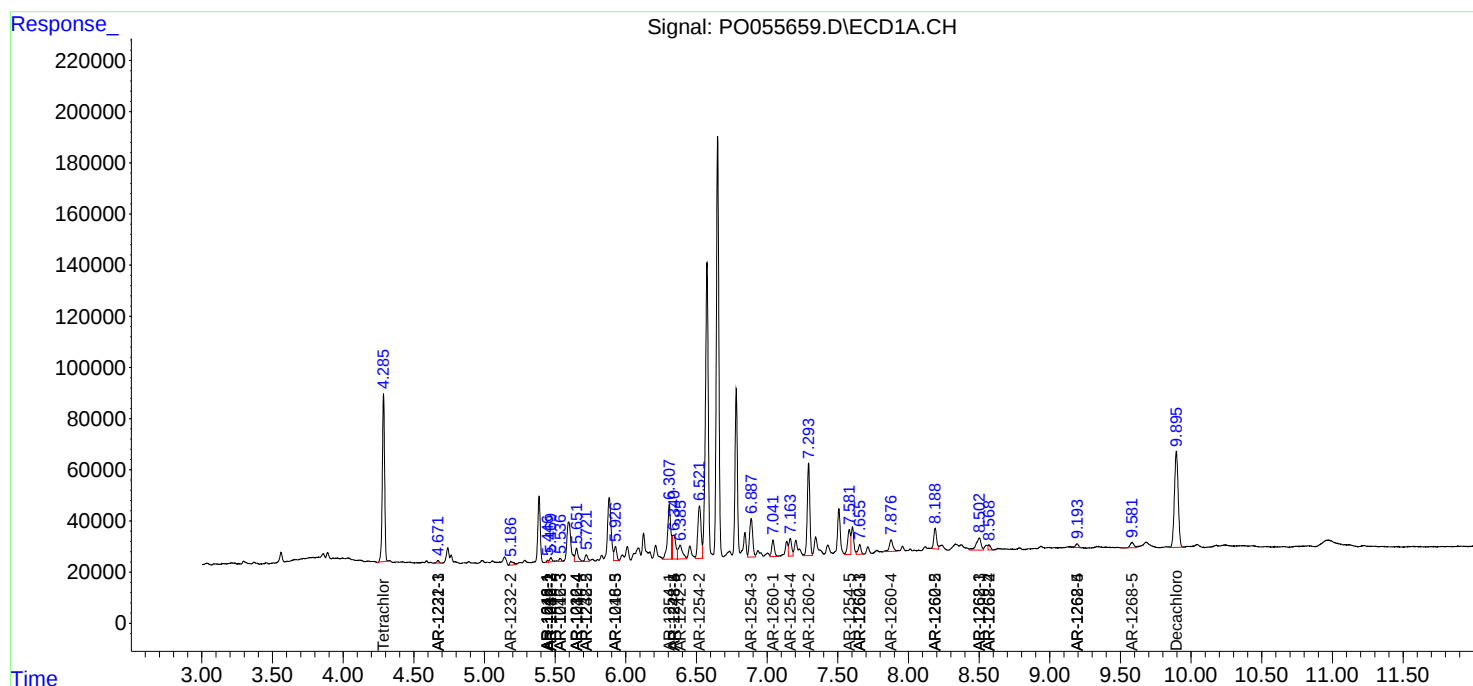


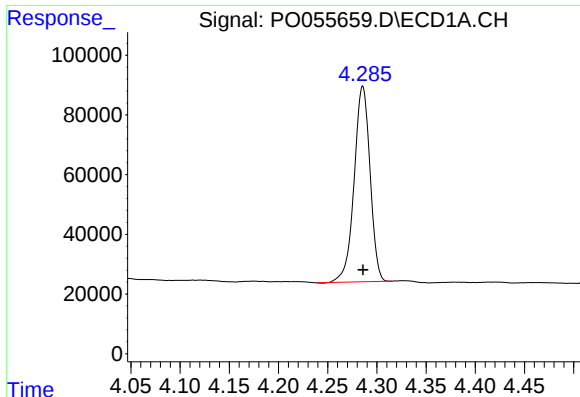

#1 Tetrachloro-m-xylene


R.T.: 4.286 min
Delta R.T.: 0.000 min
Response: 736987
Conc: 29.09 ng/ml

Instrument :
ECD_O
ClientSampleId :
FK-SF-03-007-A

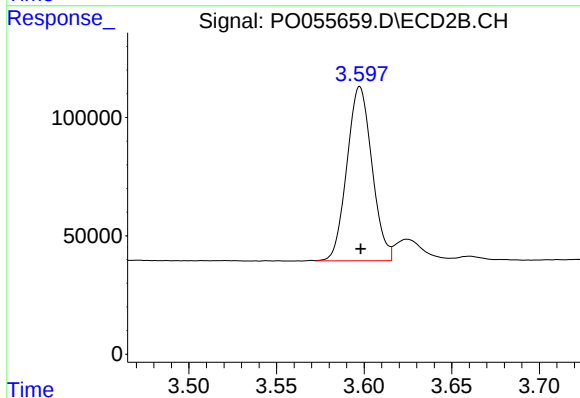


#1 Tetrachloro-m-xylene

R.T.: 3.598 min
Delta R.T.: 0.000 min
Response: 731131
Conc: 30.02 ng/ml

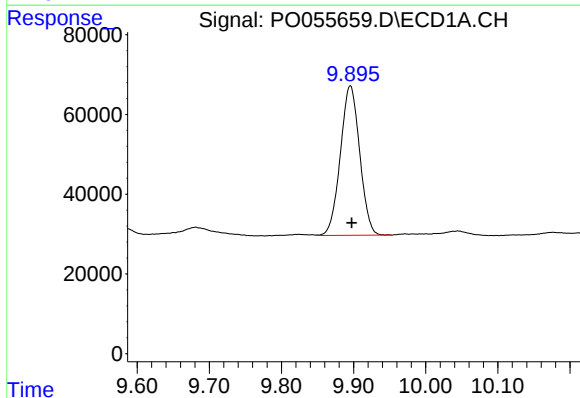


#2 Decachlorobiphenyl

R.T.: 9.895 min
Delta R.T.: -0.002 min
Response: 698492
Conc: 16.28 ng/ml

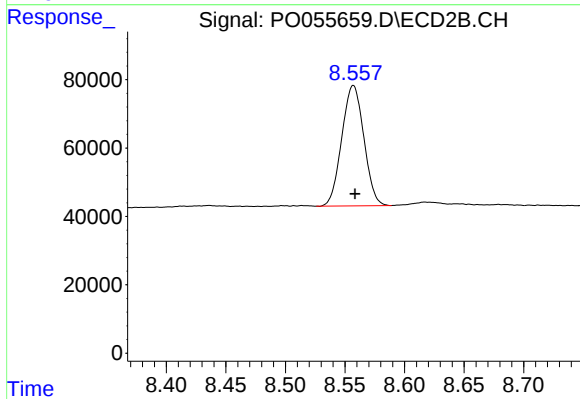

#2 Decachlorobiphenyl


R.T.: 8.557 min
Delta R.T.: -0.002 min
Response: 454717
Conc: 14.79 ng/ml

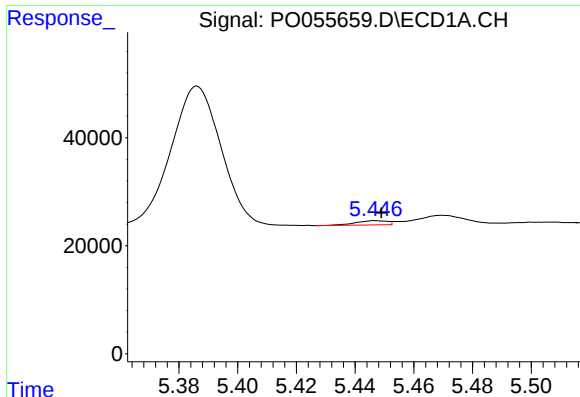

#3 AR-1016-1


R.T.: 5.447 min
Delta R.T.: -0.002 min
Response: 5881
Conc: 4.74 ng/ml

Instrument :
ECD_O
ClientSampleId :
FK-SF-03-007-A

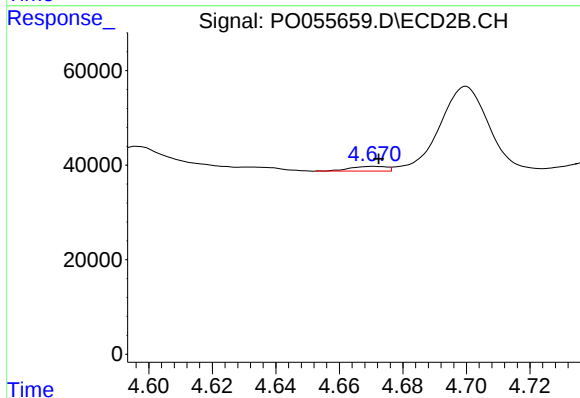


#3 AR-1016-1

R.T.: 4.671 min
Delta R.T.: -0.002 min
Response: 8146
Conc: 7.06 ng/ml

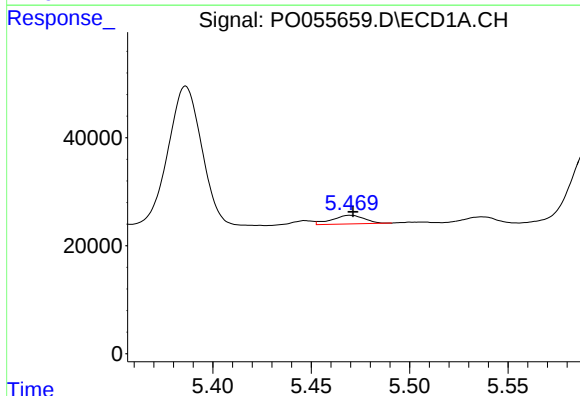


#4 AR-1016-2

R.T.: 5.470 min
Delta R.T.: -0.001 min
Response: 18477
Conc: 10.78 ng/ml

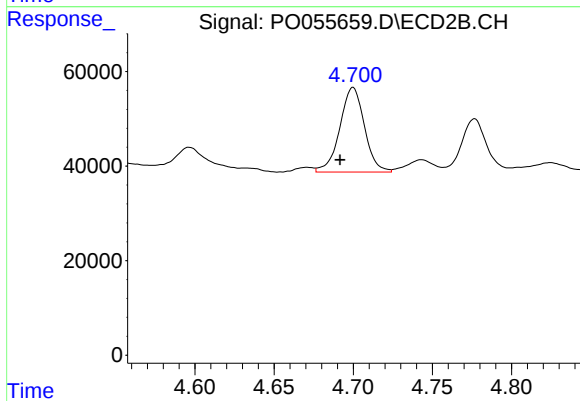

#4 AR-1016-2


R.T.: 4.700 min
Delta R.T.: 0.008 min
Response: 194288
Conc: 124.72 ng/ml

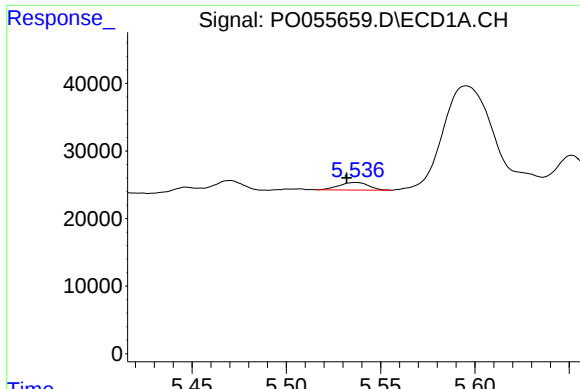

#5 AR-1016-3


R.T.: 5.537 min
Delta R.T.: 0.005 min
Response: 12084
Conc: 10.83 ng/ml

Instrument :
ECD_O
ClientSampleId :
FK-SF-03-007-A

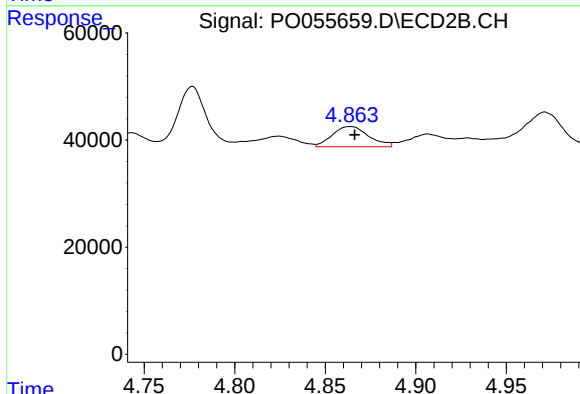


#5 AR-1016-3

R.T.: 4.864 min
Delta R.T.: -0.002 min
Response: 52744
Conc: 60.66 ng/ml

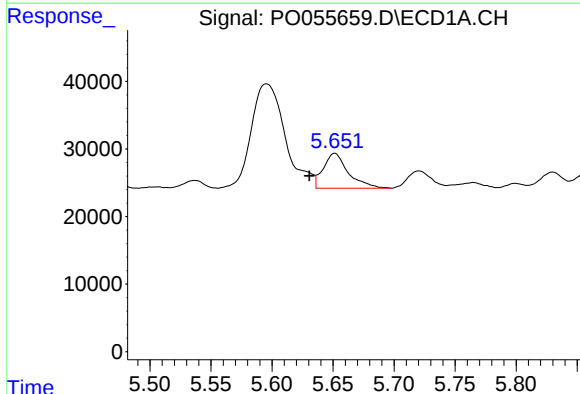


#6 AR-1016-4

R.T.: 5.651 min
Delta R.T.: 0.021 min
Response: 73602
Conc: 79.82 ng/ml

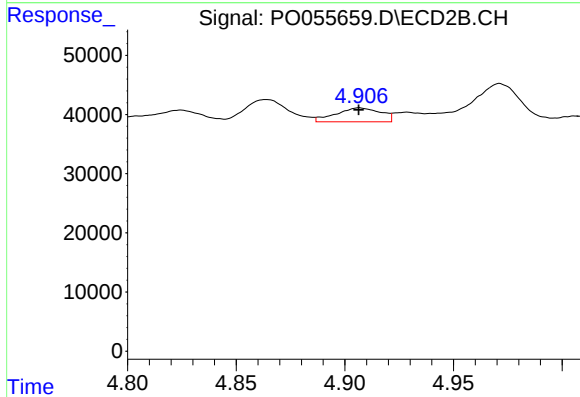

#6 AR-1016-4


R.T.: 4.907 min
Delta R.T.: 0.000 min
Response: 33894
Conc: 48.20 ng/ml

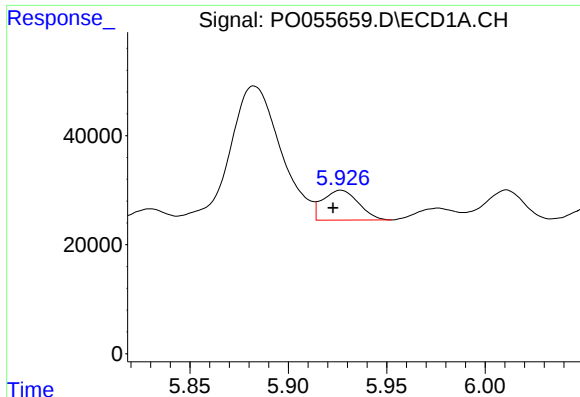

#7 AR-1016-5


R.T.: 5.927 min
Delta R.T.: 0.004 min
Response: 68918
Conc: 69.83 ng/ml

Instrument :
ECD_O
ClientSampleId :
FK-SF-03-007-A

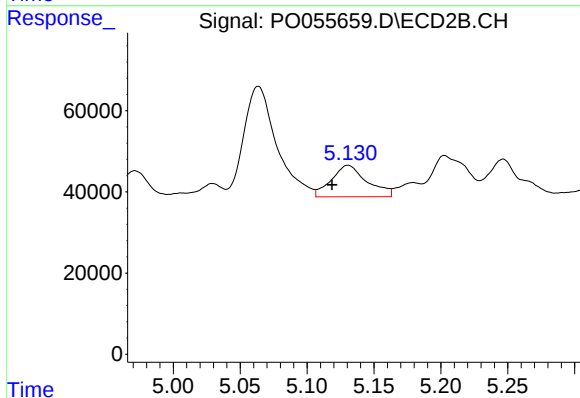


#7 AR-1016-5

R.T.: 5.131 min
Delta R.T.: 0.012 min
Response: 144248
Conc: 152.41 ng/ml

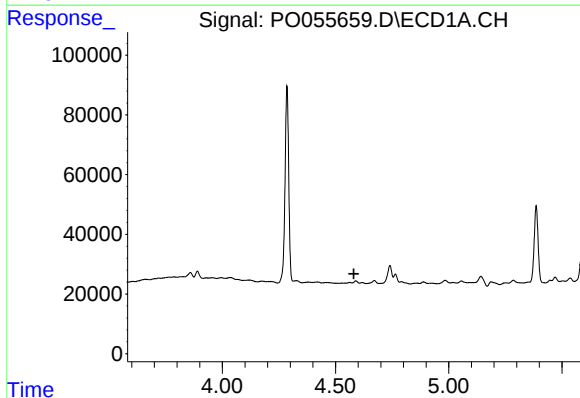


#9 AR-1221-2

R.T.: 0.000 min
Exp R.T. : 4.581 min
Response: 0
Conc: N.D.

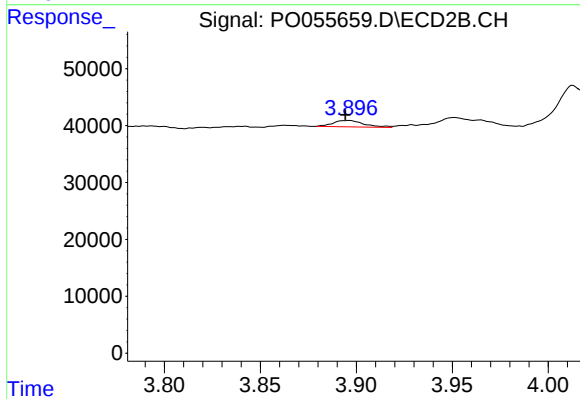

#9 AR-1221-2


R.T.: 3.896 min
Delta R.T.: 0.002 min
Response: 12800
Conc: 56.20 ng/ml

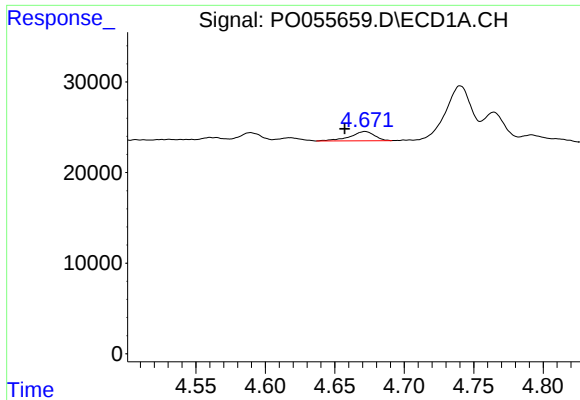

#10 AR-1221-3


R.T.: 4.672 min
Delta R.T.: 0.015 min
Response: 12436
Conc: 15.34 ng/ml

Instrument :
ECD_O
ClientSampleId :
FK-SF-03-007-A

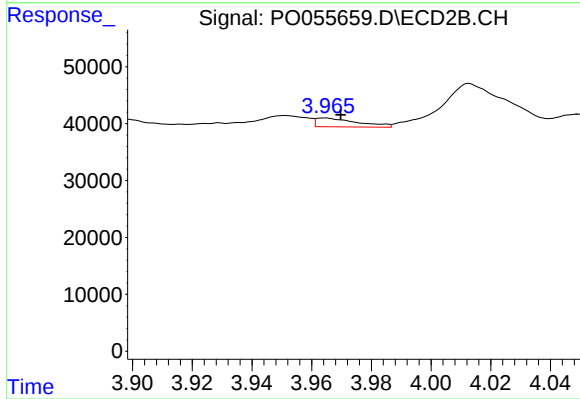


#10 AR-1221-3

R.T.: 3.965 min
Delta R.T.: -0.005 min
Response: 15065
Conc: 20.60 ng/ml

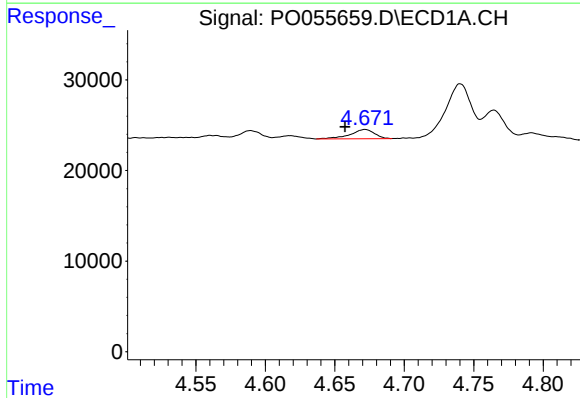


#11 AR-1232-1

R.T.: 4.672 min
Delta R.T.: 0.014 min
Response: 12436
Conc: 18.69 ng/ml

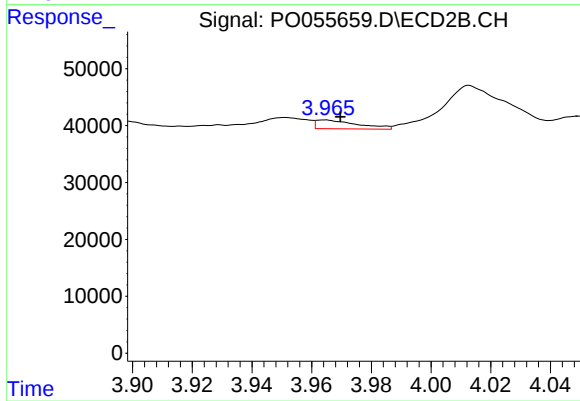

#11 AR-1232-1


R.T.: 3.965 min
Delta R.T.: -0.005 min
Response: 15065
Conc: 25.37 ng/ml

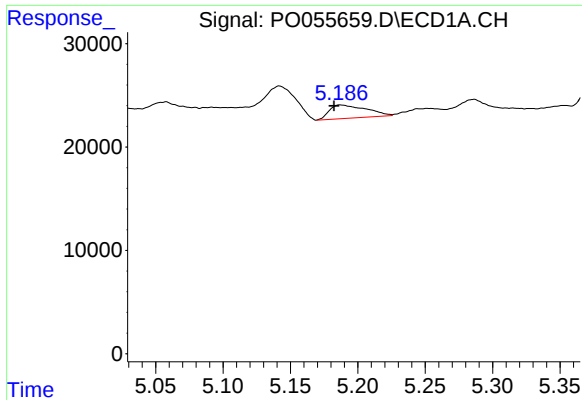

#12 AR-1232-2


R.T.: 5.186 min
Delta R.T.: 0.004 min
Response: 24626
Conc: 63.53 ng/ml

Instrument :
ECD_O
ClientSampleId :
FK-SF-03-007-A

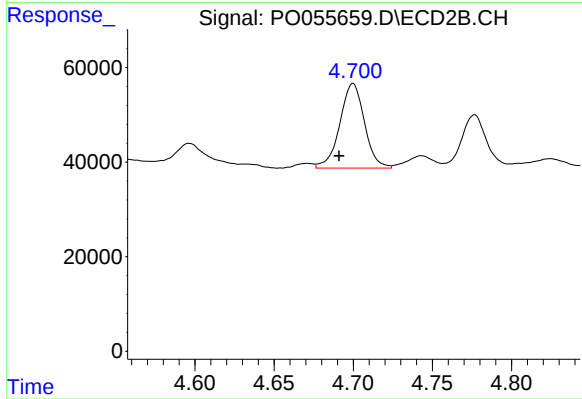


#12 AR-1232-2

R.T.: 4.700 min
Delta R.T.: 0.009 min
Response: 194288
Conc: 267.45 ng/ml

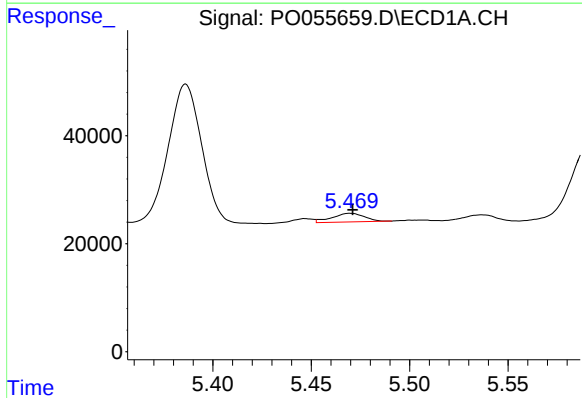


#13 AR-1232-3

R.T.: 5.470 min
Delta R.T.: -0.001 min
Response: 18477
Conc: 23.97 ng/ml

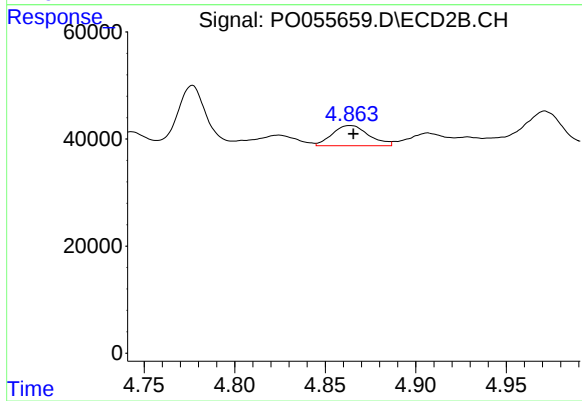

#13 AR-1232-3


R.T.: 4.864 min
Delta R.T.: -0.002 min
Response: 52744
Conc: 130.83 ng/ml

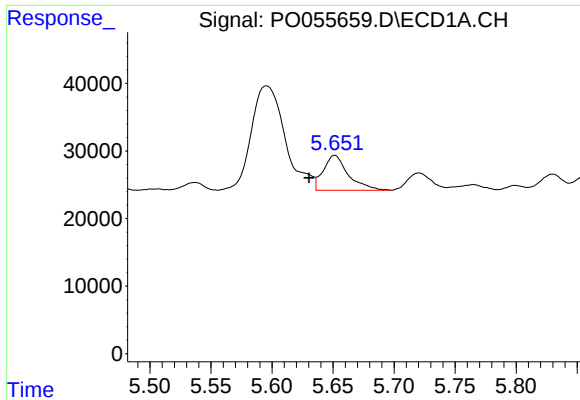

#14 AR-1232-4


R.T.: 5.651 min
Delta R.T.: 0.021 min
Response: 73602
Conc: 178.21 ng/ml

Instrument :
ECD_O
ClientSampleId :
FK-SF-03-007-A

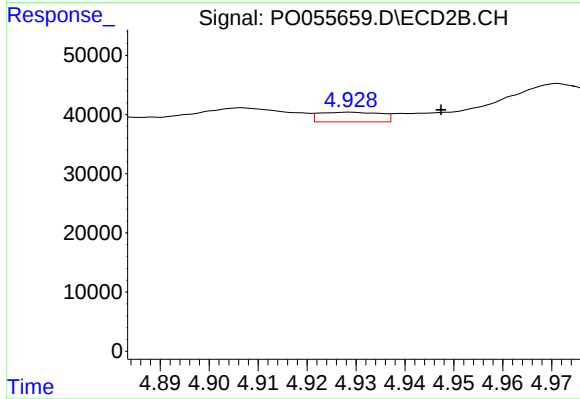


#14 AR-1232-4

R.T.: 4.929 min
Delta R.T.: -0.019 min
Response: 14122
Conc: 41.09 ng/ml

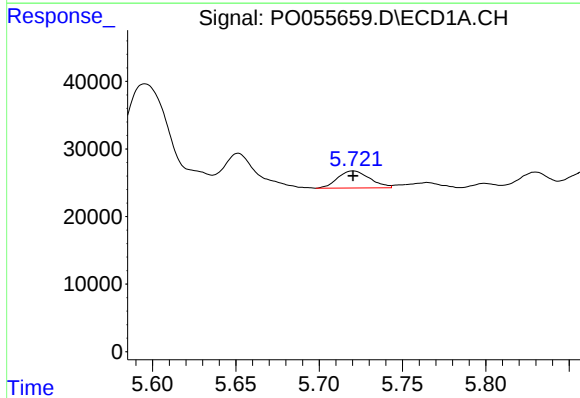


#15 AR-1232-5

R.T.: 5.720 min
Delta R.T.: 0.000 min
Response: 33855
Conc: 99.75 ng/ml

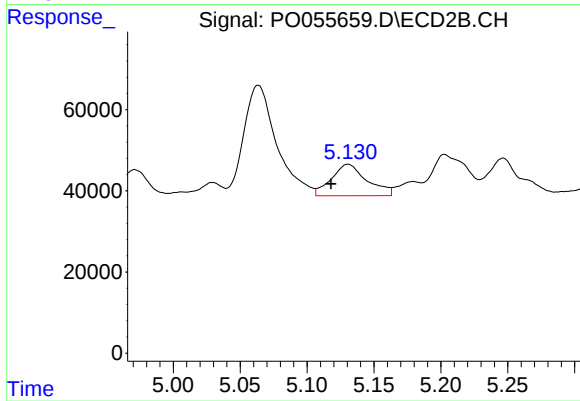

#15 AR-1232-5


R.T.: 5.131 min
Delta R.T.: 0.013 min
Response: 144248
Conc: 358.33 ng/ml

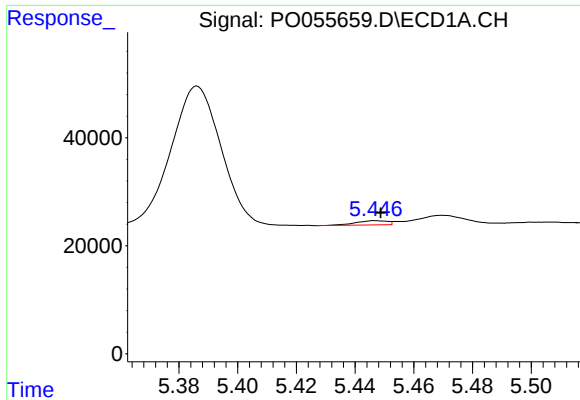

#16 AR-1242-1


R.T.: 5.447 min
Delta R.T.: -0.002 min
Response: 5881
Conc: 5.97 ng/ml

Instrument :
ECD_O
ClientSampleId :
FK-SF-03-007-A

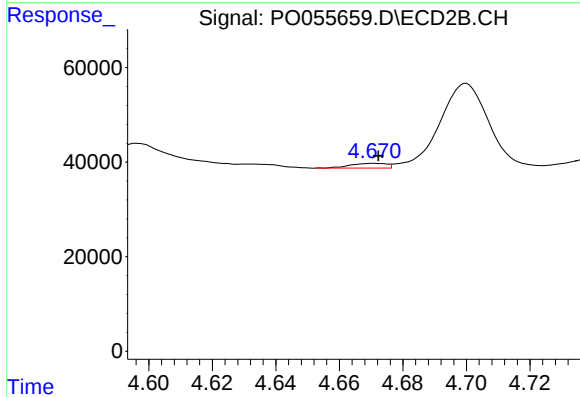


#16 AR-1242-1

R.T.: 4.671 min
Delta R.T.: -0.001 min
Response: 8146
Conc: 8.83 ng/ml

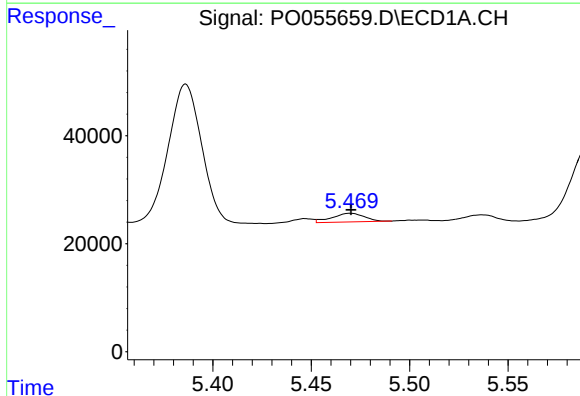


#17 AR-1242-2

R.T.: 5.470 min
Delta R.T.: 0.000 min
Response: 18477
Conc: 13.48 ng/ml

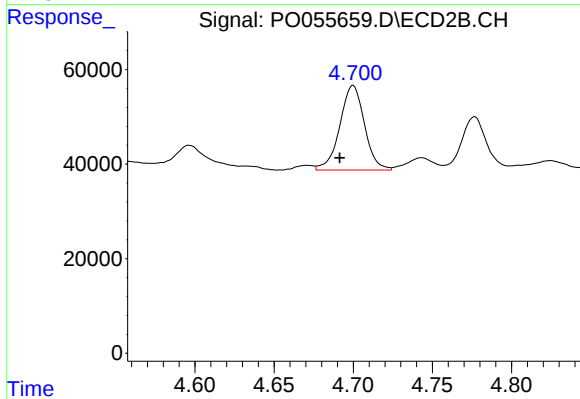

#17 AR-1242-2


R.T.: 4.700 min
Delta R.T.: 0.008 min
Response: 194288
Conc: 156.89 ng/ml

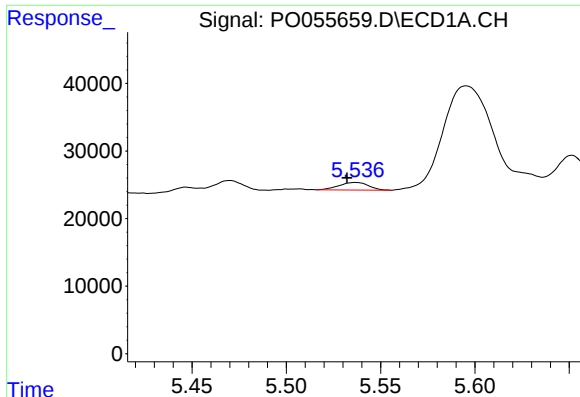

#18 AR-1242-3


R.T.: 5.537 min
Delta R.T.: 0.005 min
Response: 12084
Conc: 13.45 ng/ml

Instrument :
ECD_O
ClientSampleId :
FK-SF-03-007-A

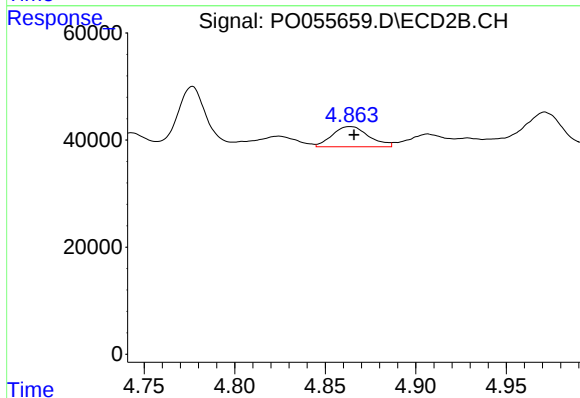


#18 AR-1242-3

R.T.: 4.864 min
Delta R.T.: -0.002 min
Response: 52744
Conc: 73.90 ng/ml

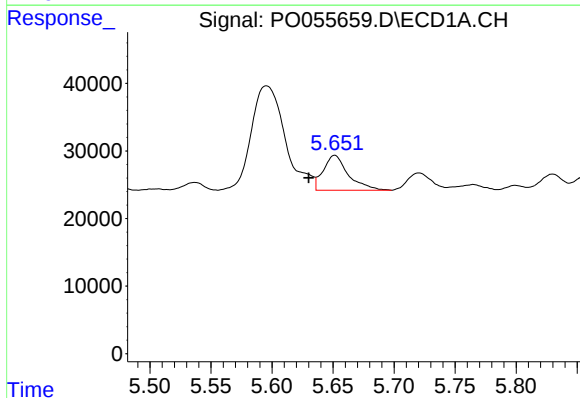


#19 AR-1242-4

R.T.: 5.651 min
Delta R.T.: 0.021 min
Response: 73602
Conc: 99.97 ng/ml

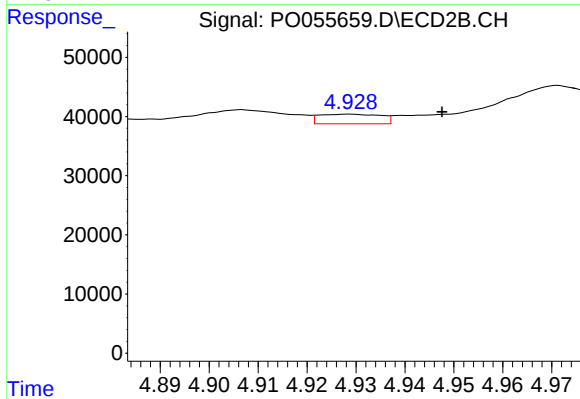

#19 AR-1242-4


R.T.: 4.929 min
Delta R.T.: -0.019 min
Response: 14122
Conc: 20.62 ng/ml

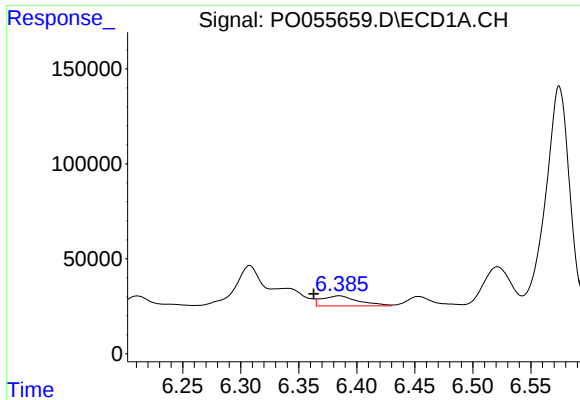

#20 AR-1242-5


R.T.: 6.385 min
Delta R.T.: 0.022 min
Response: 116514
Conc: 126.18 ng/ml

Instrument :
ECD_O
ClientSampleId :
FK-SF-03-007-A

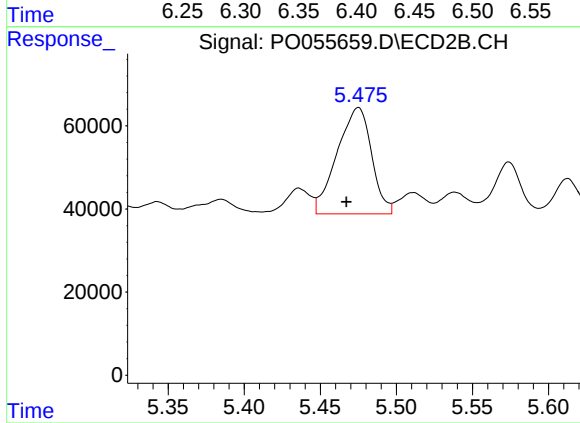


#20 AR-1242-5

R.T.: 5.475 min
Delta R.T.: 0.008 min
Response: 402663
Conc: 402.48 ng/ml

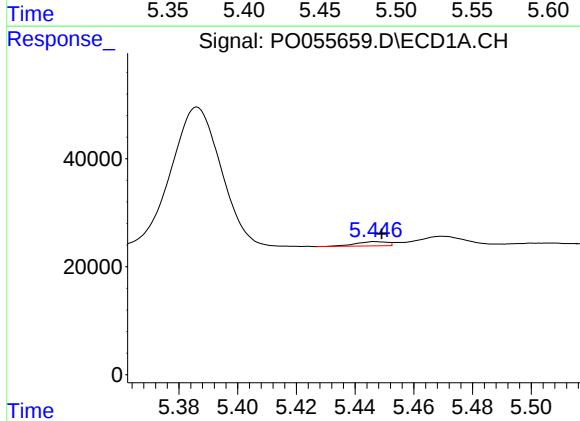


#21 AR-1248-1

R.T.: 5.447 min
Delta R.T.: -0.002 min
Response: 5881
Conc: 8.15 ng/ml

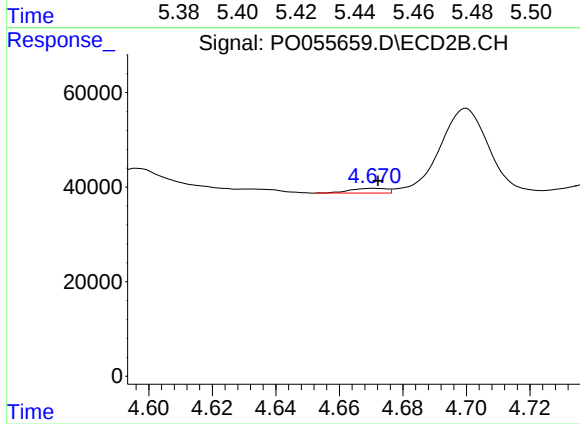

#21 AR-1248-1


R.T.: 4.671 min
Delta R.T.: -0.001 min
Response: 8146
Conc: 11.79 ng/ml

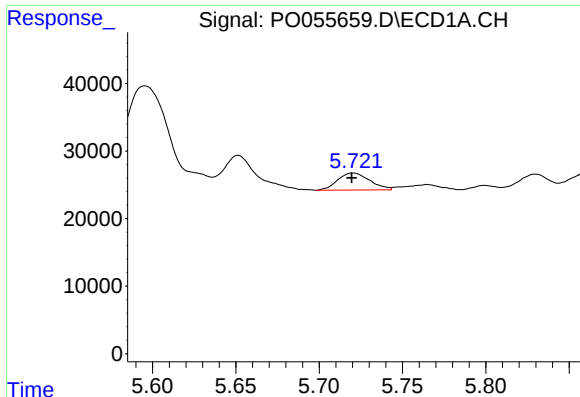

#22 AR-1248-2


R.T.: 5.720 min
Delta R.T.: 0.000 min
Response: 33855
Conc: 32.18 ng/ml

Instrument :
ECD_O
ClientSampleId :
FK-SF-03-007-A

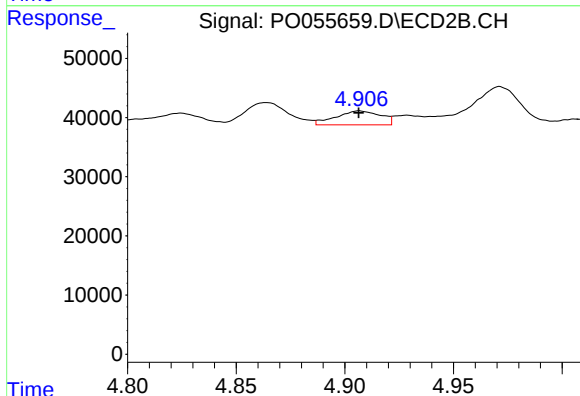


#22 AR-1248-2

R.T.: 4.907 min
Delta R.T.: 0.000 min
Response: 33894
Conc: 38.02 ng/ml

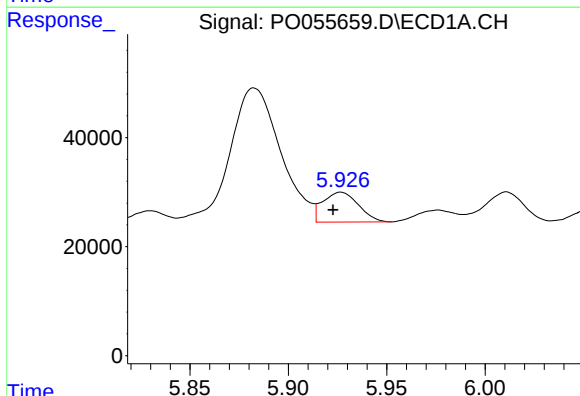


#23 AR-1248-3

R.T.: 5.927 min
Delta R.T.: 0.004 min
Response: 68918
Conc: 58.12 ng/ml

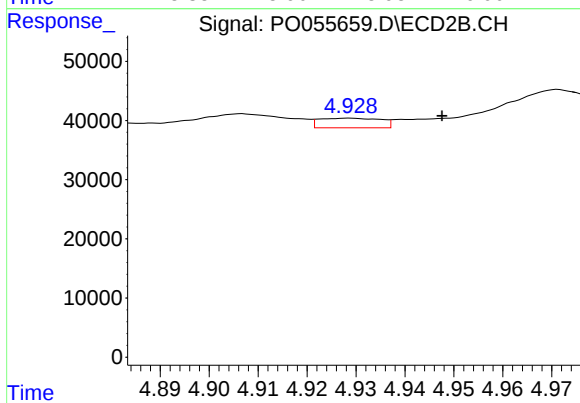

#23 AR-1248-3


R.T.: 4.929 min
Delta R.T.: -0.019 min
Response: 14122
Conc: 15.40 ng/ml

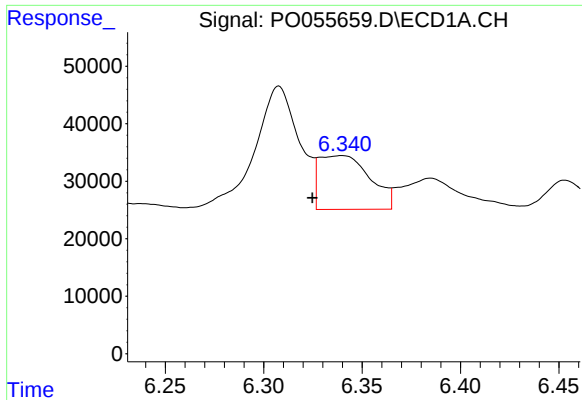

#24 AR-1248-4


R.T.: 6.340 min
Delta R.T.: 0.015 min
Response: 169049
Conc: 119.05 ng/ml

Instrument :
ECD_O
ClientSampleId :
FK-SF-03-007-A

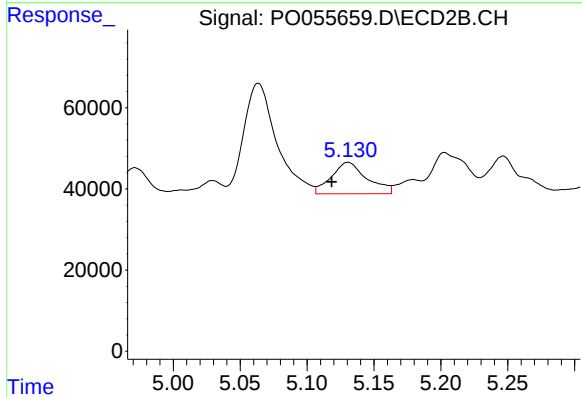


#24 AR-1248-4

R.T.: 5.131 min
Delta R.T.: 0.012 min
Response: 144248
Conc: 124.94 ng/ml

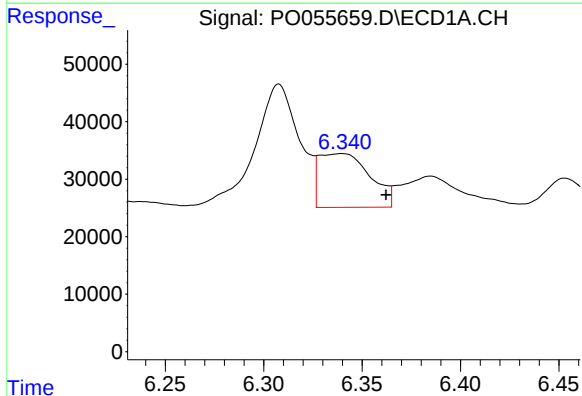


#25 AR-1248-5

R.T.: 6.340 min
Delta R.T.: -0.022 min
Response: 169049
Conc: 123.19 ng/ml

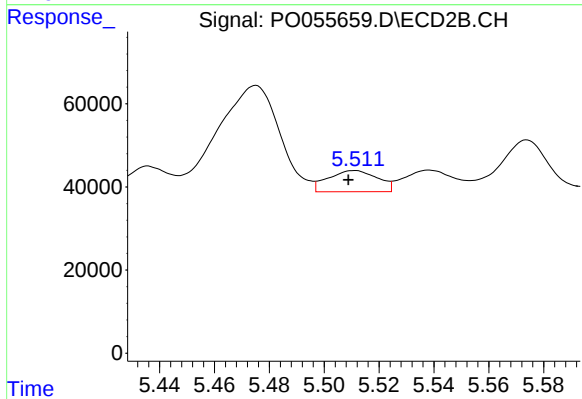

#25 AR-1248-5


R.T.: 5.511 min
Delta R.T.: 0.003 min
Response: 63420
Conc: 51.28 ng/ml

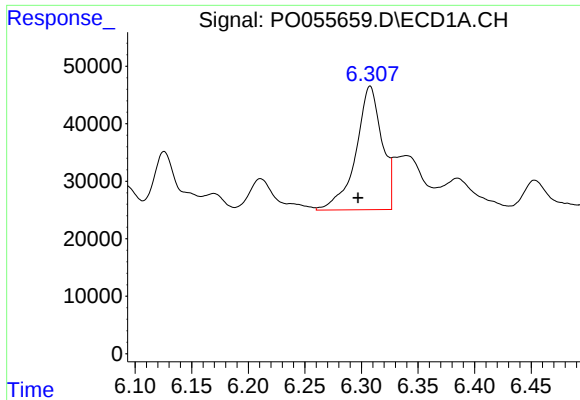

#26 AR-1254-1


R.T.: 6.308 min
Delta R.T.: 0.011 min
Response: 344606
Conc: 223.24 ng/ml

Instrument :
ECD_O
ClientSampleId :
FK-SF-03-007-A

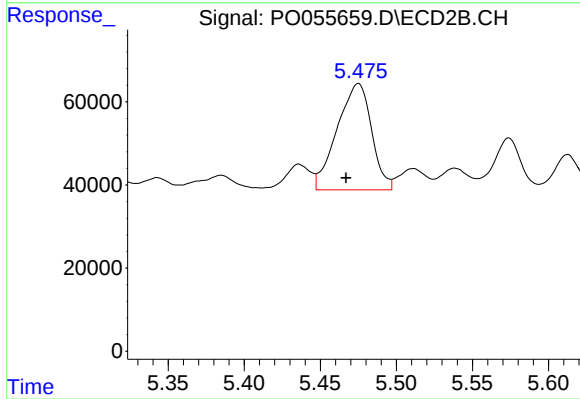


#26 AR-1254-1

R.T.: 5.475 min
Delta R.T.: 0.008 min
Response: 402663
Conc: 198.93 ng/ml

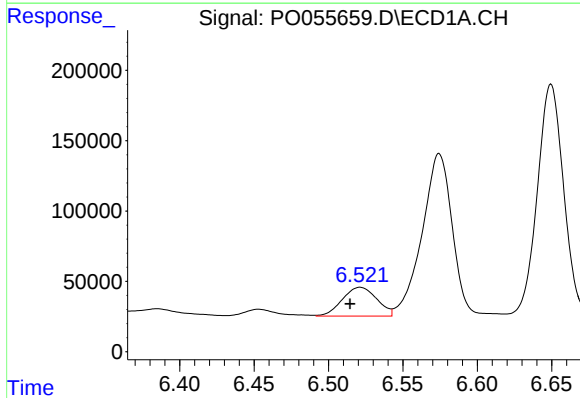


#27 AR-1254-2

R.T.: 6.521 min
Delta R.T.: 0.007 min
Response: 330422
Conc: 133.90 ng/ml

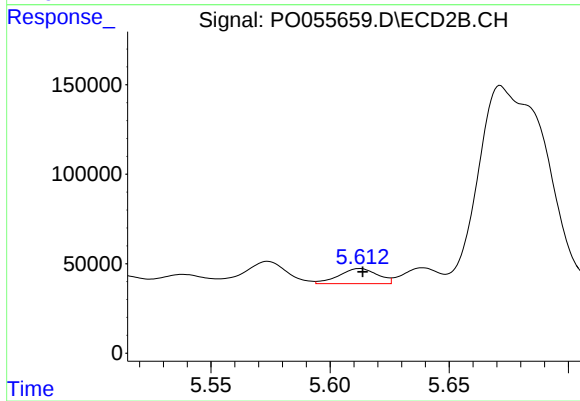

#27 AR-1254-2


R.T.: 5.613 min
Delta R.T.: -0.001 min
Response: 95146
Conc: 52.37 ng/ml

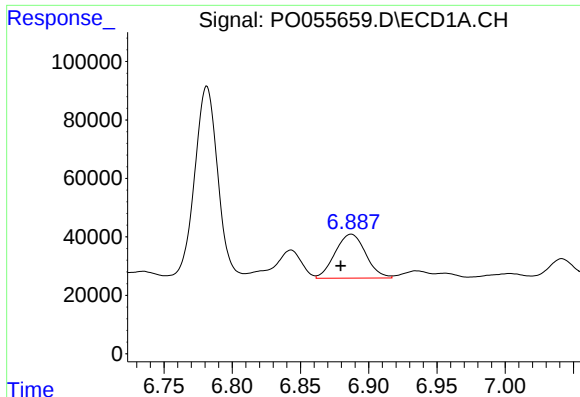

#28 AR-1254-3


R.T.: 6.887 min
Delta R.T.: 0.008 min
Response: 235123
Conc: 84.13 ng/ml

Instrument :
ECD_O
ClientSampleId :
FK-SF-03-007-A

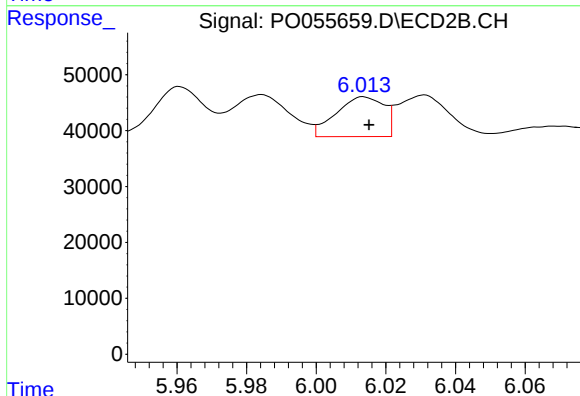


#28 AR-1254-3

R.T.: 6.014 min
Delta R.T.: -0.002 min
Response: 67998
Conc: 22.11 ng/ml

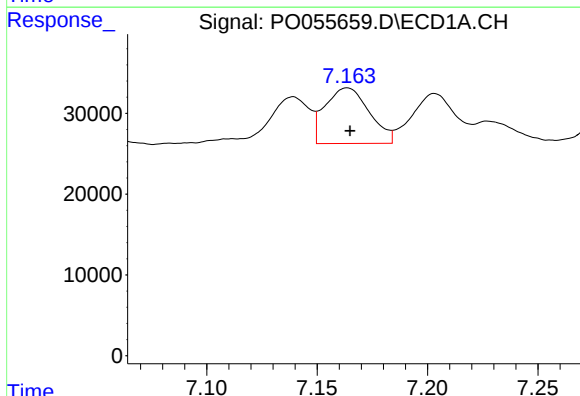


#29 AR-1254-4

R.T.: 7.164 min
Delta R.T.: -0.001 min
Response: 95931
Conc: 43.08 ng/ml

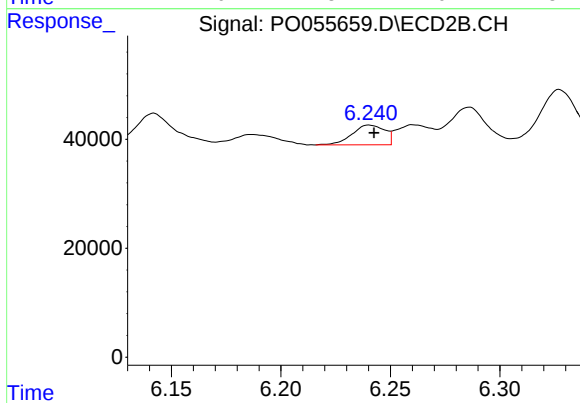

#29 AR-1254-4


R.T.: 6.240 min
Delta R.T.: -0.002 min
Response: 37748
Conc: 17.66 ng/ml

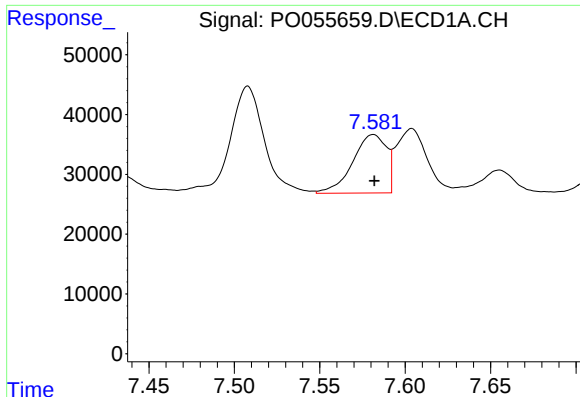

#30 AR-1254-5


R.T.: 7.581 min
Delta R.T.: 0.000 min
Response: 134543
Conc: 53.67 ng/ml

Instrument :
ECD_O
ClientSampleId :
FK-SF-03-007-A

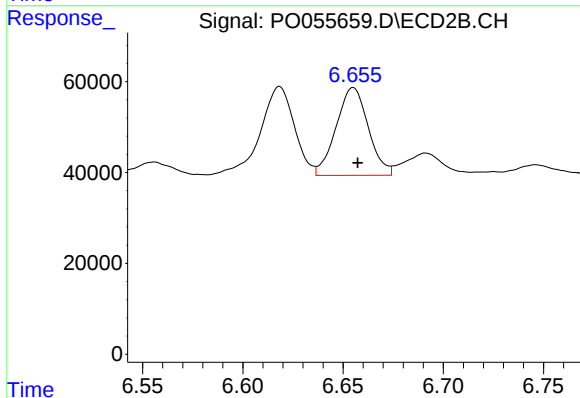


#30 AR-1254-5

R.T.: 6.655 min
Delta R.T.: -0.002 min
Response: 216429
Conc: 73.87 ng/ml

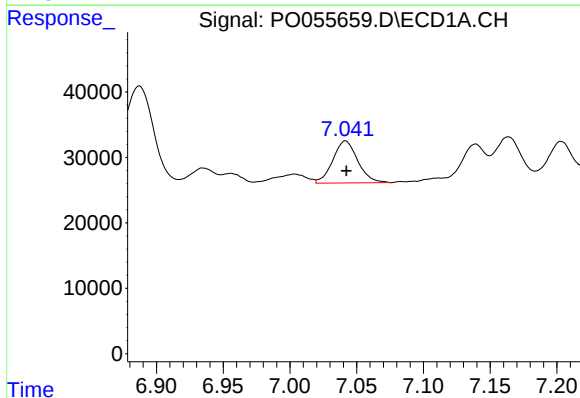


#31 AR-1260-1

R.T.: 7.042 min
Delta R.T.: 0.000 min
Response: 83863
Conc: 40.82 ng/ml

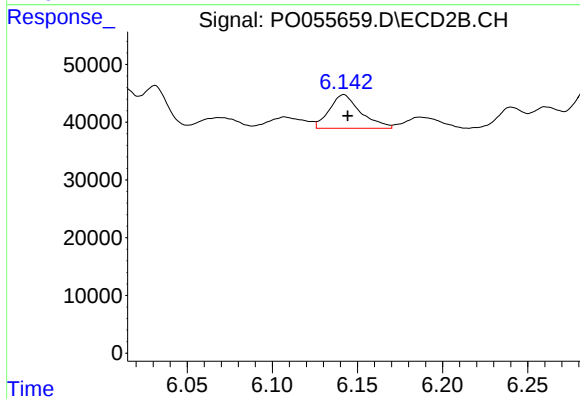

#31 AR-1260-1


R.T.: 6.142 min
Delta R.T.: -0.002 min
Response: 74770
Conc: 38.57 ng/ml

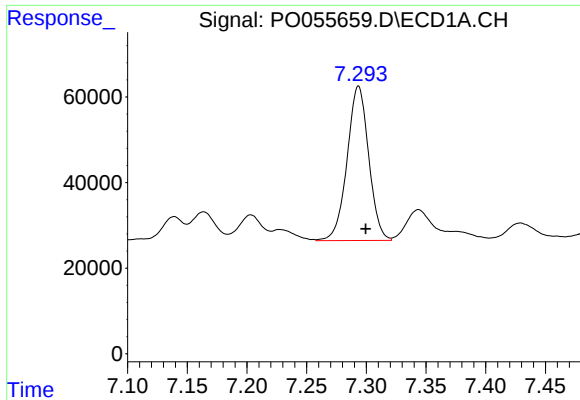

#32 AR-1260-2


R.T.: 7.293 min
Delta R.T.: -0.006 min
Response: 454433
Conc: 179.25 ng/ml

Instrument :
ECD_O
ClientSampleId :
FK-SF-03-007-A

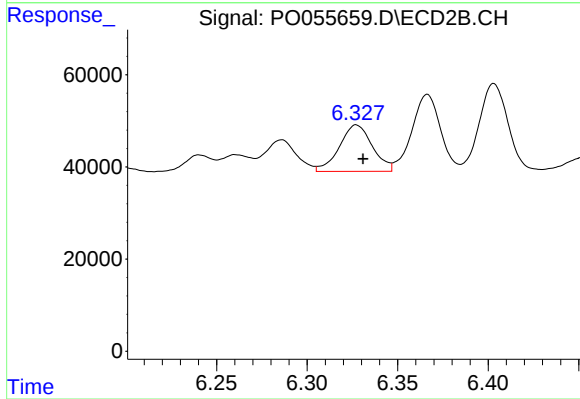


#32 AR-1260-2

R.T.: 6.327 min
Delta R.T.: -0.004 min
Response: 127646
Conc: 49.05 ng/ml

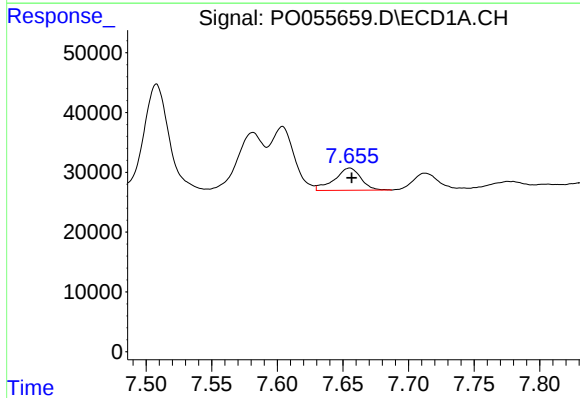


#33 AR-1260-3

R.T.: 7.655 min
Delta R.T.: -0.002 min
Response: 52522
Conc: 25.57 ng/ml

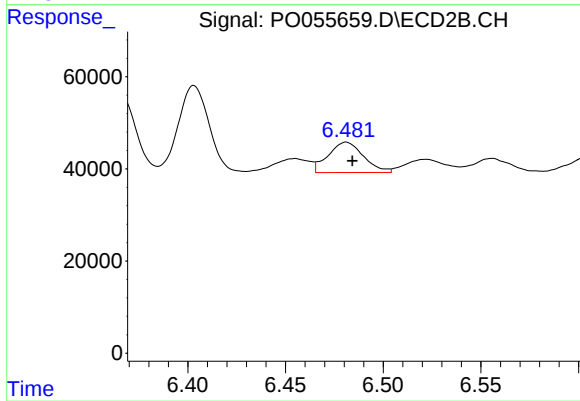

#33 AR-1260-3


R.T.: 6.481 min
Delta R.T.: -0.003 min
Response: 83379
Conc: 36.66 ng/ml

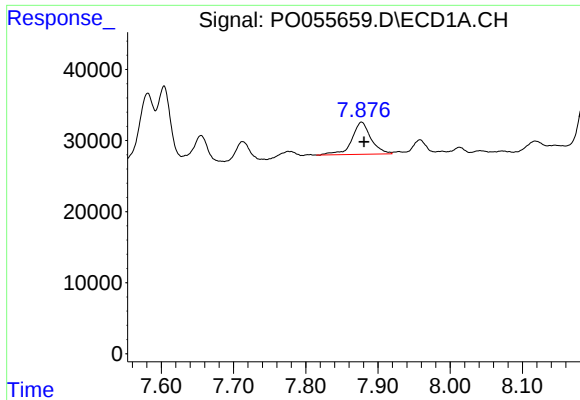

#34 AR-1260-4


R.T.: 7.877 min
Delta R.T.: -0.003 min
Response: 82881
Conc: 34.72 ng/ml

Instrument :
ECD_O
ClientSampleId :
FK-SF-03-007-A

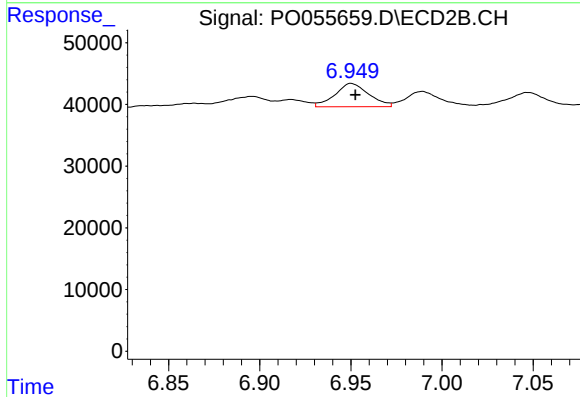


#34 AR-1260-4

R.T.: 6.950 min
Delta R.T.: -0.002 min
Response: 48795
Conc: 24.30 ng/ml

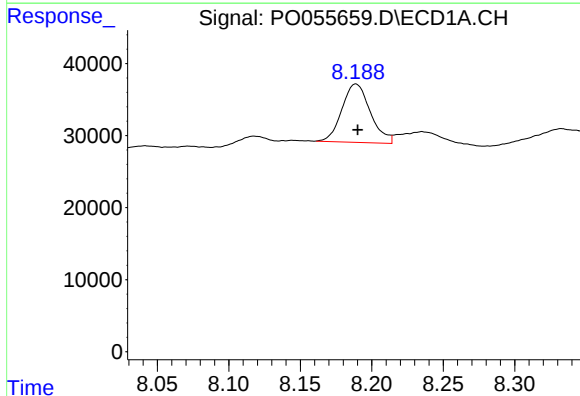


#35 AR-1260-5

R.T.: 8.189 min
Delta R.T.: -0.001 min
Response: 112340
Conc: 24.35 ng/ml

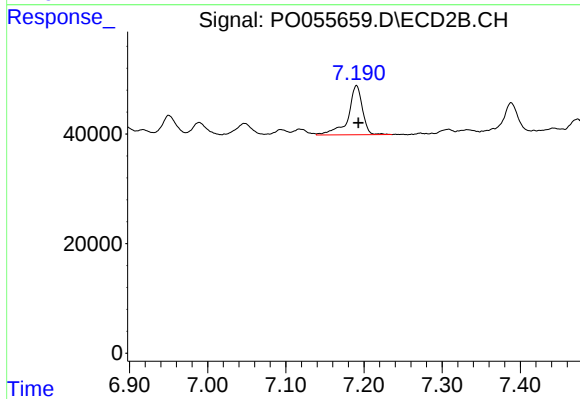

#35 AR-1260-5


R.T.: 7.190 min
Delta R.T.: -0.002 min
Response: 114255
Conc: 22.99 ng/ml

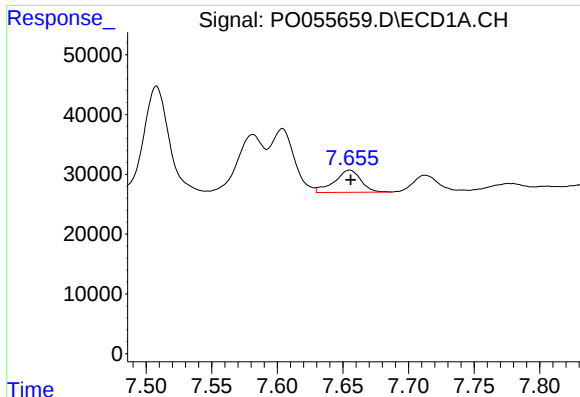

#36 AR-1262-1


R.T.: 7.655 min
Delta R.T.: 0.000 min
Response: 52522
Conc: 17.07 ng/ml

Instrument :
ECD_O
ClientSampleId :
FK-SF-03-007-A

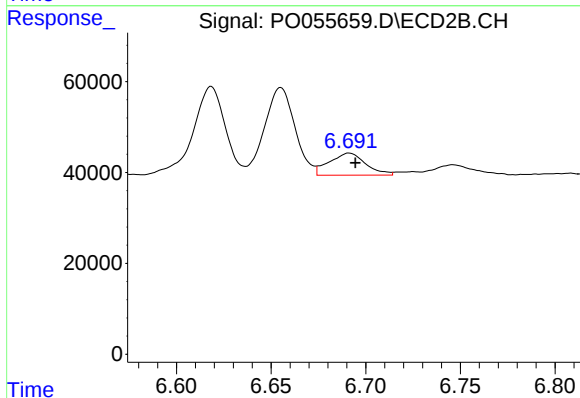


#36 AR-1262-1

R.T.: 6.691 min
Delta R.T.: -0.003 min
Response: 65631
Conc: 19.20 ng/ml

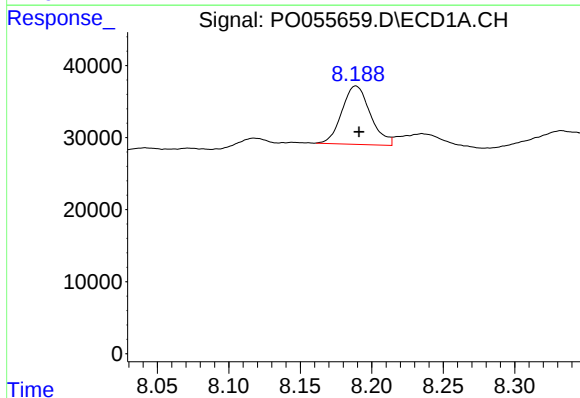


#37 AR-1262-2

R.T.: 8.189 min
Delta R.T.: -0.002 min
Response: 112340
Conc: 20.45 ng/ml

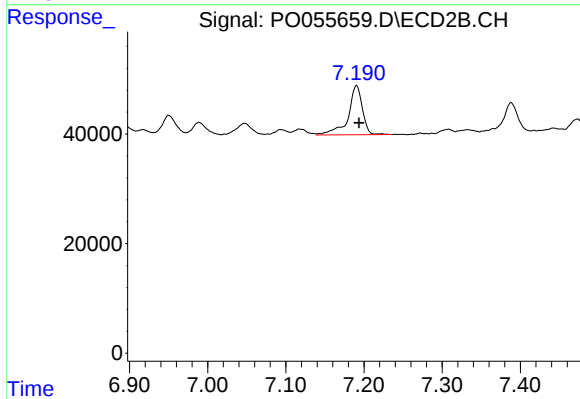

#37 AR-1262-2


R.T.: 7.190 min
Delta R.T.: -0.003 min
Response: 114255
Conc: 20.17 ng/ml

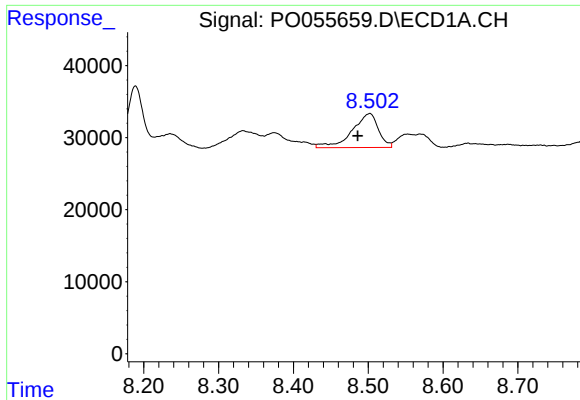

#38 AR-1262-3


R.T.: 8.502 min
Delta R.T.: 0.016 min
Response: 115006
Conc: 30.10 ng/ml

Instrument :
ECD_O
ClientSampleId :
FK-SF-03-007-A

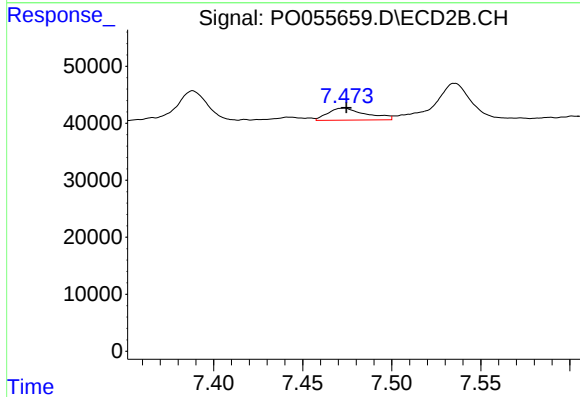


#38 AR-1262-3

R.T.: 7.473 min
Delta R.T.: -0.001 min
Response: 31758
Conc: 13.66 ng/ml

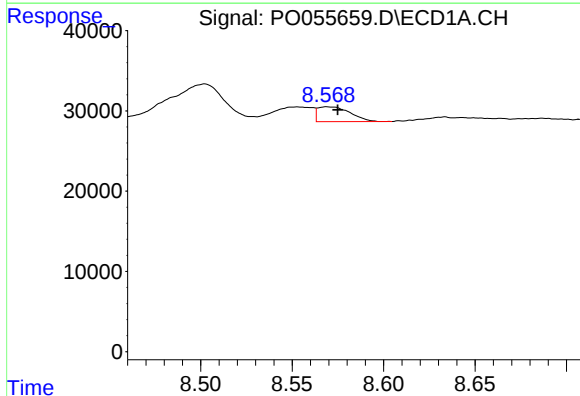


#39 AR-1262-4

R.T.: 8.569 min
Delta R.T.: -0.006 min
Response: 22731
Conc: 7.89 ng/ml

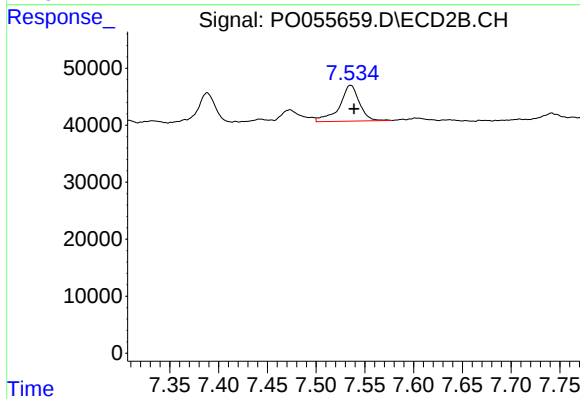

#39 AR-1262-4


R.T.: 7.535 min
Delta R.T.: -0.004 min
Response: 89819
Conc: 22.90 ng/ml

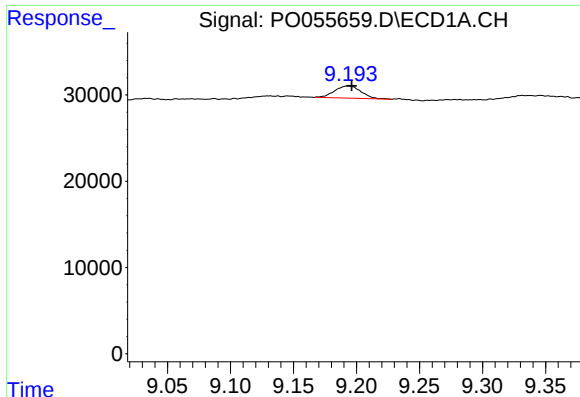

#40 AR-1262-5


R.T.: 9.194 min
Delta R.T.: -0.002 min
Response: 20808
Conc: 10.73 ng/ml

Instrument :
ECD_O
ClientSampleId :
FK-SF-03-007-A

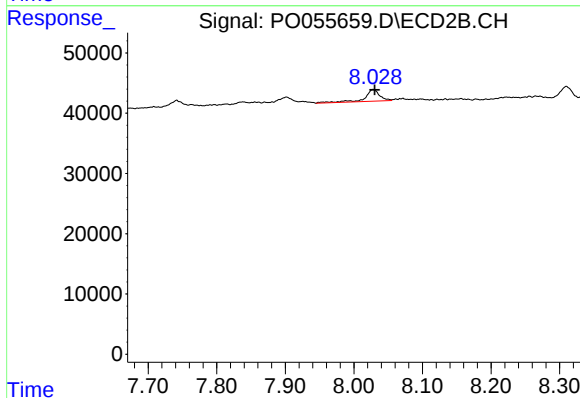


#40 AR-1262-5

R.T.: 8.028 min
Delta R.T.: -0.003 min
Response: 29500
Conc: 16.65 ng/ml

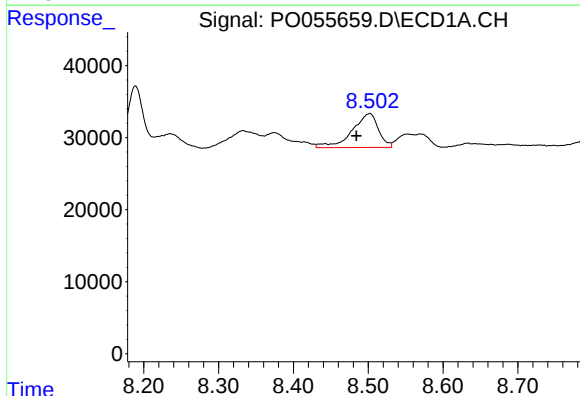


#41 AR-1268-1

R.T.: 8.502 min
Delta R.T.: 0.018 min
Response: 115006
Conc: 18.19 ng/ml

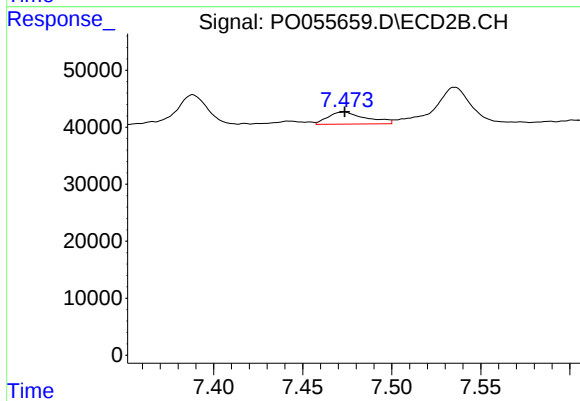

#41 AR-1268-1


R.T.: 7.473 min
Delta R.T.: 0.000 min
Response: 31758
Conc: 4.87 ng/ml

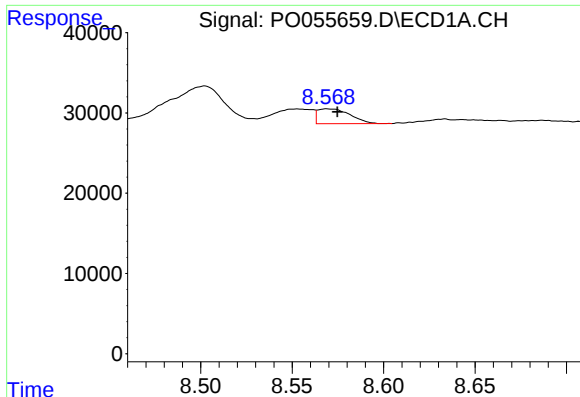

#42 AR-1268-2


R.T.: 8.569 min
Delta R.T.: -0.006 min
Response: 22731
Conc: 3.93 ng/ml

Instrument :
ECD_O
ClientSampleId :
FK-SF-03-007-A

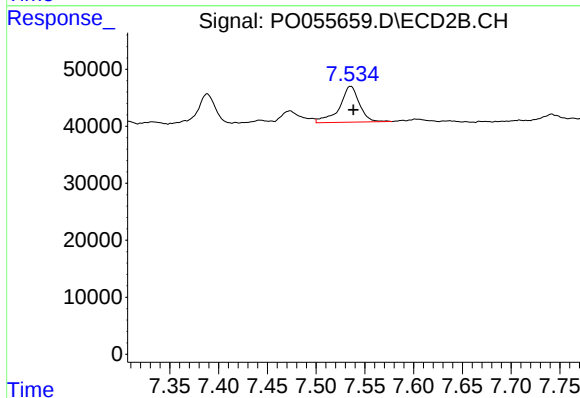


#42 AR-1268-2

R.T.: 7.535 min
Delta R.T.: -0.003 min
Response: 89819
Conc: 16.08 ng/ml

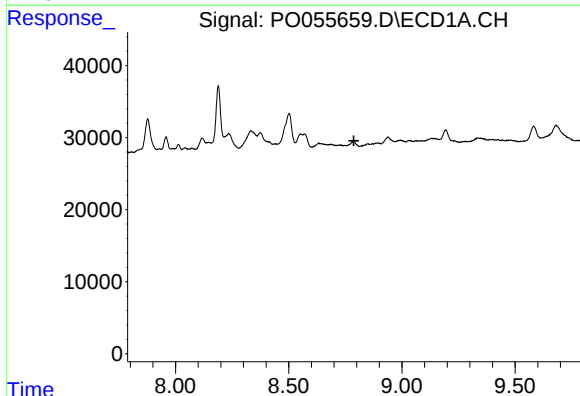


#43 AR-1268-3

R.T.: 0.000 min
Exp R.T. : 8.788 min
Response: 0
Conc: N.D.

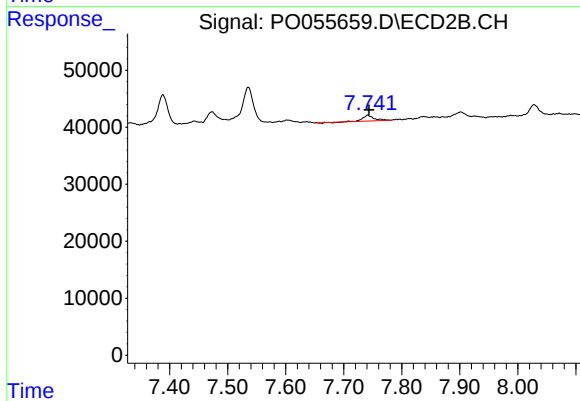

#43 AR-1268-3


R.T.: 7.742 min
Delta R.T.: -0.002 min
Response: 13398
Conc: 2.88 ng/ml

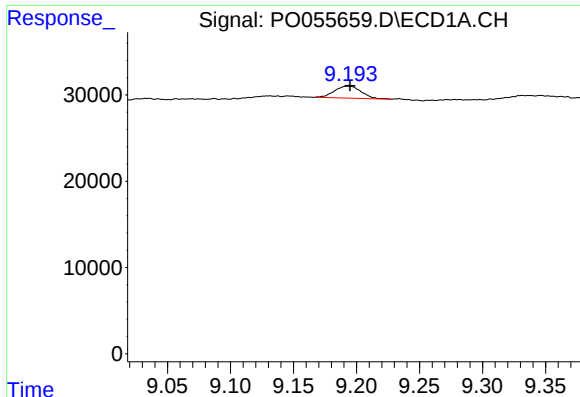

#44 AR-1268-4


R.T.: 9.194 min
Delta R.T.: -0.001 min
Response: 20808
Conc: 9.73 ng/ml

Instrument :
ECD_O
ClientSampleId :
FK-SF-03-007-A

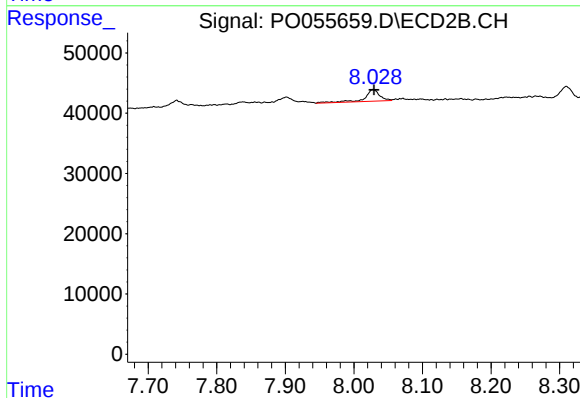


#44 AR-1268-4

R.T.: 8.028 min
Delta R.T.: -0.001 min
Response: 29500
Conc: 15.28 ng/ml

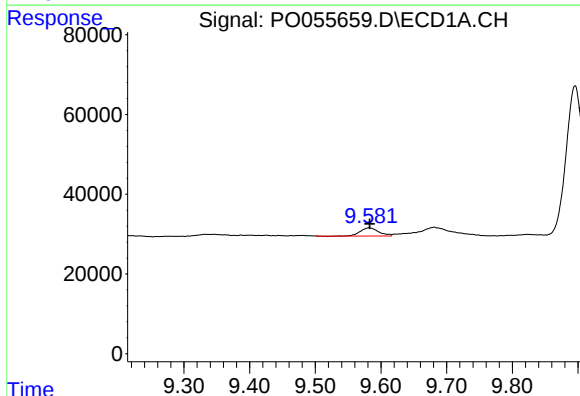

#45 AR-1268-5

R.T.: 9.582 min
Delta R.T.: -0.001 min
Response: 39648
Conc: 2.75 ng/ml

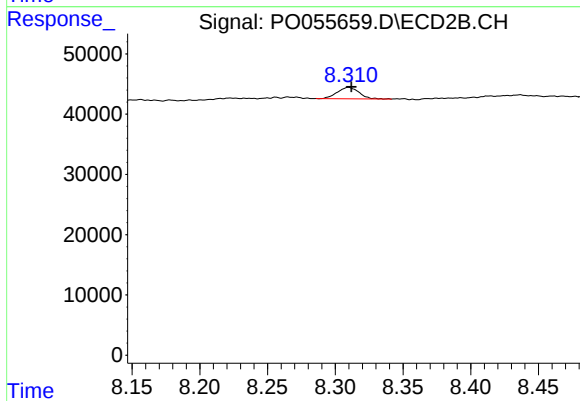

#45 AR-1268-5

R.T.: 8.310 min
Delta R.T.: -0.002 min
Response: 21336
Conc: 1.78 ng/ml