

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\P0042519\
Data File : P0055642.D
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
Acq On : 25 Apr 2019 9:29
Operator : SM/SJ
Sample : K2532-15
Misc :
ALS Vial : 7 Sample Multiplier: 1

Instrument :
ECD_O
ClientSampleId :
TP-17

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Apr 25 11:17:47 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\P0042419.M
Quant Title : GC EXTRACTABLES
QLast Update : Thu Apr 25 01:58:33 2019
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	4.284	3.597	443328	455566	17.497	18.707
2) SA Decachlor...	9.892	8.553	506706	374245	11.808	12.175

Target Compounds



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\P0042519\
Data File : P0055642.D
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
Acq On : 25 Apr 2019 9:29
Operator : SM/SJ
Sample : K2532-15
Misc :
ALS Vial : 7 Sample Multiplier: 1

Instrument :
ECD_O
ClientSampleId :
TP-17

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Apr 25 11:17:47 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\P0042419.M
Quant Title : GC EXTRACTABLES
QLast Update : Thu Apr 25 01:58:33 2019
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

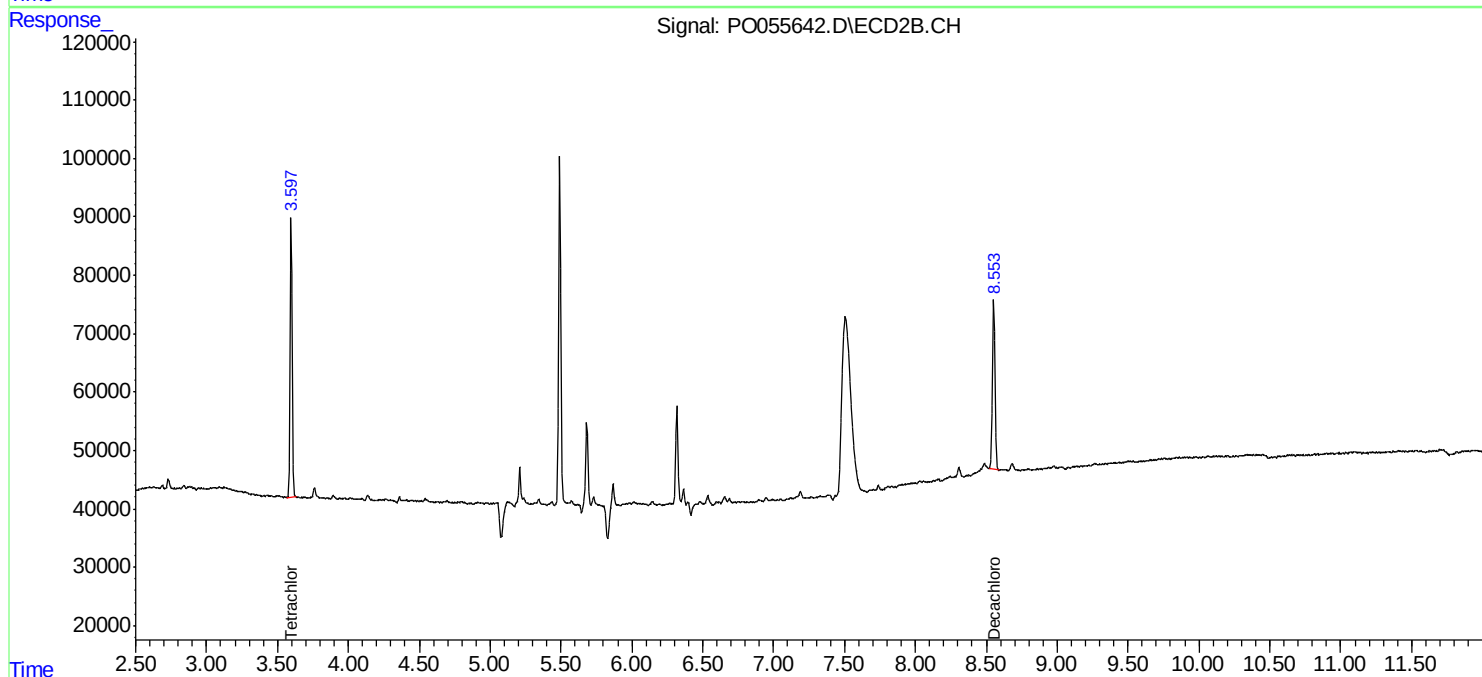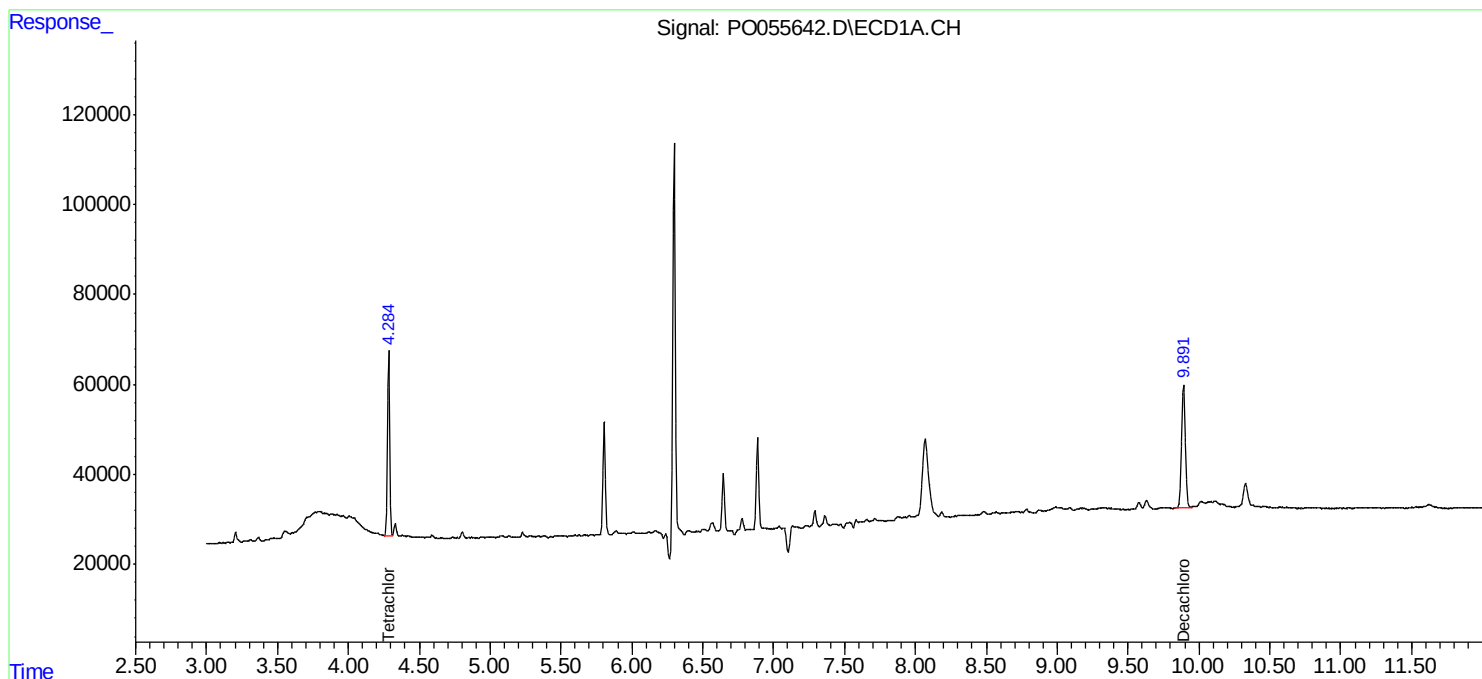


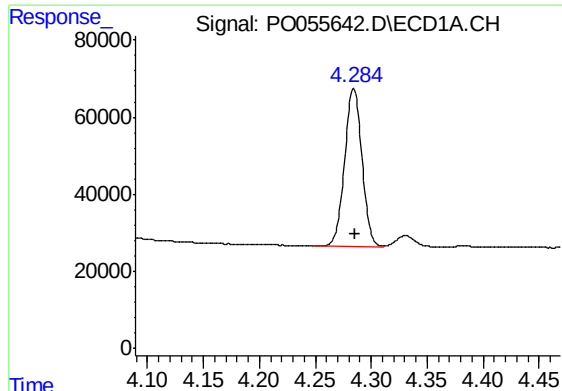

#1 Tetrachloro-m-xylene


R.T.: 4.284 min
Delta R.T.: -0.002 min
Response: 443328
Conc: 17.50 ng/ml

Instrument :
ECD_O
ClientSampleId :
TP-17

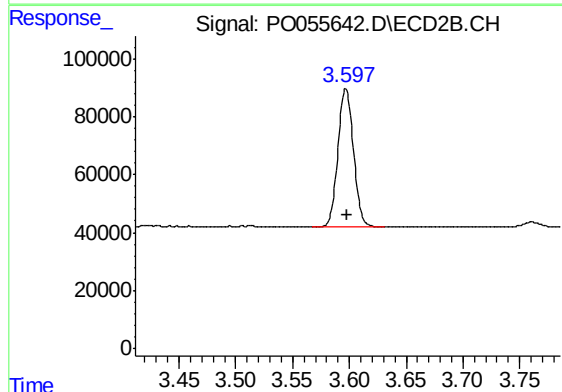


#1 Tetrachloro-m-xylene

R.T.: 3.597 min
Delta R.T.: -0.001 min
Response: 455566
Conc: 18.71 ng/ml

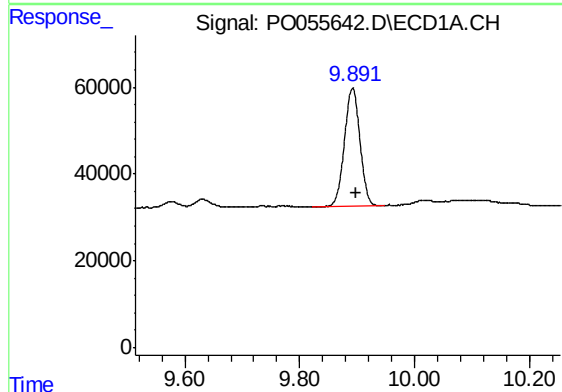

#2 Decachlorobiphenyl

R.T.: 9.892 min
Delta R.T.: -0.006 min
Response: 506706
Conc: 11.81 ng/ml

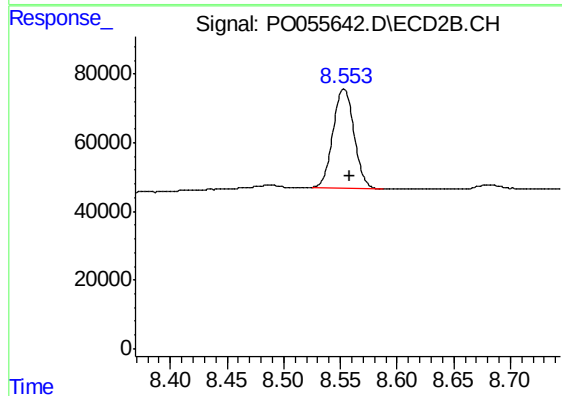

#2 Decachlorobiphenyl

R.T.: 8.553 min
Delta R.T.: -0.005 min
Response: 374245
Conc: 12.17 ng/ml