

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\P0042519\
 Data File : P0055648.D
 Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
 Acq On : 25 Apr 2019 11:36
 Operator : SM/SJ
 Sample : K2542-03
 Misc :
 ALS Vial : 6 Sample Multiplier: 1

Instrument :
 ECD_O
 ClientSampleId :
 TP-6

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Apr 26 00:40:03 2019
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\P0042419.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Thu Apr 25 01:58:33 2019
 Response via : Initial Calibration
 Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	4.285	3.596	530356	532554	20.931	21.868
2)	SA Decachlor...	9.892	8.553	591447	428282	13.782	13.933

Target Compounds



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\P0042519\
Data File : P0055648.D
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
Acq On : 25 Apr 2019 11:36
Operator : SM/SJ
Sample : K2542-03
Misc :
ALS Vial : 6 Sample Multiplier: 1

Instrument :
ECD_O
ClientSampleId :
TP-6

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Apr 26 00:40:03 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\P0042419.M
Quant Title : GC EXTRACTABLES
QLast Update : Thu Apr 25 01:58:33 2019
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

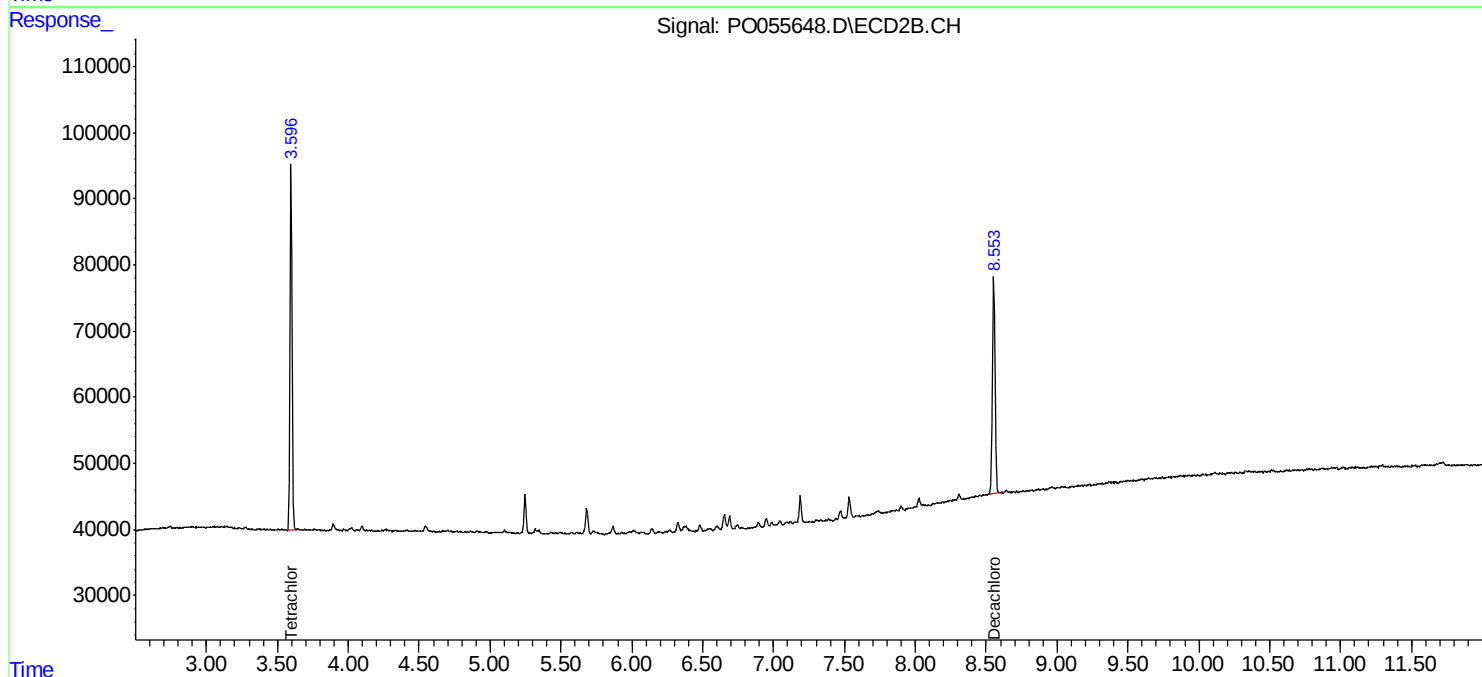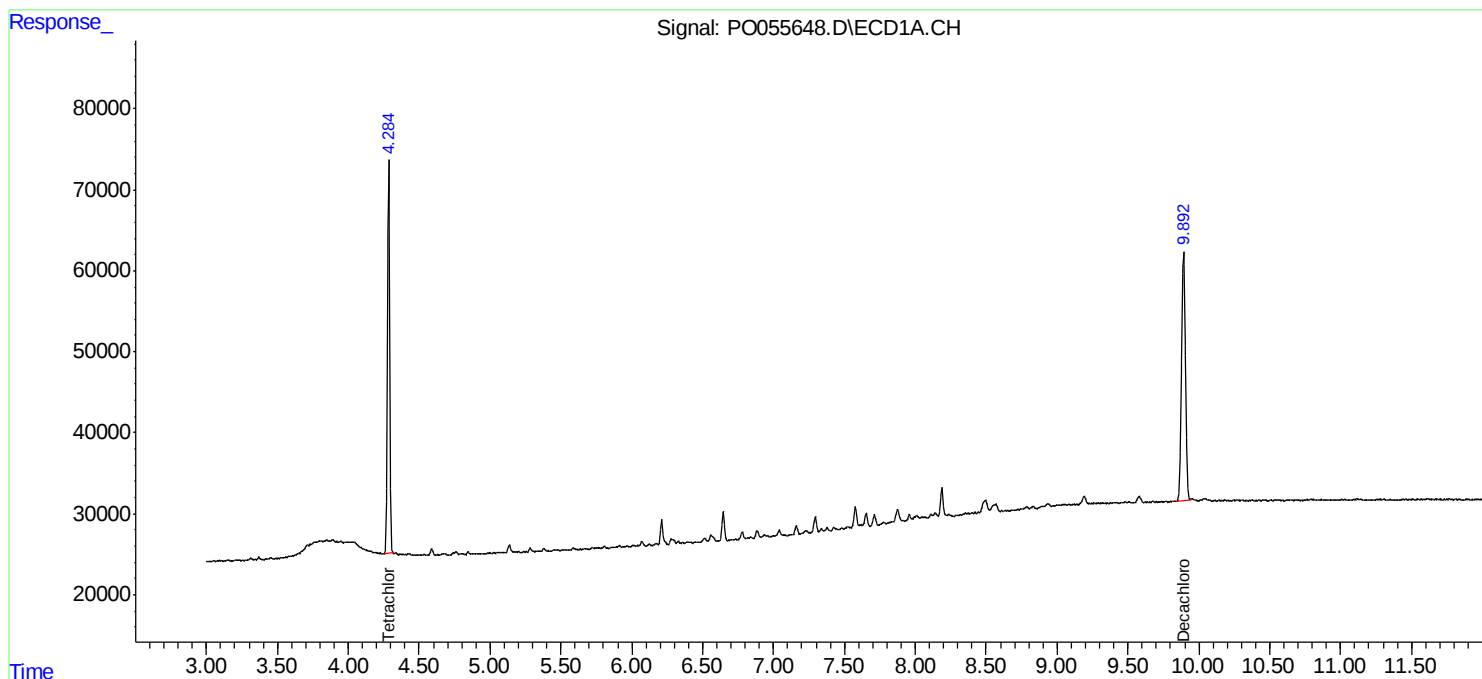


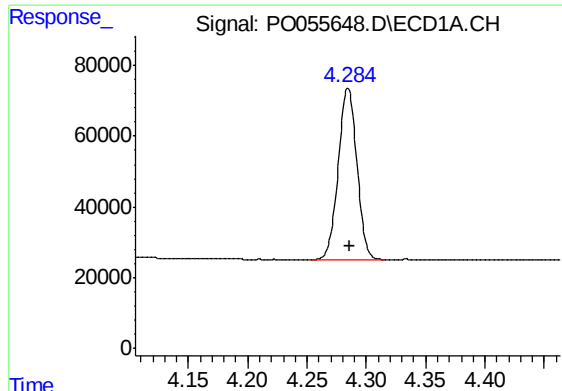

#1 Tetrachloro-m-xylene


R.T.: 4.285 min
Delta R.T.: -0.001 min
Response: 530356
Conc: 20.93 ng/ml

Instrument :
ECD_O
ClientSampleId :
TP-6

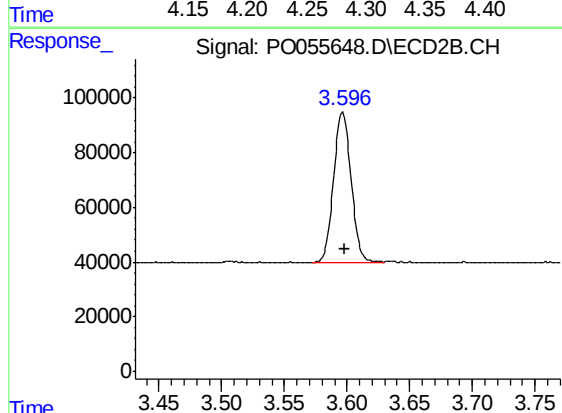


#1 Tetrachloro-m-xylene

R.T.: 3.596 min
Delta R.T.: -0.002 min
Response: 532554
Conc: 21.87 ng/ml

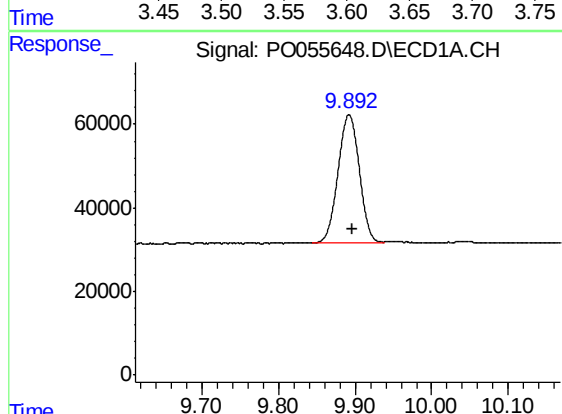

#2 Decachlorobiphenyl

R.T.: 9.892 min
Delta R.T.: -0.005 min
Response: 591447
Conc: 13.78 ng/ml

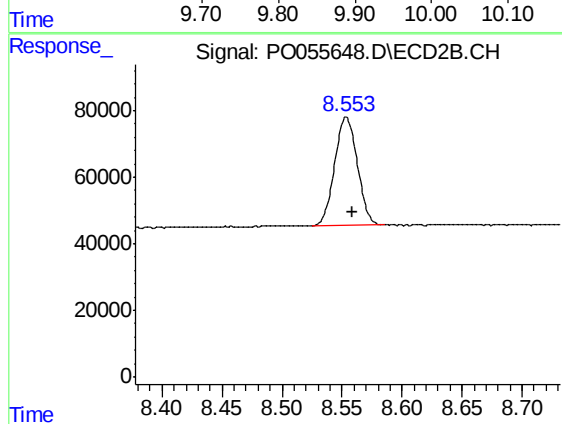

#2 Decachlorobiphenyl

R.T.: 8.553 min
Delta R.T.: -0.005 min
Response: 428282
Conc: 13.93 ng/ml