

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\P0042519\
 Data File : P0055671.D
 Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
 Acq On : 25 Apr 2019 18:29
 Operator : SM/SJ
 Sample : K2593-01
 Misc :
 ALS Vial : 15 Sample Multiplier: 1

Instrument :
 ECD_O
 ClientSampleId :
 K2593-01

Manual Integrations
 APPROVED

Sohil
 4/26/2019 5:52:23 PM

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Apr 26 00:50:32 2019
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\P0042419.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Thu Apr 25 01:58:33 2019
 Response via : Initial Calibration
 Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	4.286	3.599	656383	708616	25.905	29.098
2)	SA Decachlor...	9.892	8.555	487275	338202	11.355m	11.002m

Target Compounds

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\P0042519\
Data File : P0055671.D
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
Acq On : 25 Apr 2019 18:29
Operator : SM/SJ
Sample : K2593-01
Misc :
ALS Vial : 15 Sample Multiplier: 1



Instrument :
ECD_O
ClientSampleId :
K2593-01


Manual Integrations
APPROVED

Sohil
4/26/2019 5:52:23 PM

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Apr 26 00:50:32 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\P0042419.M
Quant Title : GC EXTRACTABLES
QLast Update : Thu Apr 25 01:58:33 2019
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

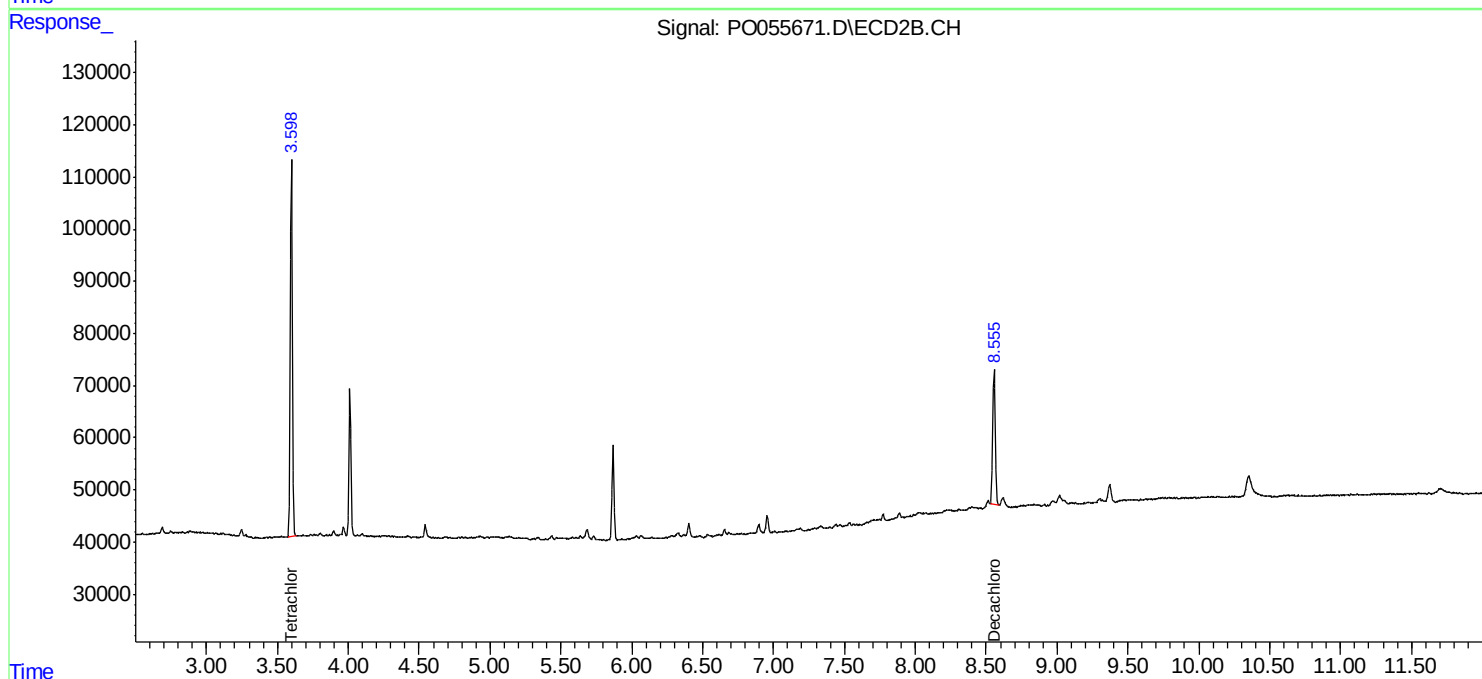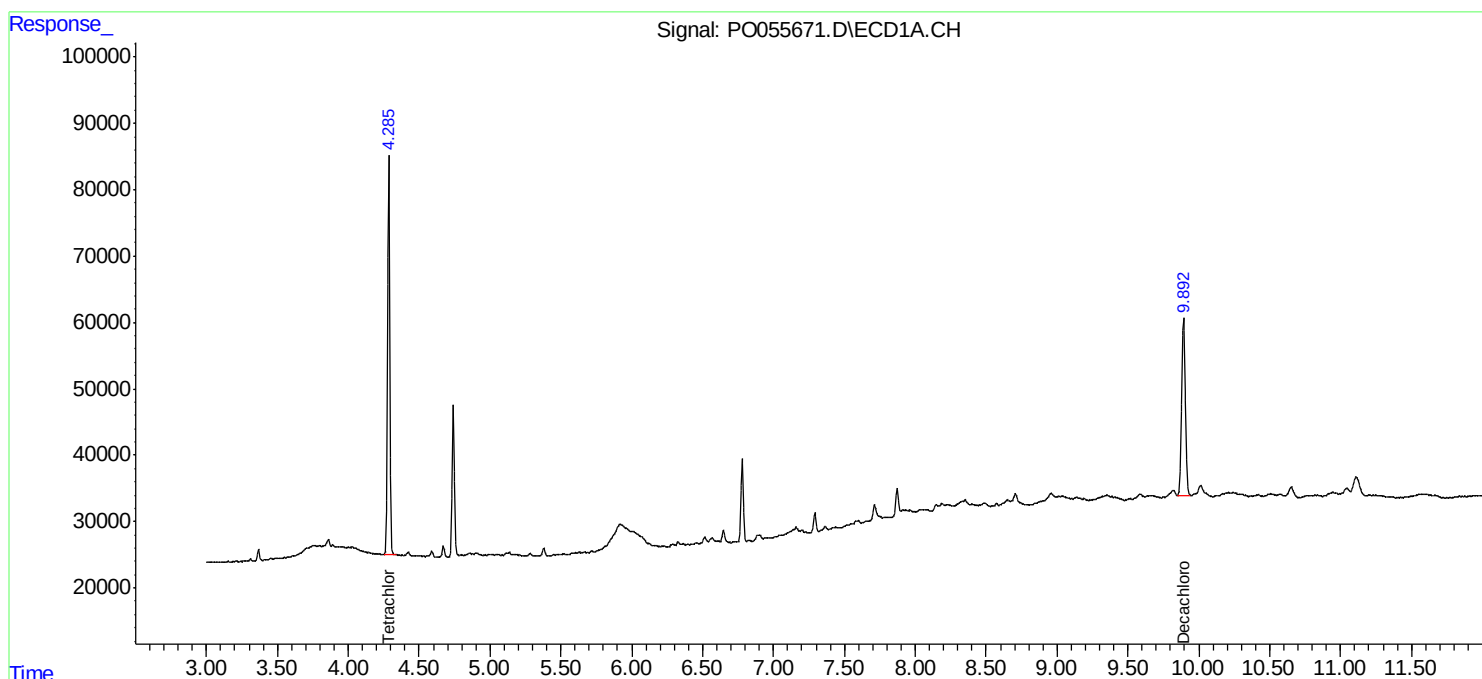

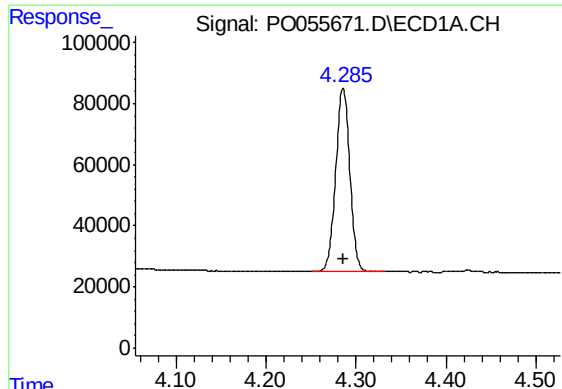


#1 Tetrachloro-m-xylene

R.T.: 4.286 min
Delta R.T.: 0.000 min
Response: 656383
Conc: 25.91 ng/ml

Instrument :
ECD_O
ClientSampleId :
K2593-01


Manual Integrations
APPROVED

Sohil
4/26/2019 5:52:23 PM

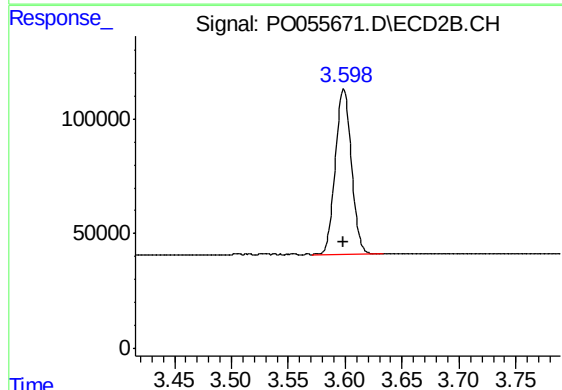


#1 Tetrachloro-m-xylene

R.T.: 3.599 min
Delta R.T.: 0.000 min
Response: 708616
Conc: 29.10 ng/ml

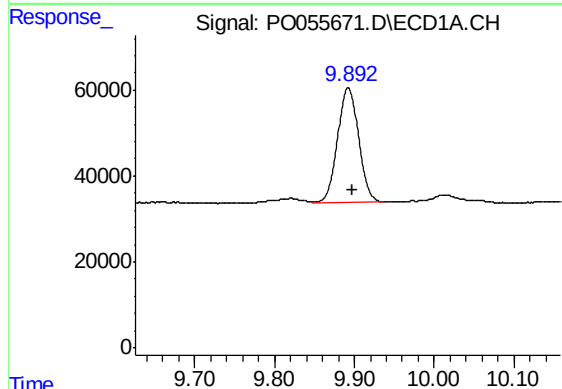

#2 Decachlorobiphenyl

R.T.: 9.892 min
Delta R.T.: -0.005 min
Response: 487275
Conc: 11.35 ng/ml m

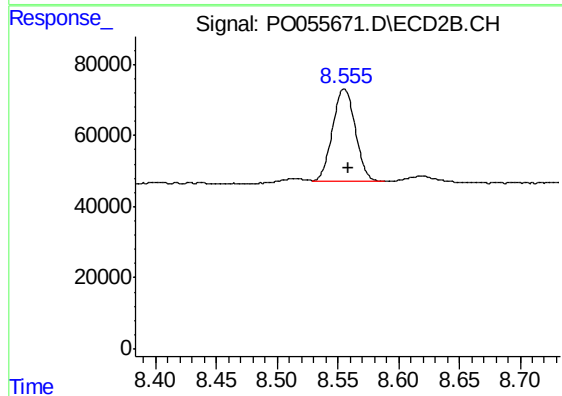

#2 Decachlorobiphenyl

R.T.: 8.555 min
Delta R.T.: -0.004 min
Response: 338202
Conc: 11.00 ng/ml m