

Data Path : P:\HPCHEM1\ECD_D\Data\PD042618\
 Data File : PD047280.D
 Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
 Acq On : 26 Apr 2018 10:05
 Operator : UA/AJ
 Sample : HEXANE
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 ECD_O
 ClientSampleId :
 HEXANE

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Apr 27 00:57:00 2018
 Quant Method : P:\HPCHEM1\ECD_D\Method\PD042518CLP.M
 Quant Title : GC Extractables
 QLast Update : Thu Apr 26 02:00:29 2018
 Response via : Initial Calibration
 Integrator: ChemStation 6890 Scale Mode: Large solvent peaks clipped

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
Target Compounds						
2) A alpha-BHC	0.000	4.454f	0	795831	N.D.	<MDL
7) B delta-BHC	0.000	5.082	0	10220038	N.D.	0.324
8) B Heptachlo...	0.000	5.908	0	32755214	N.D.	1.263
10) B trans-Chl...	0.000	6.109f	0	1582309	N.D.	<MDL


(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : P:\HPCHEM1\ECD_D\Data\PD042618\
Data File : PD047280.D
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
Acq On : 26 Apr 2018 10:05
Operator : UA/AJ
Sample : HEXANE
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
ECD_O
ClientSampleId :
HEXANE

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Apr 27 00:57:00 2018
Quant Method : P:\HPCHEM1\ECD_D\Method\PD042518CLP.M
Quant Title : GC Extractables
QLast Update : Thu Apr 26 02:00:29 2018
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Large solvent peaks clipped

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

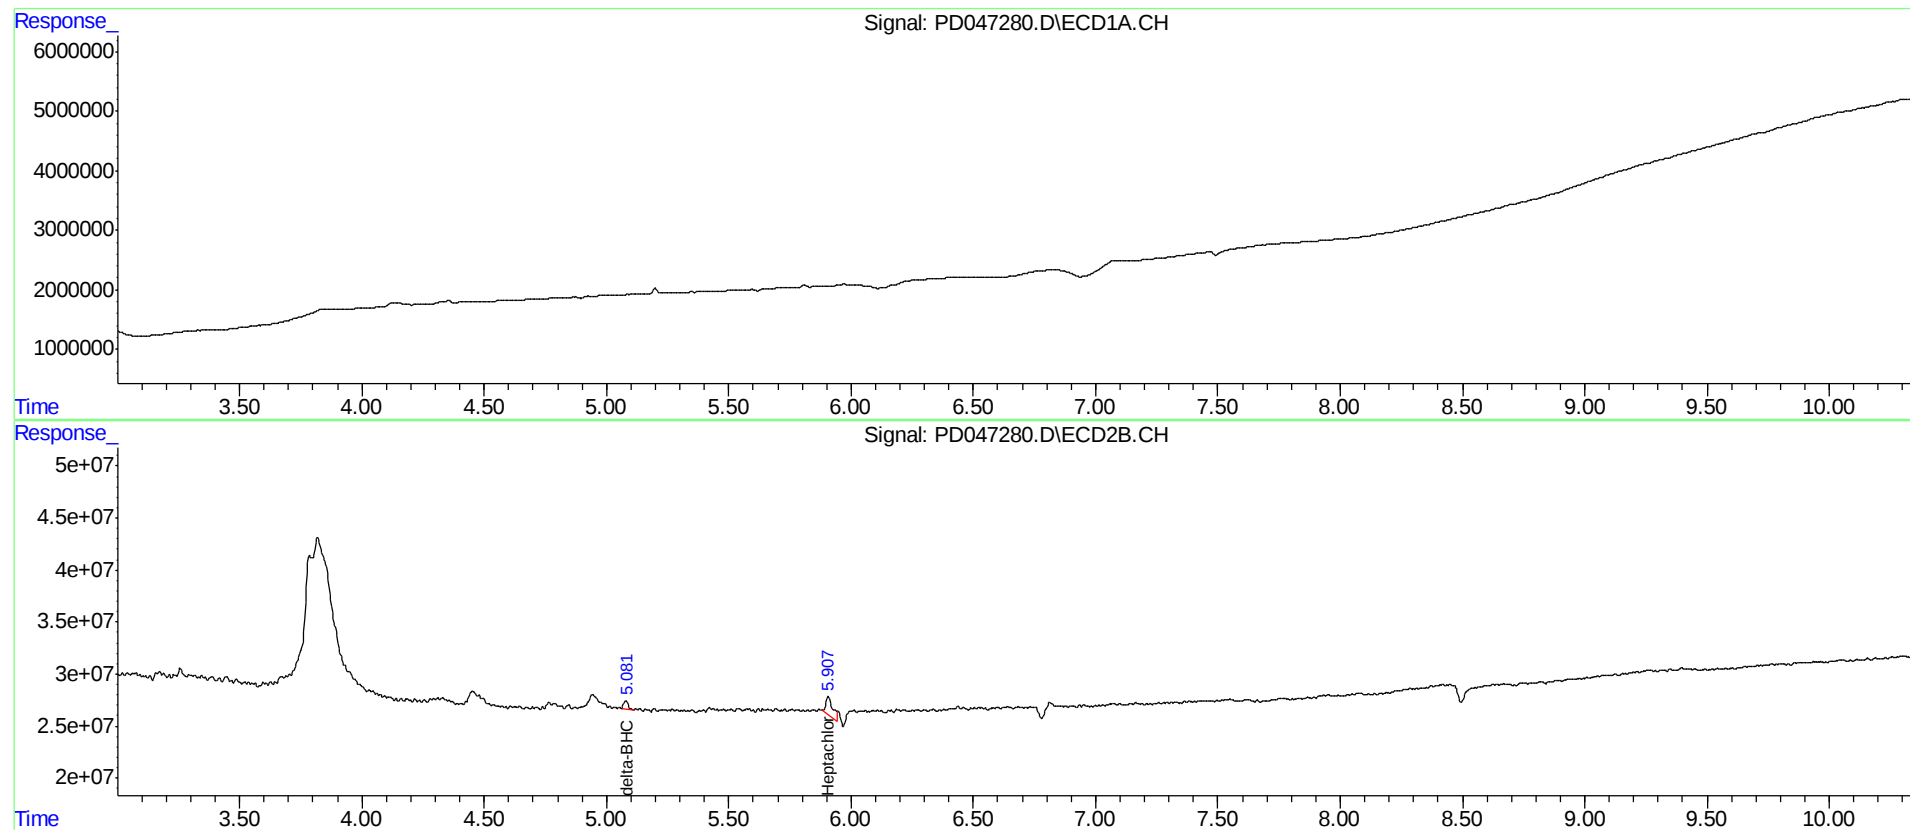


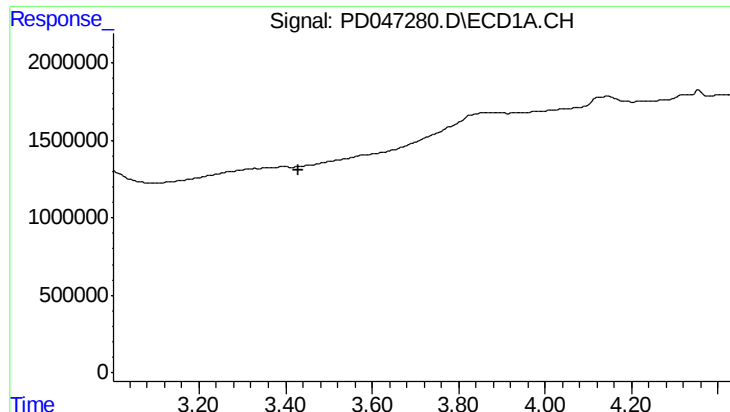

#1 Tetrachloro-m-xylene


R.T.: 0.000 min
Exp R.T.: 3.429 min
Response: 0
Conc: N.D.

Instrument :
ECD_O
ClientSampleId :
HEXANE

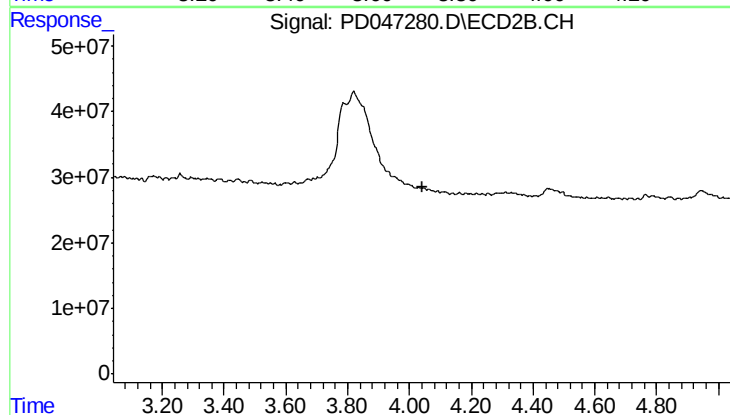


#1 Tetrachloro-m-xylene

R.T.: 0.000 min
Exp R.T.: 4.041 min
Response: 0
Conc: N.D.

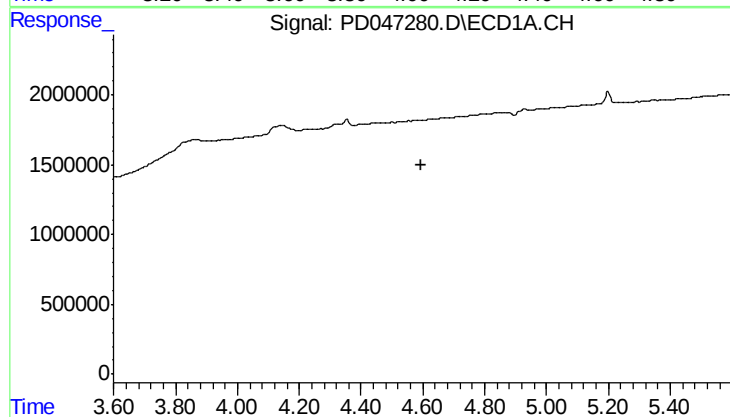


#7 delta-BHC

R.T.: 0.000 min
Exp R.T.: 4.596 min
Response: 0
Conc: N.D.

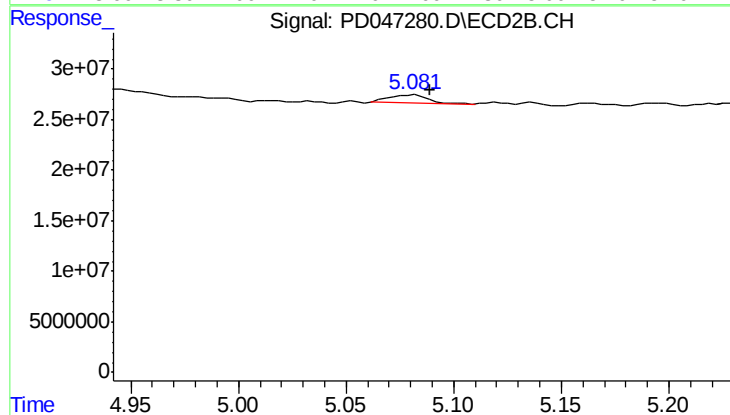

#7 delta-BHC


R.T.: 5.082 min
Delta R.T.: -0.007 min
Response: 10220038
Conc: 0.32 ng/ml

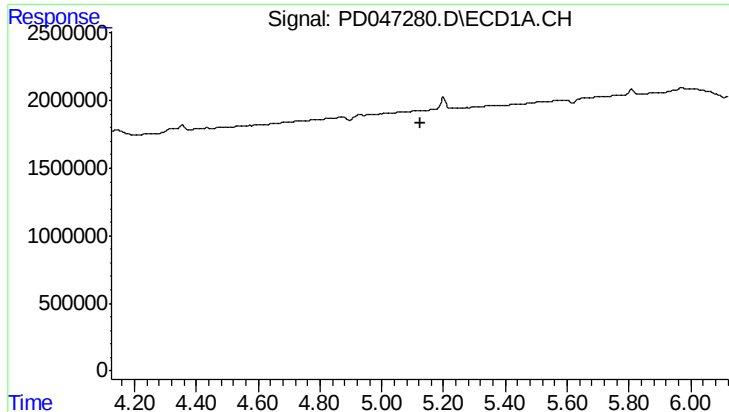

#8 Heptachlor epoxide


R.T.: 0.000 min
Exp R.T.: 5.125 min
Response: 0
Conc: N.D.

Instrument :
ECD_O
ClientSampleId :
HEXANE

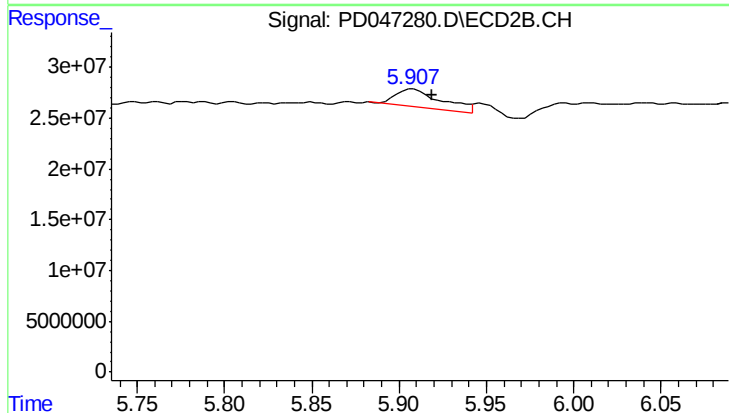


#8 Heptachlor epoxide

R.T.: 5.908 min
Delta R.T.: -0.011 min
Response: 32755214
Conc: 1.26 ng/ml

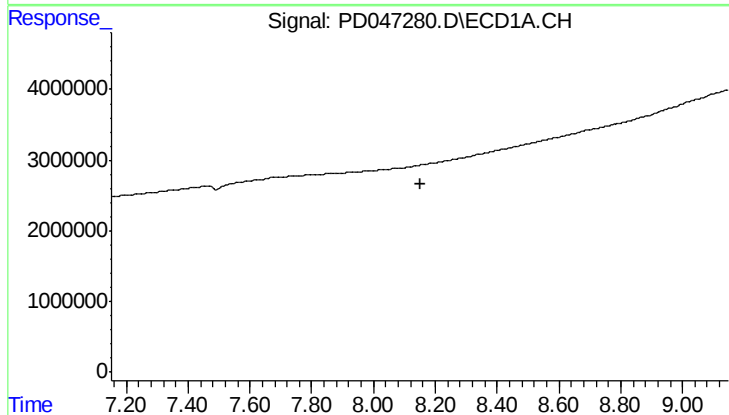

#27 Decachlorobiphenyl

R.T.: 0.000 min
Exp R.T.: 8.151 min
Response: 0
Conc: N.D.

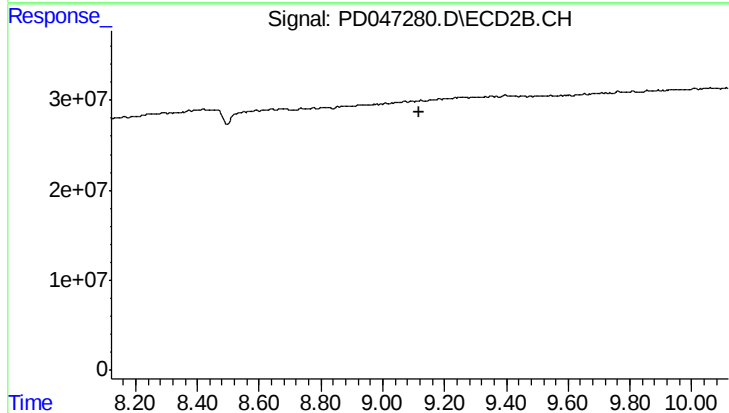

#27 Decachlorobiphenyl

R.T.: 0.000 min
Exp R.T.: 9.120 min
Response: 0
Conc: N.D.