

Data Path : P:\HPCHEM1\ECD_D\Data\PD042618\
 Data File : PD047286.D
 Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
 Acq On : 26 Apr 2018 12:03
 Operator : UA/AJ
 Sample : J2440-04
 Misc :
 ALS Vial : 7 Sample Multiplier: 1

Instrument :
 ECD_O
 ClientSampleId :
 A3Y20

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Apr 27 01:02:45 2018
 Quant Method : P:\HPCHEM1\ECD_D\Method\PD042518CLP.M
 Quant Title : GC Extractables
 QLast Update : Thu Apr 26 02:00:29 2018
 Response via : Initial Calibration
 Integrator: ChemStation 6890 Scale Mode: Large solvent peaks clipped

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	3.429	4.041	15918344	266.0E6	12.774	12.466
27)	SA Decachlor...	8.151	9.121	27146079	414.5E6	19.621	21.770
Target Compounds							
2)	A alpha-BHC	0.000	4.431	0	19432219	N.D.	0.593
3)	MA gamma-BHC...	0.000	4.682f	0	2519981	N.D.	<MDL
6)	B beta-BHC	4.358f	0.000	3438527	0	4.413	N.D. #
7)	B delta-BHC	0.000	5.080	0	40609360	N.D.	1.289
9)	A Endosulfan I	0.000	6.302	0	9128377	N.D.	0.375
10)	B trans-Chl...	0.000	6.116f	0	19303910	N.D.	0.769
14)	MA Endrin	0.000	6.816f	0	6581946	N.D.	0.358
15)	B Endosulfa...	0.000	6.940	0	3367330	N.D.	0.159
16)	A 4,4'-DDD	0.000	6.816f	0	6581946	N.D.	0.333


(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : P:\HPCHEM1\ECD_D\Data\PD042618\
Data File : PD047286.D
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
Acq On : 26 Apr 2018 12:03
Operator : UA/AJ
Sample : J2440-04
Misc :
ALS Vial : 7 Sample Multiplier: 1

Instrument :
ECD_O
ClientSampleId :
A3Y20

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Apr 27 01:02:45 2018
Quant Method : P:\HPCHEM1\ECD_D\Method\PD042518CLP.M
Quant Title : GC Extractables
QLast Update : Thu Apr 26 02:00:29 2018
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Large solvent peaks clipped

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

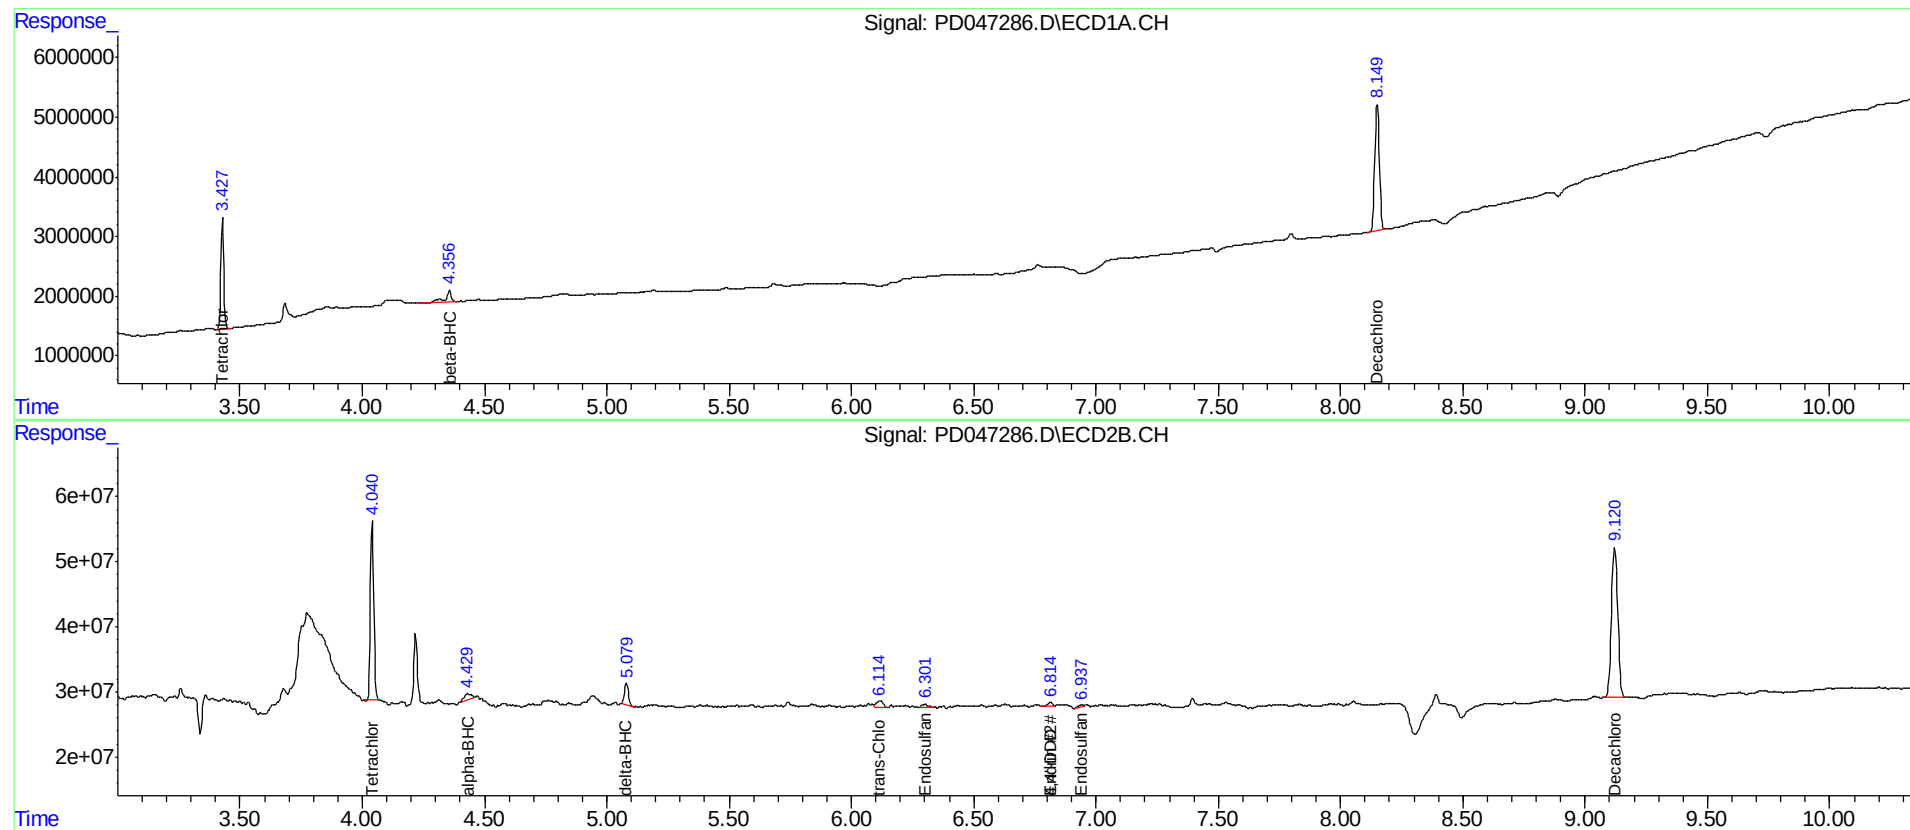


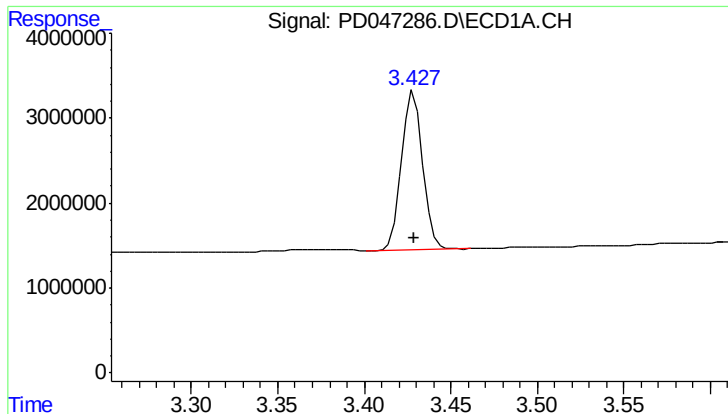

#1 Tetrachloro-m-xylene


R.T.: 3.429 min
Delta R.T.: 0.000 min
Response: 15918344
Conc: 12.77 ng/ml

Instrument :
ECD_O
ClientSampleId :
A3Y20

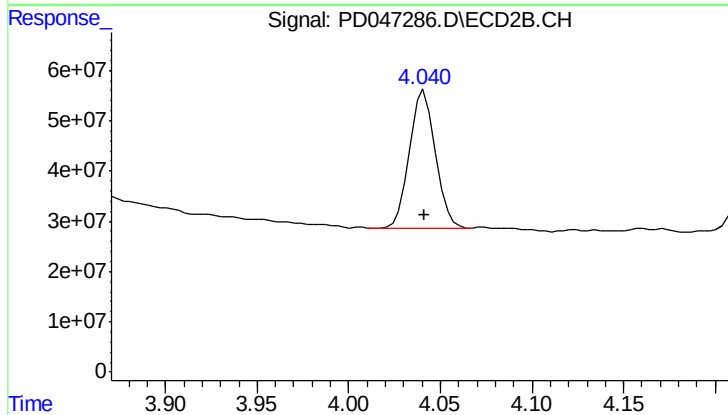


#1 Tetrachloro-m-xylene

R.T.: 4.041 min
Delta R.T.: 0.000 min
Response: 265973031
Conc: 12.47 ng/ml

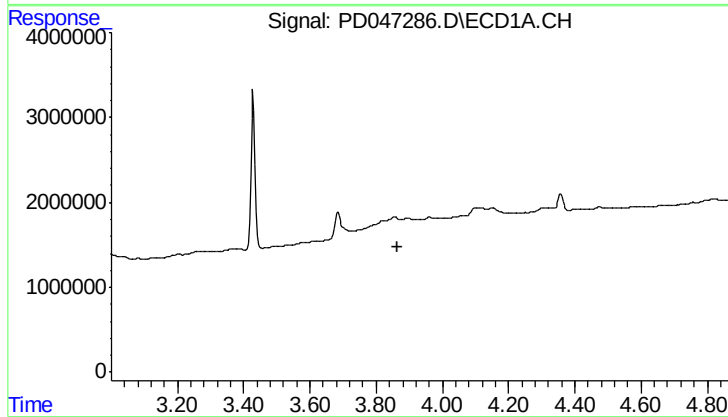


#2 alpha-BHC

R.T.: 0.000 min
Exp R.T.: 3.866 min
Response: 0
Conc: N.D.

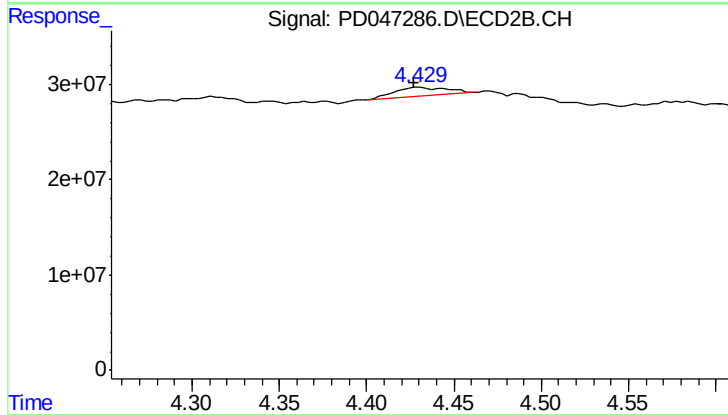

#2 alpha-BHC


R.T.: 4.431 min
Delta R.T.: 0.004 min
Response: 19432219
Conc: 0.59 ng/ml

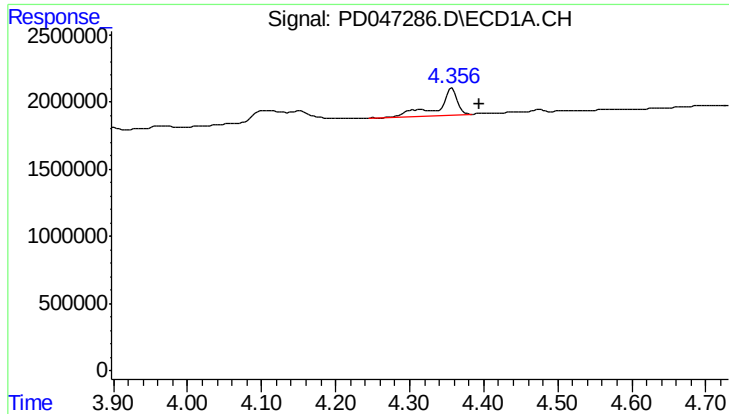

#6 beta-BHC


R.T.: 4.358 min
Delta R.T.: -0.036 min
Response: 3438527
Conc: 4.41 ng/ml

Instrument :
ECD_O
ClientSampleId :
A3Y20

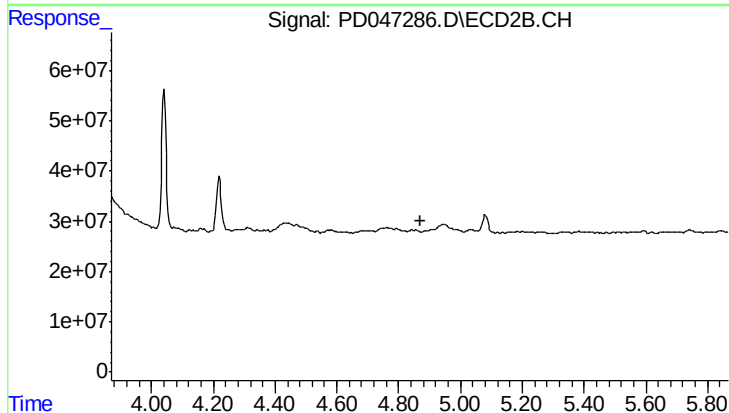


#6 beta-BHC

R.T.: 0.000 min
Exp R.T.: 4.870 min
Response: 0
Conc: N.D.

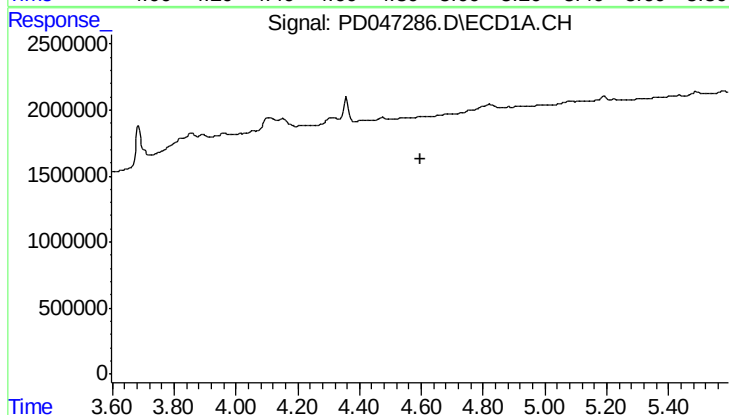


#7 delta-BHC

R.T.: 0.000 min
Exp R.T.: 4.596 min
Response: 0
Conc: N.D.

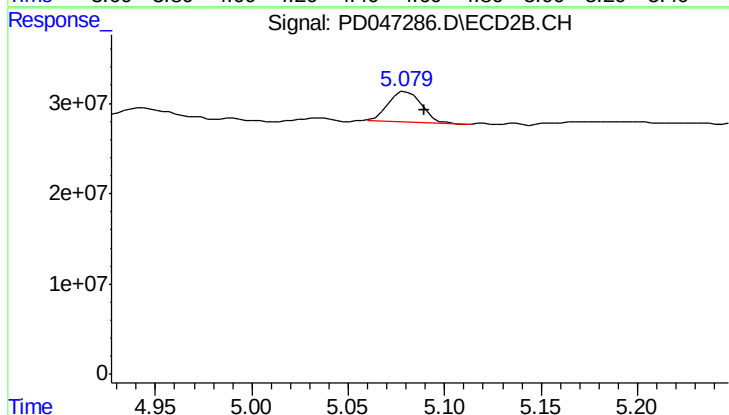

#7 delta-BHC


R.T.: 5.080 min
Delta R.T.: -0.009 min
Response: 40609360
Conc: 1.29 ng/ml

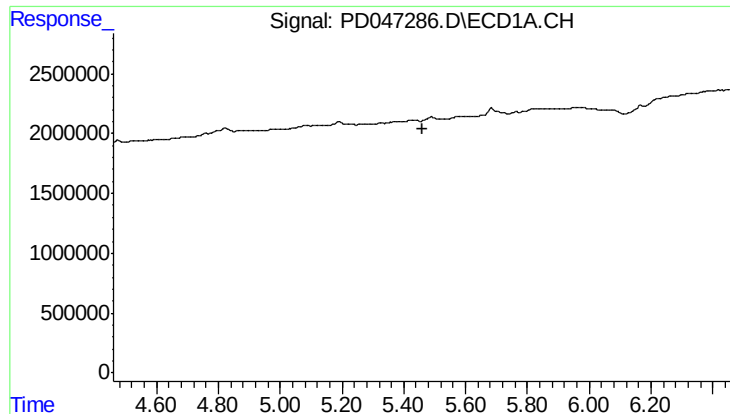

#9 Endosulfan I


R.T.: 0.000 min
Exp R.T.: 5.460 min
Response: 0
Conc: N.D.

Instrument :
ECD_O
ClientSampleId :
A3Y20

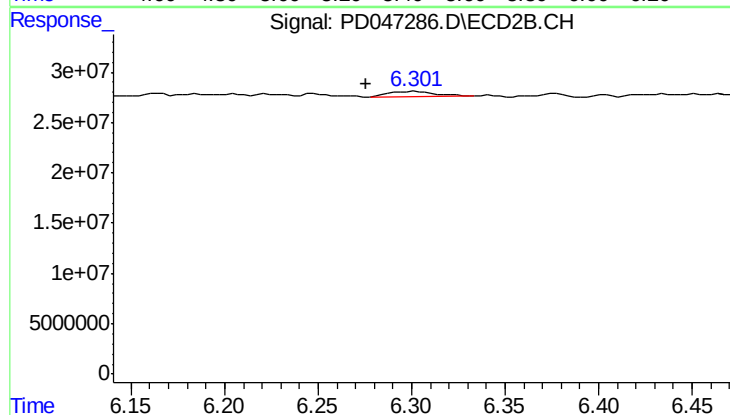


#9 Endosulfan I

R.T.: 6.302 min
Delta R.T.: 0.026 min
Response: 9128377
Conc: 0.37 ng/ml

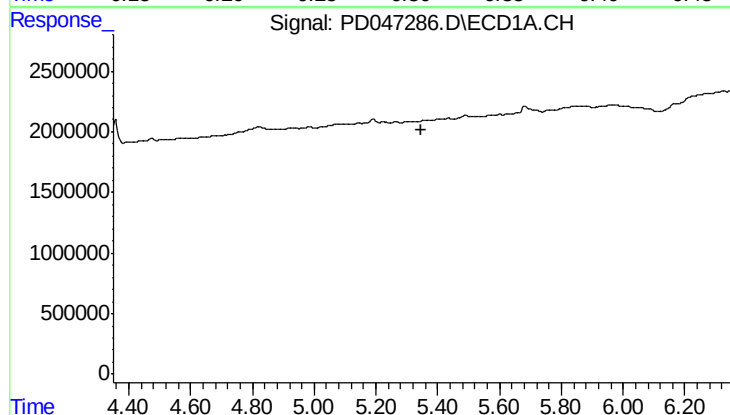


#10 trans-Chlordane

R.T.: 0.000 min
Exp R.T.: 5.348 min
Response: 0
Conc: N.D.

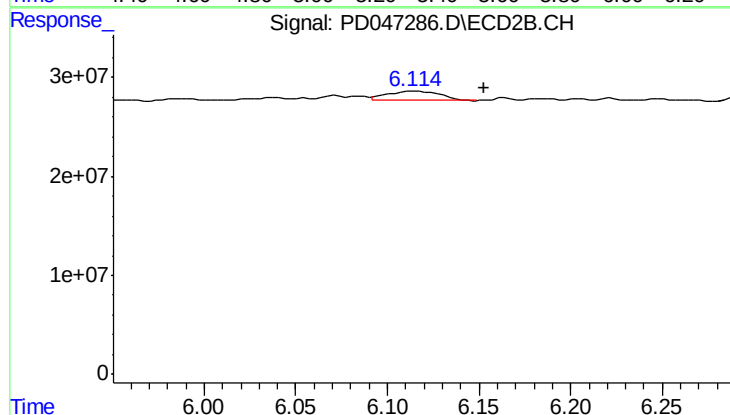

#10 trans-Chlordane


R.T.: 6.116 min
Delta R.T.: -0.037 min
Response: 19303910
Conc: 0.77 ng/ml

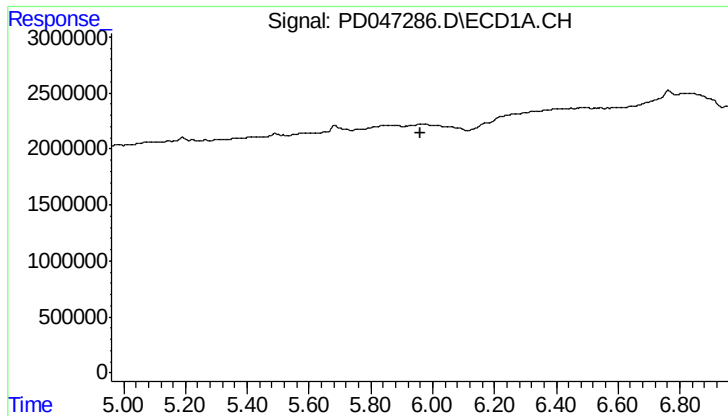

#14 Endrin


R.T.: 0.000 min
Exp R.T.: 5.959 min
Response: 0
Conc: N.D.

Instrument :
ECD_O
ClientSampleId :
A3Y20

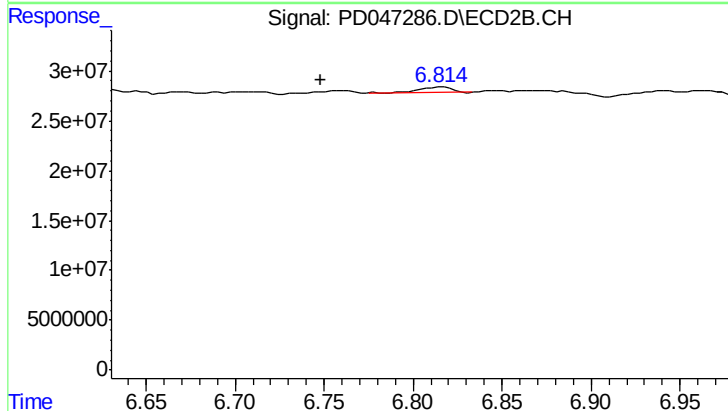


#14 Endrin

R.T.: 6.816 min
Delta R.T.: 0.068 min
Response: 6581946
Conc: 0.36 ng/ml

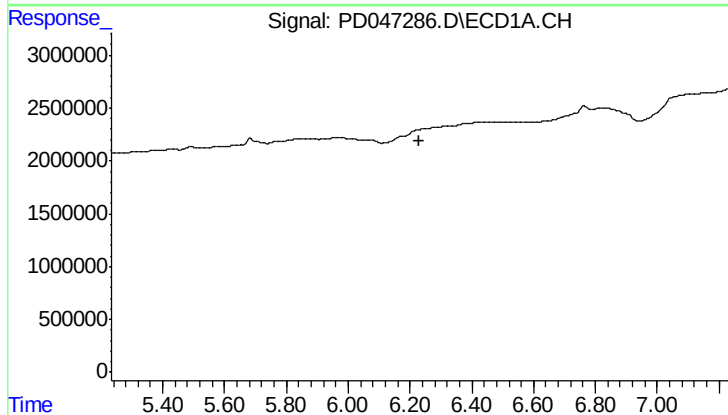


#15 Endosulfan II

R.T.: 0.000 min
Exp R.T.: 6.231 min
Response: 0
Conc: N.D.

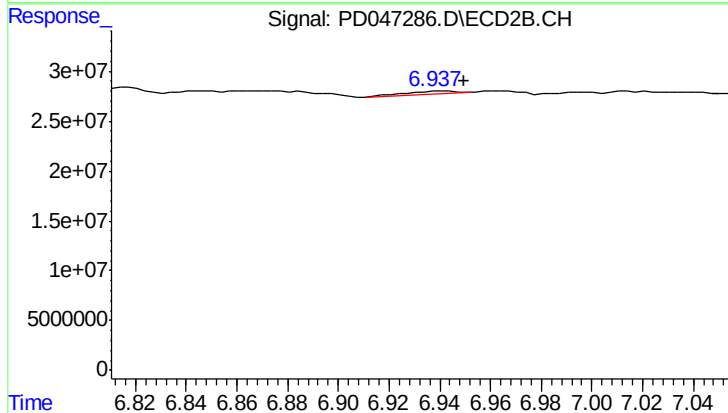

#15 Endosulfan II


R.T.: 6.940 min
Delta R.T.: -0.010 min
Response: 3367330
Conc: 0.16 ng/ml

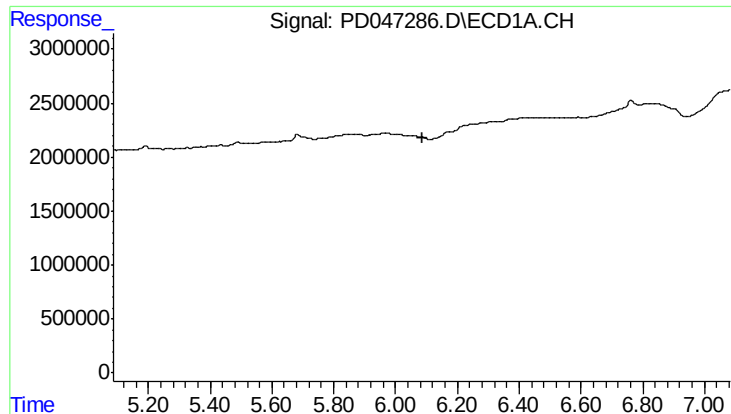

#16 4,4'-DDD


R.T.: 0.000 min
Exp R.T.: 6.086 min
Response: 0
Conc: N.D.

Instrument :
ECD_O
ClientSampleId :
A3Y20

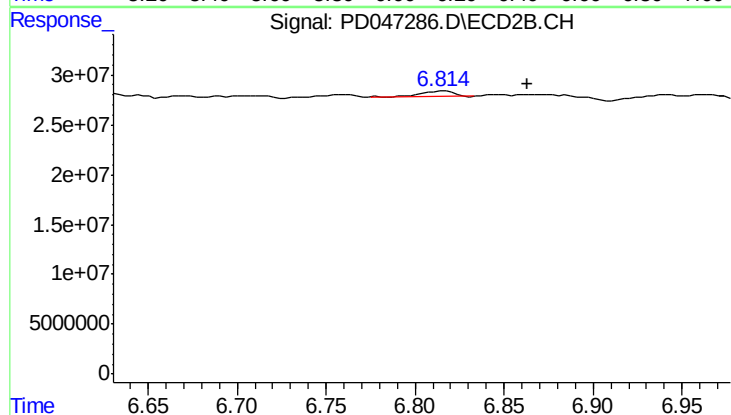


#16 4,4'-DDD

R.T.: 6.816 min
Delta R.T.: -0.047 min
Response: 6581946
Conc: 0.33 ng/ml

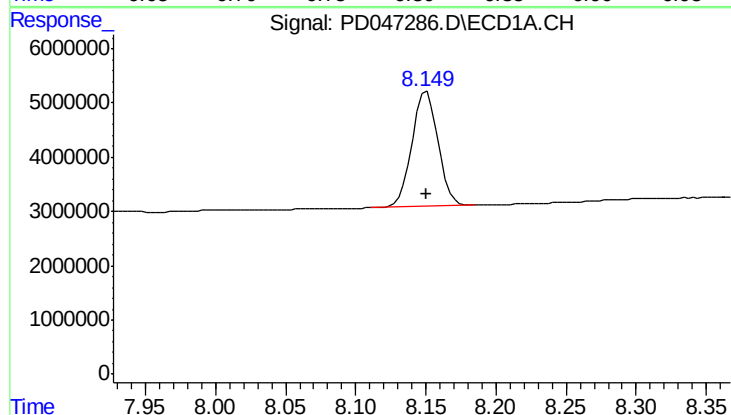

#27 Decachlorobiphenyl

R.T.: 8.151 min
Delta R.T.: 0.000 min
Response: 27146079
Conc: 19.62 ng/ml

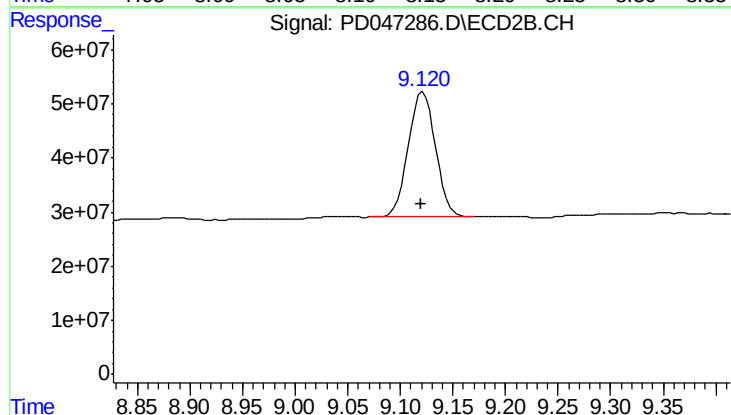

#27 Decachlorobiphenyl

R.T.: 9.121 min
Delta R.T.: 0.001 min
Response: 414470452
Conc: 21.77 ng/ml