

Data Path : P:\HPCHEM1\ECD_0\Data\P0042618\
 Data File : P0044123.D
 Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
 Acq On : 26 Apr 2018 17:01
 Operator : SM/UA
 Sample : J2541-01
 Misc :
 ALS Vial : 8 Sample Multiplier: 1

Instrument :
 ECD_O
 ClientSampleId :
 TP-4-11

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Apr 27 06:58:23 2018
 Quant Method : P:\HPCHEM1\ECD_0\methods\P0042518.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Thu Apr 26 04:36:05 2018
 Response via : Initial Calibration
 Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	4.041	3.295	9836932	12814150	13.742	13.246
2) SA Decachlor...	9.392	8.063	7099286	9176169	11.526	11.057
Target Compounds						
9) L2 AR-1221-2	0.000	3.581	0	189262	N.D.	19.813 #
12) L3 AR-1232-2	5.112	0.000	288863	0	38.152	N.D. #
24) L5 AR-1248-4	6.096	0.000	791453	0	41.934	N.D. #
25) L5 AR-1248-5	6.268	0.000	186716	0	15.176	N.D. #
26) L6 AR-1254-1	6.268	0.000	186716	0	5.372	N.D. #
34) L7 AR-1260-4	7.851	0.000	88123	0	1.337	N.D. #
40) L8 AR-1262-5	7.851	0.000	88123	0	1.110	N.D. #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : P:\HPCHEM1\ECD_0\Data\PO042618\
Data File : PO044123.D
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
Acq On : 26 Apr 2018 17:01
Operator : SM/UA
Sample : J2541-01
Misc :
ALS Vial : 8 Sample Multiplier: 1

Instrument :
ECD_O
ClientSampled :
TP-4-11

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Apr 27 06:58:23 2018
Quant Method : P:\HPCHEM1\ECD_0\methods\PO042518.M
Quant Title : GC EXTRACTABLES
QLast Update : Thu Apr 26 04:36:05 2018
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

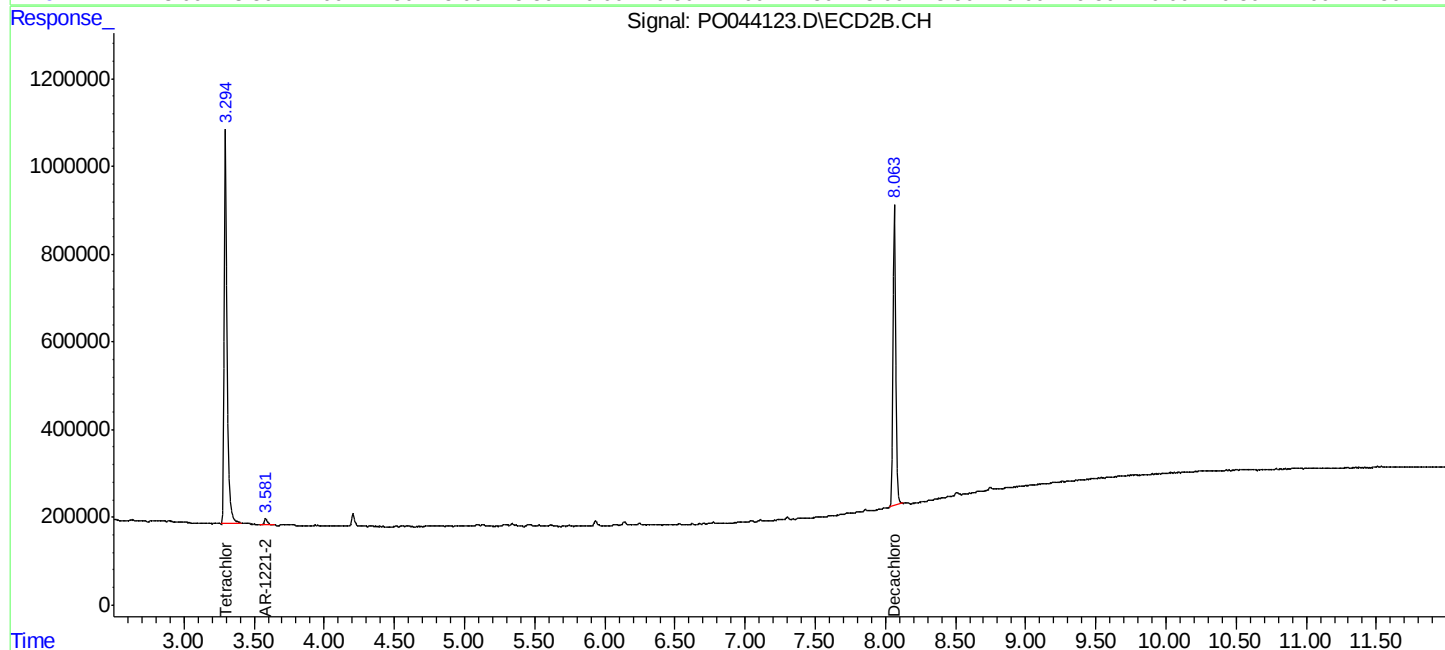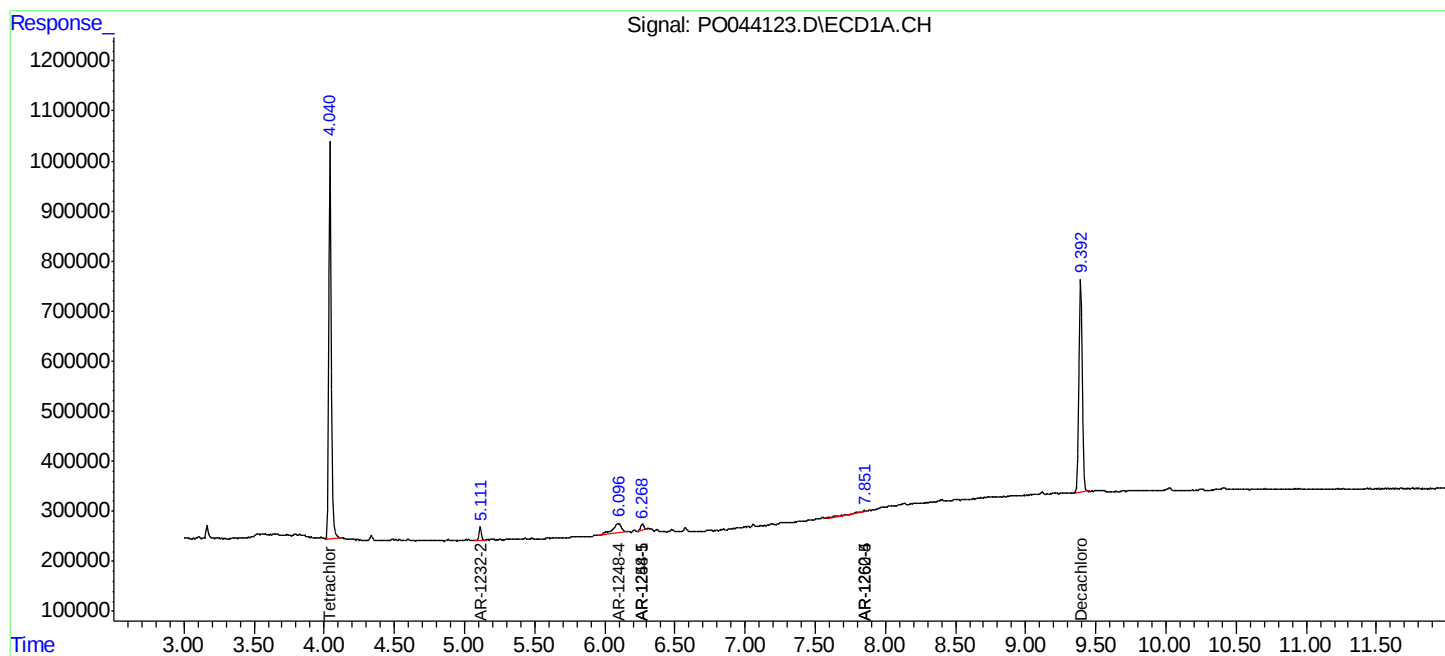


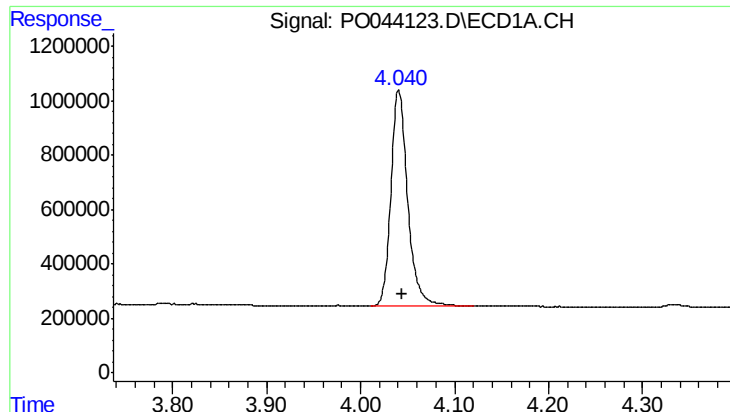

#1 Tetrachloro-m-xylene


R.T.: 4.041 min
Delta R.T.: -0.003 min
Response: 9836932
Conc: 13.74 ng/ml

Instrument :
ECD_O
ClientSampleId :
TP-4-11

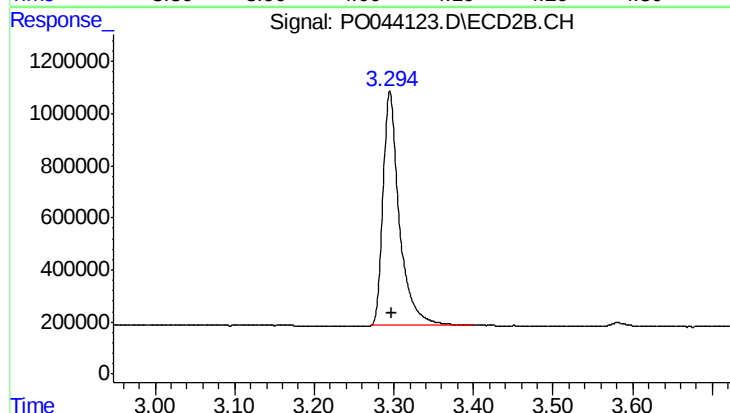


#1 Tetrachloro-m-xylene

R.T.: 3.295 min
Delta R.T.: -0.003 min
Response: 12814150
Conc: 13.25 ng/ml

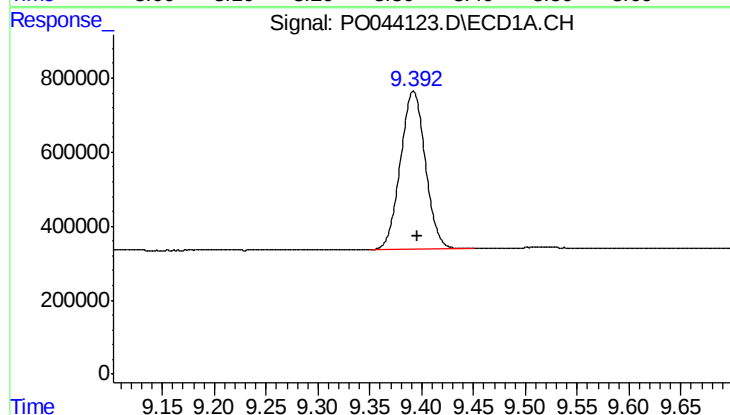


#2 Decachlorobiphenyl

R.T.: 9.392 min
Delta R.T.: -0.004 min
Response: 7099286
Conc: 11.53 ng/ml

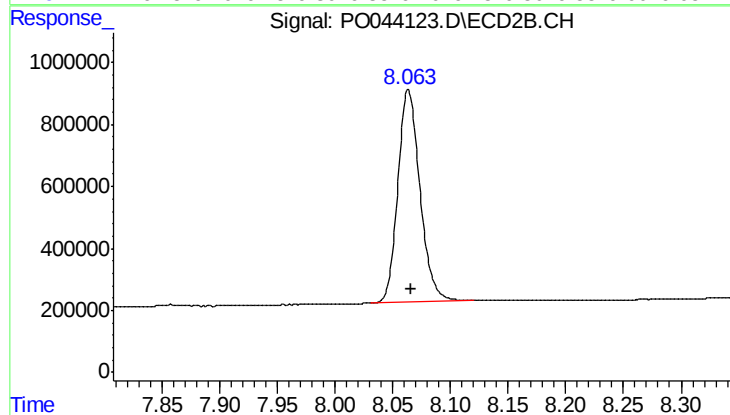

#2 Decachlorobiphenyl


R.T.: 8.063 min
Delta R.T.: -0.003 min
Response: 9176169
Conc: 11.06 ng/ml

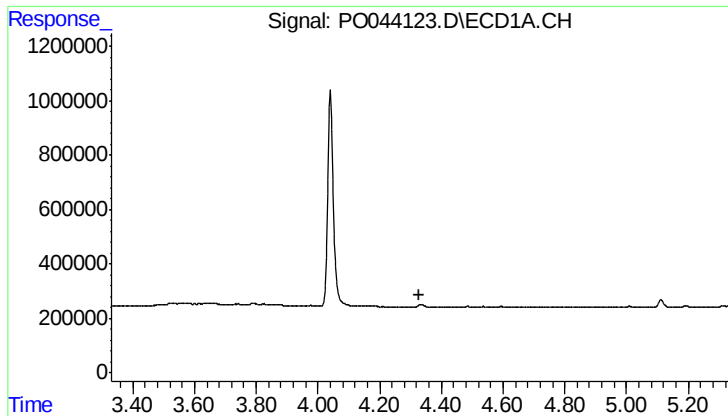

#9 AR-1221-2


R.T.: 0.000 min
Exp R.T.: 4.331 min
Response: 0
Conc: N.D.

Instrument :
ECD_O
ClientSampleId :
TP-4-11

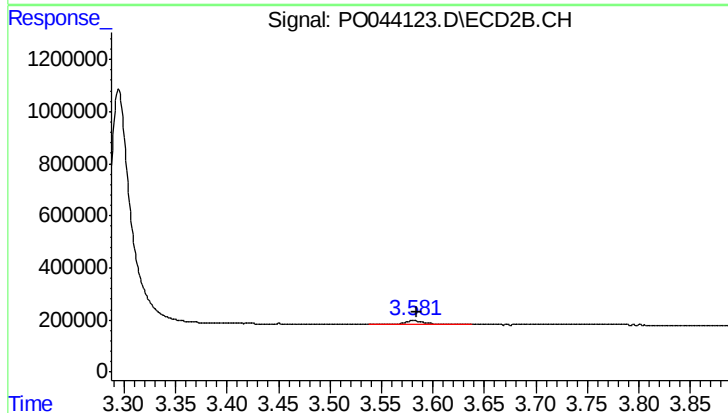


#9 AR-1221-2

R.T.: 3.581 min
Delta R.T.: -0.003 min
Response: 189262
Conc: 19.81 ng/ml

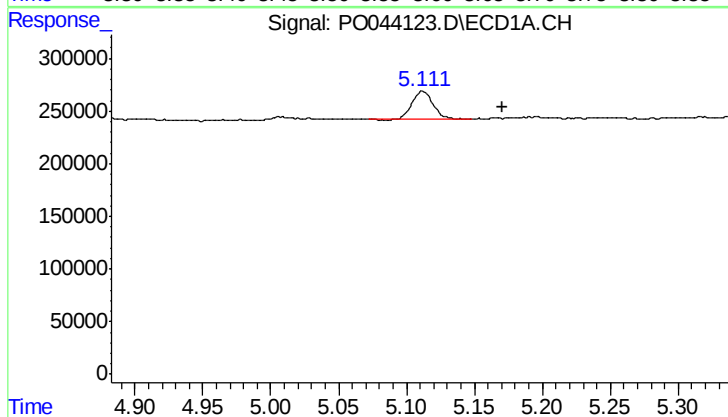


#12 AR-1232-2

R.T.: 5.112 min
Delta R.T.: -0.059 min
Response: 288863
Conc: 38.15 ng/ml

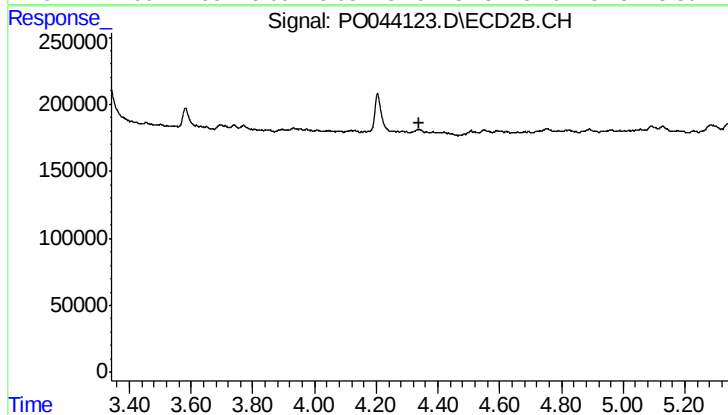

#12 AR-1232-2


R.T.: 0.000 min
Exp R.T.: 4.341 min
Response: 0
Conc: N.D.

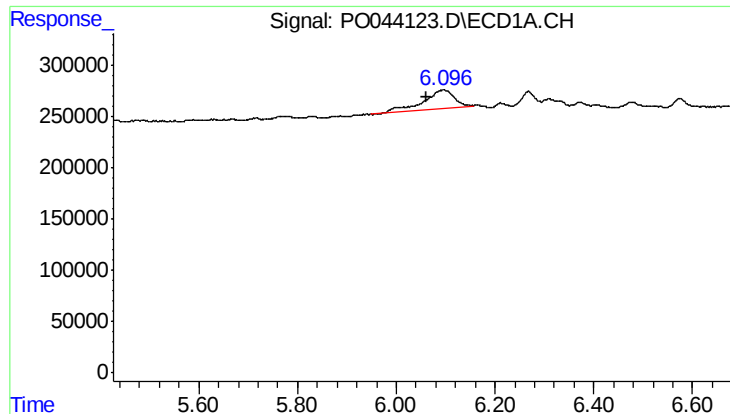

#24 AR-1248-4


R.T.: 6.096 min
Delta R.T.: 0.036 min
Response: 791453
Conc: 41.93 ng/ml

Instrument :
ECD_O
ClientSampleId :
TP-4-11

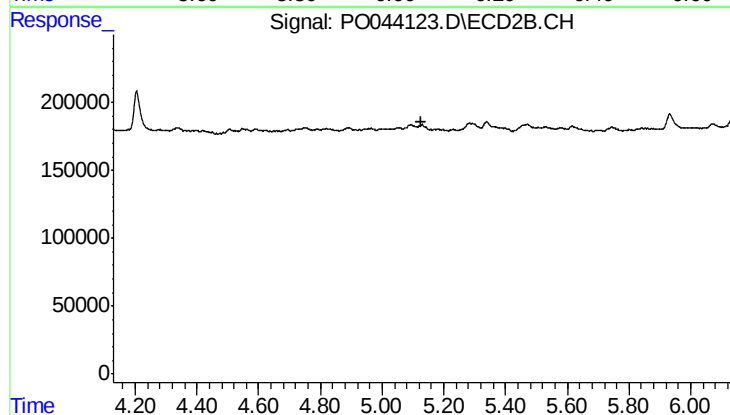


#24 AR-1248-4

R.T.: 0.000 min
Exp R.T.: 5.129 min
Response: 0
Conc: N.D.

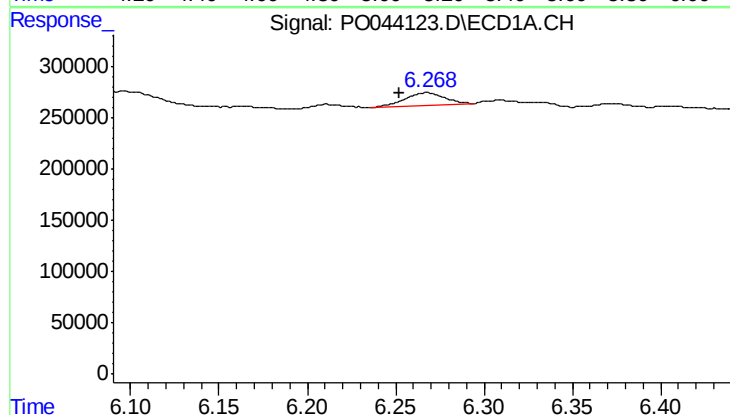


#25 AR-1248-5

R.T.: 6.268 min
Delta R.T.: 0.016 min
Response: 186716
Conc: 15.18 ng/ml

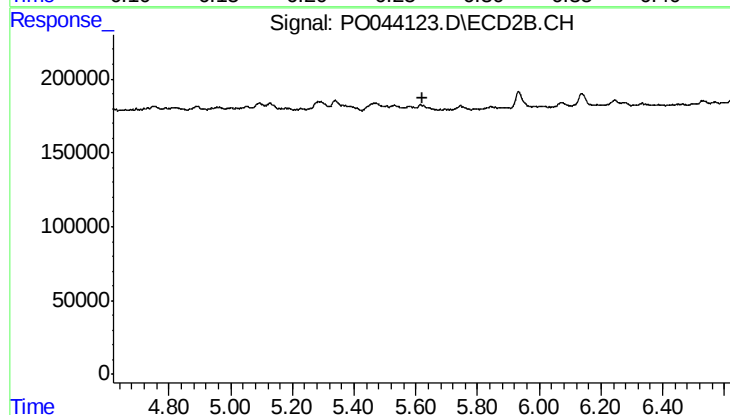

#25 AR-1248-5


R.T.: 0.000 min
Exp R.T.: 5.620 min
Response: 0
Conc: N.D.

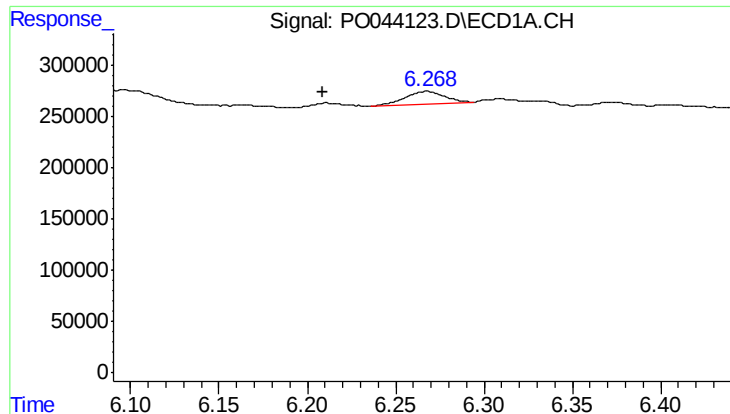

#26 AR-1254-1


R.T.: 6.268 min
Delta R.T.: 0.059 min
Response: 186716
Conc: 5.37 ng/ml

Instrument :
ECD_O
ClientSampleId :
TP-4-11

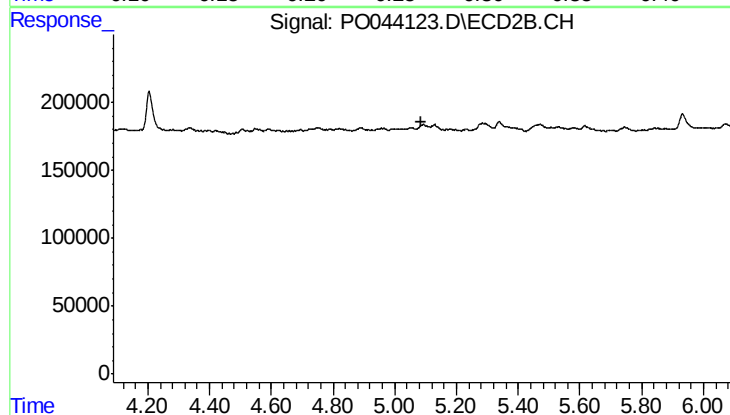


#26 AR-1254-1

R.T.: 0.000 min
Exp R.T.: 5.088 min
Response: 0
Conc: N.D.

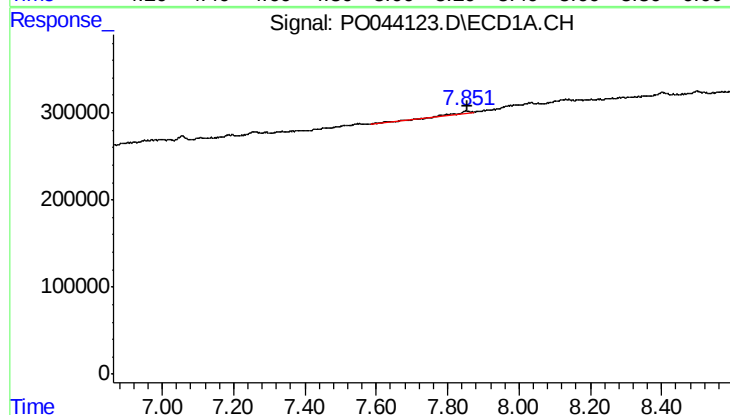


#34 AR-1260-4

R.T.: 7.851 min
Delta R.T.: -0.003 min
Response: 88123
Conc: 1.34 ng/ml

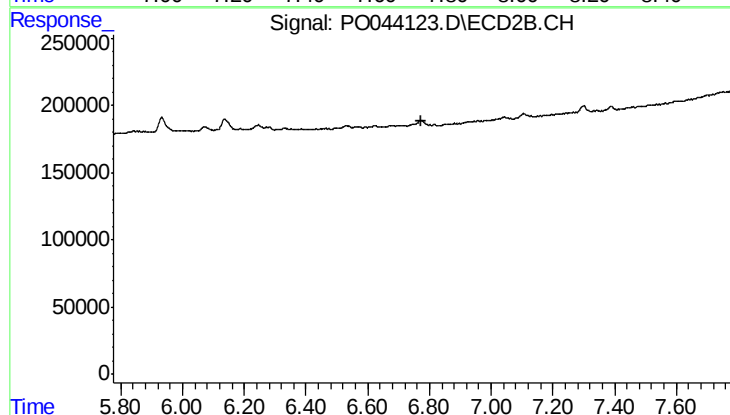

#34 AR-1260-4


R.T.: 0.000 min
Exp R.T.: 6.775 min
Response: 0
Conc: N.D.

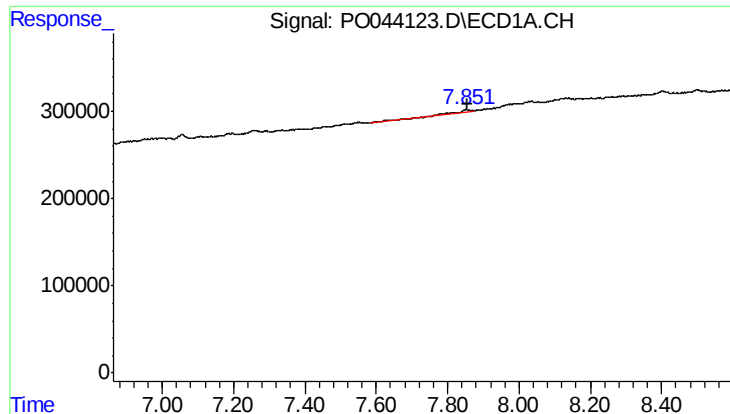

#40 AR-1262-5

R.T.: 7.851 min
Delta R.T.: -0.003 min
Response: 88123
Conc: 1.11 ng/ml

Instrument :
ECD_O
ClientSampleId :
TP-4-11

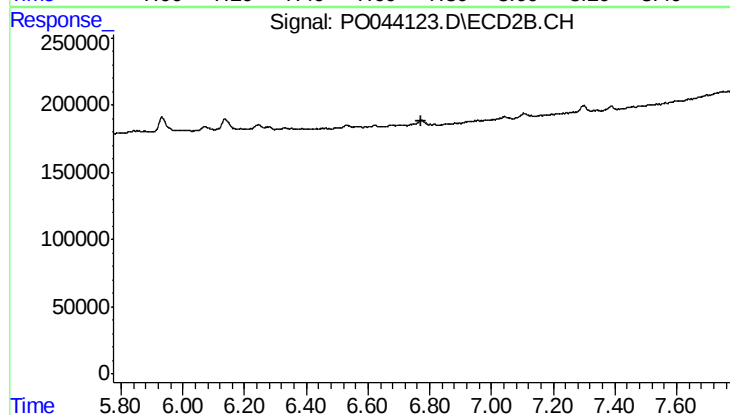

#40 AR-1262-5

R.T.: 0.000 min
Exp R.T. : 6.775 min
Response: 0
Conc: N.D.