

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\P0042920\
 Data File : P0068073.D
 Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
 Acq On : 29 Apr 2020 10:18
 Operator : DD\AJ
 Sample : L2428-01
 Misc :
 ALS Vial : 6 Sample Multiplier: 1

Instrument :
 ECD_O
 ClientSampleId :
 S-7

Manual Integrations
 APPROVED

Sohil
 4/30/2020 8:36:42 AM

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Apr 29 10:53:30 2020
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\P0042720.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Tue Apr 28 07:12:58 2020
 Response via : Initial Calibration
 Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	4.915	3.935	535867	698350	22.393	21.854m
2) SA Decachlor...	10.878	9.210	751444	791860	19.912m	20.517m

Target Compounds

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\P0042920\
Data File : P0068073.D
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
Acq On : 29 Apr 2020 10:18
Operator : DD\AJ
Sample : L2428-01
Misc :
ALS Vial : 6 Sample Multiplier: 1


Instrument :
ECD_O
ClientSampleId :
S-7


Manual Integrations
APPROVED

Sohil
4/30/2020 8:36:42 AM

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Apr 29 10:53:30 2020
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\P0042720.M
Quant Title : GC EXTRACTABLES
QLast Update : Tue Apr 28 07:12:58 2020
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

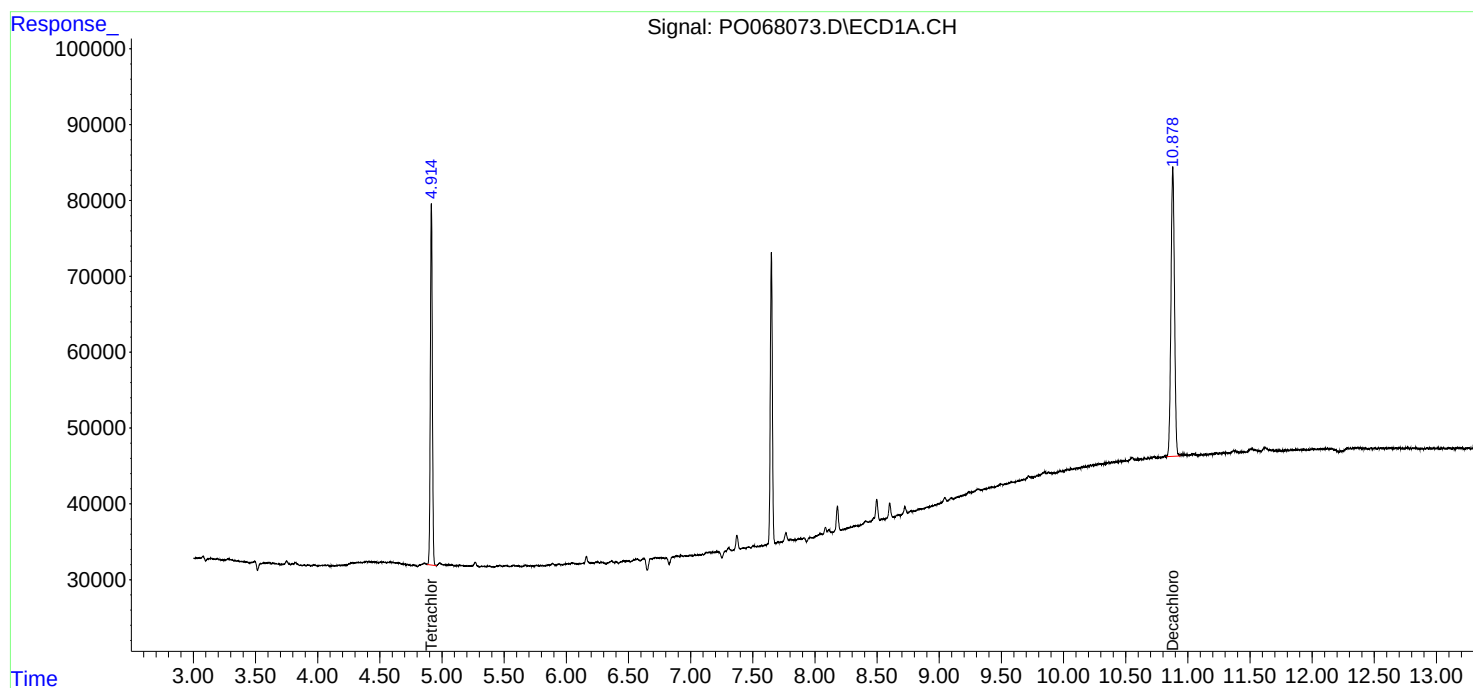

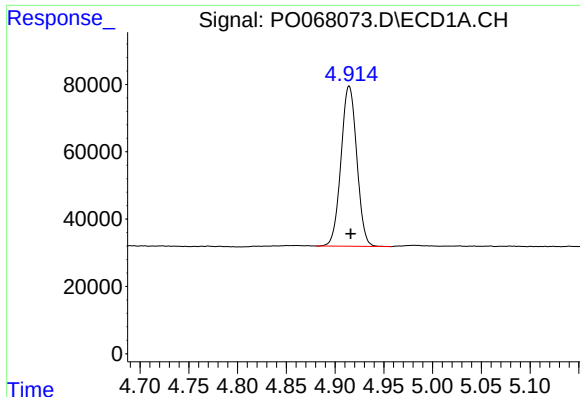


#1 Tetrachloro-m-xylene

R.T.: 4.915 min
Delta R.T.: -0.001 min
Response: 535867
Conc: 22.39 ng/ml

Instrument :
ECD_O
ClientSampleId :
S-7


Manual Integrations
APPROVED

Sohil
4/30/2020 8:36:42 AM

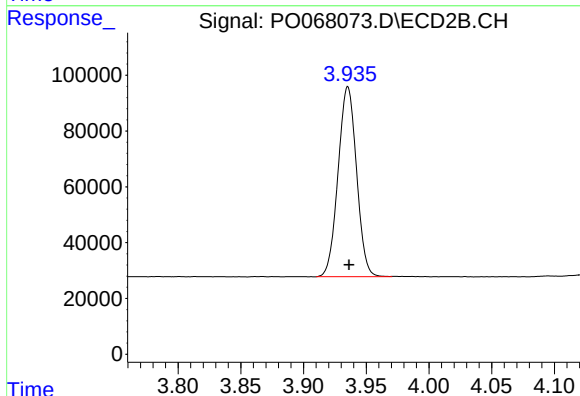


#1 Tetrachloro-m-xylene

R.T.: 3.935 min
Delta R.T.: -0.001 min
Response: 698350
Conc: 21.85 ng/ml m

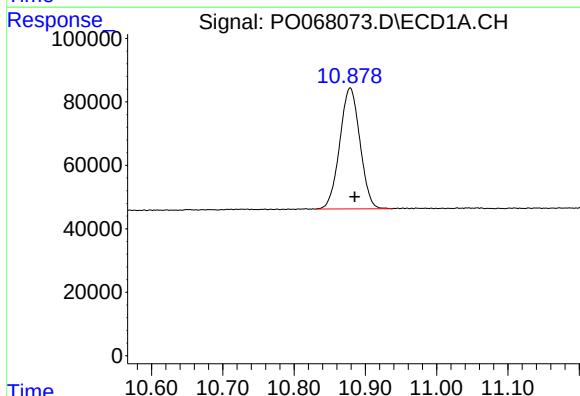

#2 Decachlorobiphenyl

R.T.: 10.878 min
Delta R.T.: -0.007 min
Response: 751444
Conc: 19.91 ng/ml m

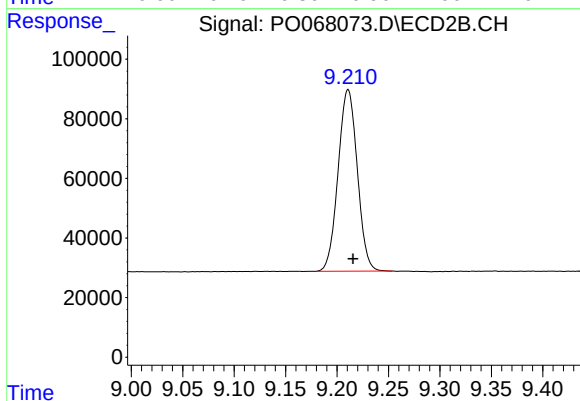

#2 Decachlorobiphenyl

R.T.: 9.210 min
Delta R.T.: -0.005 min
Response: 791860
Conc: 20.52 ng/ml m