

Data Path : P:\HPCHEM1\ECD_0\Data\P0043018\
 Data File : P0044243.D
 Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
 Acq On : 30 Apr 2018 20:40
 Operator : SM/UA
 Sample : J2553-02
 Misc :
 ALS Vial : 17 Sample Multiplier: 1

Instrument :
 ECD_O
 ClientSampleId :
 BPS1-SB4017-2025

Manual Integrations
 APPROVED

ugo
 5/1/2018 3:37:30 PM

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: May 01 03:26:16 2018
 Quant Method : P:\HPCHEM1\ECD_0\methods\P0042518.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Thu Apr 26 04:36:05 2018
 Response via : Initial Calibration
 Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	4.041	3.297	13474885	16743267	18.824	17.308
2)	SA Decachlor...	9.385	8.058	10582685	11507442	17.181m	13.866

Target Compounds

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : P:\HPCHEM1\ECD_0\Data\PO043018\
Data File : PO044243.D
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
Acq On : 30 Apr 2018 20:40
Operator : SM/UA
Sample : J2553-02
Misc :
ALS Vial : 17 Sample Multiplier: 1



Instrument :
ECD_O
ClientSampleId :
BPS1-SB4017-2025


Manual Integrations
APPROVED

ugo
5/1/2018 3:37:30 PM

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: May 01 03:26:16 2018
Quant Method : P:\HPCHEM1\ECD_0\methods\PO042518.M
Quant Title : GC EXTRACTABLES
QLast Update : Thu Apr 26 04:36:05 2018
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

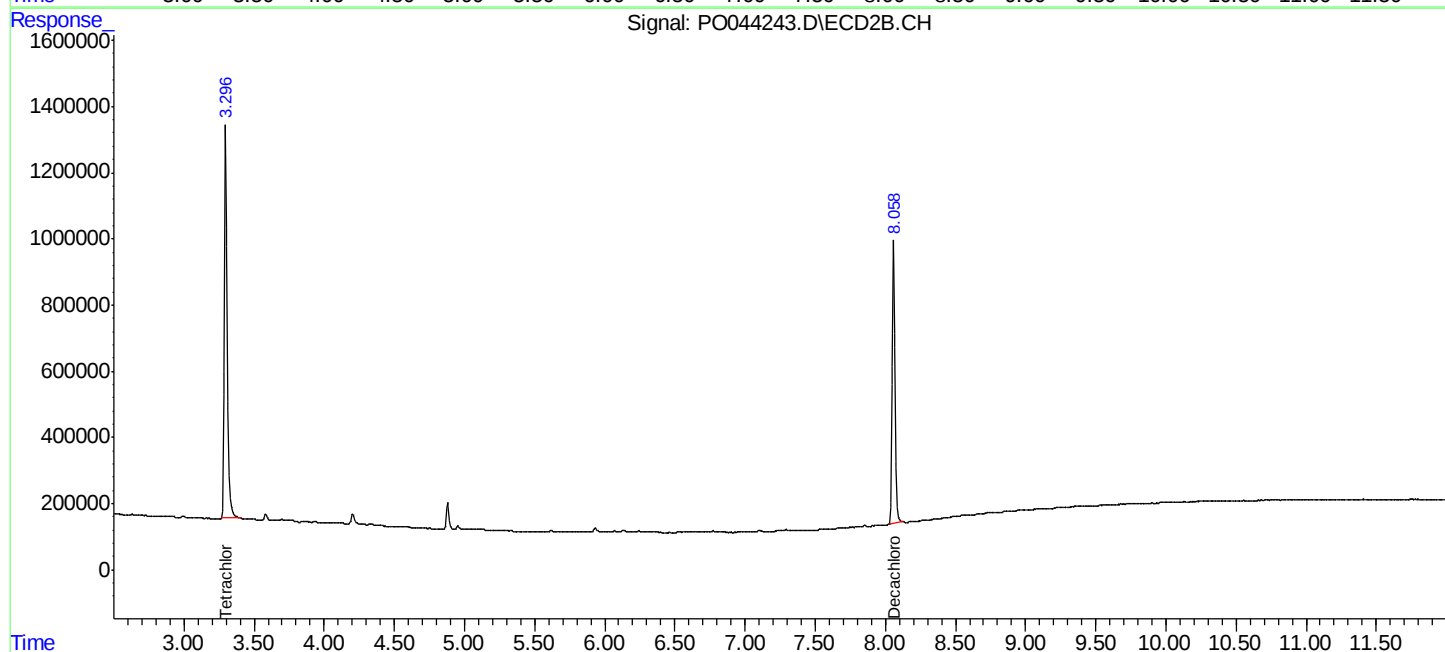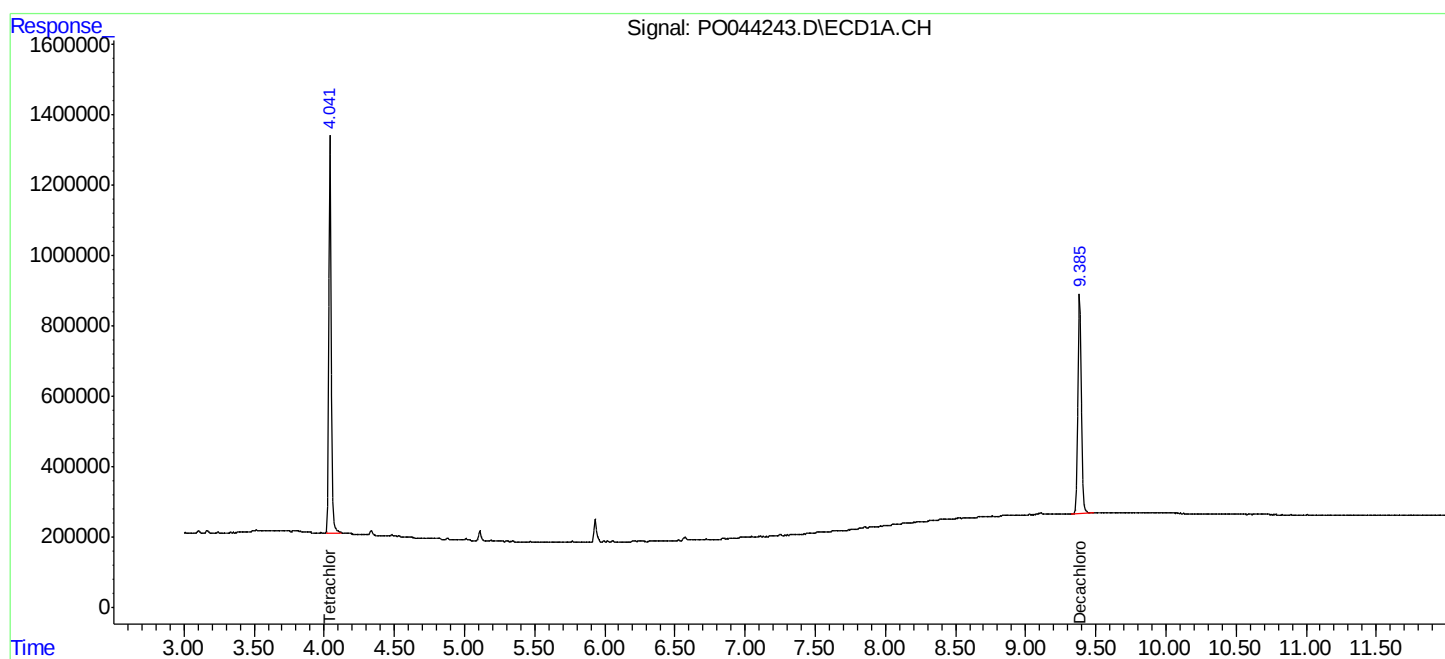

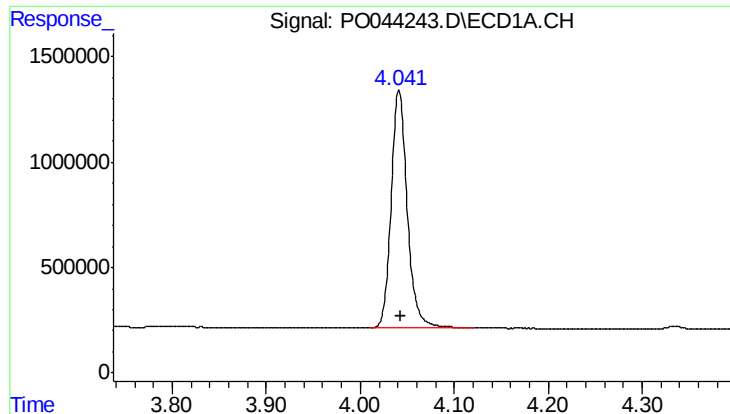


#1 Tetrachloro-m-xylene

R.T.: 4.041 min
Delta R.T.: -0.003 min
Response: 13474885
Conc: 18.82 ng/ml

Instrument :
ECD_O
ClientSampleId :
BPS1-SB4017-2025


Manual Integrations
APPROVED

ugo
5/1/2018 3:37:30 PM

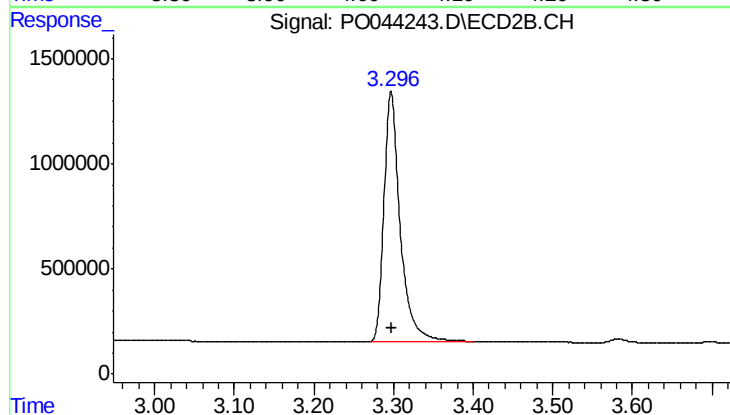


#1 Tetrachloro-m-xylene

R.T.: 3.297 min
Delta R.T.: -0.001 min
Response: 16743267
Conc: 17.31 ng/ml

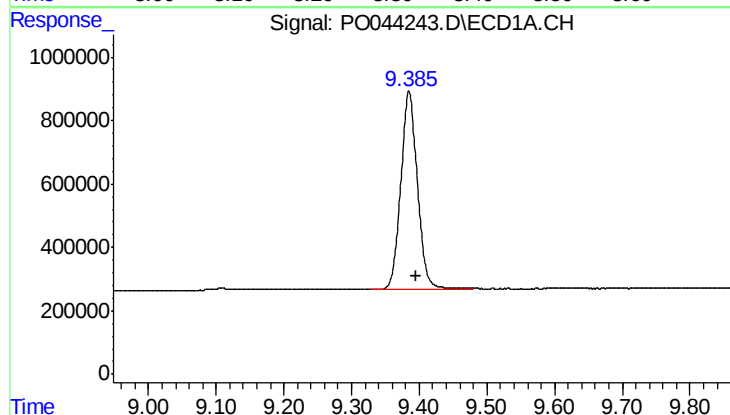

#2 Decachlorobiphenyl

R.T.: 9.385 min
Delta R.T.: -0.011 min
Response: 10582685
Conc: 17.18 ng/ml m

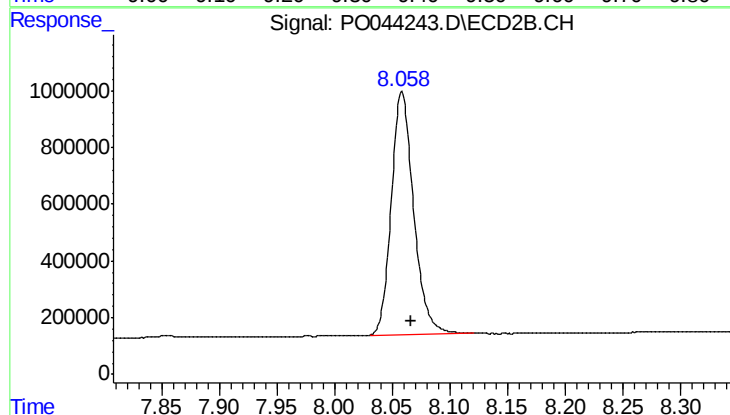

#2 Decachlorobiphenyl

R.T.: 8.058 min
Delta R.T.: -0.008 min
Response: 11507442
Conc: 13.87 ng/ml