

Data Path : P:\HPCHEM1\ECD_0\Data\P0043018\
Data File : P0044245.D
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
Acq On : 30 Apr 2018 21:10
Operator : SM/UA
Sample : J2553-04
Misc :
ALS Vial : 19 Sample Multiplier: 1

Instrument :
ECD_O
ClientSampleId :
BPS1-SB4018-1520

Manual Integrations
APPROVED

ugo
5/1/2018 3:37:24 PM

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: May 01 03:31:26 2018
Quant Method : P:\HPCHEM1\ECD_0\methods\P0042518.M
Quant Title : GC EXTRACTABLES
QLast Update : Thu Apr 26 04:36:05 2018
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	4.041	3.296	13751546	16984220	19.210	17.557
2) SA Decachlor...	9.384	8.058	10412626	11527989	16.905m	13.891

Target Compounds

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : P:\HPCHEM1\ECD_0\Data\P0043018\
Data File : P0044245.D
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
Acq On : 30 Apr 2018 21:10
Operator : SM/UA
Sample : J2553-04
Misc :
ALS Vial : 19 Sample Multiplier: 1



Instrument :
ECD_O
ClientSampleId :
BPS1-SB4018-1520


Manual Integrations
APPROVED

ugo
5/1/2018 3:37:24 PM

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: May 01 03:31:26 2018
Quant Method : P:\HPCHEM1\ECD_0\methods\P0042518.M
Quant Title : GC EXTRACTABLES
QLast Update : Thu Apr 26 04:36:05 2018
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

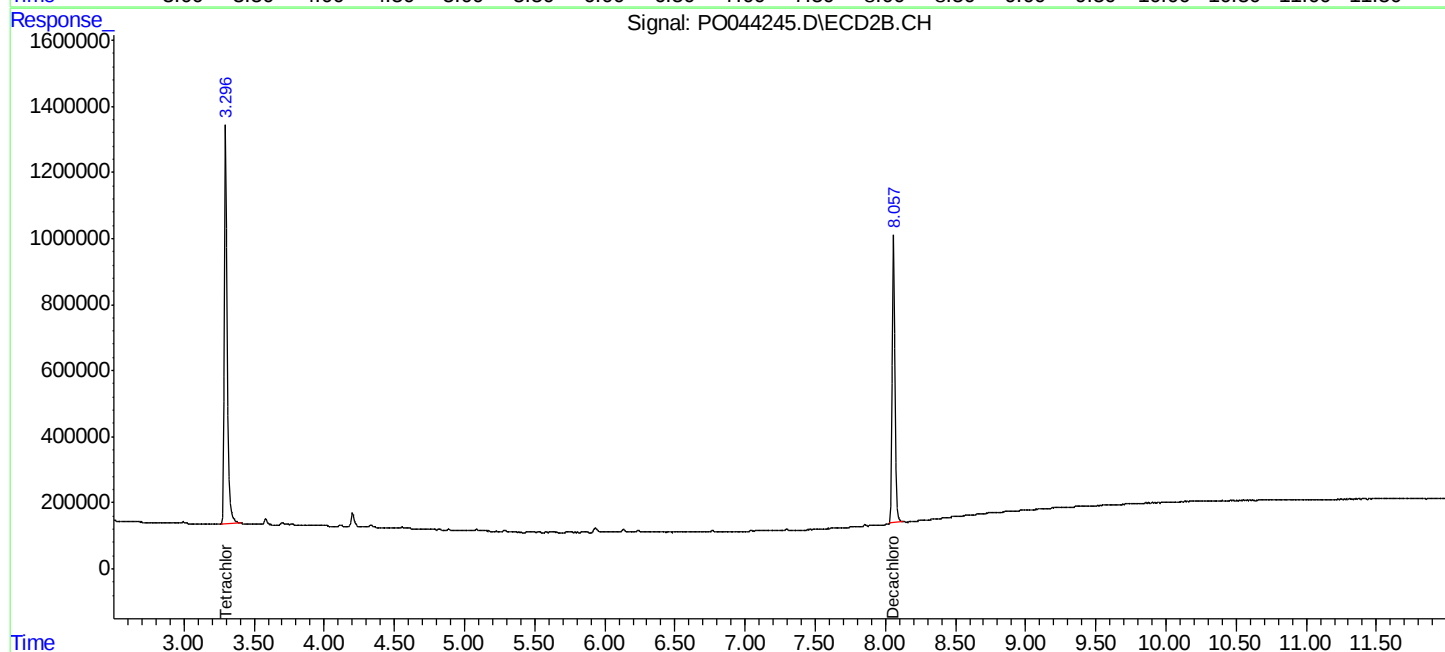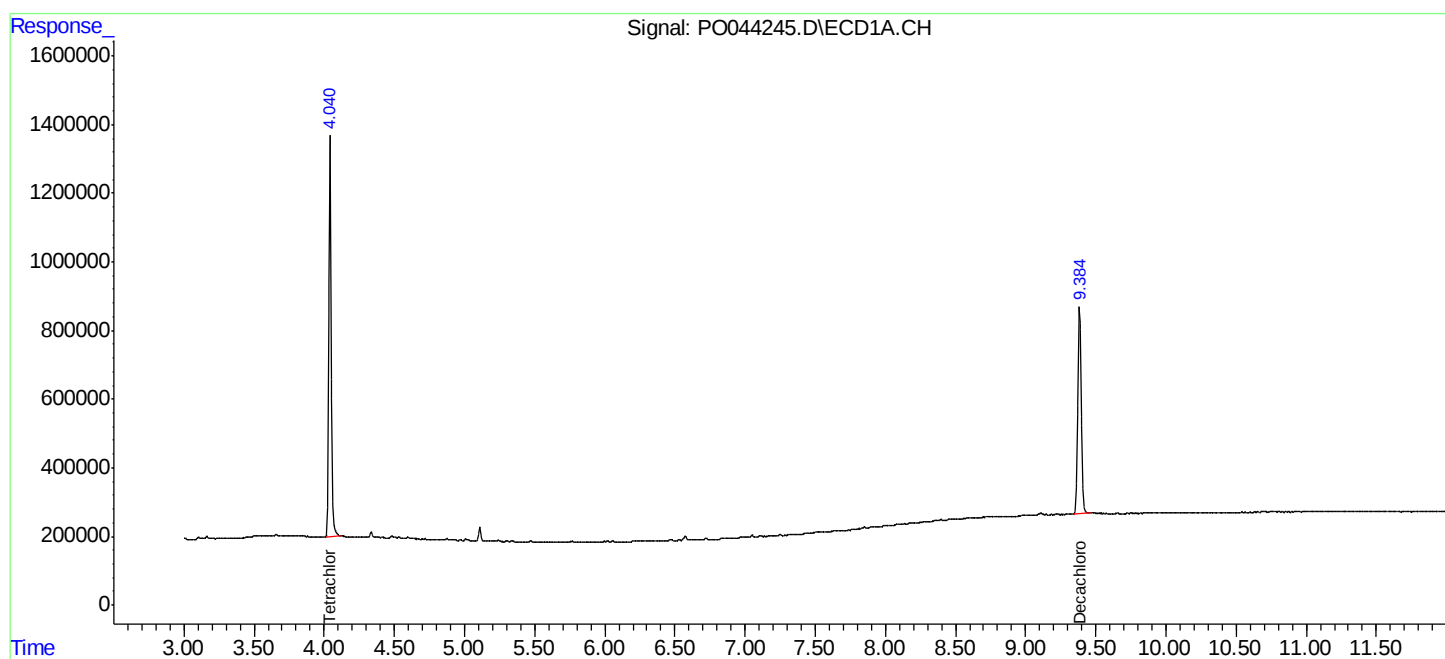

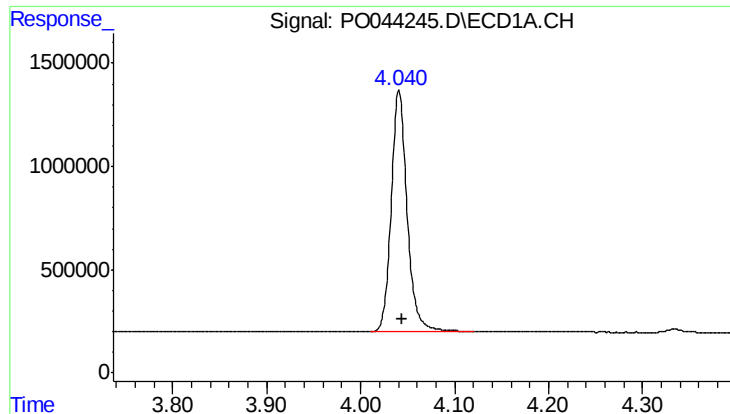


#1 Tetrachloro-m-xylene

R.T.: 4.041 min
Delta R.T.: -0.003 min
Response: 13751546
Conc: 19.21 ng/ml

Instrument :
ECD_O
ClientSampleId :
BPS1-SB4018-1520


Manual Integrations
APPROVED

ugo
5/1/2018 3:37:24 PM

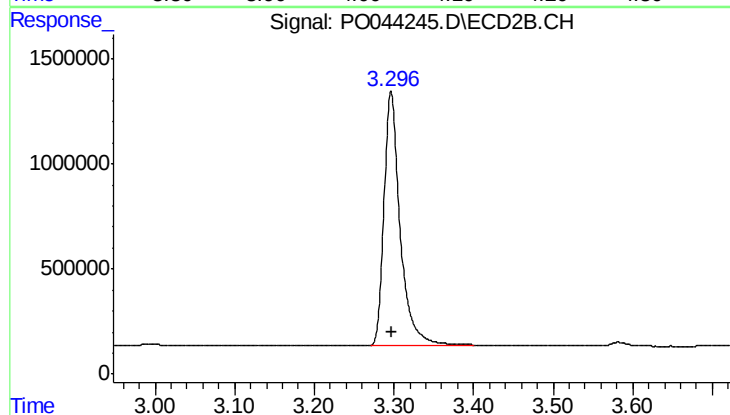


#1 Tetrachloro-m-xylene

R.T.: 3.296 min
Delta R.T.: -0.002 min
Response: 16984220
Conc: 17.56 ng/ml

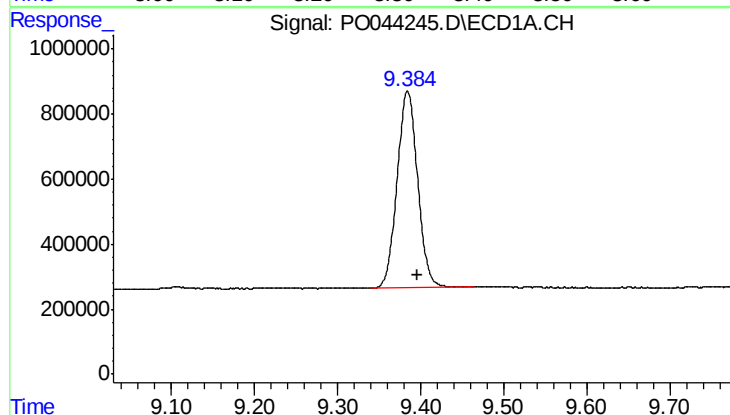

#2 Decachlorobiphenyl

R.T.: 9.384 min
Delta R.T.: -0.012 min
Response: 10412626
Conc: 16.90 ng/ml m

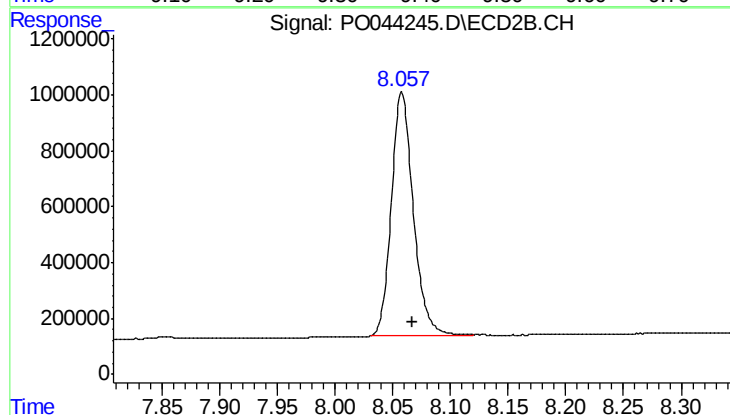

#2 Decachlorobiphenyl

R.T.: 8.058 min
Delta R.T.: -0.009 min
Response: 11527989
Conc: 13.89 ng/ml