

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\P0043019\
 Data File : P0055712.D
 Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
 Acq On : 30 Apr 2019 12:11
 Operator : SM/SJ
 Sample : I.BLK
 Misc :
 ALS Vial : 2 Sample Multiplier: 1

Instrument :
 ECD_O
 ClientSampleId :

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Apr 30 12:56:05 2019
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\P0042919.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Tue Apr 30 05:21:50 2019
 Response via : Initial Calibration
 Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	4.285	3.597	684184	755005	24.325	25.881
2)	SA Decachlor...	9.886	8.551	608590	397763	14.249	12.521
Target Compounds							
20)	L4 AR-1242-5	6.297	5.490	60097	39198	51.983	29.328 #
24)	L5 AR-1248-4	6.297	0.000	60097	0	34.080	N.D. #
25)	L5 AR-1248-5	6.297	5.490	60097	39198	35.425	23.843 #
26)	L6 AR-1254-1	6.297	5.490	60097	39198	31.816	15.012 #
28)	L6 AR-1254-3	6.886	0.000	25076	0	7.537	N.D. #
29)	L6 AR-1254-4	7.128	0.000	55294	0	21.540	N.D. #
35)	L7 AR-1260-5	8.160	0.000	79796	0	16.460	N.D. #
37)	L8 AR-1262-2	8.160	0.000	79796	0	12.903	N.D. #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\P0043019\
Data File : P0055712.D
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
Acq On : 30 Apr 2019 12:11
Operator : SM/SJ
Sample : I.BLK
Misc :
ALS Vial : 2 Sample Multiplier: 1

Instrument :
ECD_O
ClientSampleId :

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Apr 30 12:56:05 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\P0042919.M
Quant Title : GC EXTRACTABLES
QLast Update : Tue Apr 30 05:21:50 2019
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

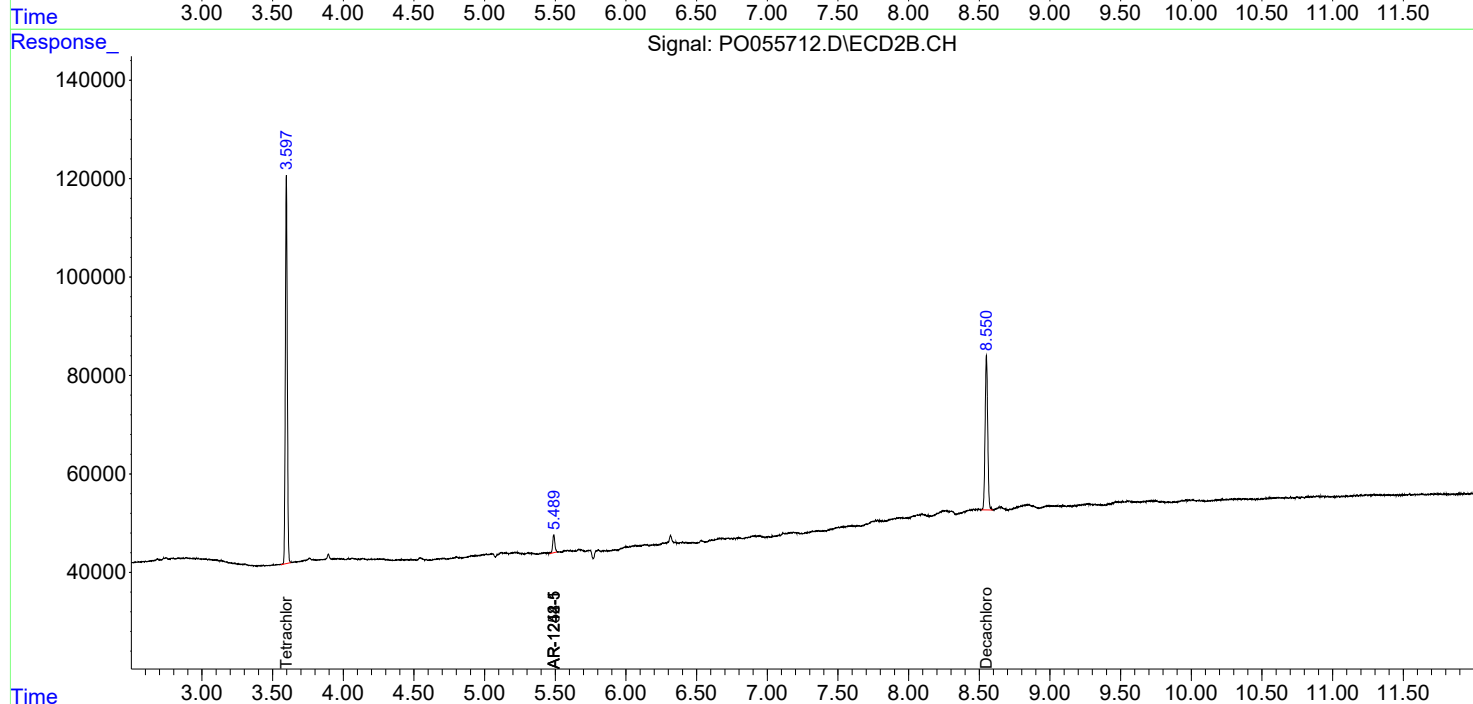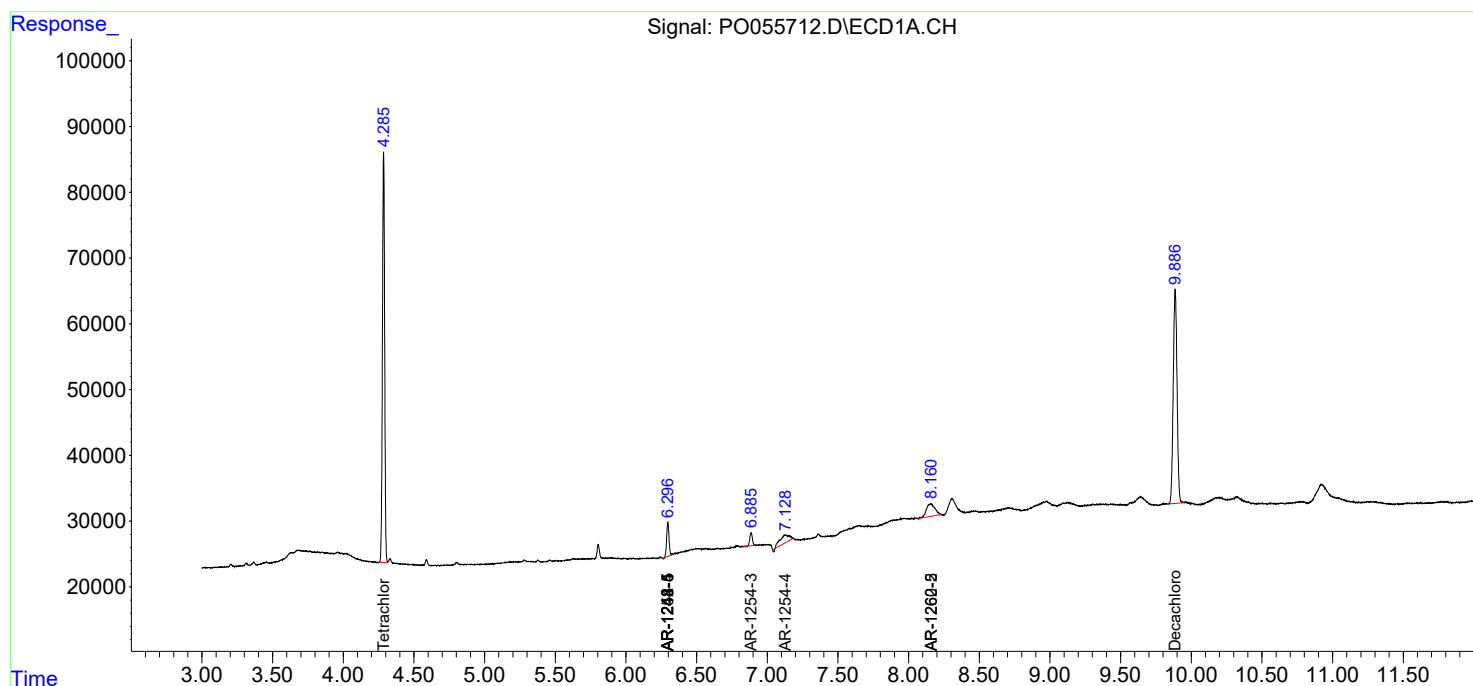


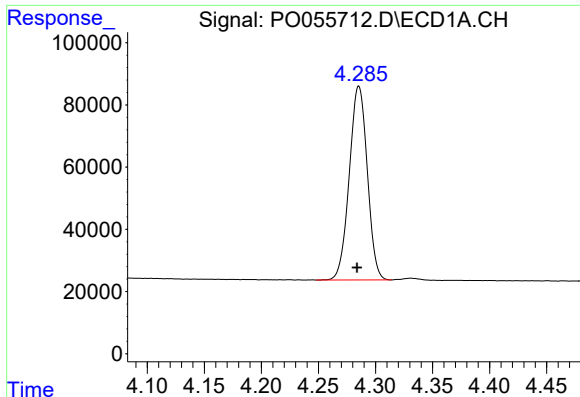

#1 Tetrachloro-m-xylene


R.T.: 4.285 min
Delta R.T.: 0.001 min
Response: 684184
Conc: 24.33 ng/ml

Instrument :
ECD_O
ClientSampleId :

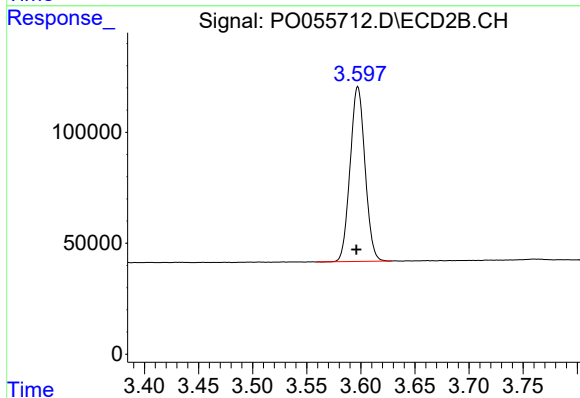


#1 Tetrachloro-m-xylene

R.T.: 3.597 min
Delta R.T.: 0.001 min
Response: 755005
Conc: 25.88 ng/ml

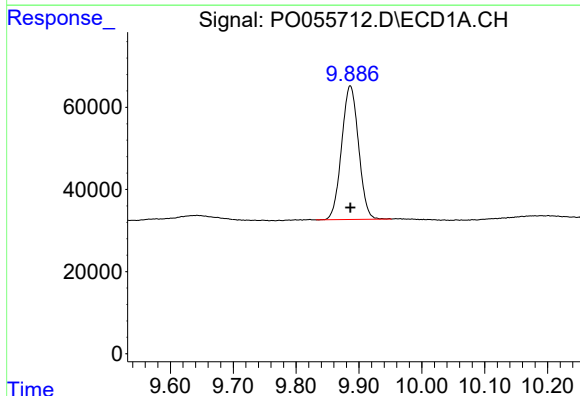


#2 Decachlorobiphenyl

R.T.: 9.886 min
Delta R.T.: 0.000 min
Response: 608590
Conc: 14.25 ng/ml

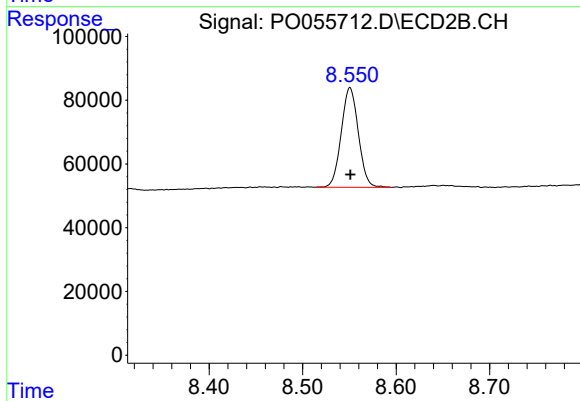

#2 Decachlorobiphenyl


R.T.: 8.551 min
Delta R.T.: 0.000 min
Response: 397763
Conc: 12.52 ng/ml

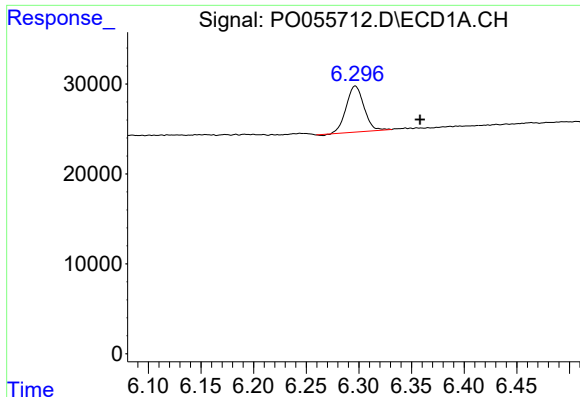

#20 AR-1242-5


R.T.: 6.297 min
Delta R.T.: -0.062 min
Response: 60097
Conc: 51.98 ng/ml

Instrument :
ECD_O
ClientSampleId :

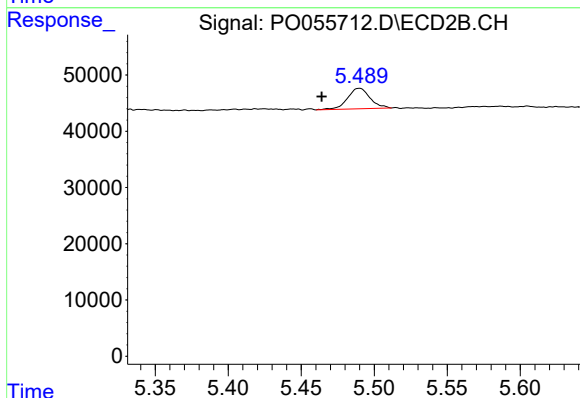


#20 AR-1242-5

R.T.: 5.490 min
Delta R.T.: 0.026 min
Response: 39198
Conc: 29.33 ng/ml

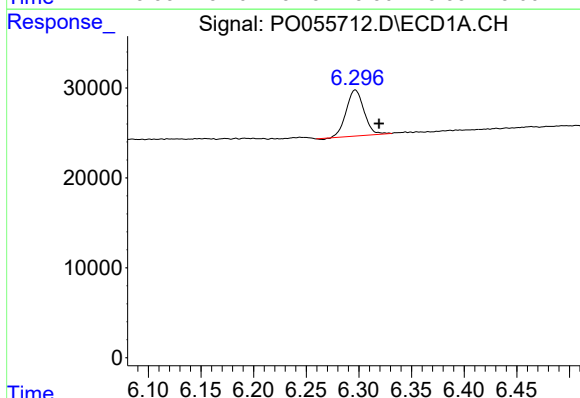


#24 AR-1248-4

R.T.: 6.297 min
Delta R.T.: -0.023 min
Response: 60097
Conc: 34.08 ng/ml

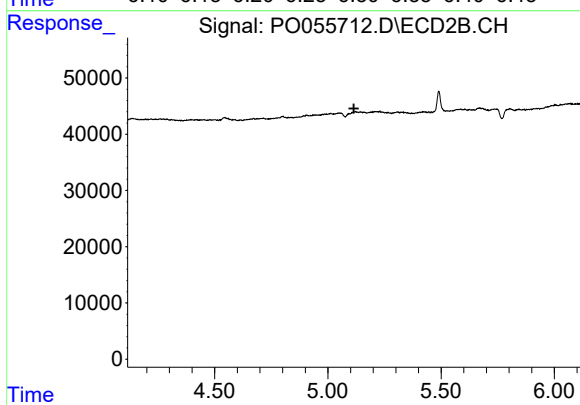

#24 AR-1248-4


R.T.: 0.000 min
Exp R.T.: 5.115 min
Response: 0
Conc: N.D.

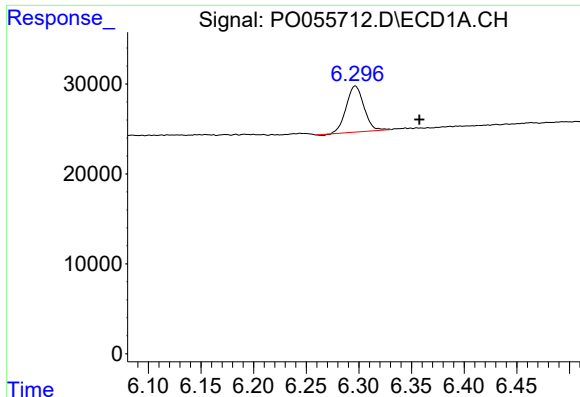

#25 AR-1248-5


R.T.: 6.297 min
Delta R.T.: -0.061 min
Response: 60097
Conc: 35.43 ng/ml

Instrument :
ECD_O
ClientSampleId :

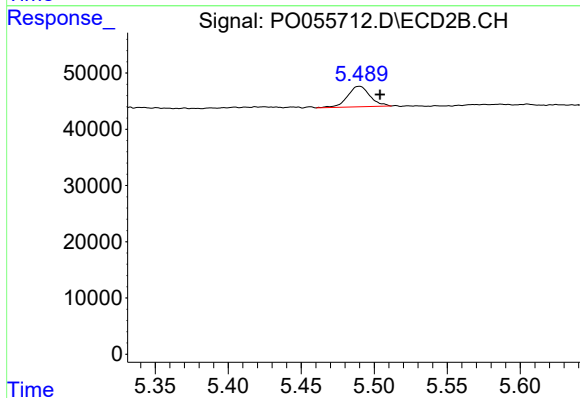


#25 AR-1248-5

R.T.: 5.490 min
Delta R.T.: -0.014 min
Response: 39198
Conc: 23.84 ng/ml

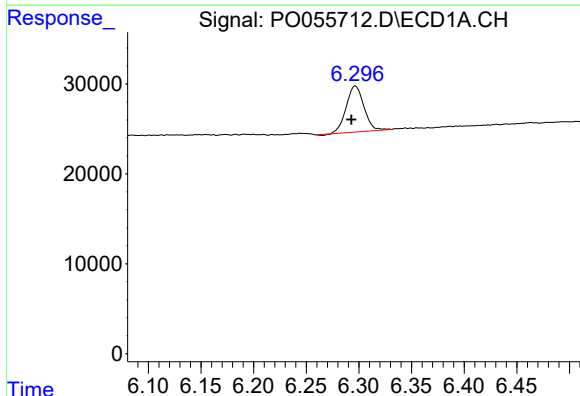


#26 AR-1254-1

R.T.: 6.297 min
Delta R.T.: 0.004 min
Response: 60097
Conc: 31.82 ng/ml

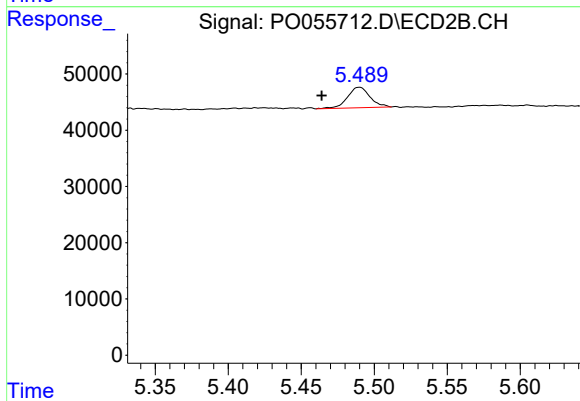

#26 AR-1254-1


R.T.: 5.490 min
Delta R.T.: 0.026 min
Response: 39198
Conc: 15.01 ng/ml

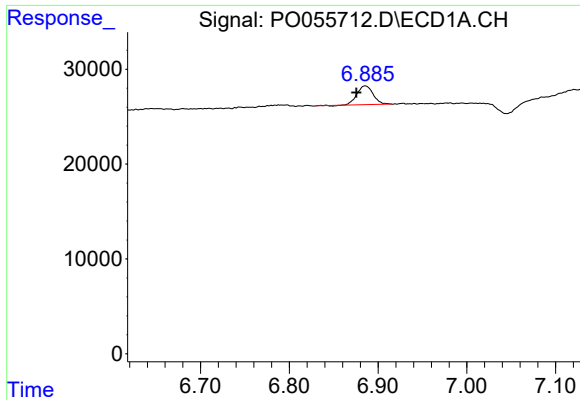

#28 AR-1254-3


R.T.: 6.886 min
Delta R.T.: 0.010 min
Response: 25076
Conc: 7.54 ng/ml

Instrument :
ECD_O
ClientSampleId :

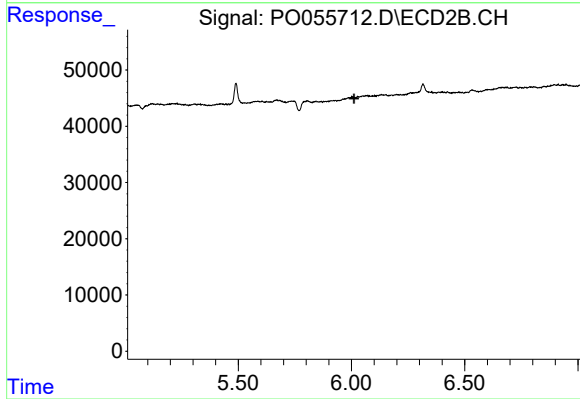


#28 AR-1254-3

R.T.: 0.000 min
Exp R.T. : 6.011 min
Response: 0
Conc: N.D.

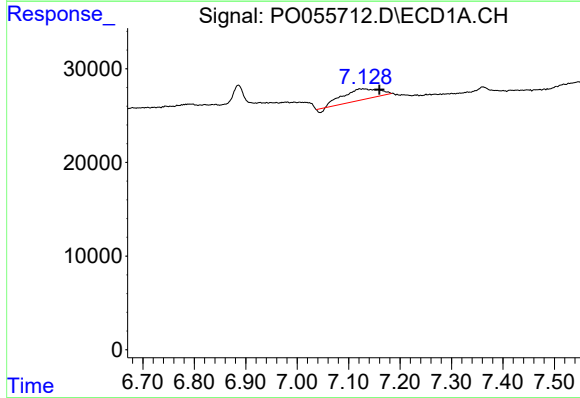


#29 AR-1254-4

R.T.: 7.128 min
Delta R.T.: -0.032 min
Response: 55294
Conc: 21.54 ng/ml

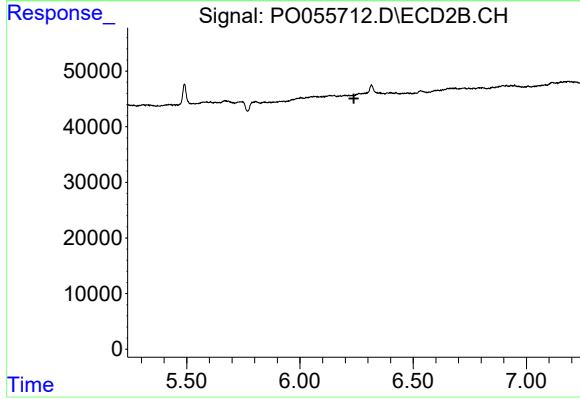

#29 AR-1254-4


R.T.: 0.000 min
Exp R.T. : 6.238 min
Response: 0
Conc: N.D.

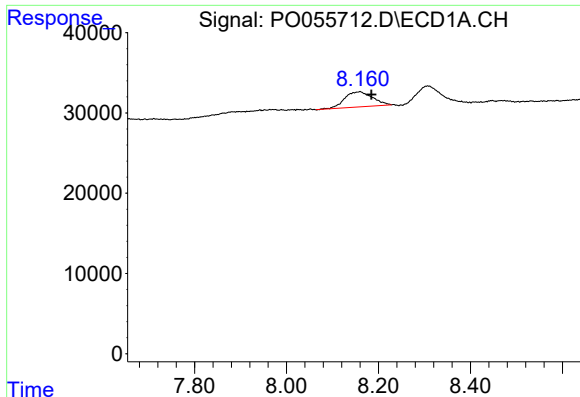

#35 AR-1260-5


R.T.: 8.160 min
Delta R.T.: -0.024 min
Response: 79796
Conc: 16.46 ng/ml

Instrument :
ECD_O
ClientSampleId :

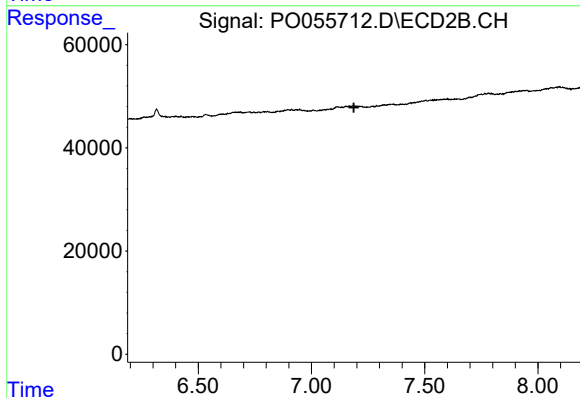


#35 AR-1260-5

R.T.: 0.000 min
Exp R.T. : 7.187 min
Response: 0
Conc: N.D.

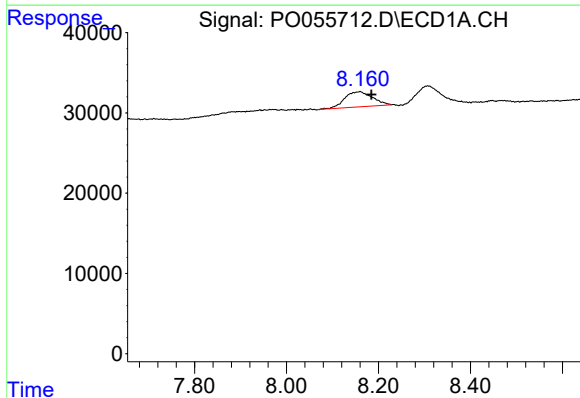

#37 AR-1262-2

R.T.: 8.160 min
Delta R.T.: -0.025 min
Response: 79796
Conc: 12.90 ng/ml

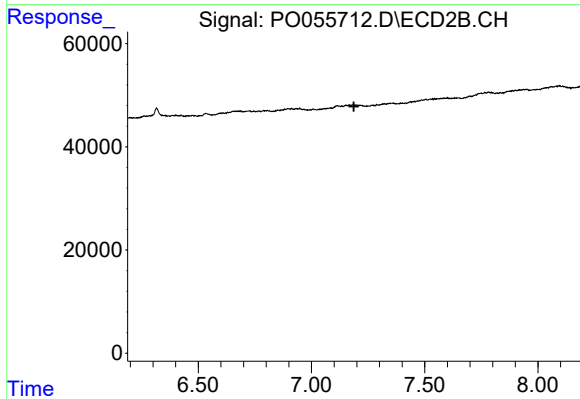

#37 AR-1262-2

R.T.: 0.000 min
Exp R.T. : 7.187 min
Response: 0
Conc: N.D.