

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\P0043019\
 Data File : P0055725.D
 Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
 Acq On : 30 Apr 2019 18:22
 Operator : SM/SJ
 Sample : K2564-02
 Misc :
 ALS Vial : 10 Sample Multiplier: 1

Instrument :
 ECD_O
 ClientSampleId :

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: May 01 00:51:55 2019
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\P0042919.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Tue Apr 30 05:21:50 2019
 Response via : Initial Calibration
 Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	4.280	3.594	589564	631418	20.961	21.645
2)	SA Decachlor...	9.881	8.546	559019	364436	13.089	11.472
Target Compounds							
7)	L1 AR-1016-5	0.000	5.128	0	50640	N.D.	40.950 #
15)	L3 AR-1232-5	0.000	5.128	0	50640	N.D.	99.417 #
24)	L5 AR-1248-4	0.000	5.128	0	50640	N.D.	31.765 #
28)	L6 AR-1254-3	6.881	0.000	41434	0	12.454	N.D. #
31)	L7 AR-1260-1	0.000	6.136	0	23839	N.D.	9.923 #
32)	L7 AR-1260-2	0.000	6.315	0	24421	N.D.	7.360 #
33)	L7 AR-1260-3	0.000	6.449	0	46326	N.D.	16.609 #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\P0043019\
Data File : P0055725.D
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
Acq On : 30 Apr 2019 18:22
Operator : SM/SJ
Sample : K2564-02
Misc :
ALS Vial : 10 Sample Multiplier: 1

Instrument :
ECD_O
ClientSampled :

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: May 01 00:51:55 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\P0042919.M
Quant Title : GC EXTRACTABLES
QLast Update : Tue Apr 30 05:21:50 2019
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µm Signal #2 Info : 30M x 0.32mm x 0.25µm

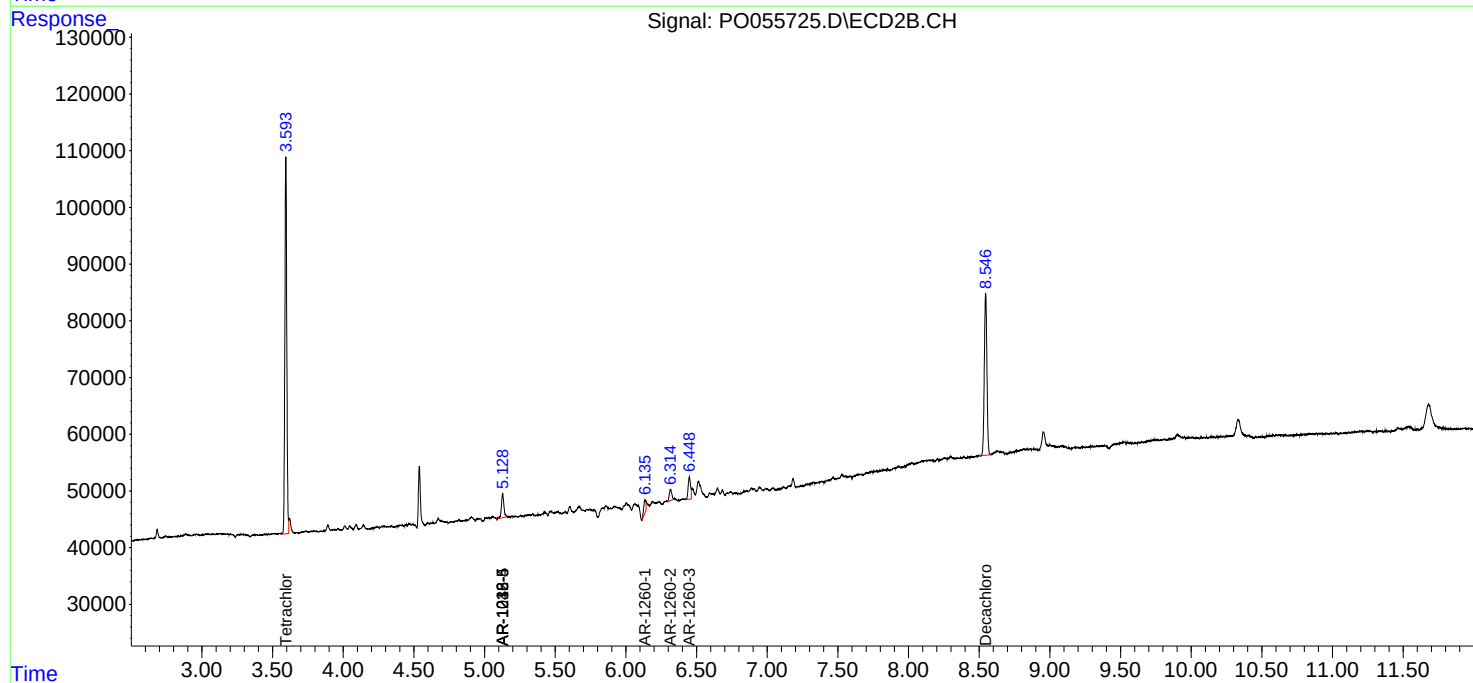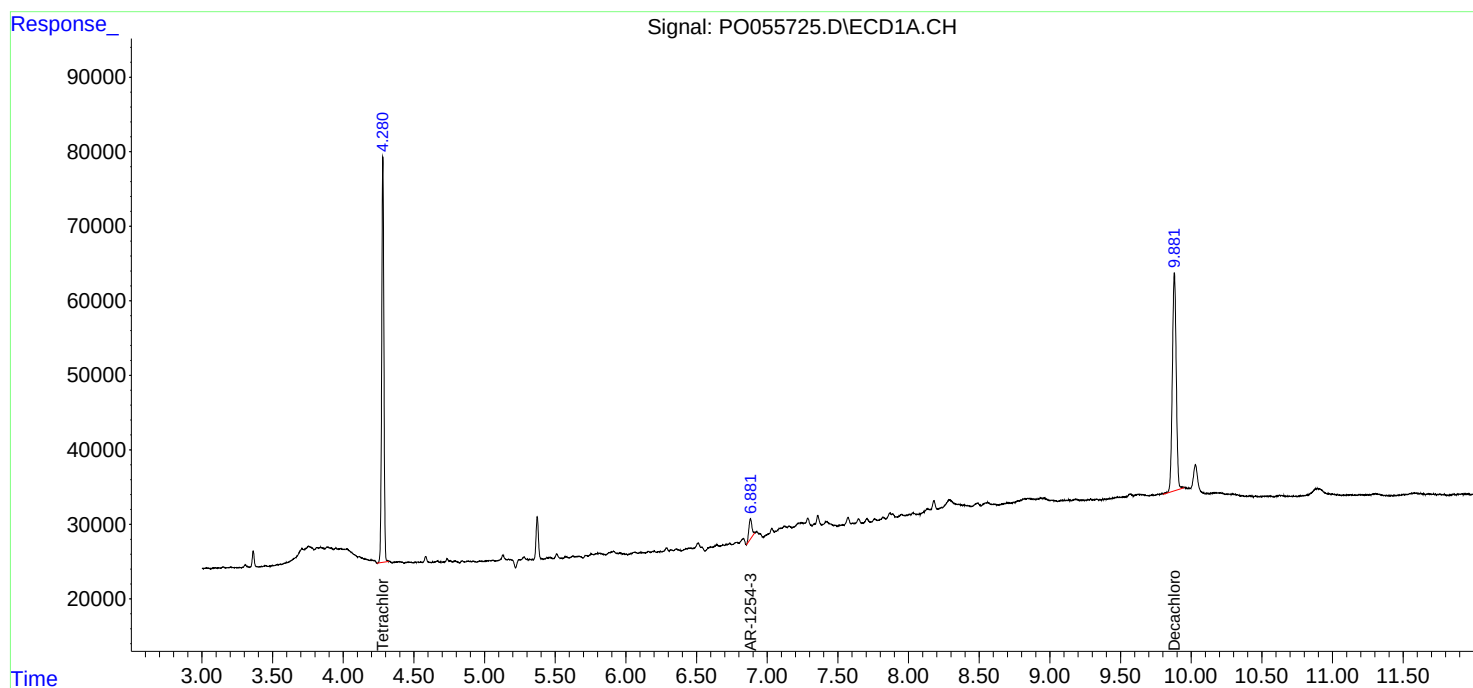


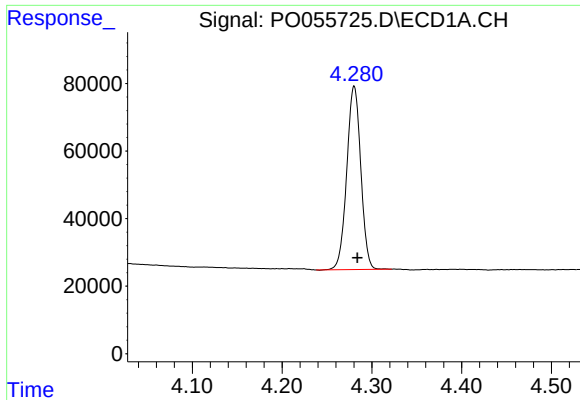

#1 Tetrachloro-m-xylene


R.T.: 4.280 min
Delta R.T.: -0.004 min
Response: 589564
Conc: 20.96 ng/ml

Instrument :
ECD_O
ClientSampleId :

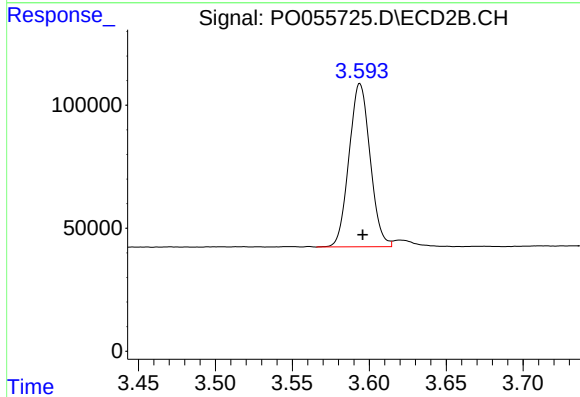


#1 Tetrachloro-m-xylene

R.T.: 3.594 min
Delta R.T.: -0.002 min
Response: 631418
Conc: 21.64 ng/ml

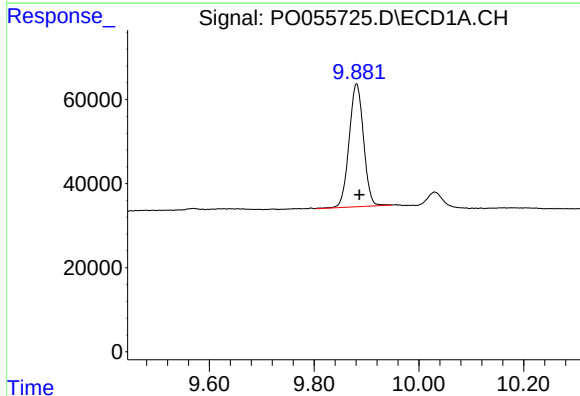


#2 Decachlorobiphenyl

R.T.: 9.881 min
Delta R.T.: -0.005 min
Response: 559019
Conc: 13.09 ng/ml

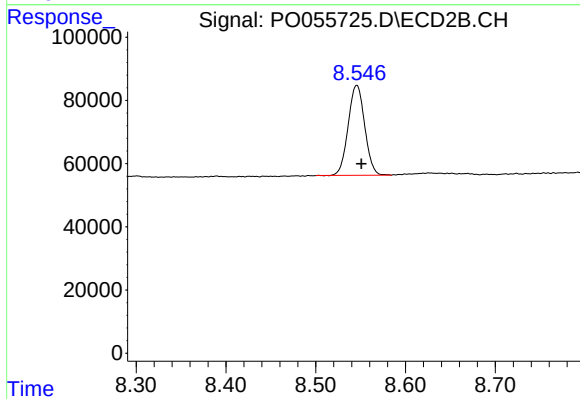

#2 Decachlorobiphenyl


R.T.: 8.546 min
Delta R.T.: -0.005 min
Response: 364436
Conc: 11.47 ng/ml

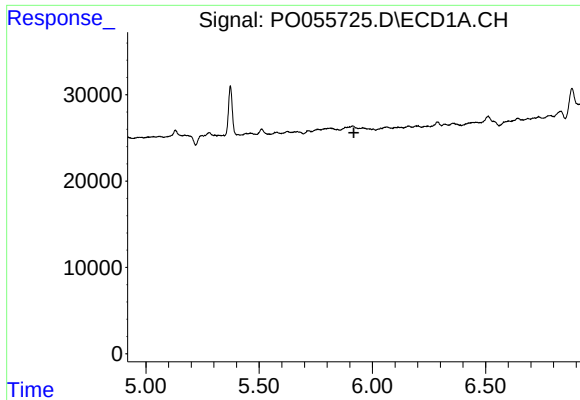

#7 AR-1016-5


R.T.: 0.000 min
Exp R.T. : 5.919 min
Response: 0
Conc: N.D.

Instrument :
ECD_O
ClientSampleId :

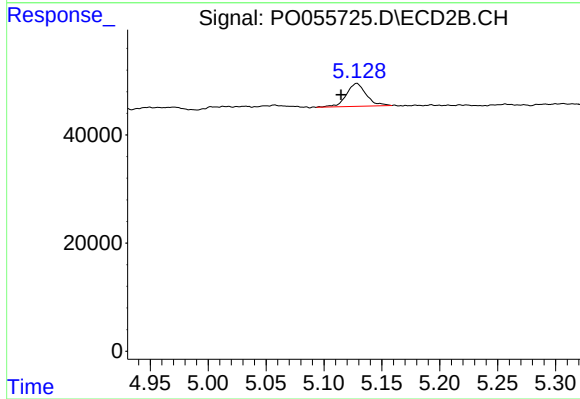


#7 AR-1016-5

R.T.: 5.128 min
Delta R.T.: 0.014 min
Response: 50640
Conc: 40.95 ng/ml

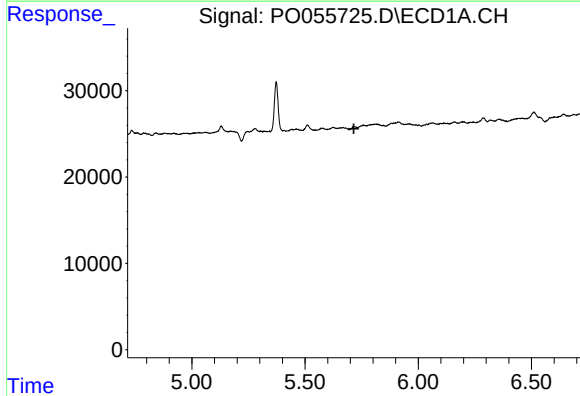


#15 AR-1232-5

R.T.: 0.000 min
Exp R.T. : 5.716 min
Response: 0
Conc: N.D.

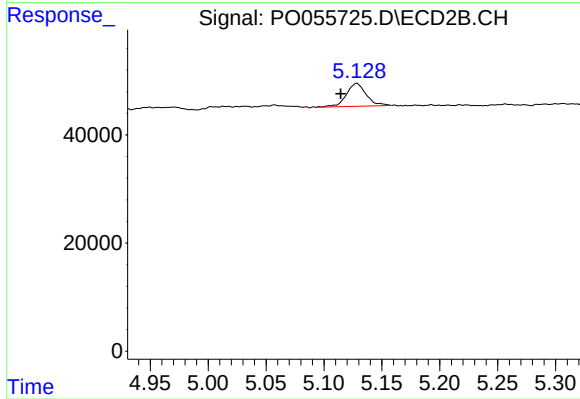

#15 AR-1232-5


R.T.: 5.128 min
Delta R.T.: 0.014 min
Response: 50640
Conc: 99.42 ng/ml

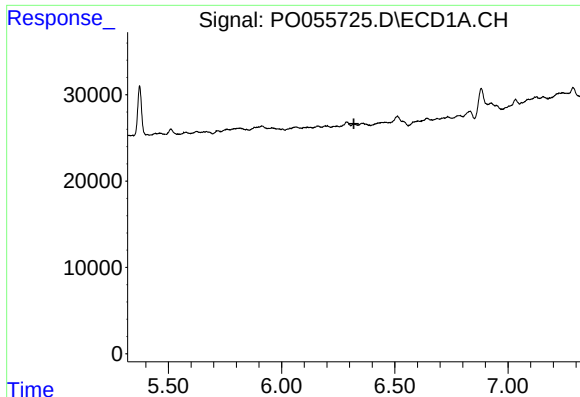

#24 AR-1248-4


R.T.: 0.000 min
Exp R.T.: 6.319 min
Response: 0
Conc: N.D.

Instrument :
ECD_O
ClientSampleId :

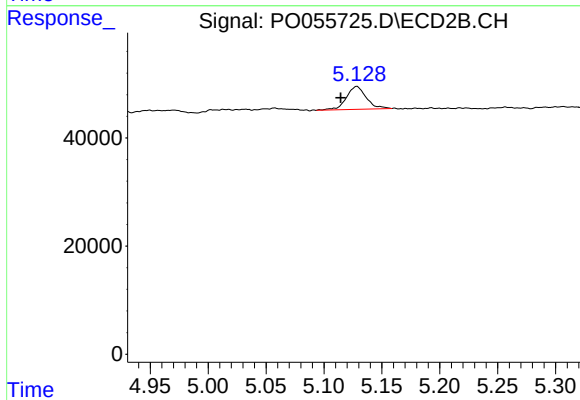


#24 AR-1248-4

R.T.: 5.128 min
Delta R.T.: 0.014 min
Response: 50640
Conc: 31.76 ng/ml

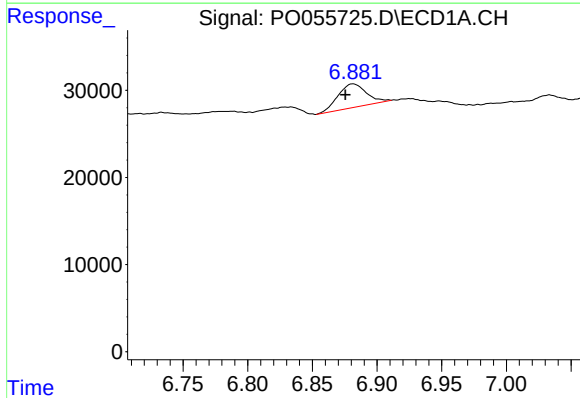


#28 AR-1254-3

R.T.: 6.881 min
Delta R.T.: 0.006 min
Response: 41434
Conc: 12.45 ng/ml

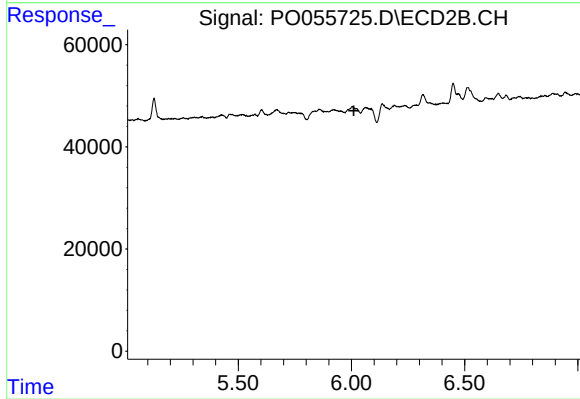

#28 AR-1254-3


R.T.: 0.000 min
Exp R.T.: 6.011 min
Response: 0
Conc: N.D.

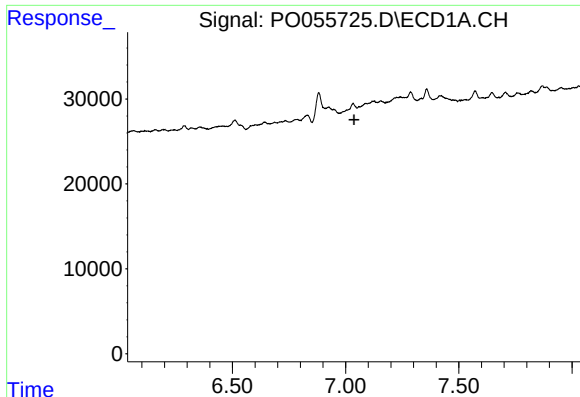

#31 AR-1260-1


R.T.: 0.000 min
Exp R.T.: 7.037 min
Response: 0
Conc: N.D.

Instrument :
ECD_O
ClientSampleId :

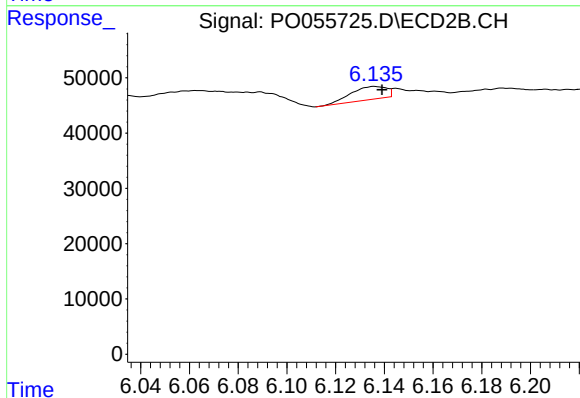


#31 AR-1260-1

R.T.: 6.136 min
Delta R.T.: -0.003 min
Response: 23839
Conc: 9.92 ng/ml

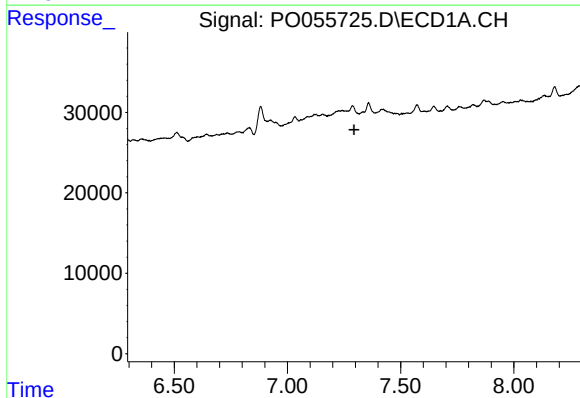


#32 AR-1260-2

R.T.: 0.000 min
Exp R.T.: 7.294 min
Response: 0
Conc: N.D.

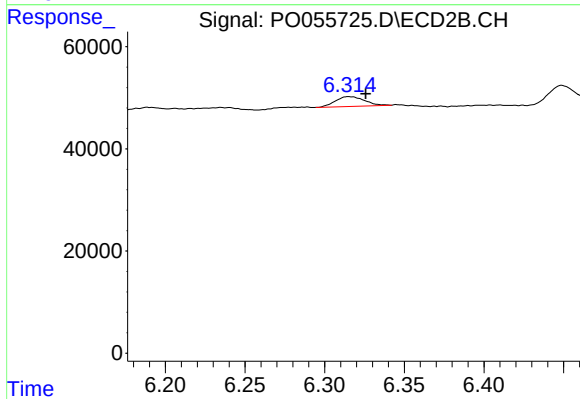

#32 AR-1260-2


R.T.: 6.315 min
Delta R.T.: -0.011 min
Response: 24421
Conc: 7.36 ng/ml

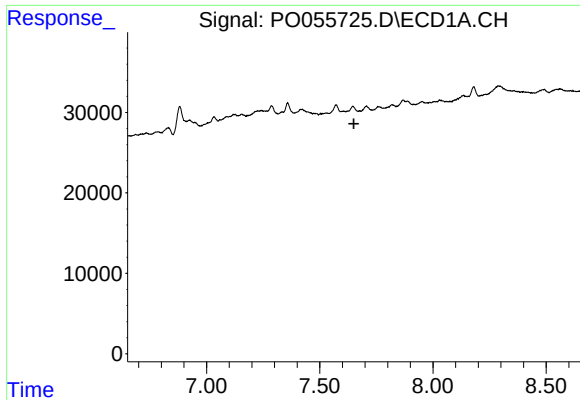

#33 AR-1260-3

R.T.: 0.000 min
Exp R.T.: 7.650 min
Response: 0
Conc: N.D.

Instrument :
ECD_O
ClientSampleId :

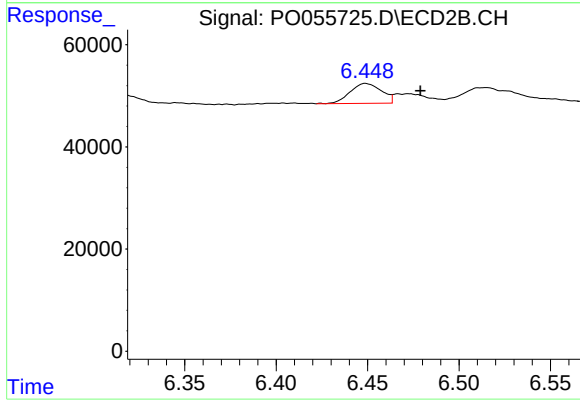

#33 AR-1260-3

R.T.: 6.449 min
Delta R.T.: -0.030 min
Response: 46326
Conc: 16.61 ng/ml