

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\P0043019\
 Data File : P0055705.D
 Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
 Acq On : 30 Apr 2019 10:12
 Operator : SM/SJ
 Sample : K2578-01
 Misc :
 ALS Vial : 4 Sample Multiplier: 1

Instrument :
 ECD_O
 ClientSampleId :
 WATER-COMP

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Apr 30 11:39:32 2019
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\P0042919.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Tue Apr 30 05:21:50 2019
 Response via : Initial Calibration
 Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	4.298	3.598	548263	622839	19.493	21.351
2) SA Decachlor...	9.910	8.556	350869	190832	8.215	6.007 #

Target Compounds



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\P0043019\
Data File : P0055705.D
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
Acq On : 30 Apr 2019 10:12
Operator : SM/SJ
Sample : K2578-01
Misc :
ALS Vial : 4 Sample Multiplier: 1

Instrument :
ECD_O
ClientSampleId :
WATER-COMP

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Apr 30 11:39:32 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\P0042919.M
Quant Title : GC EXTRACTABLES
QLast Update : Tue Apr 30 05:21:50 2019
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

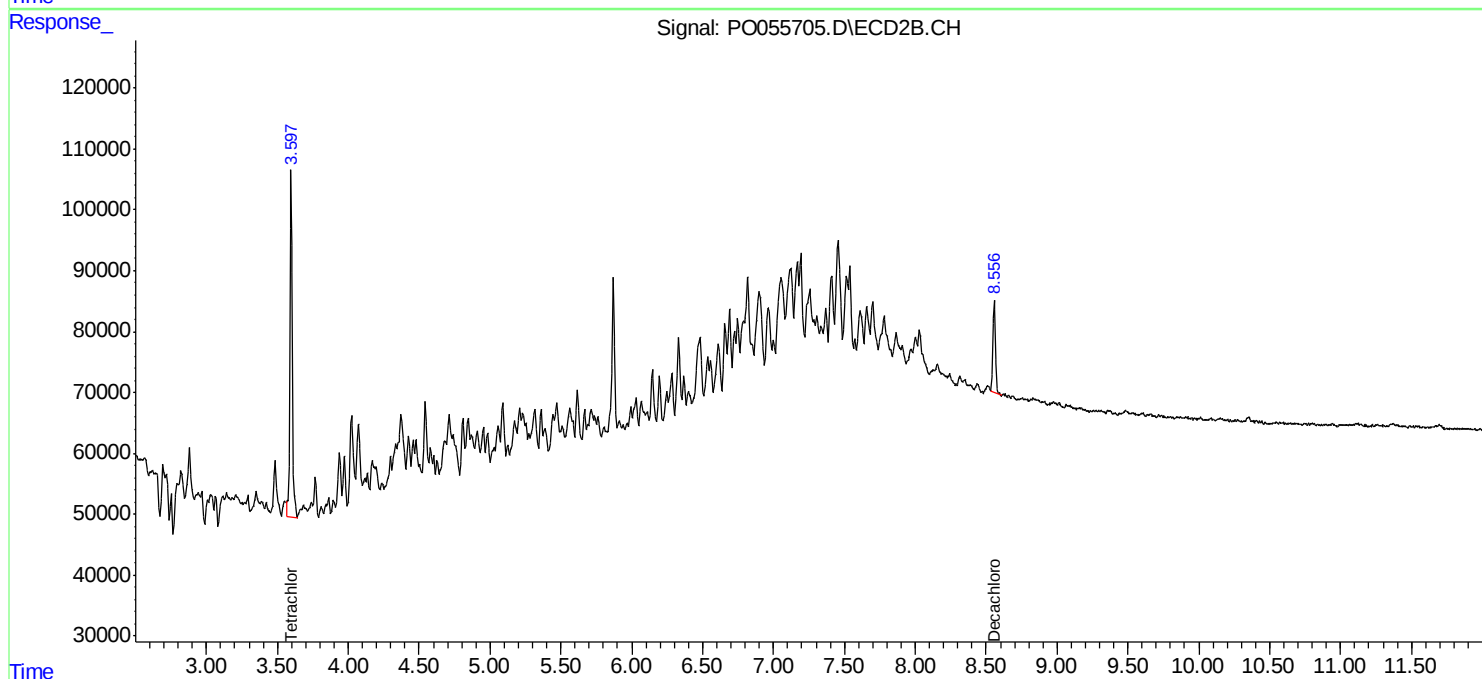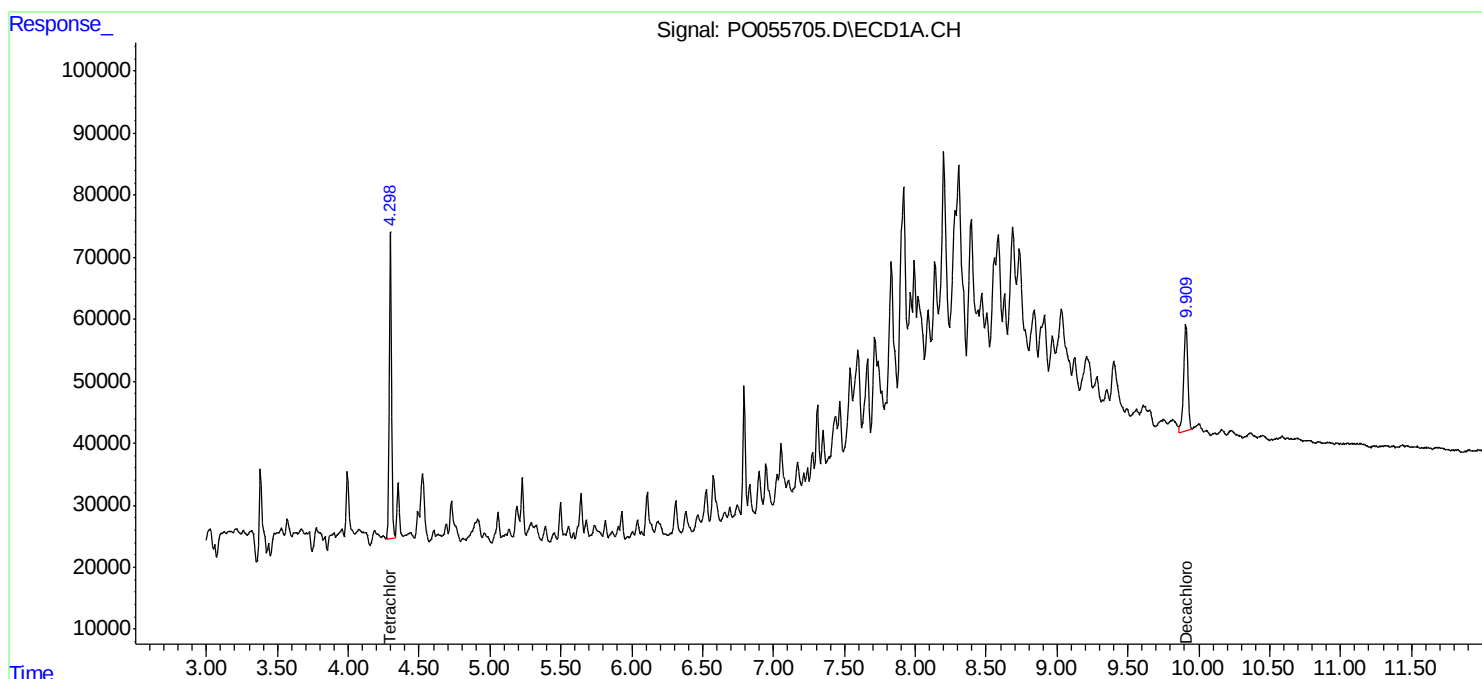


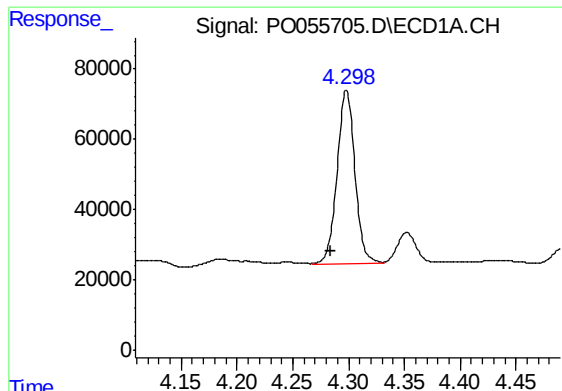

#1 Tetrachloro-m-xylene


R.T.: 4.298 min
Delta R.T.: 0.014 min
Response: 548263
Conc: 19.49 ng/ml

Instrument :
ECD_O
ClientSampleId :
WATER-COMP

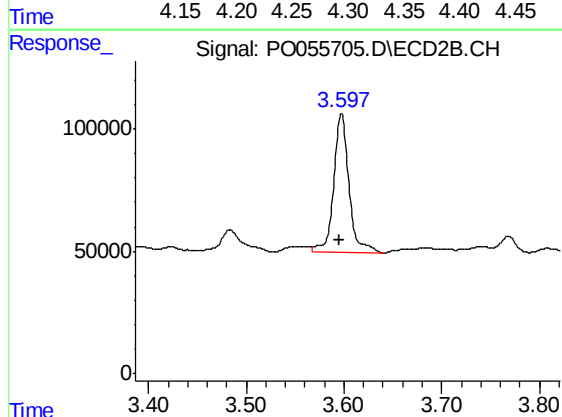


#1 Tetrachloro-m-xylene

R.T.: 3.598 min
Delta R.T.: 0.002 min
Response: 622839
Conc: 21.35 ng/ml

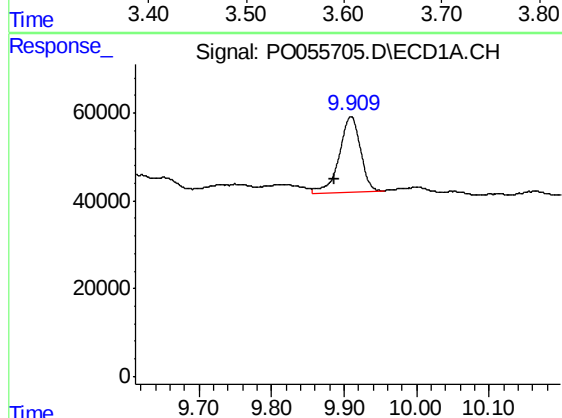

#2 Decachlorobiphenyl

R.T.: 9.910 min
Delta R.T.: 0.023 min
Response: 350869
Conc: 8.22 ng/ml

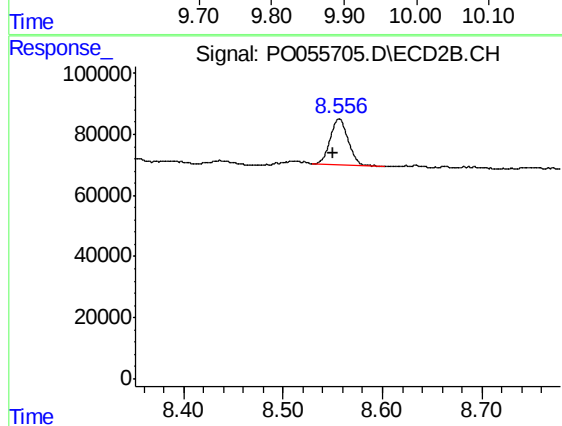

#2 Decachlorobiphenyl

R.T.: 8.556 min
Delta R.T.: 0.005 min
Response: 190832
Conc: 6.01 ng/ml