

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\P0043020\
 Data File : P0068084.D
 Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
 Acq On : 30 Apr 2020 8:59
 Operator : DD\AJ
 Sample : PB128515BL
 Misc :
 ALS Vial : 4 Sample Multiplier: 1

Instrument :
 ECD_O
 ClientSampleId :
 PB128515BL

Manual Integrations
 APPROVED

Sohil
 5/1/2020 8:35:00 AM

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Apr 30 10:38:17 2020
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\P0042720.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Tue Apr 28 07:12:58 2020
 Response via : Initial Calibration
 Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	4.914	3.936	471262	622667	19.693	19.486
2) SA Decachlor...	10.879	9.212	762945	837229	20.216m	21.693

Target Compounds

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\P0043020\
Data File : P0068084.D
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
Acq On : 30 Apr 2020 8:59
Operator : DD\AJ
Sample : PB128515BL
Misc :
ALS Vial : 4 Sample Multiplier: 1



Instrument :
ECD_O
ClientSampleId :
PB128515BL


Manual Integrations
APPROVED

Sohil
5/1/2020 8:35:00 AM

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Apr 30 10:38:17 2020
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\P0042720.M
Quant Title : GC EXTRACTABLES
QLast Update : Tue Apr 28 07:12:58 2020
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

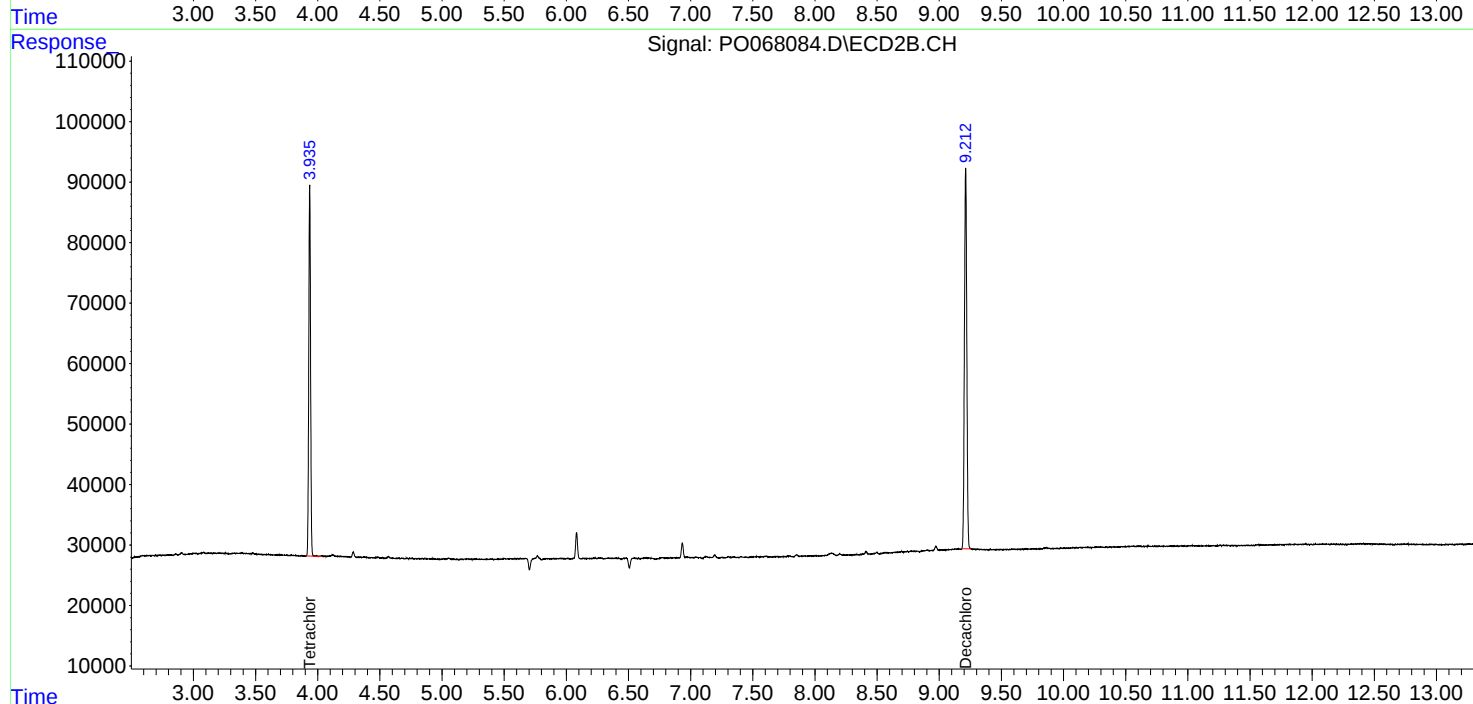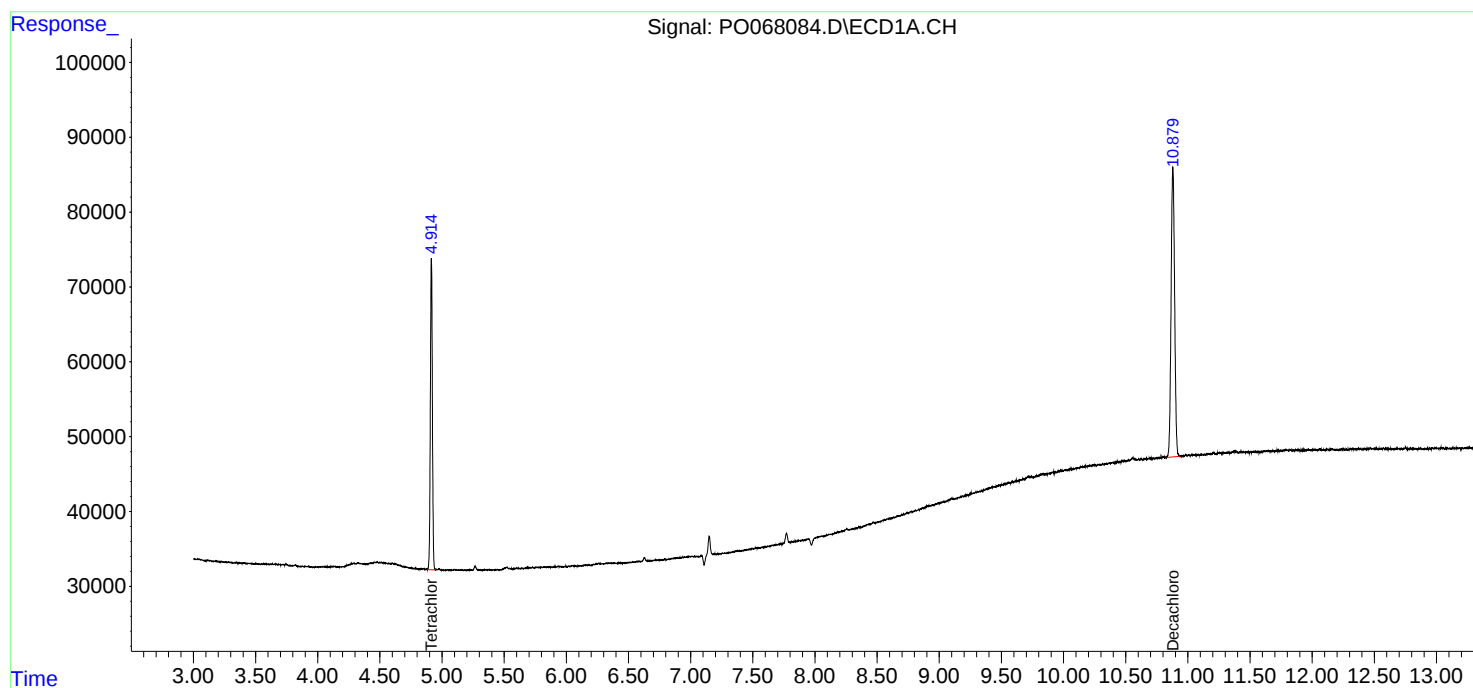

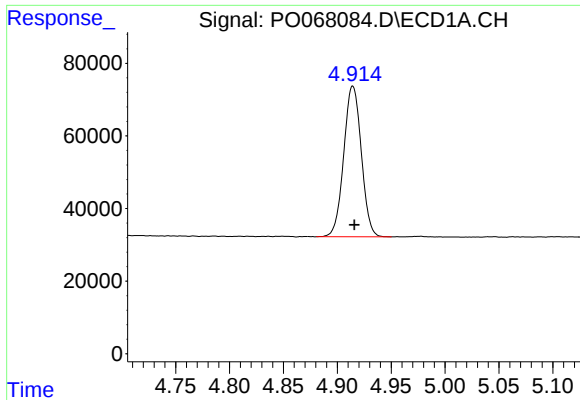


#1 Tetrachloro-m-xylene

R.T.: 4.914 min
Delta R.T.: -0.002 min
Response: 471262
Conc: 19.69 ng/ml

Instrument :
ECD_O
ClientSampleId :
PB128515BL


Manual Integrations
APPROVED

Sohil
5/1/2020 8:35:00 AM

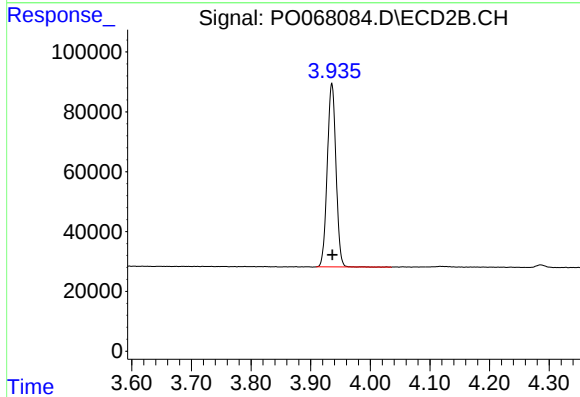


#1 Tetrachloro-m-xylene

R.T.: 3.936 min
Delta R.T.: 0.000 min
Response: 622667
Conc: 19.49 ng/ml

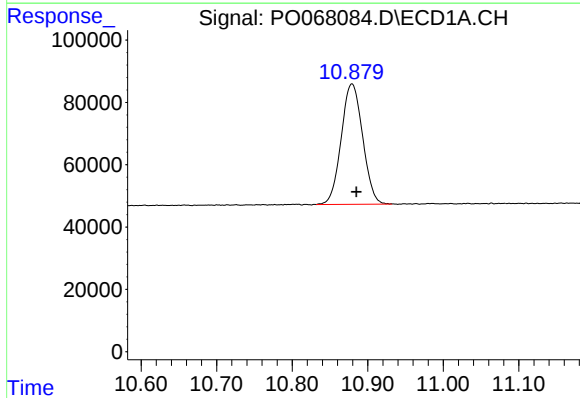

#2 Decachlorobiphenyl

R.T.: 10.879 min
Delta R.T.: -0.006 min
Response: 762945
Conc: 20.22 ng/ml m

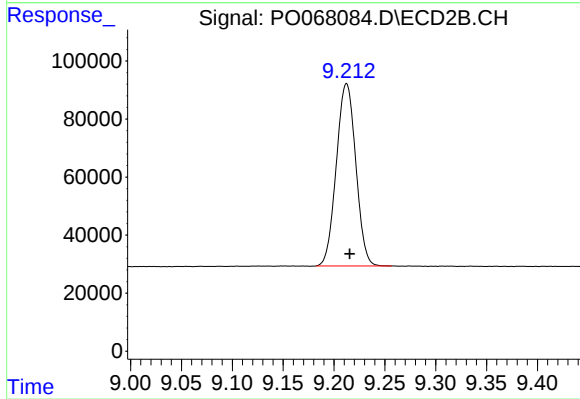

#2 Decachlorobiphenyl

R.T.: 9.212 min
Delta R.T.: -0.003 min
Response: 837229
Conc: 21.69 ng/ml