

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\P0043020\
 Data File : P0068088.D
 Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
 Acq On : 30 Apr 2020 10:27
 Operator : DD\AJ
 Sample : L2430-01 5X
 Misc :
 ALS Vial : 8 Sample Multiplier: 1

Instrument :
 ECD_O
 ClientSampleId :
 37-ST-2020

Manual Integrations
 APPROVED

Sohil
 5/1/2020 8:35:04 AM

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Apr 30 10:47:30 2020
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\P0042720.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Tue Apr 28 07:12:58 2020
 Response via : Initial Calibration
 Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	4.915	3.934	85847	134413	3.587m	4.206m
2) SA Decachlor...	10.879	9.211	221904	252509	5.880m	6.543m

Target Compounds

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\P0043020\
Data File : P0068088.D
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
Acq On : 30 Apr 2020 10:27
Operator : DD\AJ
Sample : L2430-01 5X
Misc :
ALS Vial : 8 Sample Multiplier: 1



Instrument :
ECD_O
ClientSampleID :
37-ST-2020


Manual Integrations
APPROVED

Sohil
5/1/2020 8:35:04 AM

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Apr 30 10:47:30 2020
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\P0042720.M
Quant Title : GC EXTRACTABLES
QLast Update : Tue Apr 28 07:12:58 2020
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

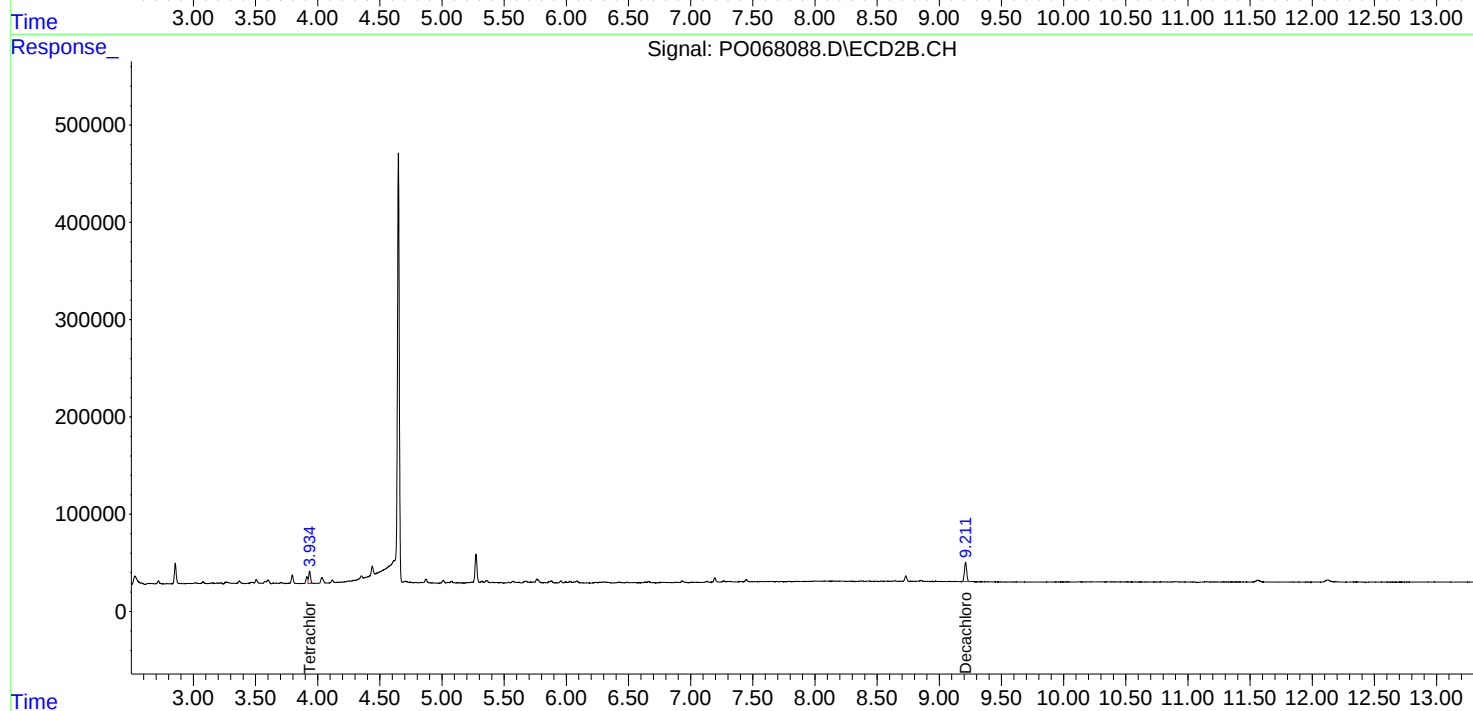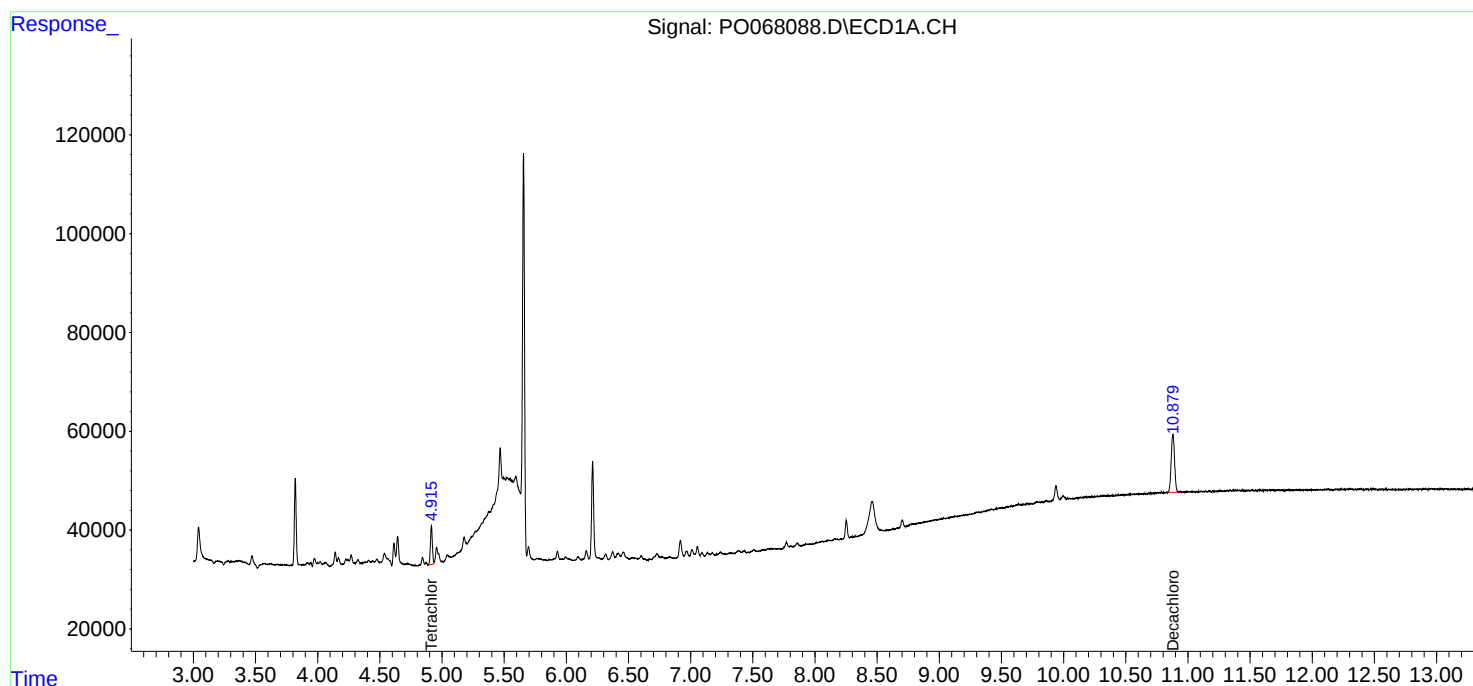

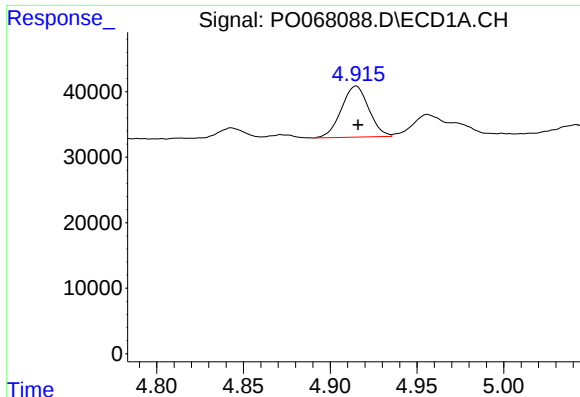


#1 Tetrachloro-m-xylene

R.T.: 4.915 min
Delta R.T.: -0.001 min
Response: 85847
Conc: 3.59 ng/ml m

Instrument :
ECD_O
ClientSampleId :
37-ST-2020


Manual Integrations
APPROVED

Sohil
5/1/2020 8:35:04 AM

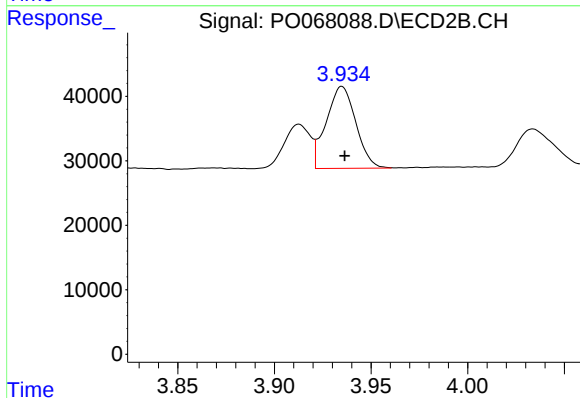


#1 Tetrachloro-m-xylene

R.T.: 3.934 min
Delta R.T.: -0.002 min
Response: 134413
Conc: 4.21 ng/ml m

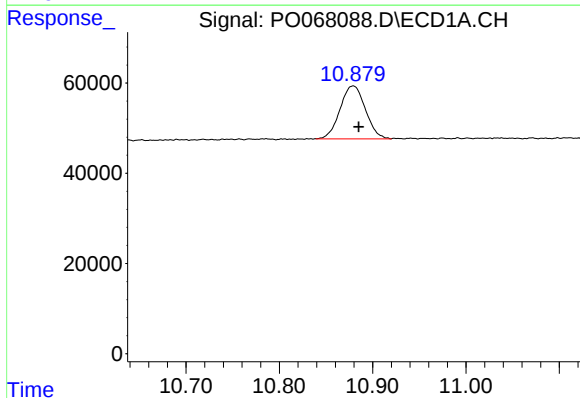

#2 Decachlorobiphenyl

R.T.: 10.879 min
Delta R.T.: -0.006 min
Response: 221904
Conc: 5.88 ng/ml m

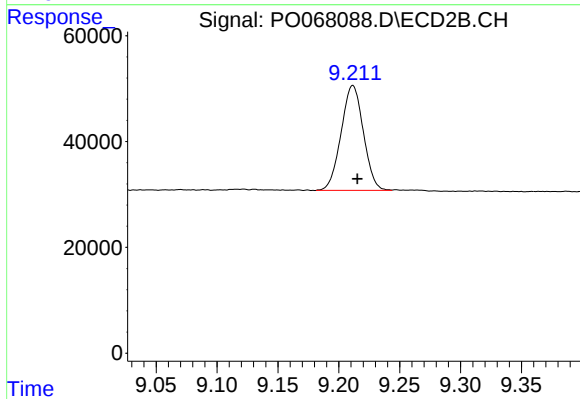

#2 Decachlorobiphenyl

R.T.: 9.211 min
Delta R.T.: -0.004 min
Response: 252509
Conc: 6.54 ng/ml m