

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\P0043020\
 Data File : P0068090.D
 Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
 Acq On : 30 Apr 2020 11:01
 Operator : DD\AJ
 Sample : L2408-05MS
 Misc :
 ALS Vial : 10 Sample Multiplier: 1

Instrument :
 ECD_O
 ClientSampleId :
 HP-627MS

Manual Integrations
 APPROVED

Sohil
 5/1/2020 8:35:07 AM

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Apr 30 12:27:08 2020
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\P0042720.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Tue Apr 28 07:12:58 2020
 Response via : Initial Calibration
 Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	4.914	3.935	1313357	1042479	54.883	32.623m#
2) SA Decachlor...	10.879	9.213	577044	542695	15.290	14.061

Target Compounds

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\PO043020\
Data File : PO068090.D
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
Acq On : 30 Apr 2020 11:01
Operator : DD\AJ
Sample : L2408-05MS
Misc :
ALS Vial : 10 Sample Multiplier: 1



Instrument :
ECD_O
ClientSampleId :
HP-627MS


Manual Integrations
APPROVED

Sohil
5/1/2020 8:35:07 AM

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Apr 30 12:27:08 2020
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\PO042720.M
Quant Title : GC EXTRACTABLES
QLast Update : Tue Apr 28 07:12:58 2020
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

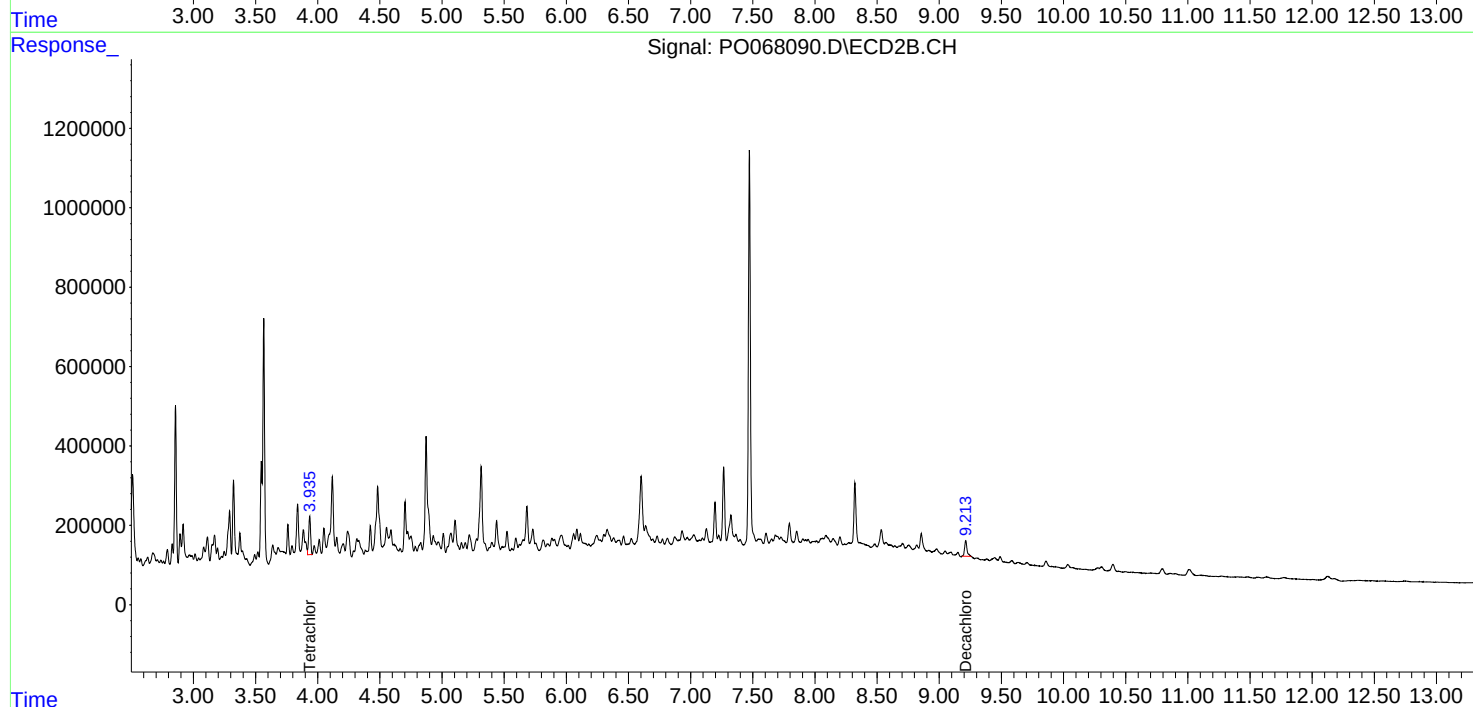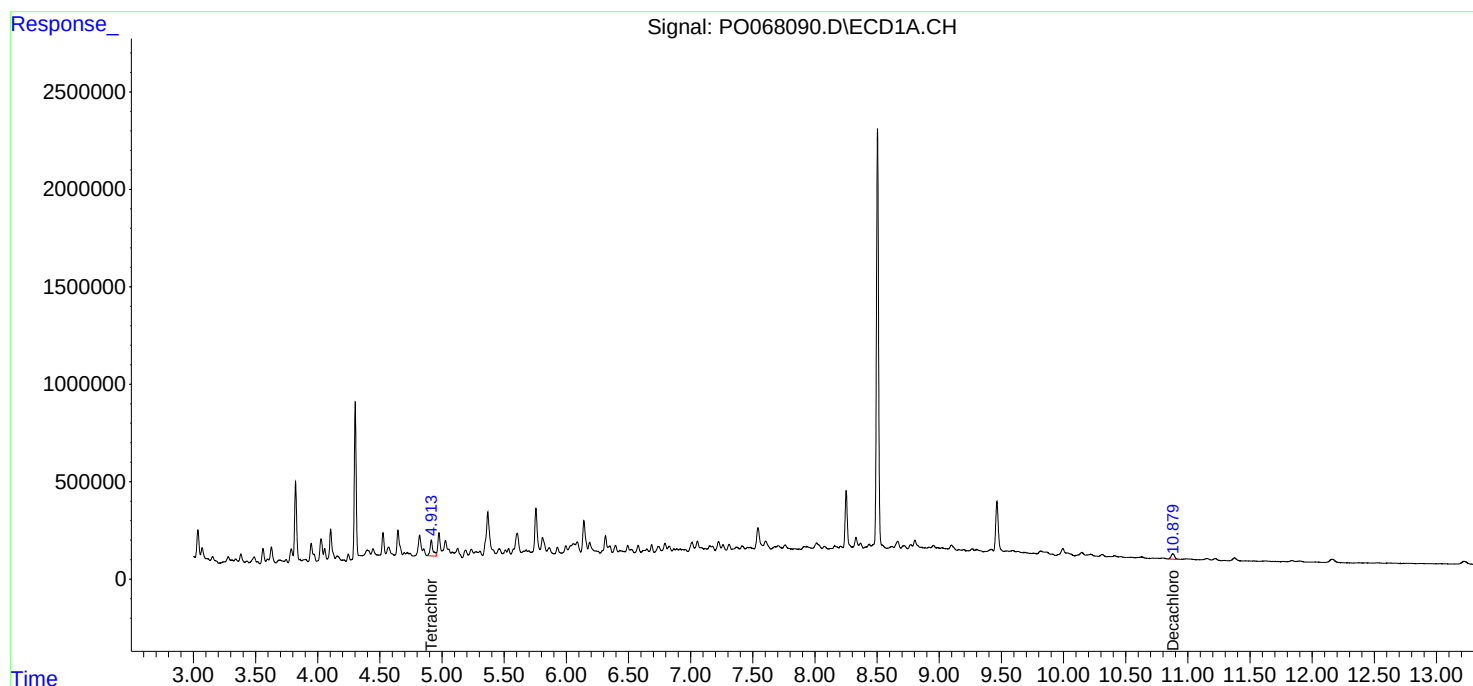

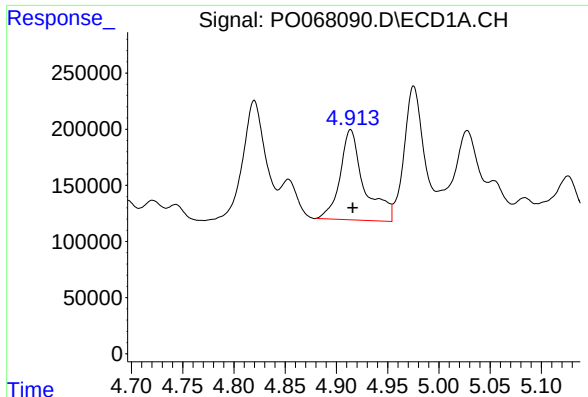


#1 Tetrachloro-m-xylene

R.T.: 4.914 min
Delta R.T.: -0.002 min
Response: 1313357
Conc: 54.88 ng/ml

Instrument :
ECD_O
ClientSampleId :
HP-627MS


Manual Integrations
APPROVED

Sohil
5/1/2020 8:35:07 AM

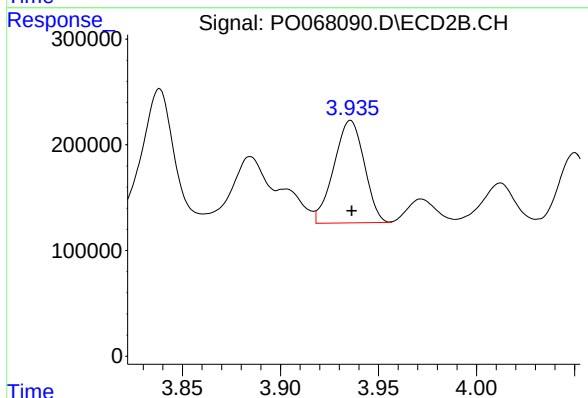


#1 Tetrachloro-m-xylene

R.T.: 3.935 min
Delta R.T.: 0.000 min
Response: 1042479
Conc: 32.62 ng/ml m

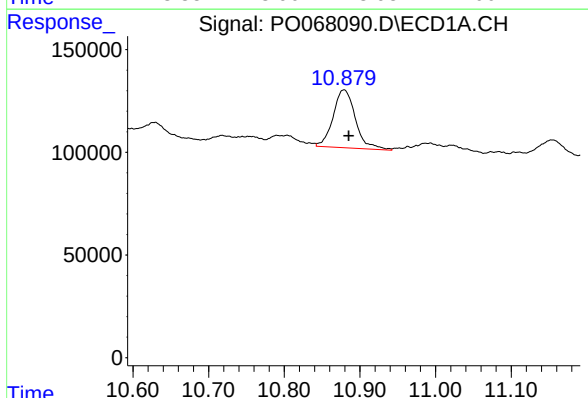

#2 Decachlorobiphenyl

R.T.: 10.879 min
Delta R.T.: -0.006 min
Response: 577044
Conc: 15.29 ng/ml

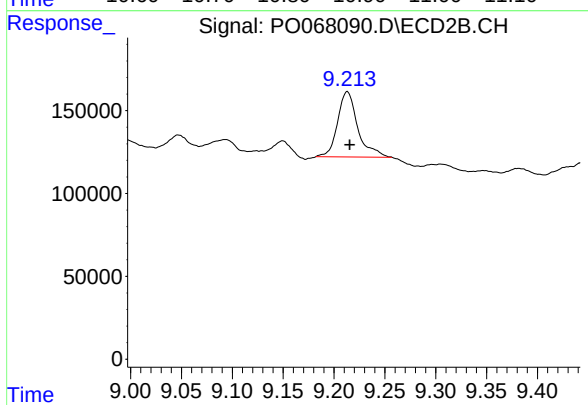

#2 Decachlorobiphenyl

R.T.: 9.213 min
Delta R.T.: -0.002 min
Response: 542695
Conc: 14.06 ng/ml