

Data Path : P:\HPCHEM1\ECD_0\Data\P0050118\
Data File : P0044295.D
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
Acq On : 01 May 2018 23:06
Operator : SM/UA
Sample : J2553-10
Misc :
ALS Vial : 25 Sample Multiplier: 1

Instrument :
ECD_O
ClientSampleId :
BPS1-SB4019-2025

Manual Integrations
APPROVED

UGO
5/2/2018 12:12:21 PM

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: May 02 03:31:08 2018
Quant Method : P:\HPCHEM1\ECD_0\methods\P0042518.M
Quant Title : GC EXTRACTABLES
QLast Update : Thu Apr 26 04:36:05 2018
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	4.038	3.295	12155847	14575230	16.981	15.067
2)	SA Decachlor...	9.376	8.052	10243930	12872935	16.631m	15.512m

Target Compounds

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : P:\HPCHEM1\ECD_0\Data\P0050118\
Data File : P0044295.D
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
Acq On : 01 May 2018 23:06
Operator : SM/UA
Sample : J2553-10
Misc :
ALS Vial : 25 Sample Multiplier: 1



Instrument :
ECD_O
ClientSampleId :
BPS1-SB4019-2025


Manual Integrations
APPROVED

UGO
5/2/2018 12:12:21 PM

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: May 02 03:31:08 2018
Quant Method : P:\HPCHEM1\ECD_0\methods\P0042518.M
Quant Title : GC EXTRACTABLES
QLast Update : Thu Apr 26 04:36:05 2018
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

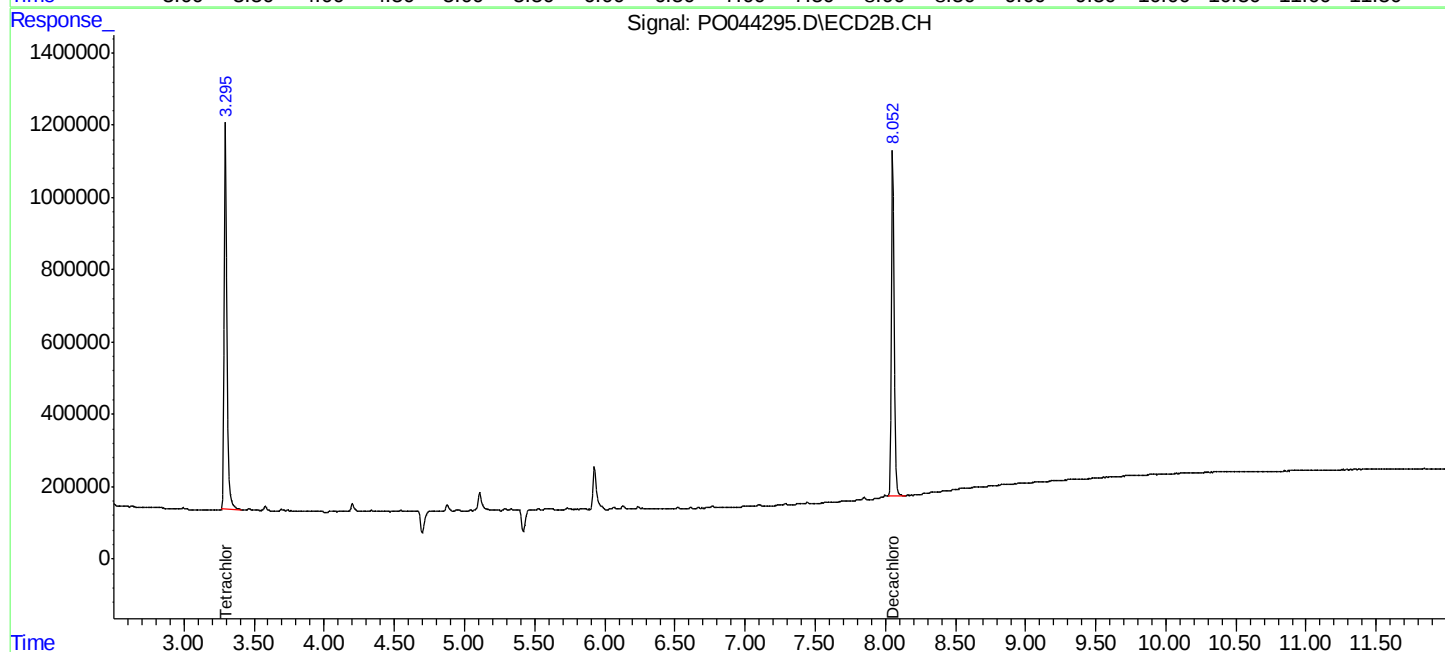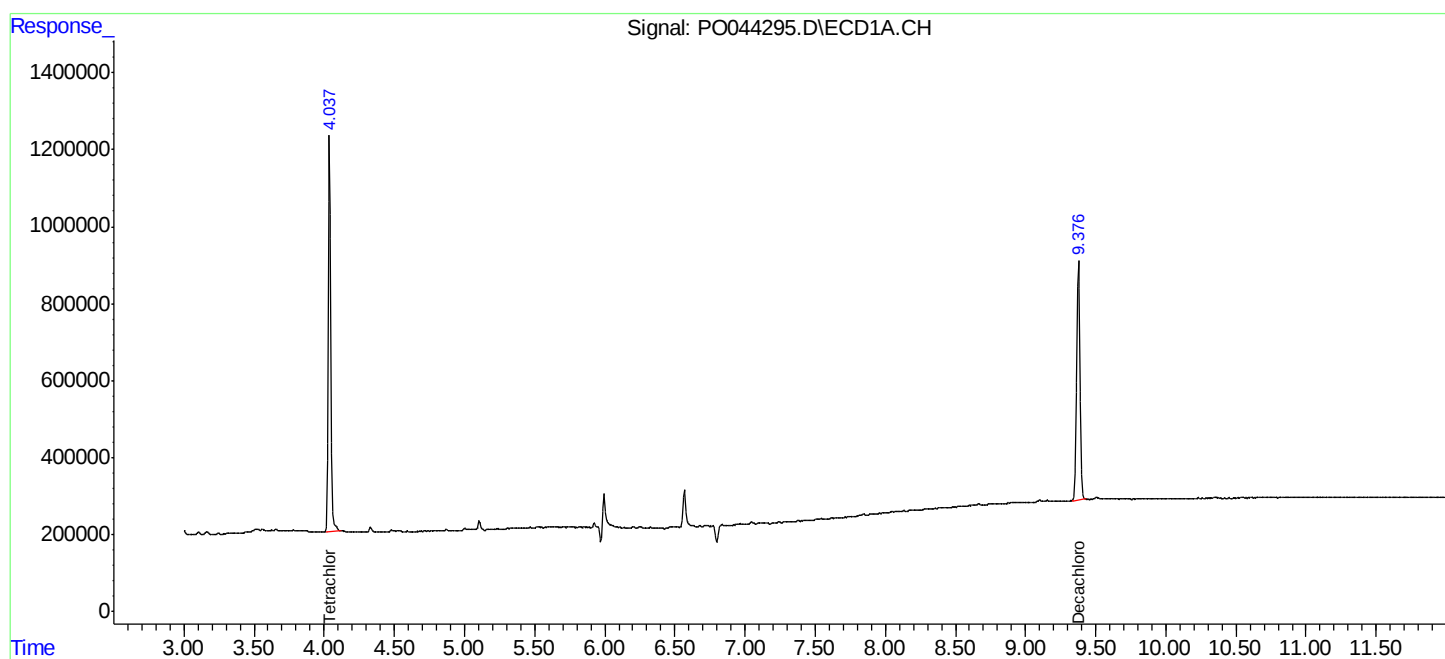

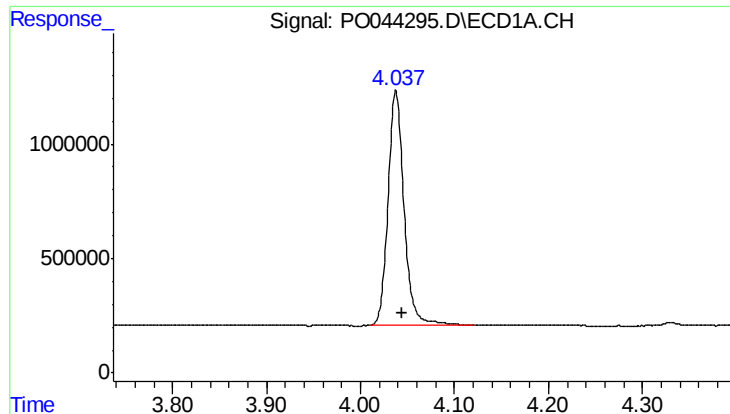


#1 Tetrachloro-m-xylene

R.T.: 4.038 min
Delta R.T.: -0.006 min
Response: 12155847
Conc: 16.98 ng/ml

Instrument :
ECD_O
ClientSampleId :
BPS1-SB4019-2025


Manual Integrations
APPROVED

UGO
5/2/2018 12:12:21 PM

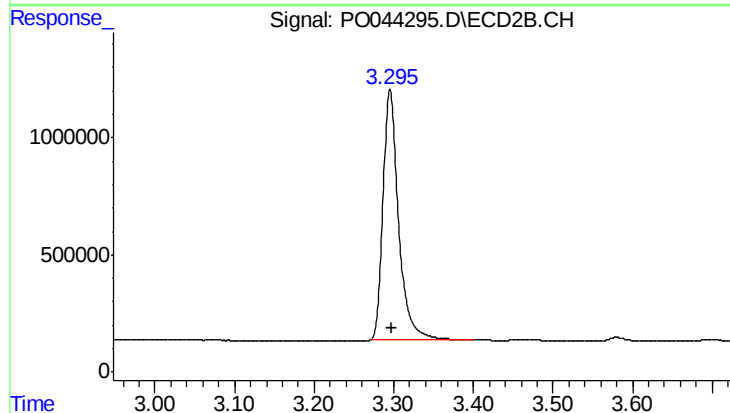


#1 Tetrachloro-m-xylene

R.T.: 3.295 min
Delta R.T.: -0.003 min
Response: 14575230
Conc: 15.07 ng/ml

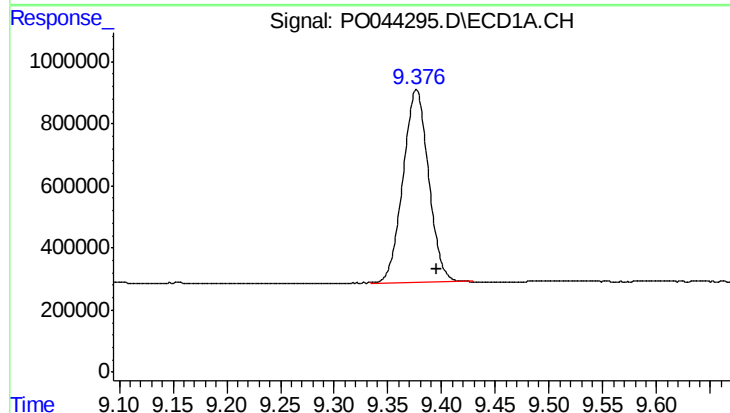

#2 Decachlorobiphenyl

R.T.: 9.376 min
Delta R.T.: -0.020 min
Response: 10243930
Conc: 16.63 ng/ml m

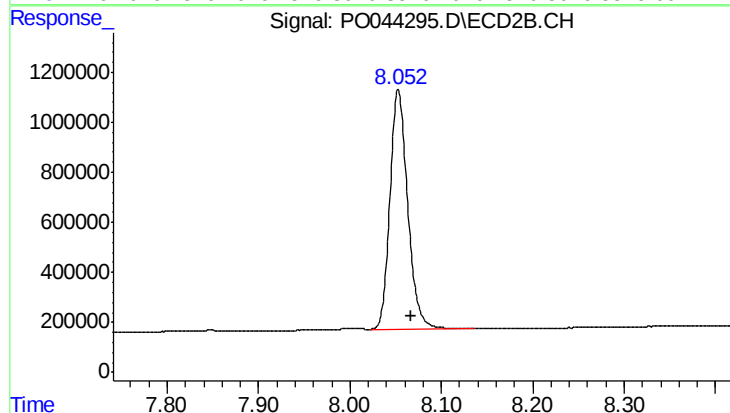

#2 Decachlorobiphenyl

R.T.: 8.052 min
Delta R.T.: -0.014 min
Response: 12872935
Conc: 15.51 ng/ml m